

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090518\
 Data File : BE097410.D
 Acq On : 5 Sep 2018 17:50
 Operator : SJ/JU
 Sample : PB112580BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Sep 06 01:29:55 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 06 01:29:05 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	827	0.40	ng/ul	0.00
2) Naphthalene-d8	10.12	136	4262	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.01	164	2891	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.86	188	647573	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-20.97
20) Perylene-d12	23.20	264	13563	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.72	152	2587	0.39	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.01	166	882	0.085	ng/ul#	21
23) Benzo(a)pyrene	23.06	252	2655	0.079	ng/ul	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090518\
Data File : BE097410.D
Acq On : 5 Sep 2018 17:50
Operator : SJ/JU
Sample : PB112580BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Sep 06 01:29:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 06 01:29:05 2018
Response via : Initial Calibration




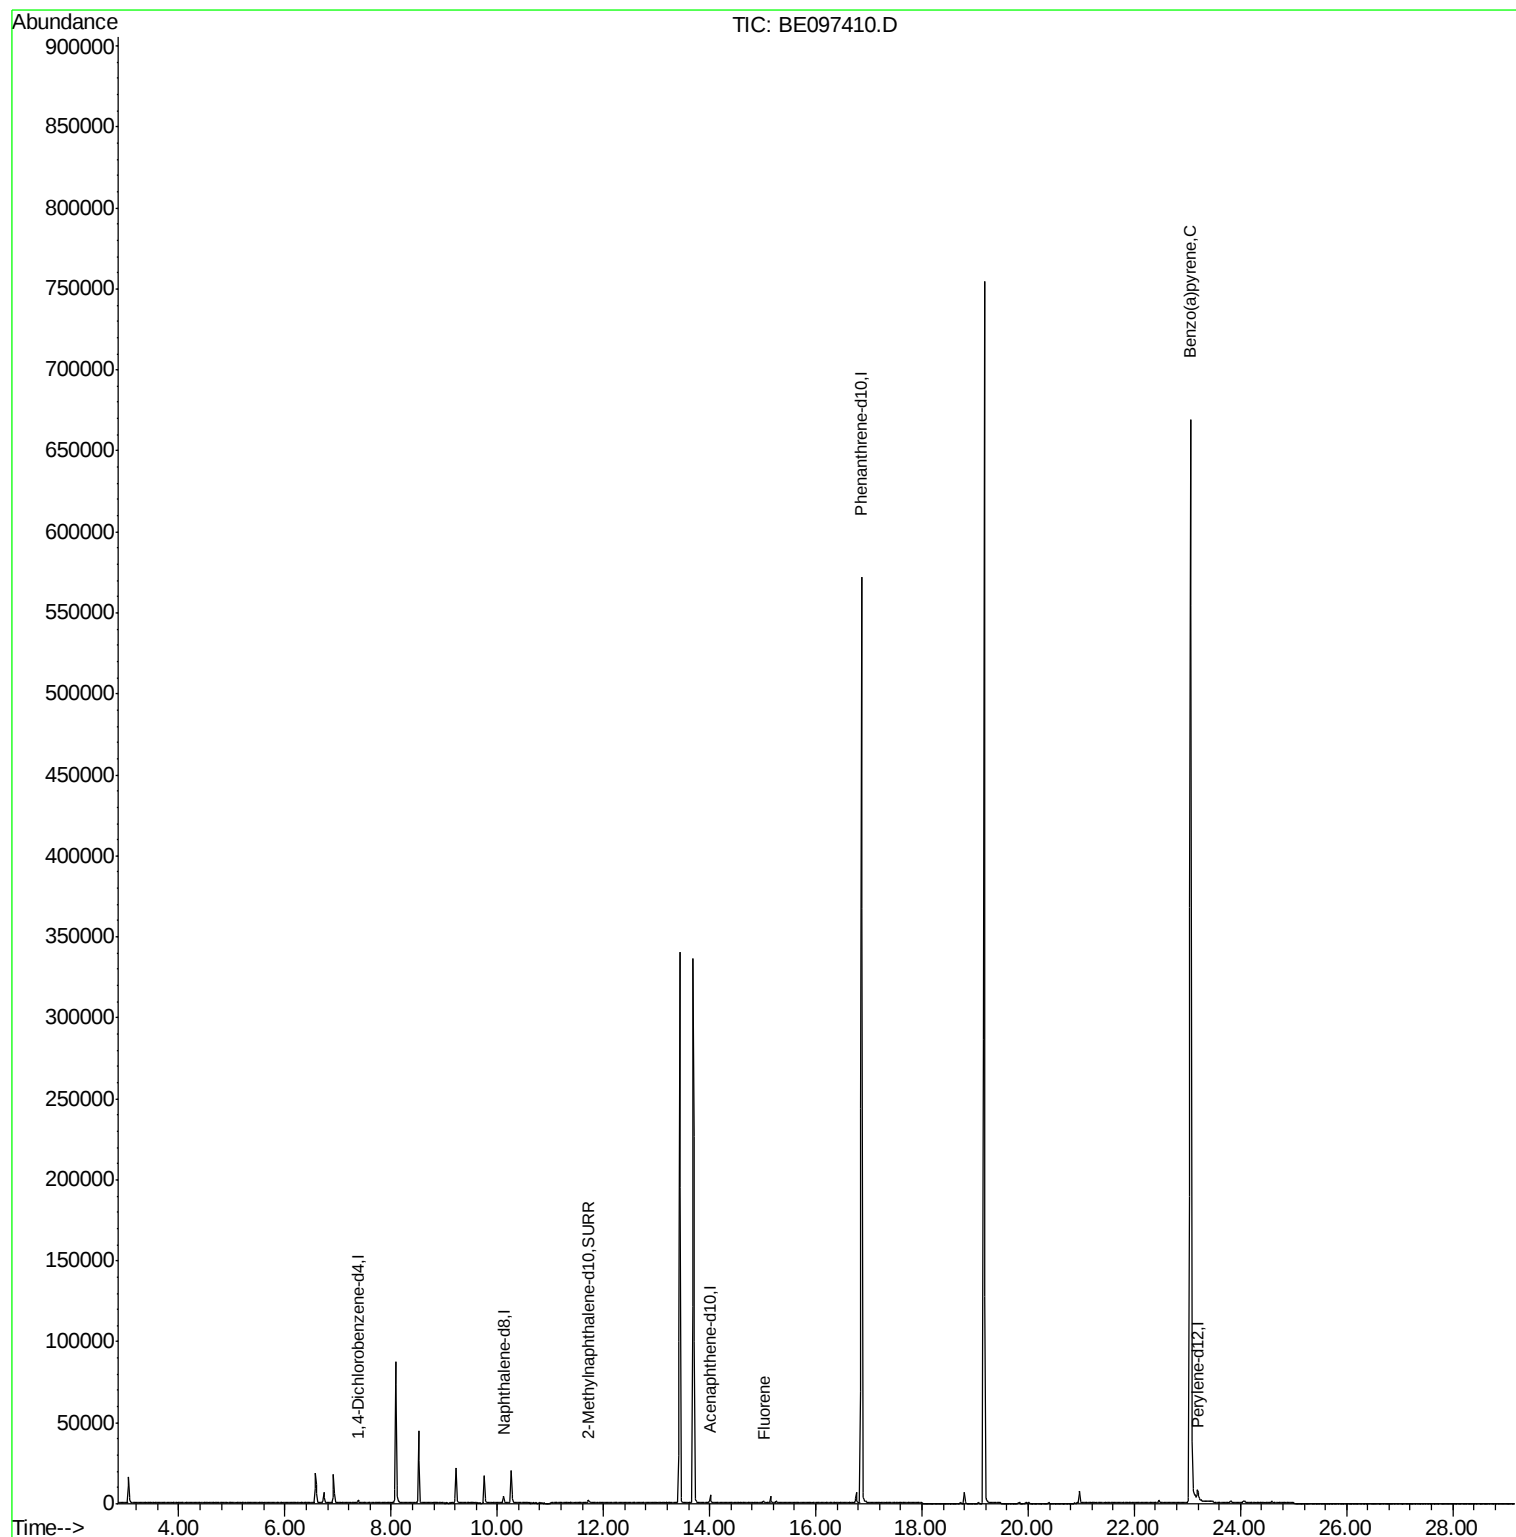


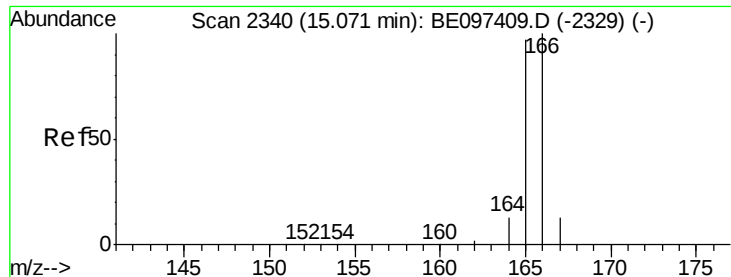

#9
Fluorene
 Concen: 0.085 ng/ul
 RT: 15.01 min Scan# 2331
 Delta R.T. -0.06 min
 Lab File: BE097410.D
 Acq: 5 Sep 2018 17:50

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:166 Resp: 882
 Ion Ratio Lower Upper
 166 100
 165 10.7 73.4 110.2#
 167 39.0 14.6 22.0#

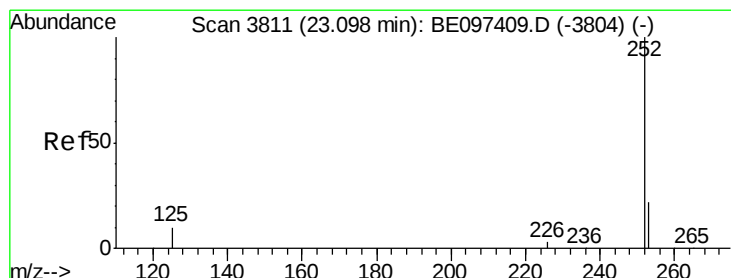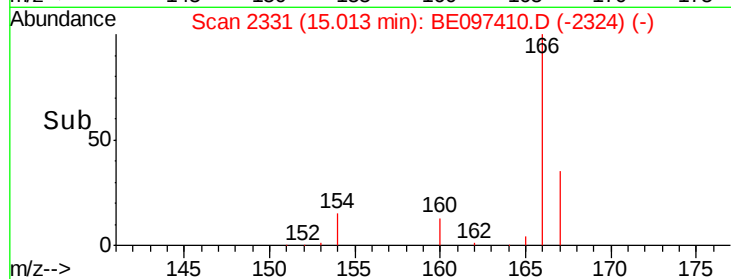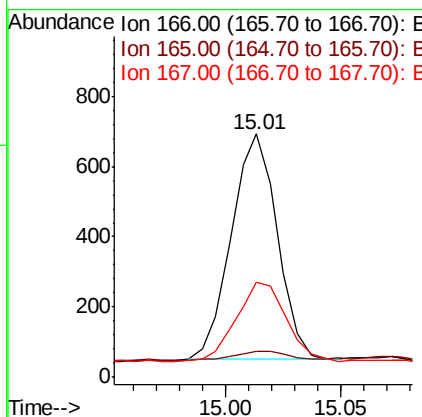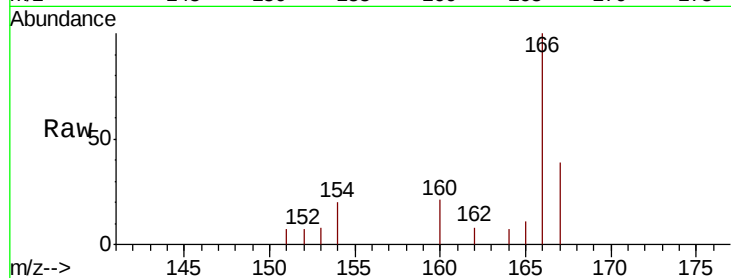

#23
Benzo(a)pyrene
 Concen: 0.079 ng/ul
 RT: 23.06 min Scan# 3808
 Delta R.T. -0.04 min
 Lab File: BE097410.D
 Acq: 5 Sep 2018 17:50

Tgt Ion:252 Resp: 2655
 Ion Ratio Lower Upper
 252 100
 253 31.4 28.5 42.7
 125 19.0 18.1 27.1

