

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090518\
 Data File : BE097412.D
 Acq On : 5 Sep 2018 19:05
 Operator : SJ/JU
 Sample : PB112369BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Sep 06 01:30:05 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 06 01:29:05 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	928	0.40	ng/ul	0.00
2) Naphthalene-d8	10.12	136	4768	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.01	164	3137	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.86	188	683029	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-20.97
20) Perylene-d12	23.20	264	14337	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.72	152	2852	0.38	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.01	166	950	0.084	ng/ul#	21
23) Benzo(a)pyrene	23.06	252	2831	0.080	ng/ul	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090518\
Data File : BE097412.D
Acq On : 5 Sep 2018 19:05
Operator : SJ/JU
Sample : PB112369BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Sep 06 01:30:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 06 01:29:05 2018
Response via : Initial Calibration




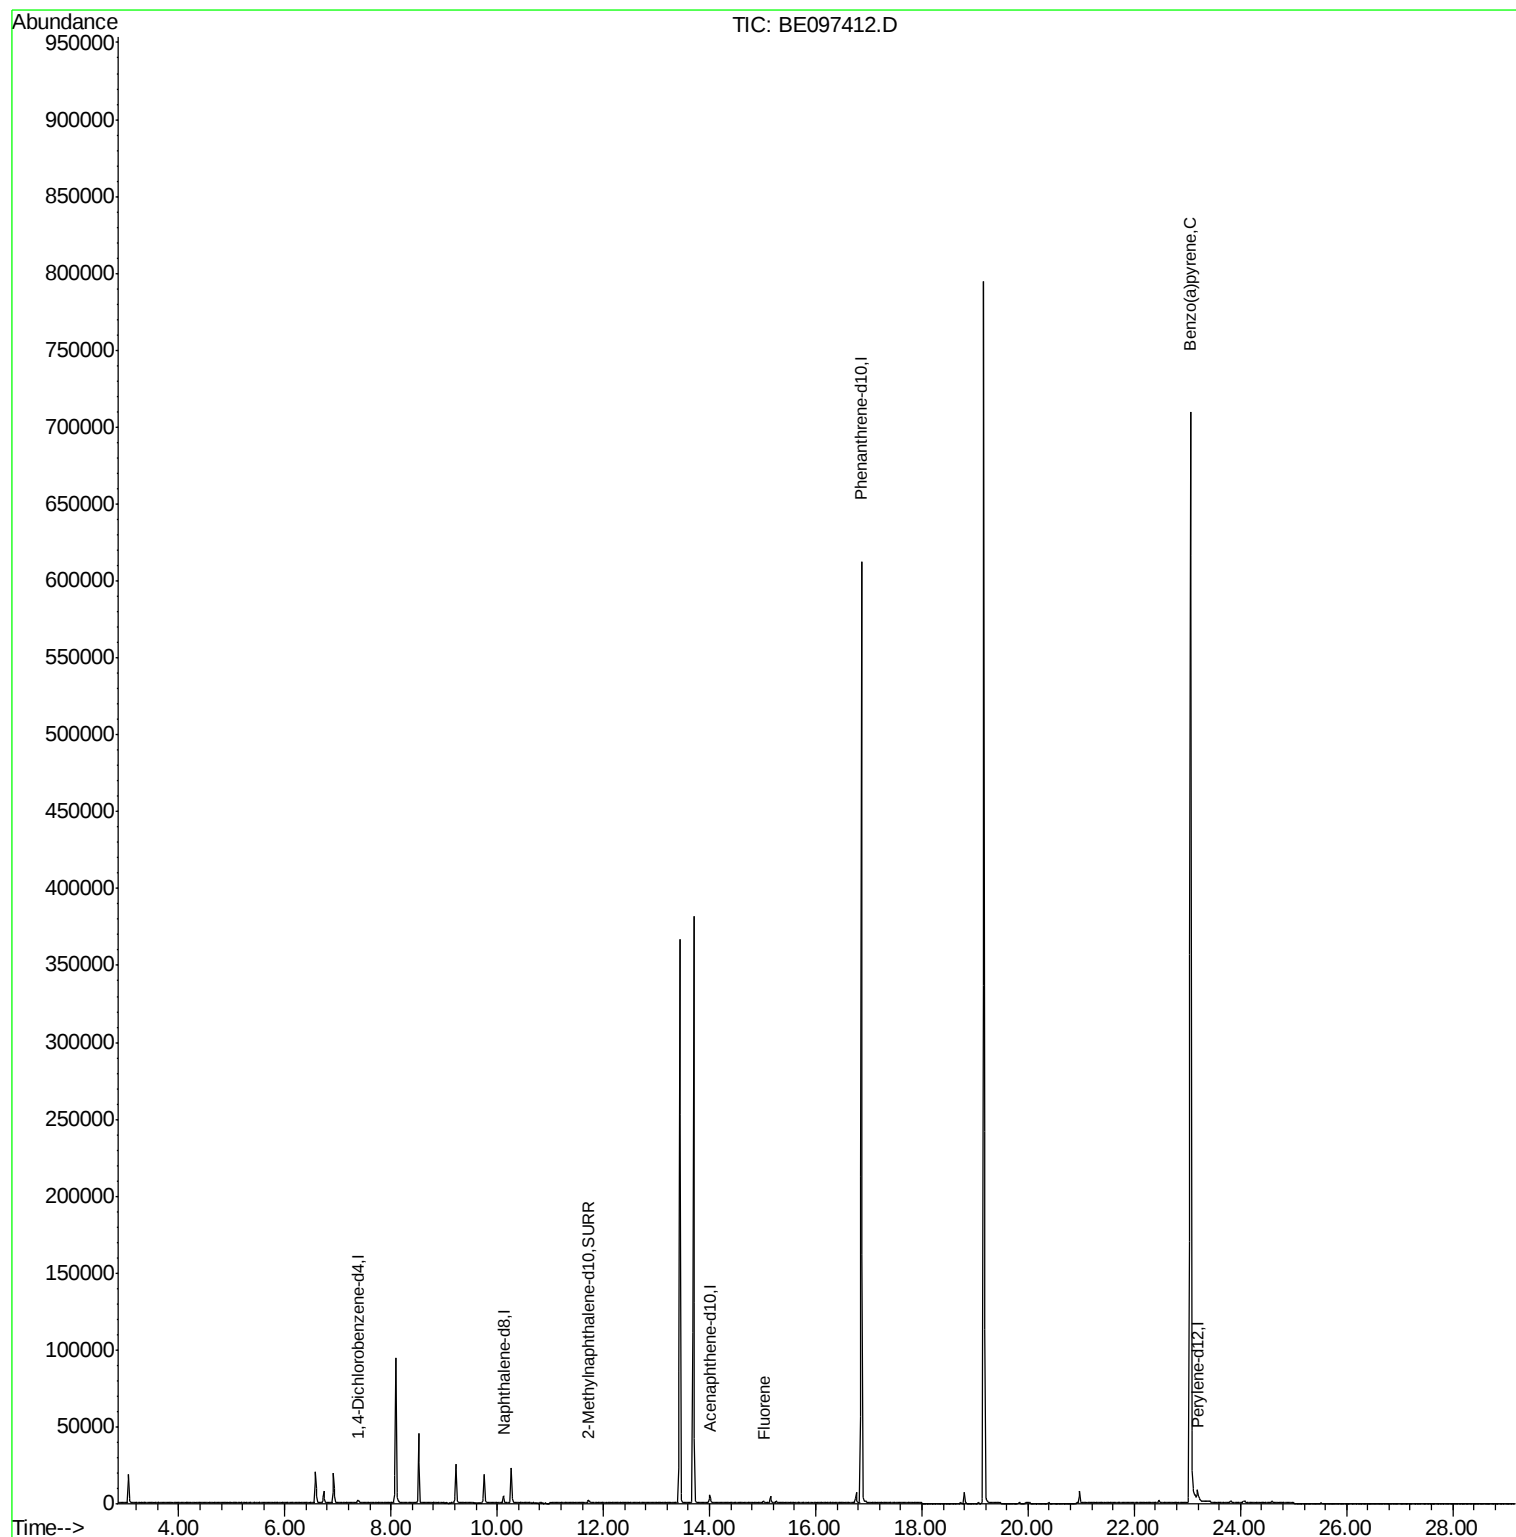


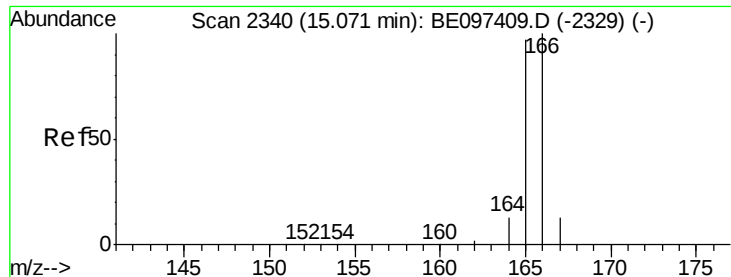

#9
Fluorene
 Concen: 0.084 ng/ul
 RT: 15.01 min Scan# 2330
 Delta R.T. -0.06 min
 Lab File: BE097412.D
 Acq: 5 Sep 2018 19:05

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:166 Resp: 950
 Ion Ratio Lower Upper
 166 100
 165 9.8 73.4 110.2#
 167 38.3 14.6 22.0#

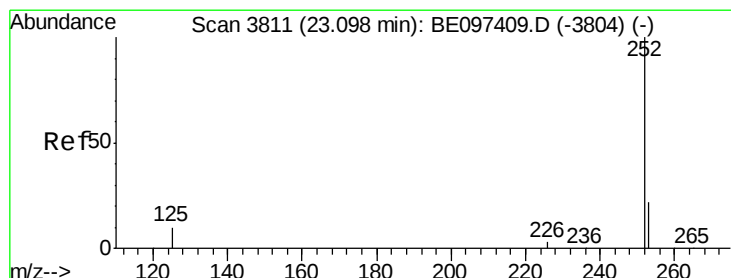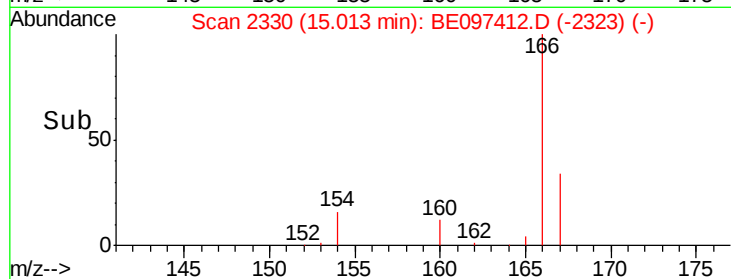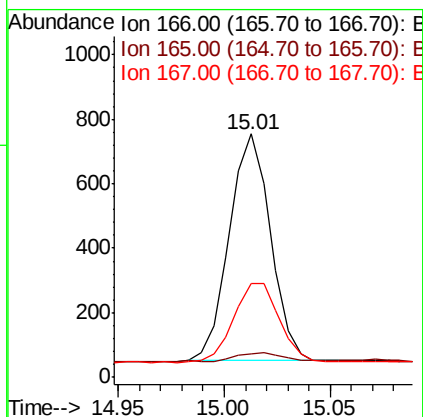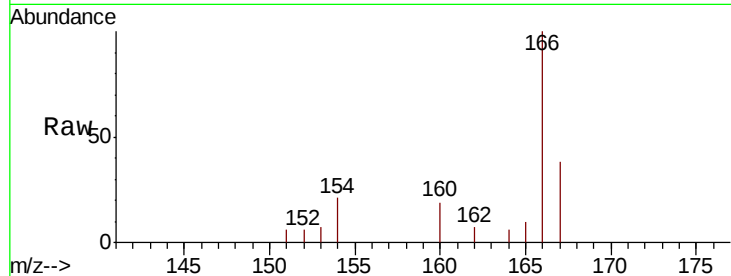

#23
Benzo(a)pyrene
 Concen: 0.080 ng/ul
 RT: 23.06 min Scan# 3806
 Delta R.T. -0.04 min
 Lab File: BE097412.D
 Acq: 5 Sep 2018 19:05

Tgt Ion:252 Resp: 2831
 Ion Ratio Lower Upper
 252 100
 253 31.5 28.5 42.7
 125 19.3 18.1 27.1

