


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090518\
Data File : BE097413.D
Acq On : 5 Sep 2018 19:41
Operator : SJ/JU
Sample : J4688-21
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3YT2

Manual Integrations
APPROVED

Sohil
9/6/2018 4:33:10 PM

Quant Time: Sep 06 02:09:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 06 01:29:05 2018
Response via : Initial Calibration

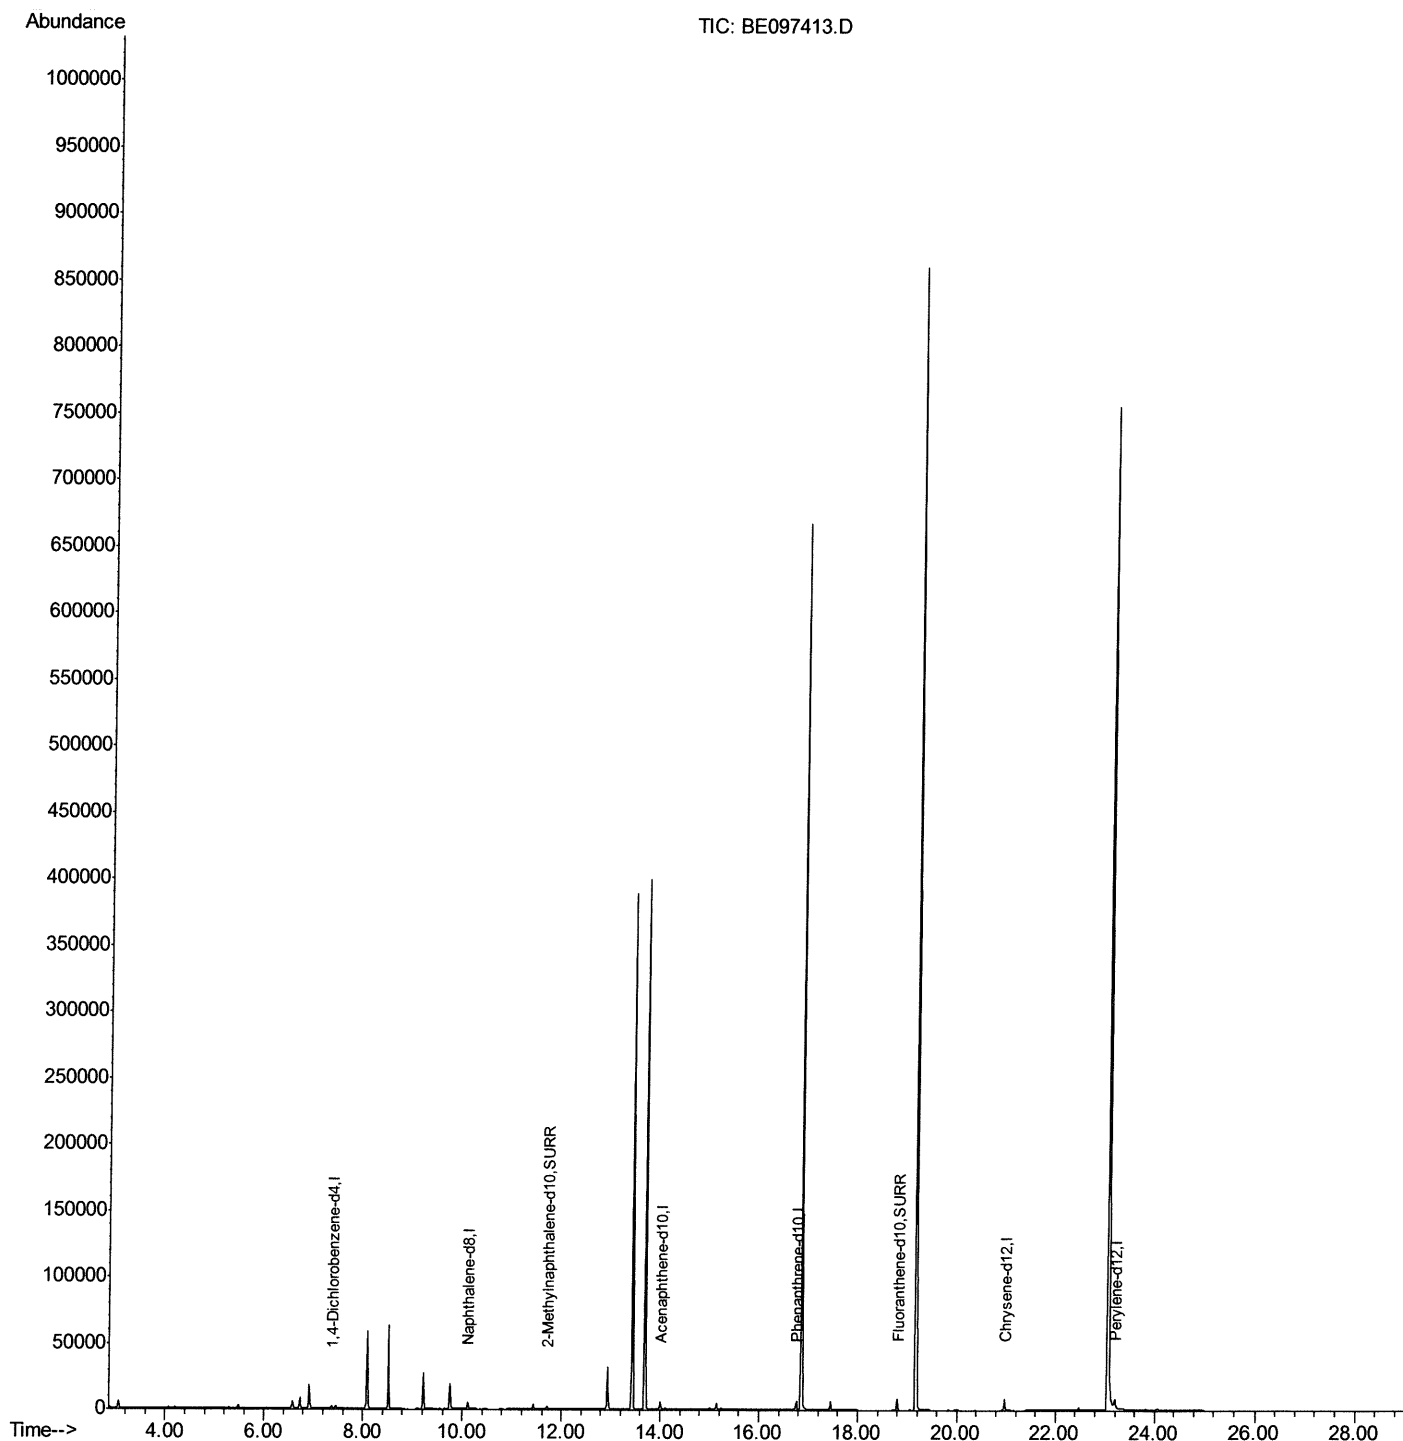

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090518\
 Data File : BE097413.D
 Acq On : 5 Sep 2018 19:41
 Operator : SJ/JU
 Sample : J4688-21
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3YT2

Manual Integrations
 APPROVED

Sohil
 9/6/2018 4:33:10 PM

Quant Time: Sep 06 01:30:11 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 06 01:29:05 2018
 Response via : Initial Calibration

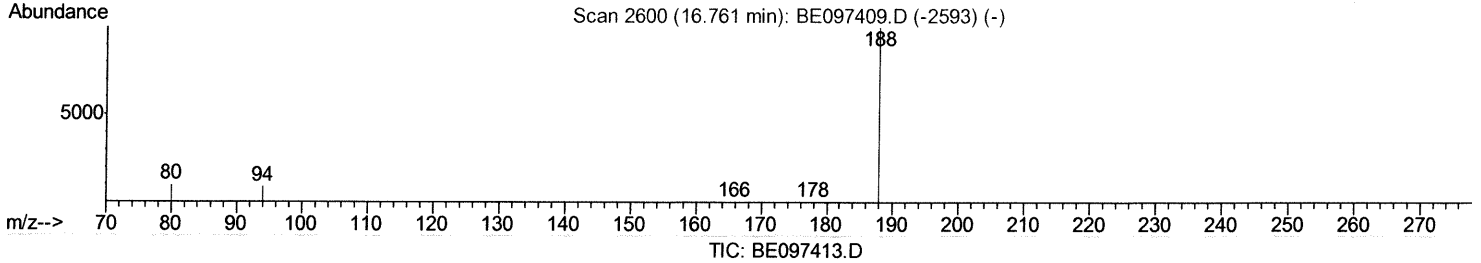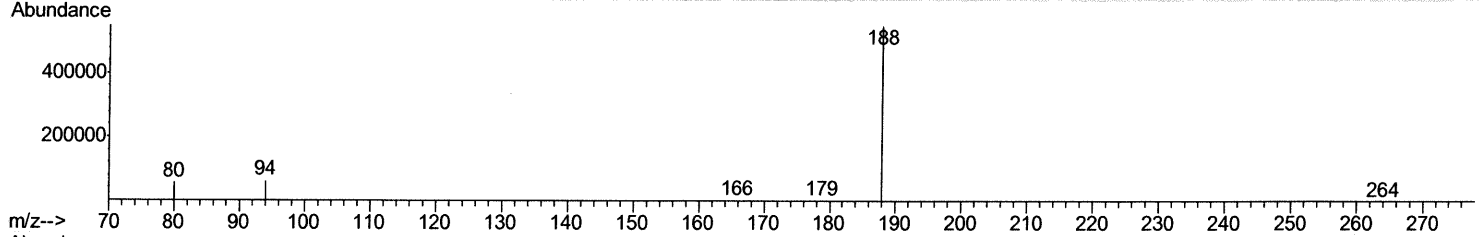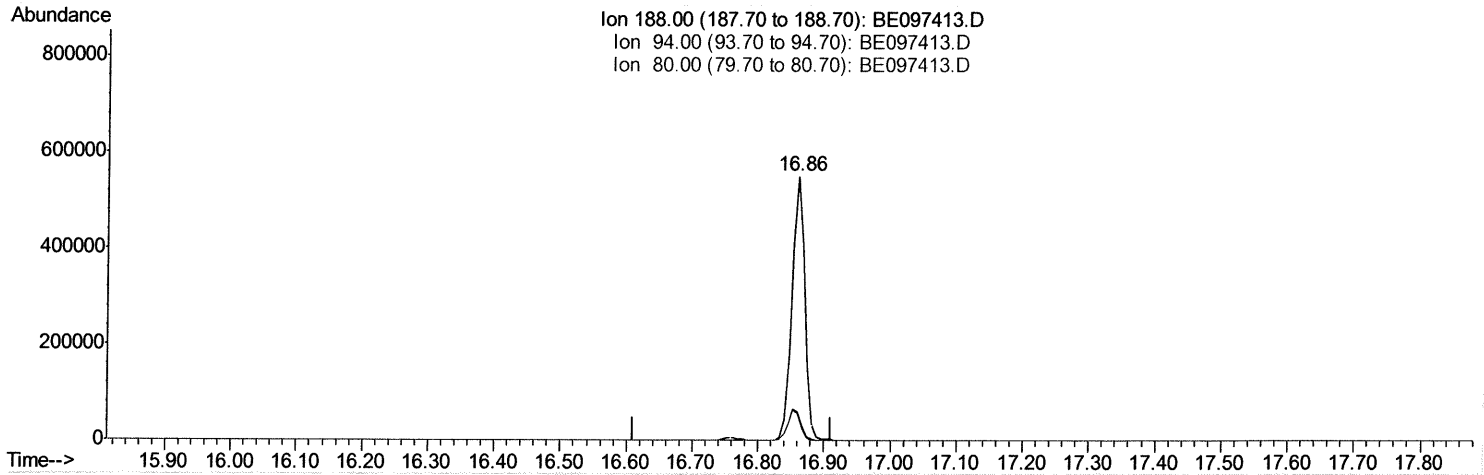

(10) Phenanthrene-d10 (I)

16.860min (+0.100) 0.40ng/ul

response 751737

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	11.04
80.00	11.80	10.11
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090518\
 Data File : BE097413.D
 Acq On : 5 Sep 2018 19:41
 Operator : SJ/JU
 Sample : J4688-21
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3YT2

Manual Integrations
 APPROVED

Sohil
 9/6/2018 4:33:10 PM

Quant Time: Sep 06 01:30:11 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 06 01:29:05 2018
 Response via : Initial Calibration

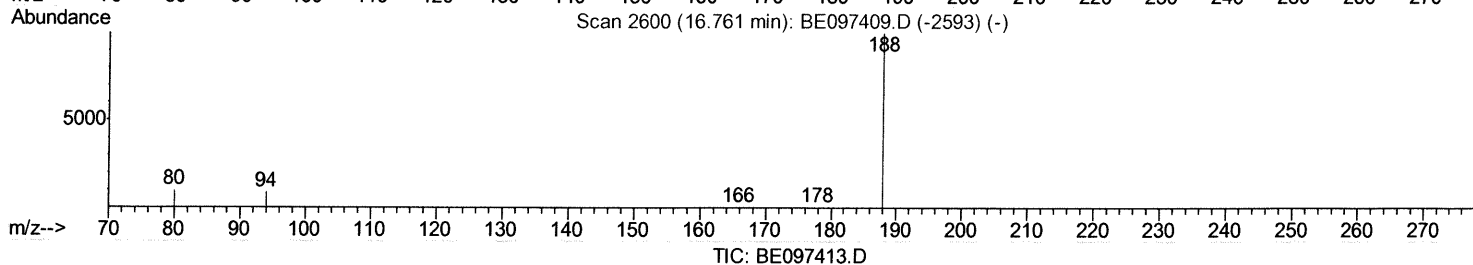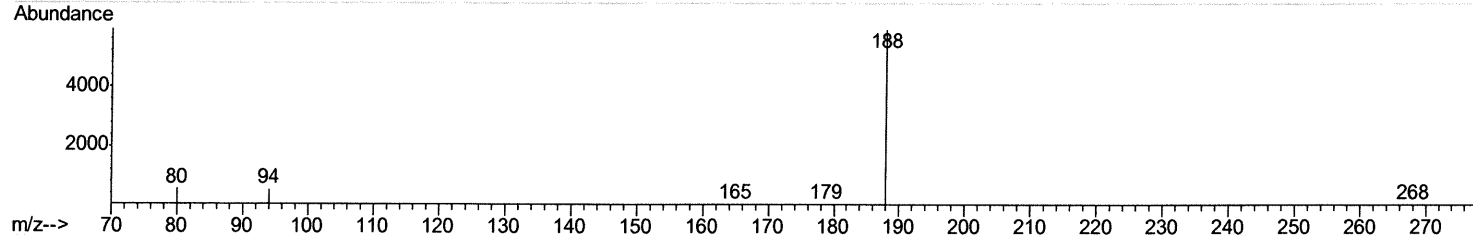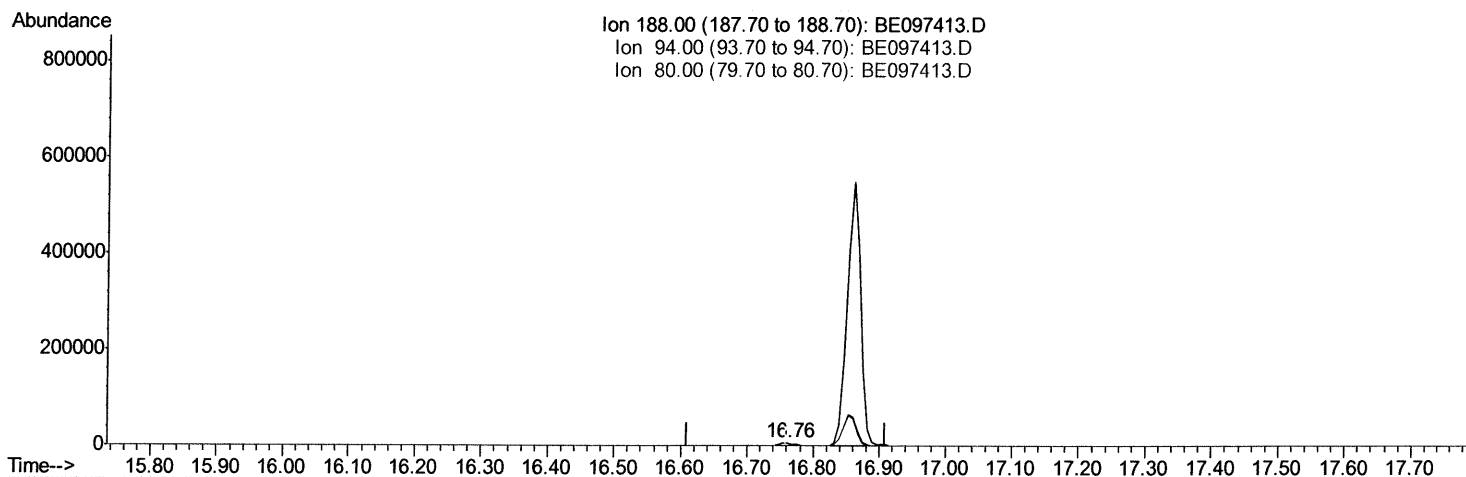

(10) Phenanthrene-d10 (I)

16.762min (+0.001) 0.40ng/ul m > SJ 9/7/18

response 8383

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	8.96
80.00	11.80	9.29#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090518\
Data File : BE097413.D
Acq On : 5 Sep 2018 19:41
Operator : SJ/JU
Sample : J4688-21
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3YT2

Manual Integrations
APPROVED

Sohil
9/6/2018 4:33:10 PM

Quant Time: Sep 06 02:08:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 06 01:29:05 2018
Response via : Initial Calibration

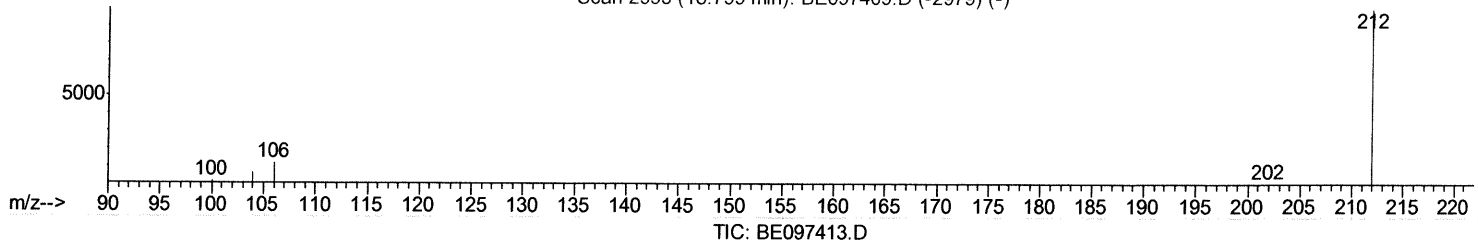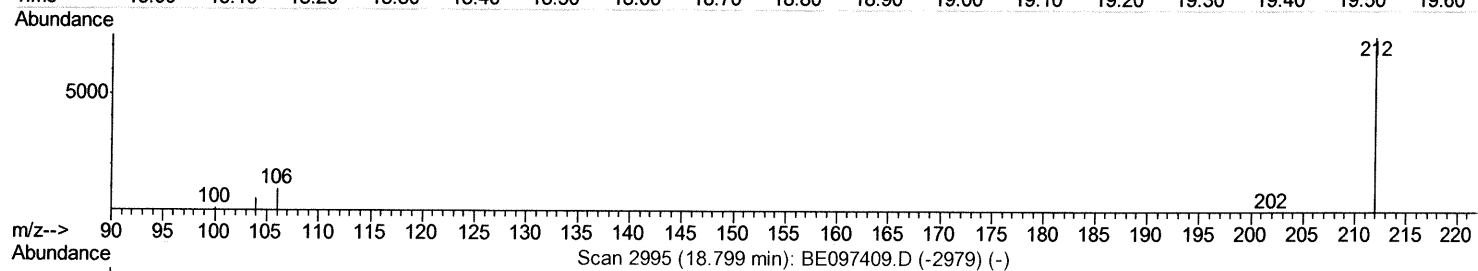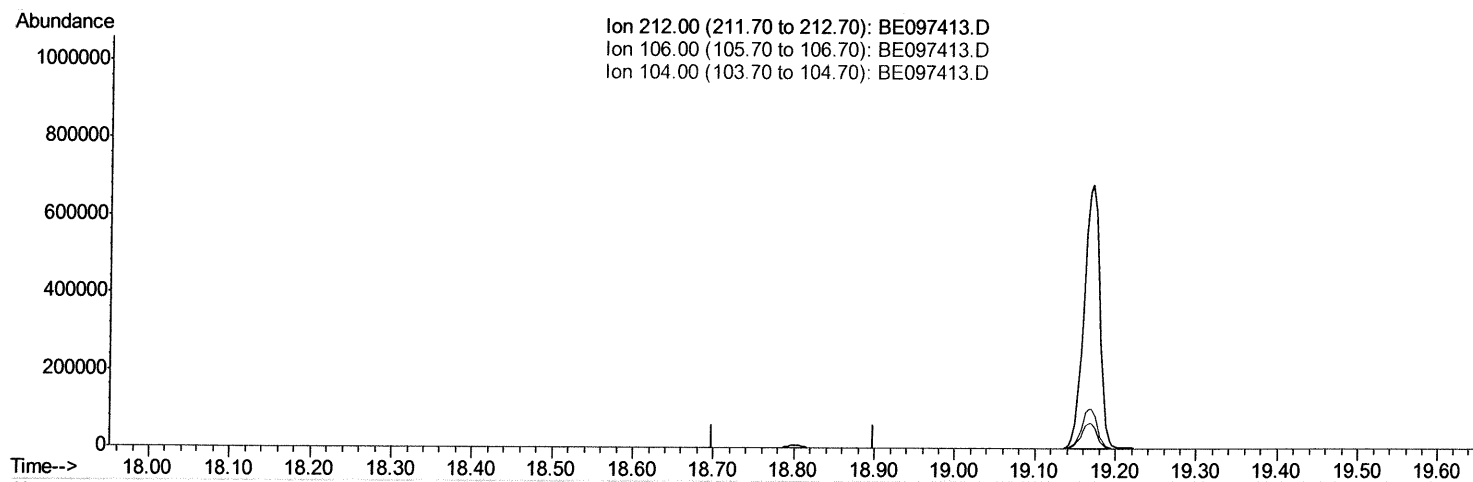

(14) Fluoranthene-d10 (SURR)

18.799min (-18.799) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090518\
 Data File : BE097413.D
 Acq On : 5 Sep 2018 19:41
 Operator : SJ/JU
 Sample : J4688-21
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 A3YT2

Manual Integrations
 APPROVED

Sohil
 9/6/2018 4:33:10 PM

Quant Time: Sep 06 02:08:29 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 06 01:29:05 2018
 Response via : Initial Calibration

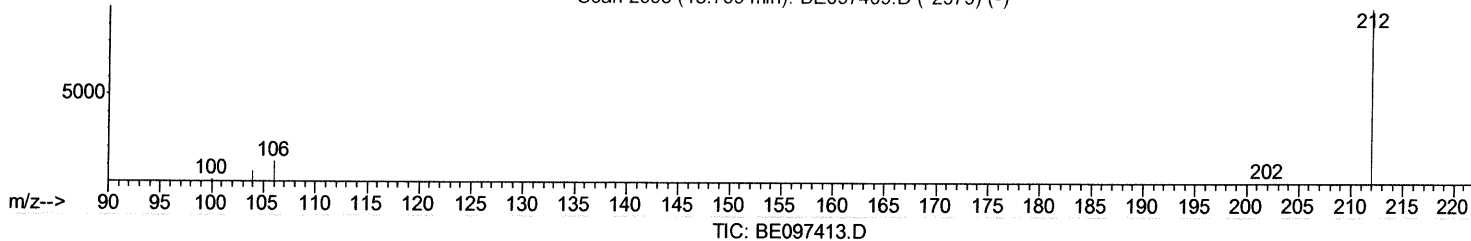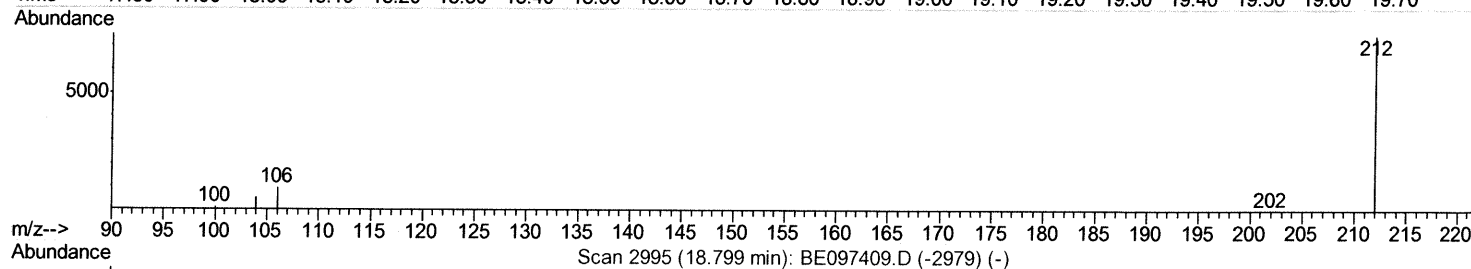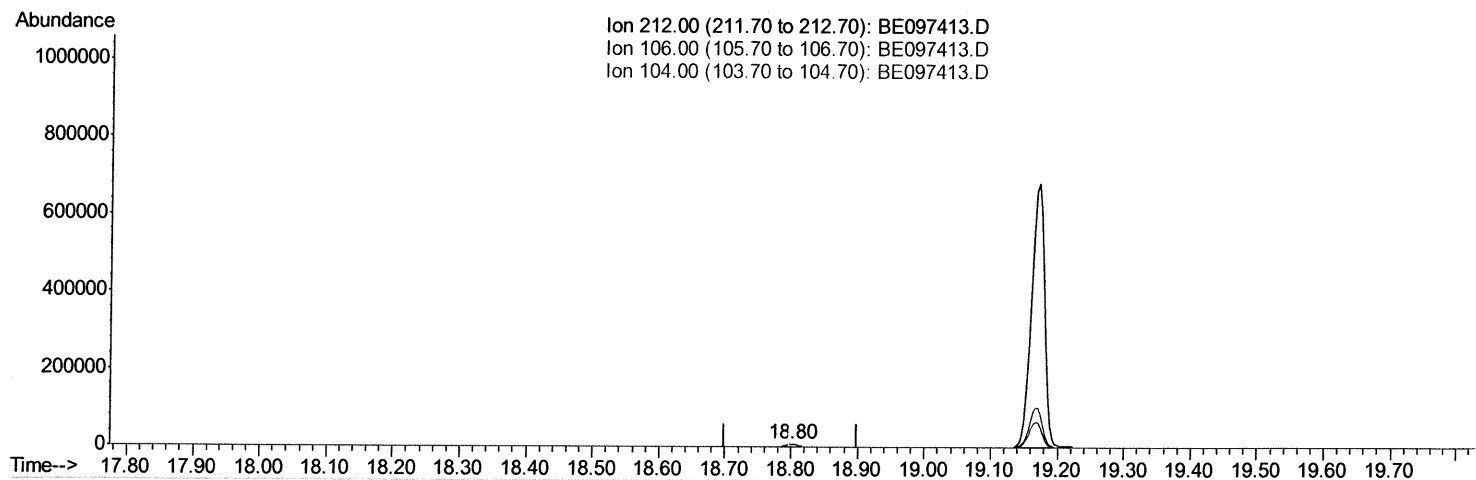

(14) Fluoranthene-d10 (SURR)

18.799min (+0.000) 0.37ng/ul m> 50 9/7/18

response 10288

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090518\
 Data File : BE097413.D
 Acq On : 5 Sep 2018 19:41
 Operator : SJ/JU
 Sample : J4688-21
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3YT2

Manual Integrations
 APPROVED

Sohil
 9/6/2018 4:33:10 PM

Quant Time: Sep 06 02:08:29 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 06 01:29:05 2018
 Response via : Initial Calibration

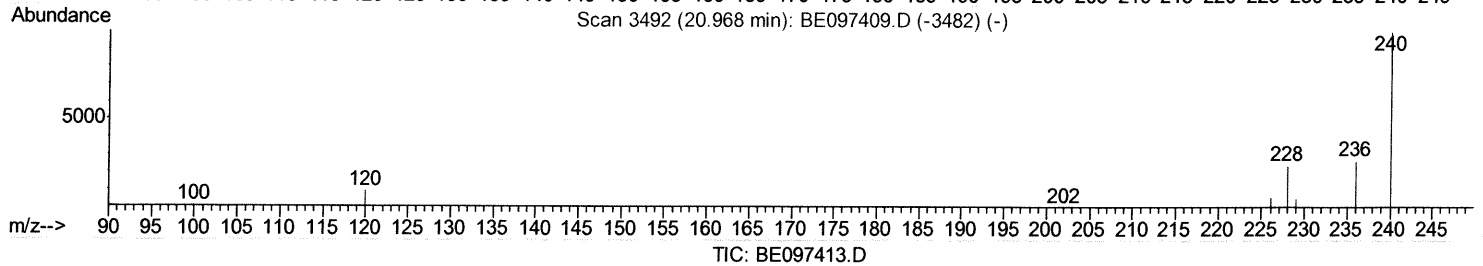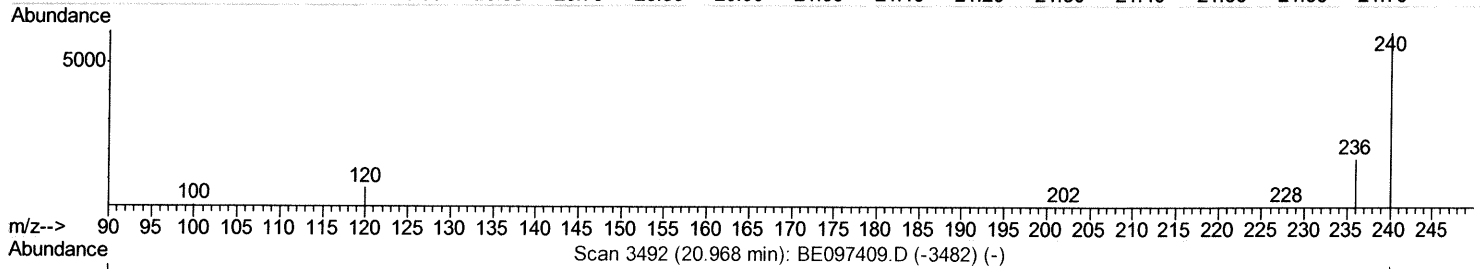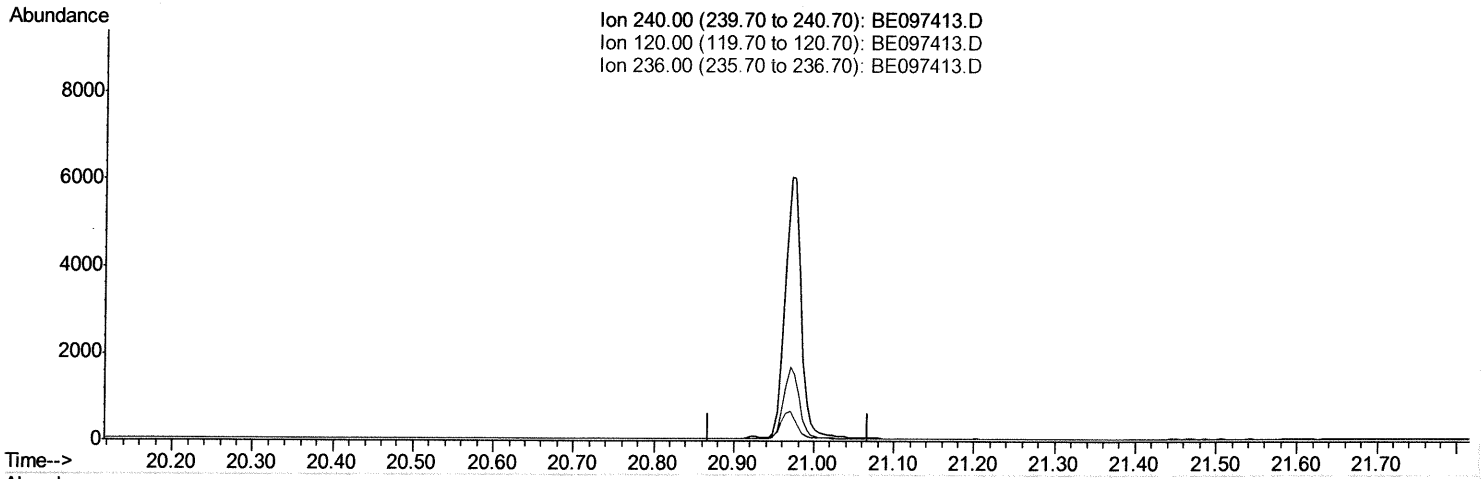

(16) Chrysene-d12 (I)

20.968min (-20.968) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	20.60	0.00#
236.00	34.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090518\
 Data File : BE097413.D
 Acq On : 5 Sep 2018 19:41
 Operator : SJ/JU
 Sample : J4688-21
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 A3YT2

Manual Integrations
 APPROVED

Sohil
 9/6/2018 4:33:10 PM

Quant Time: Sep 06 02:08:29 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 06 01:29:05 2018
 Response via : Initial Calibration

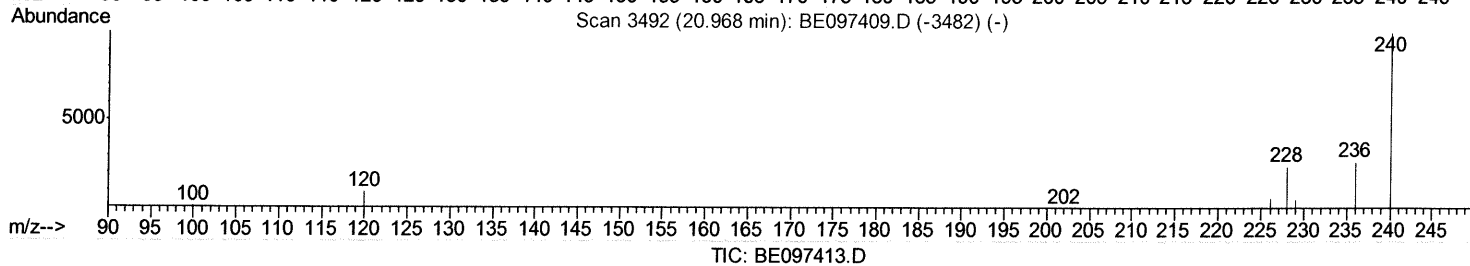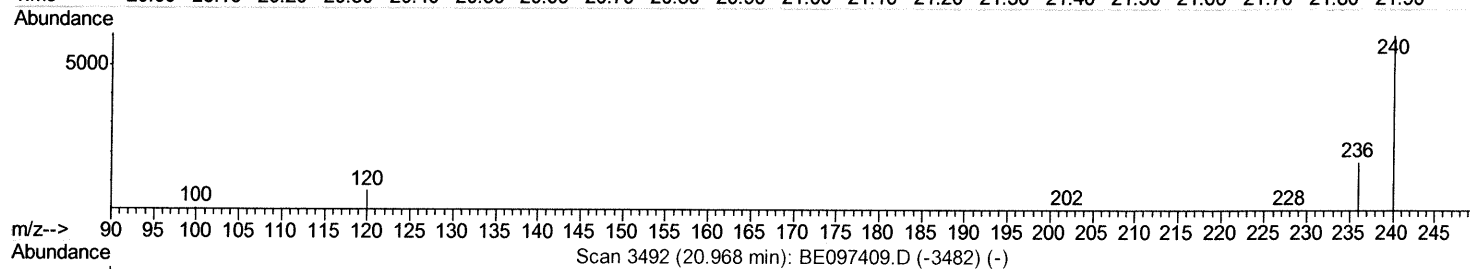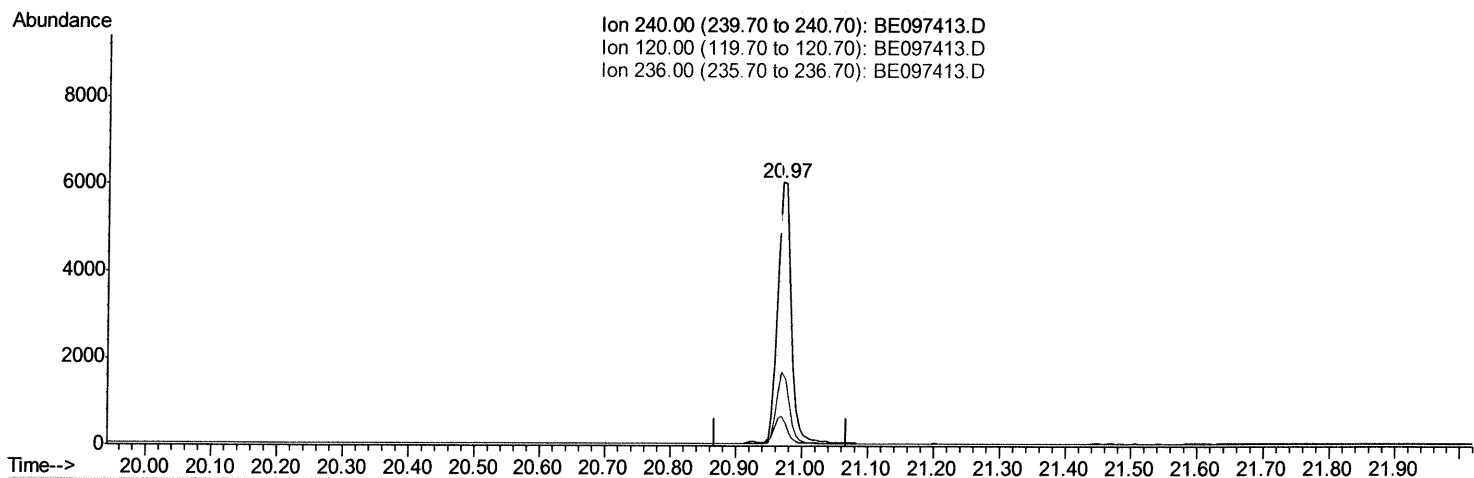

(16) Chrysene-d12 (I)

20.970min (+0.001) 0.40ng/ul m> SJ 9/7/18

response 8382

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	11.50#
236.00	34.90	28.15
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090518\
 Data File : BE097413.D
 Acq On : 5 Sep 2018 19:41
 Operator : SJ/JU
 Sample : J4688-21
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 A3YT2

Manual Integrations
 APPROVED

Sohil
 9/6/2018 4:33:10 PM

Quant Time: Sep 06 02:09:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 06 01:29:05 2018
 Response via : Initial Calibration

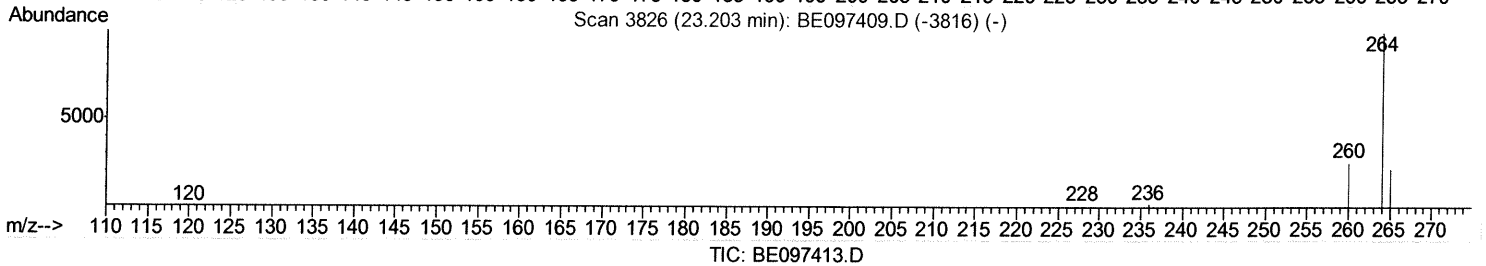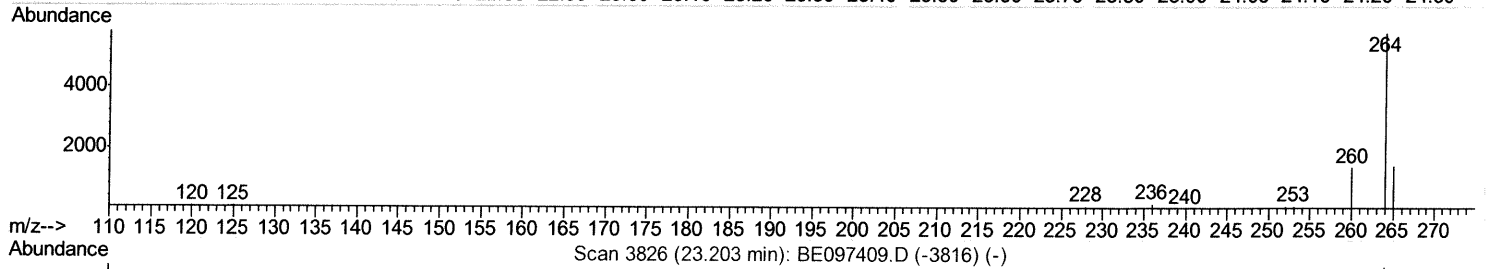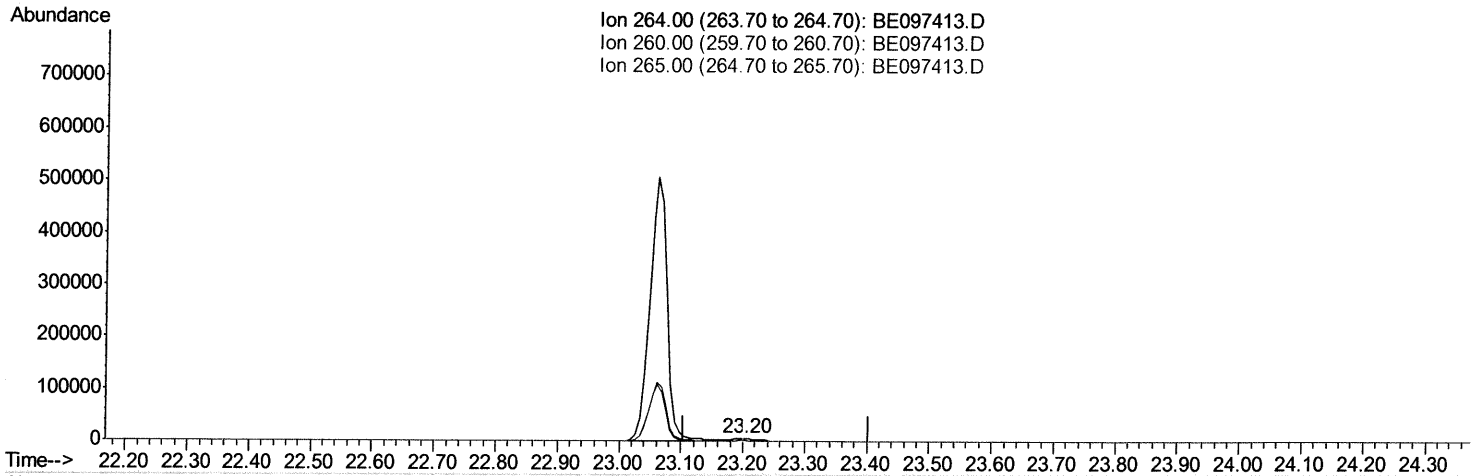

(20) Perylene-d12 (I)
 23.202min (-0.001) 0.40ng/ul
 response 15072

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	23.93#
265.00	103.50	24.57#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090518\
Data File : BE097413.D
Acq On : 5 Sep 2018 19:41
Operator : SJ/JU
Sample : J4688-21
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
A3YT2

Manual Integrations
APPROVED

Sohil
9/6/2018 4:33:10 PM

Quant Time: Sep 06 02:09:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 06 01:29:05 2018
Response via : Initial Calibration

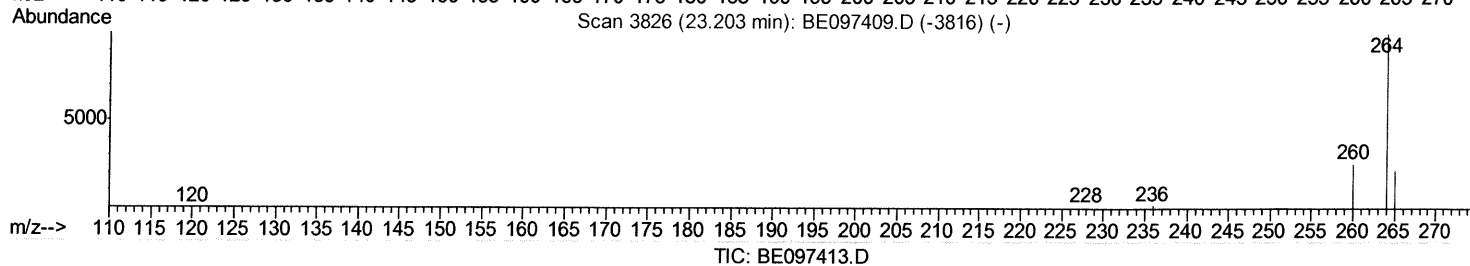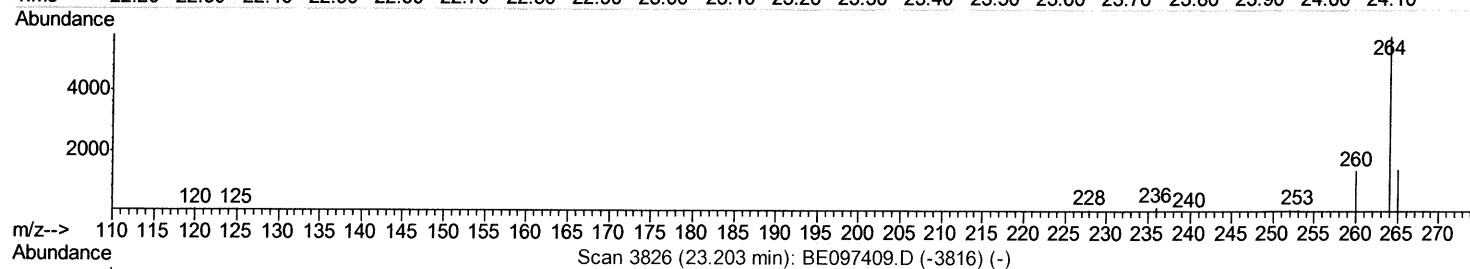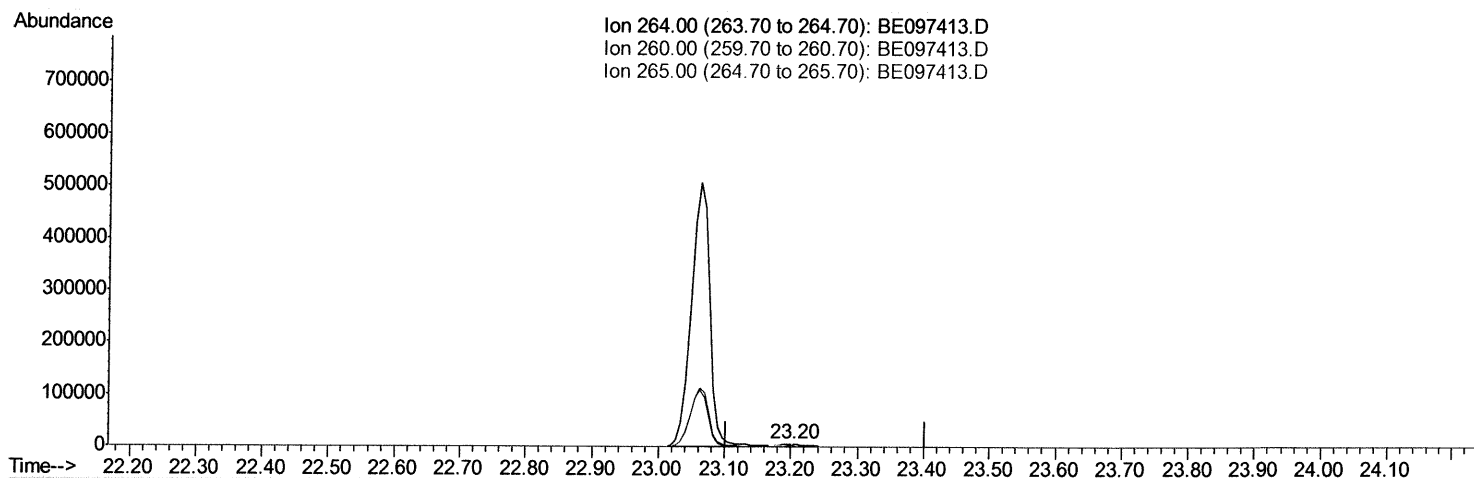

(20) Perylene-d12 (I)

23.202min (-0.001) 0.40ng/ul m) > SJ 9/7/18

response 7418

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	23.93#
265.00	103.50	24.57#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090518\
Data File : BE097413.D
Acq On : 5 Sep 2018 19:41
Operator : SJ/JU
Sample : J4688-21
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3YT2

Manual Integrations
APPROVED

Sohil
9/6/2018 4:33:10 PM

Quant Time: Sep 06 02:09:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 06 01:29:05 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	991	0.40	ng/ul	0.00
2) Naphthalene-d8	10.12	136	4931	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.01	164	3327	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.76	188	8383m	0.40	ng/ul	0.00
16) Chrysene-d12	20.97	240	8382m	0.40	ng/ul	0.00
20) Perylene-d12	23.20	264	7418m	0.40	ng/ul	0.00

SJ 9/7/18

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.72	152	3241	0.42	ng/ul	0.00
14) Fluoranthene-d10	18.80	212	10288m	0.37	ng/ul	0.00

SJ 9/7/18

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed