

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090718\
 Data File : BE097419.D
 Acq On : 7 Sep 2018 11:29
 Operator : SJ/JU
 Sample : J4688-12
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Sep 07 23:50:59 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 07 23:49:56 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	972	0.40	ng/ul	0.00
2) Naphthalene-d8	10.12	136	4937	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.01	164	3112	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.86	188	294468	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-20.97
20) Perylene-d12	23.19	264	12246	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.72	152	1320	0.17	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.05	252	1347	0.044	ng/ul	Ovalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090718\
Data File : BE097419.D
Acq On : 7 Sep 2018 11:29
Operator : SJ/JU
Sample : J4688-12
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Sep 07 23:50:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 07 23:49:56 2018
Response via : Initial Calibration

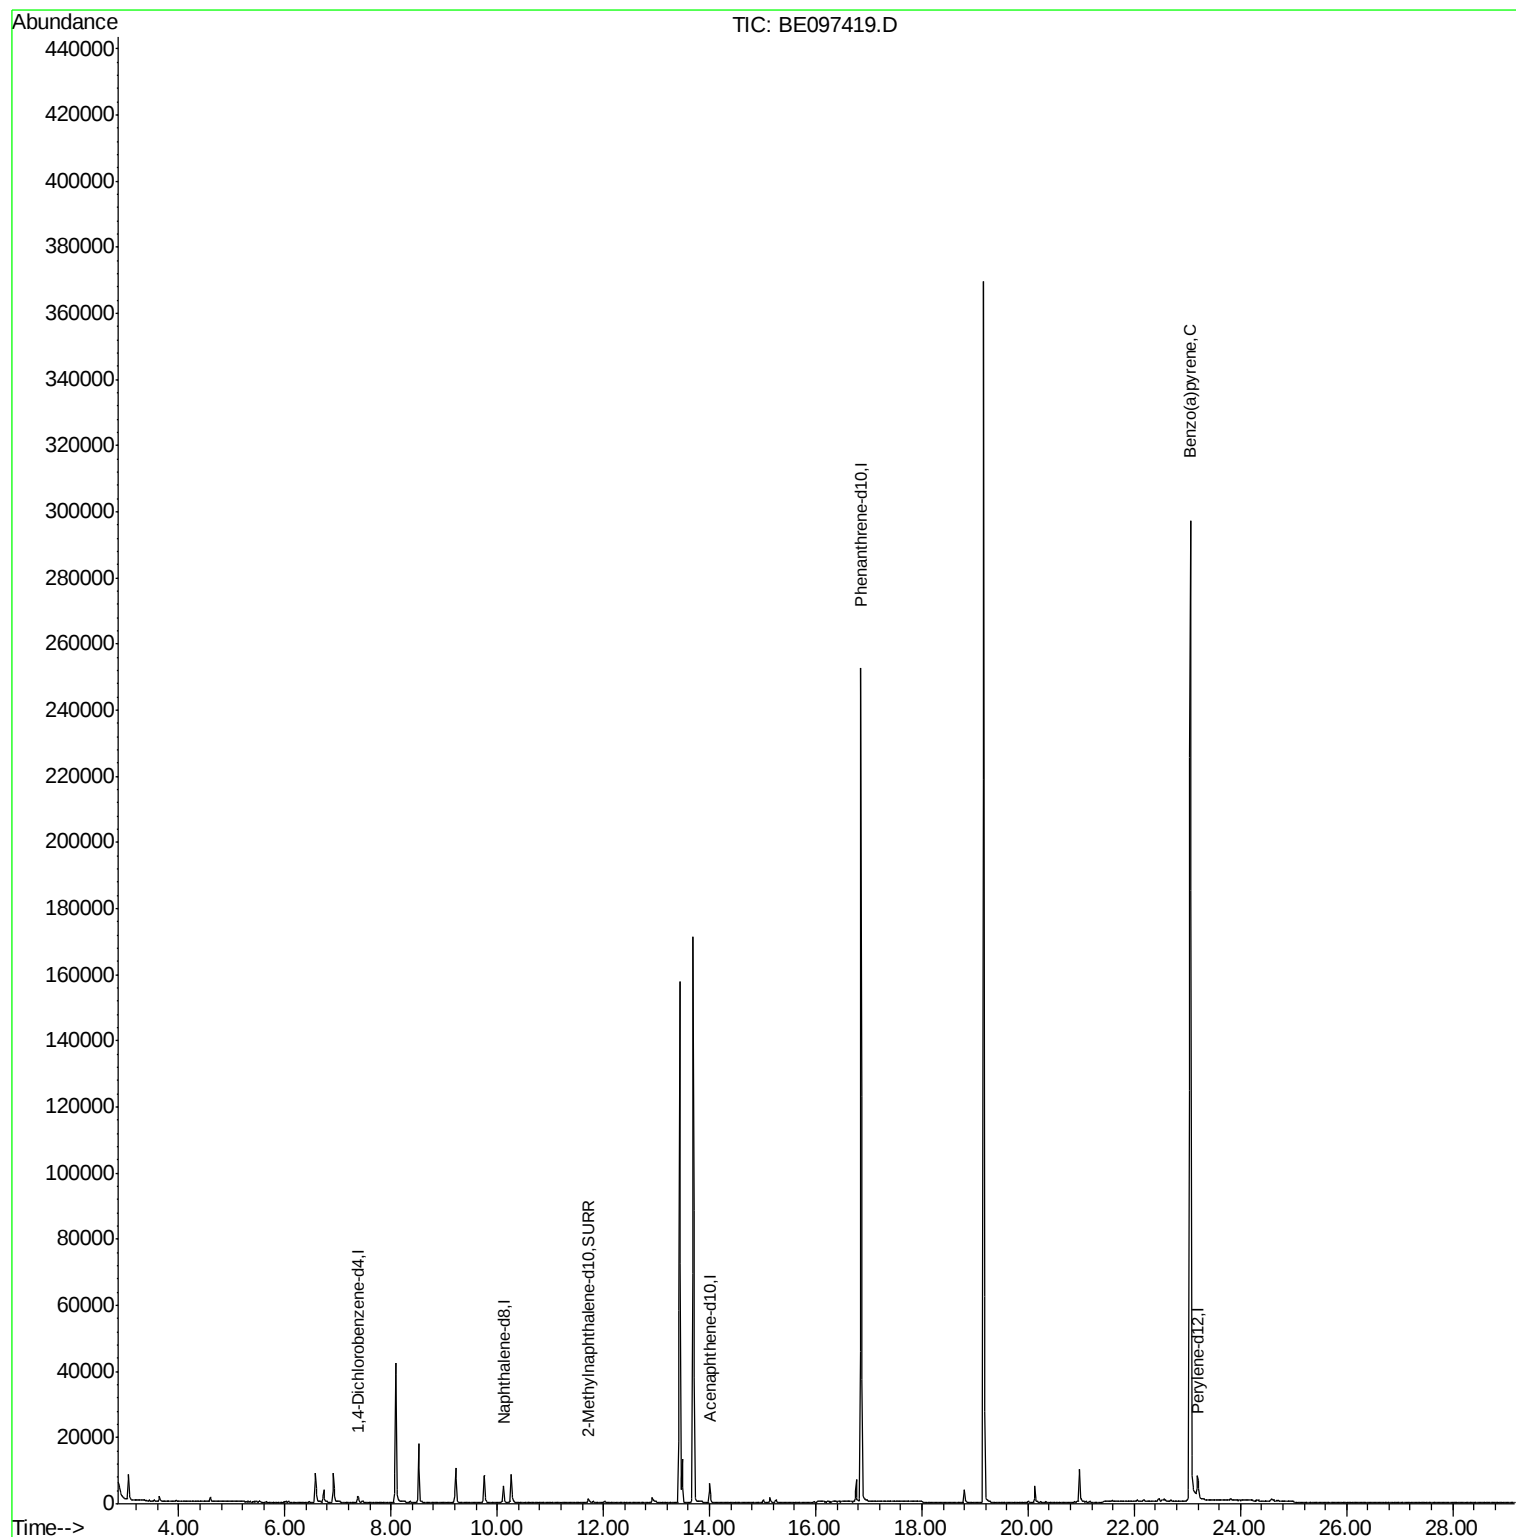

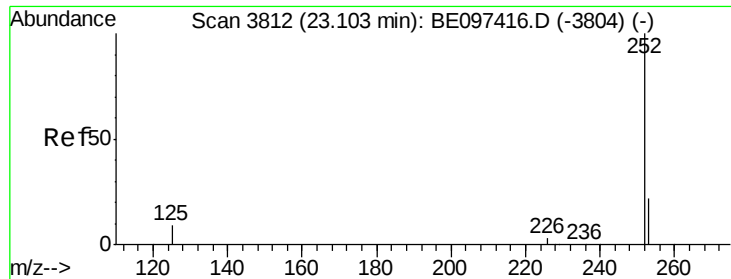

#23

Benzo(a)pyrene

Concen: 0.044 ng/ul

RT: 23.05 min Scan# 3806

Delta R.T. -0.05 min


Lab File: BE097419.D

Acq: 7 Sep 2018 11:29

Instrument :

BNA_E

ClientSampleId :

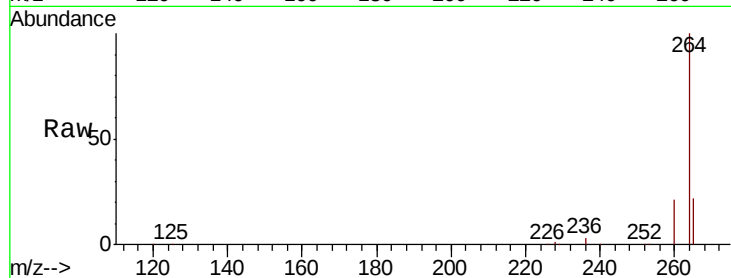


Tot Ion: 252 Resp: 1347

Ion Ratio Lower Upper

252 100

253 37.8 28.5 42.7

125 26.5 18.1 27.1

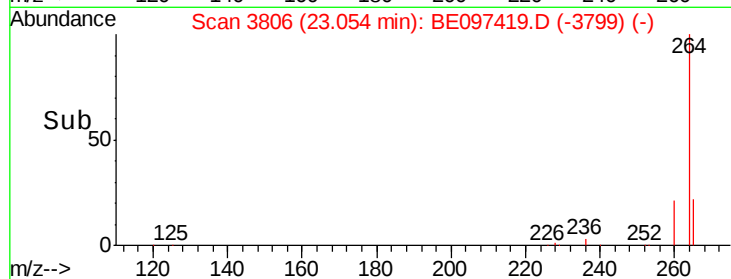

Abundance Ion 252.00 (251.70 to 252.70): E

1000 Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

