


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090718\
Data File : BE097420.D
Acq On : 7 Sep 2018 12:05
Operator : SJ/JU
Sample : J4688-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Z17

Manual Integrations
APPROVED

Sohil
9/11/2018 2:42:26 PM

Quant Time: Sep 08 00:10:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 07 23:49:56 2018
Response via : Initial Calibration

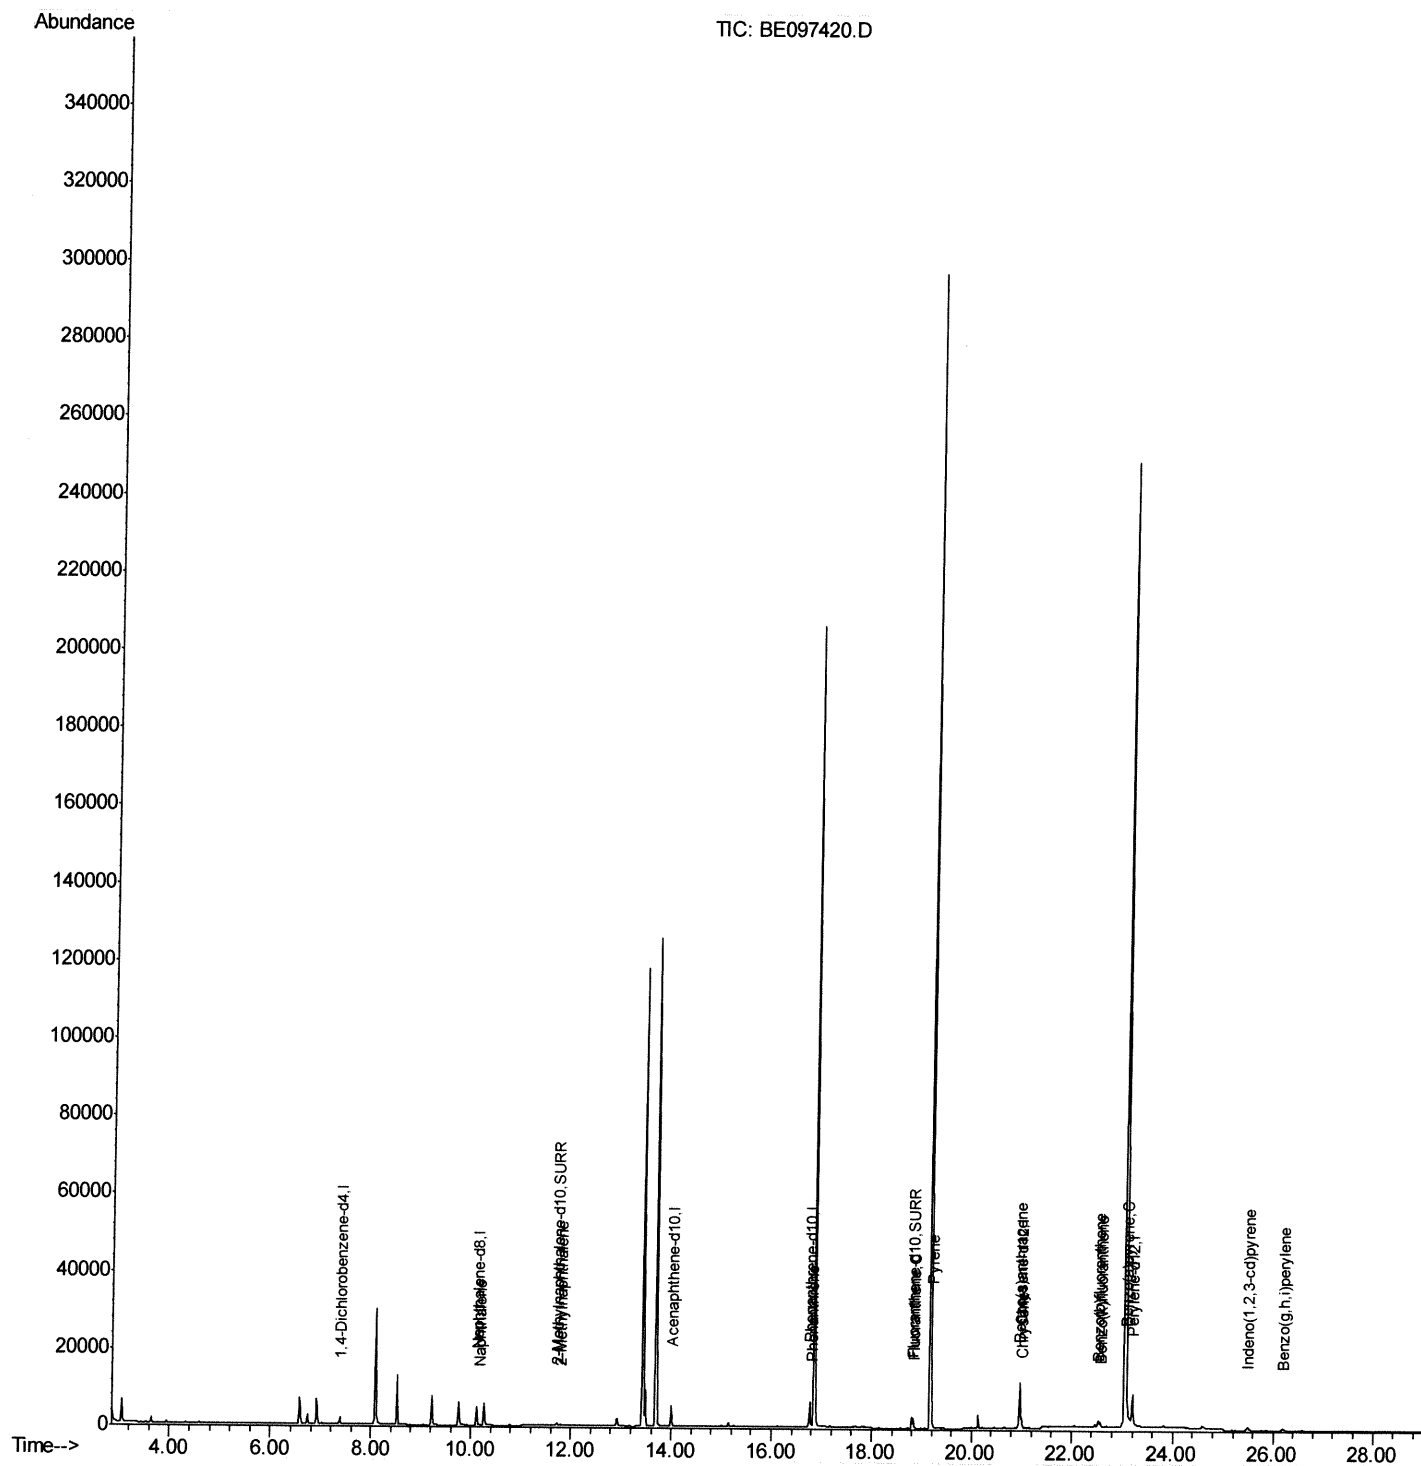

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090718\
 Data File : BE097420.D
 Acq On : 7 Sep 2018 12:05
 Operator : SJ/JU
 Sample : J4688-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Z17

Manual Integrations
 APPROVED

Sohil
 9/11/2018 2:42:26 PM

Quant Time: Sep 07 23:51:03 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 07 23:49:56 2018
 Response via : Initial Calibration

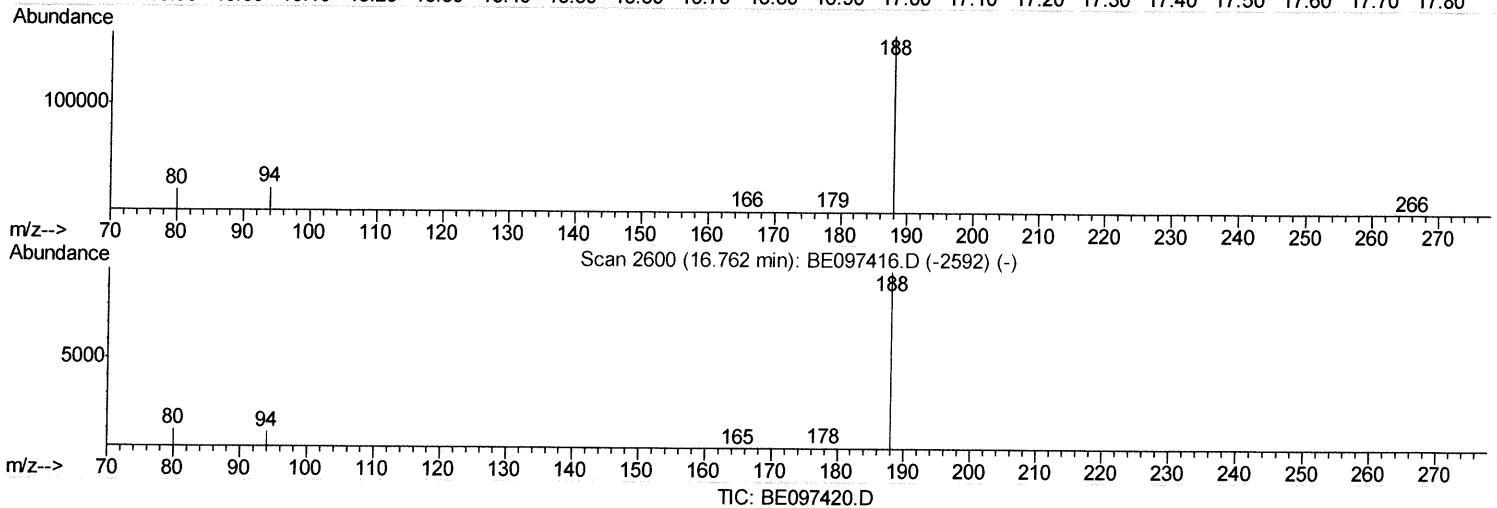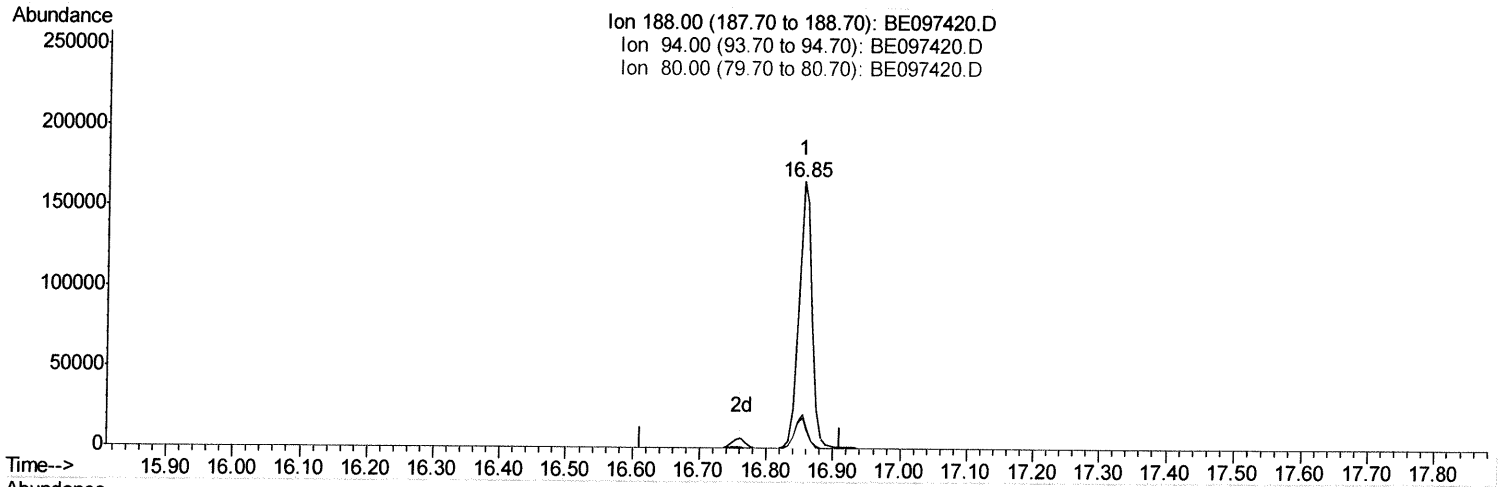

(10) Phenanthrene-d10 (I)

16.853min (+0.092) 0.40ng/ul

response 231271

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	12.59
80.00	11.80	11.38
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090718\
 Data File : BE097420.D
 Acq On : 7 Sep 2018 12:05
 Operator : SJ/JU
 Sample : J4688-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Z17

Manual Integrations
 APPROVED

Sohil
 9/11/2018 2:42:26 PM

Quant Time: Sep 07 23:51:03 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 07 23:49:56 2018
 Response via : Initial Calibration

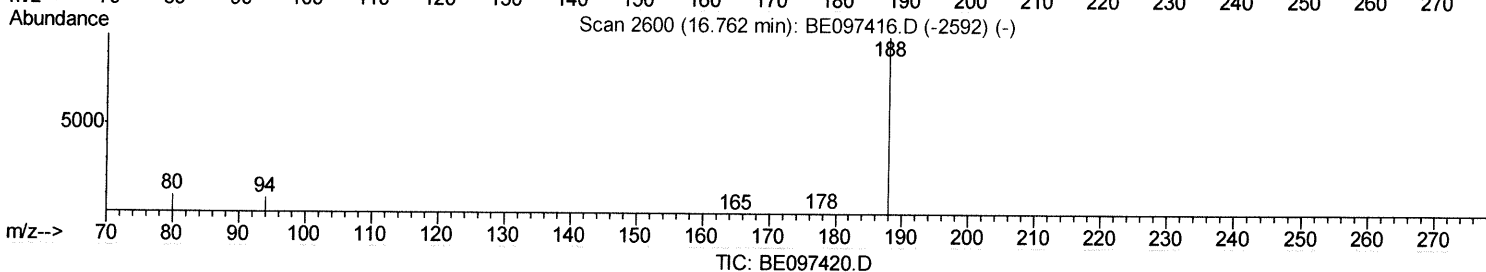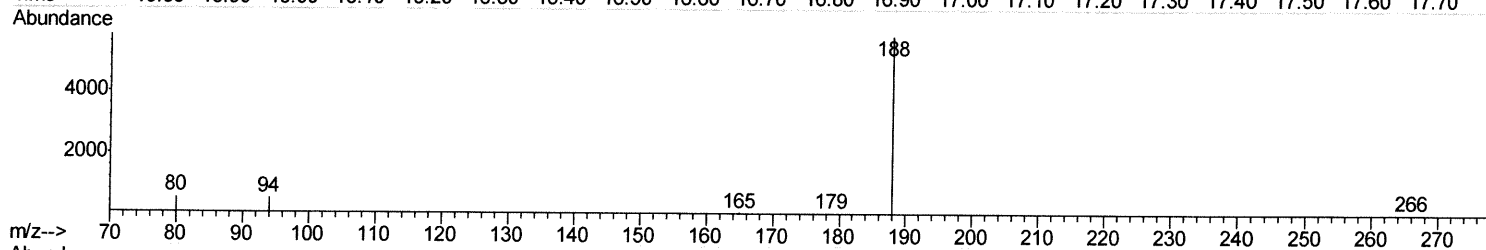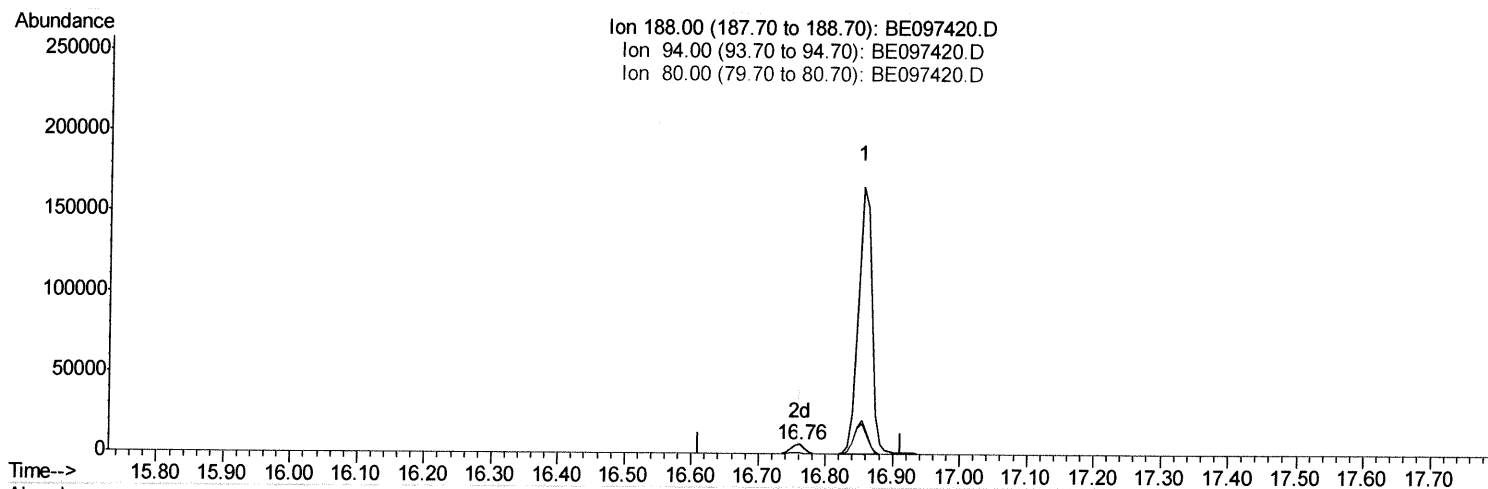

(10) Phenanthrene-d10 (I)

16.762min (+0.000) 0.40ng/ul m

response 8323

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	8.70#
80.00	11.80	9.15#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090718\
 Data File : BE097420.D
 Acq On : 7 Sep 2018 12:05
 Operator : SJ/JU
 Sample : J4688-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Z17

Manual Integrations
 APPROVED

Sohil
 9/11/2018 2:42:26 PM

Quant Time: Sep 08 00:06:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 07 23:49:56 2018
 Response via : Initial Calibration

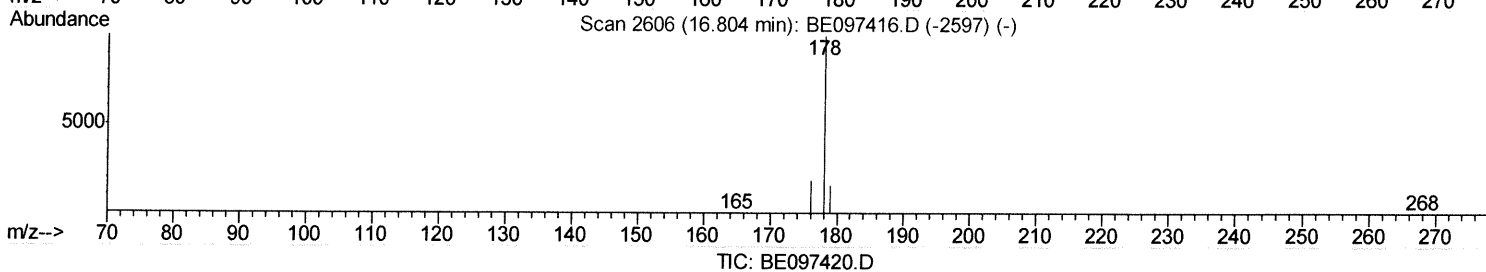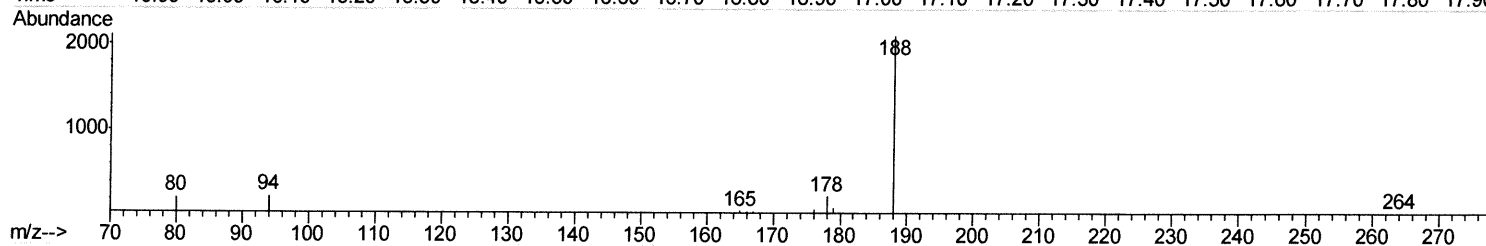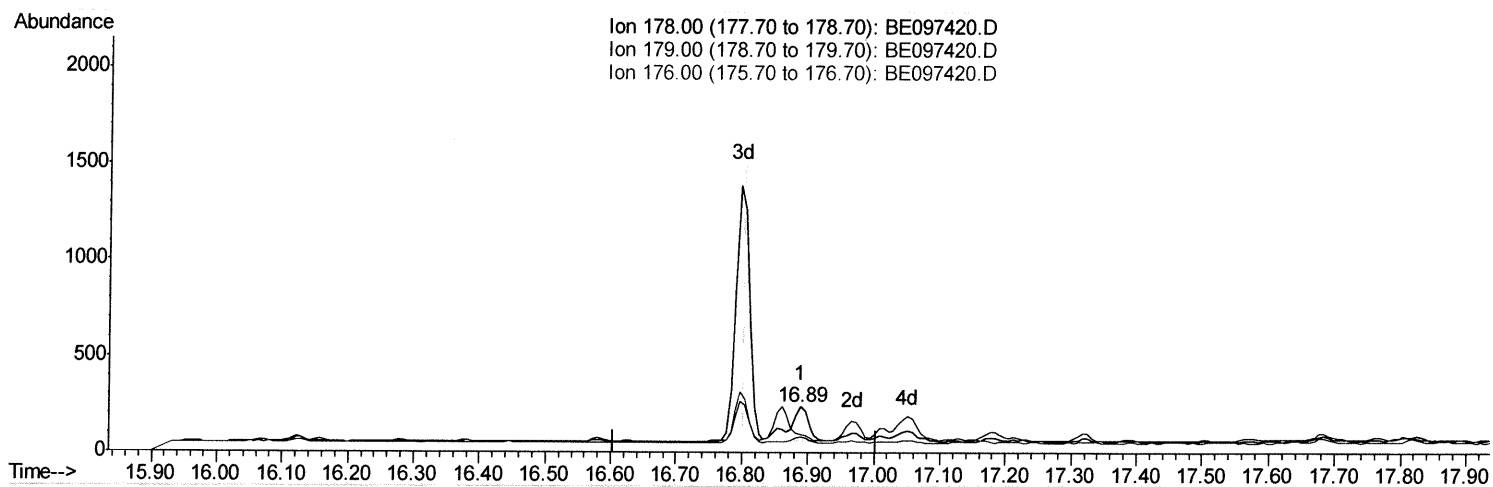

(12) Phenanthrene

16.888min (+0.084) 0.02ng/ul

response 364

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	40.34#
176.00	17.00	35.29#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090718\
 Data File : BE097420.D
 Acq On : 7 Sep 2018 12:05
 Operator : SJ/JU
 Sample : J4688-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Z17

Manual Integrations
 APPROVED

Sohil
 9/11/2018 2:42:26 PM

Quant Time: Sep 08 00:06:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 07 23:49:56 2018
 Response via : Initial Calibration

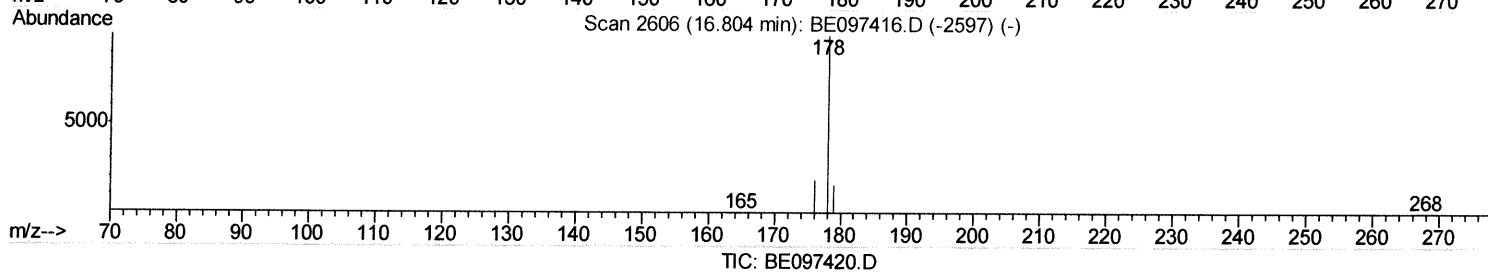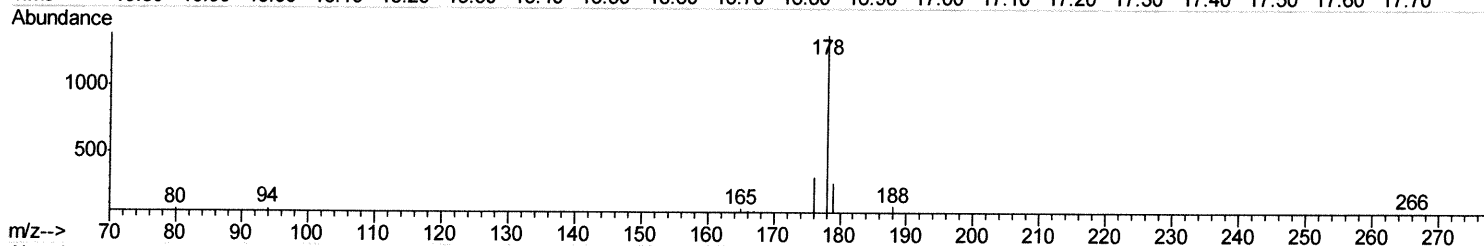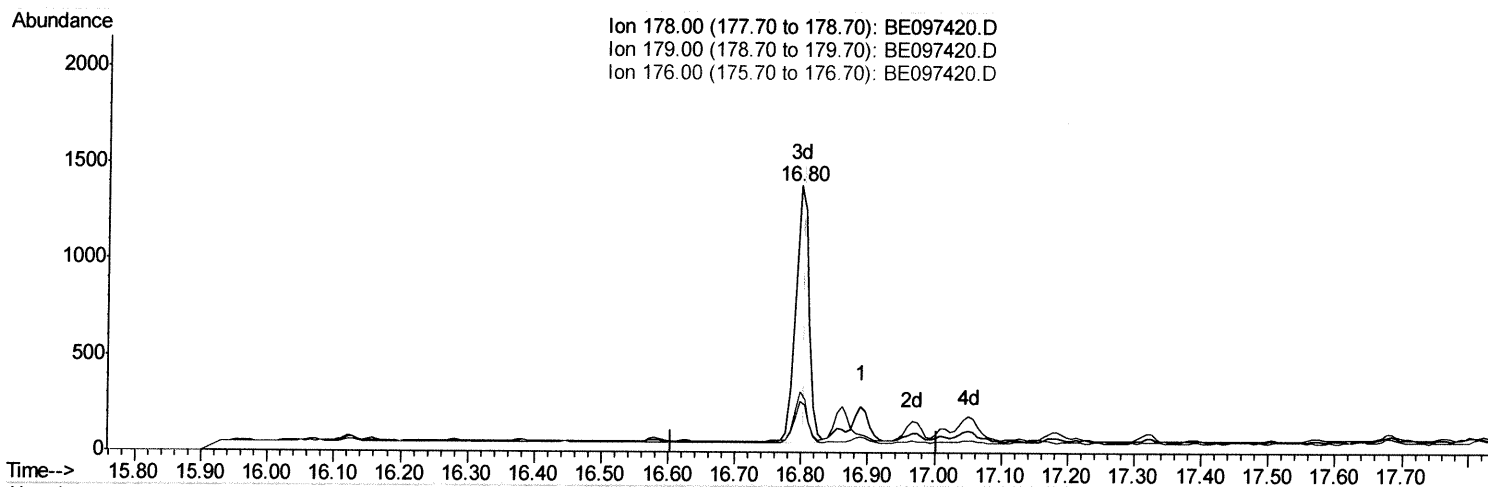

(12) Phenanthrene

16.797min (-0.007) 0.09ng/ul m

85 9/12/18

response 1914

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	18.96
176.00	17.00	22.57#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090718\
Data File : BE097420.D
Acq On : 7 Sep 2018 12:05
Operator : SJ/JU
Sample : J4688-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Z17

Manual Integrations
APPROVED

Sohil
9/11/2018 2:42:26 PM

Quant Time: Sep 08 00:06:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 07 23:49:56 2018
Response via : Initial Calibration

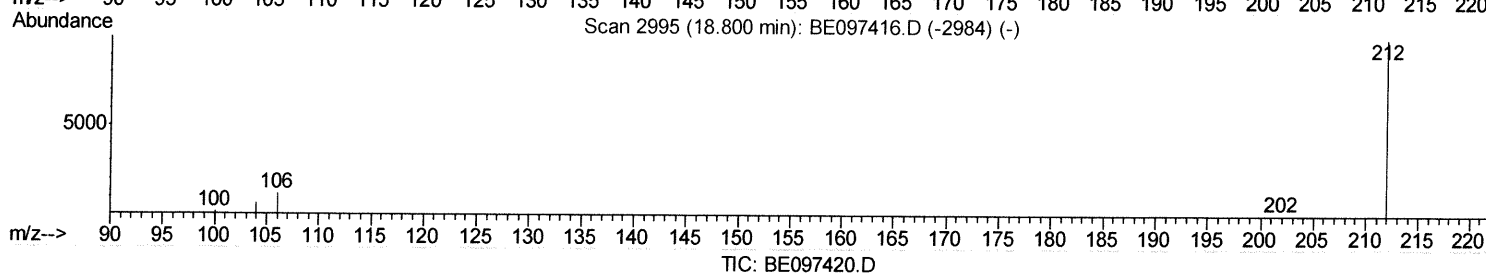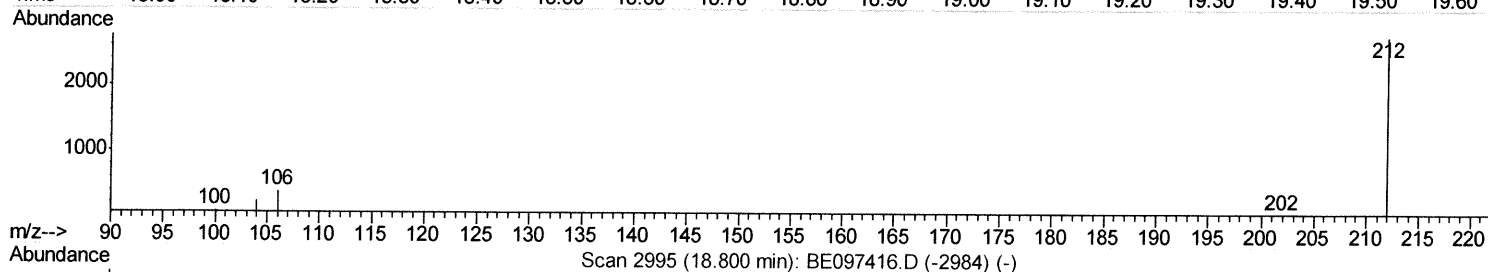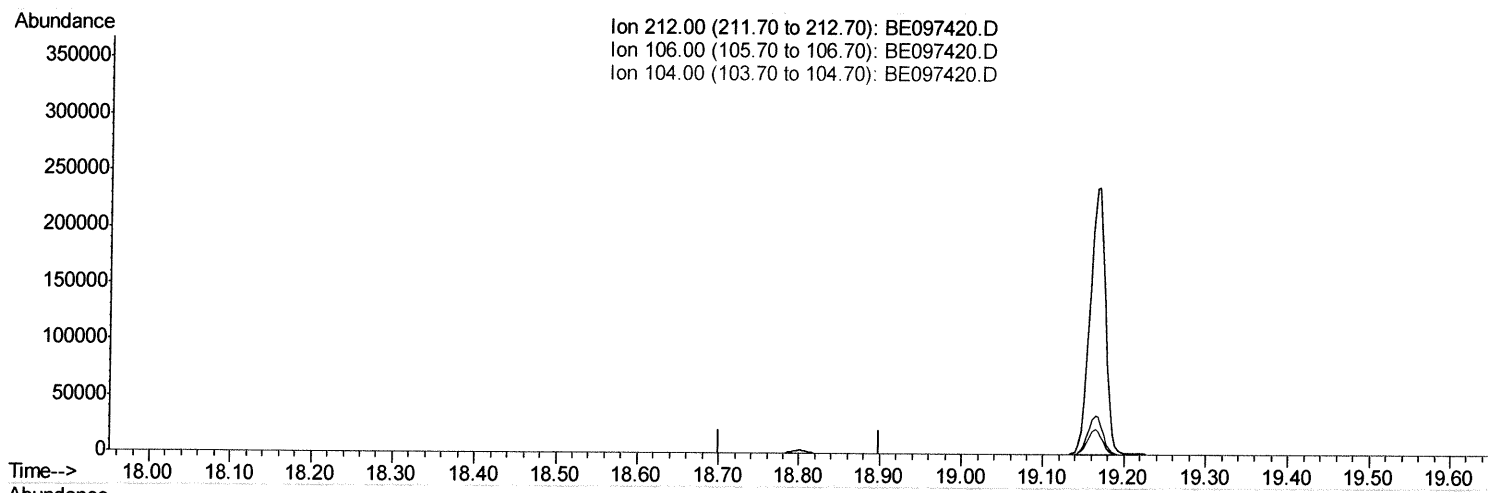

(14) Fluoranthene-d10 (SURR)

18.800min (-18.800) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090718\
 Data File : BE097420.D
 Acq On : 7 Sep 2018 12:05
 Operator : SJ/JU
 Sample : J4688-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Z17

Manual Integrations
 APPROVED

Sohil
 9/11/2018 2:42:26 PM

Quant Time: Sep 08 00:06:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 07 23:49:56 2018
 Response via : Initial Calibration

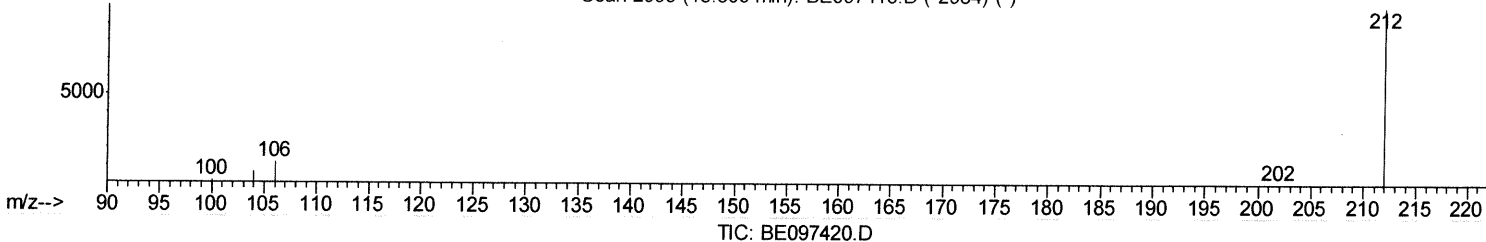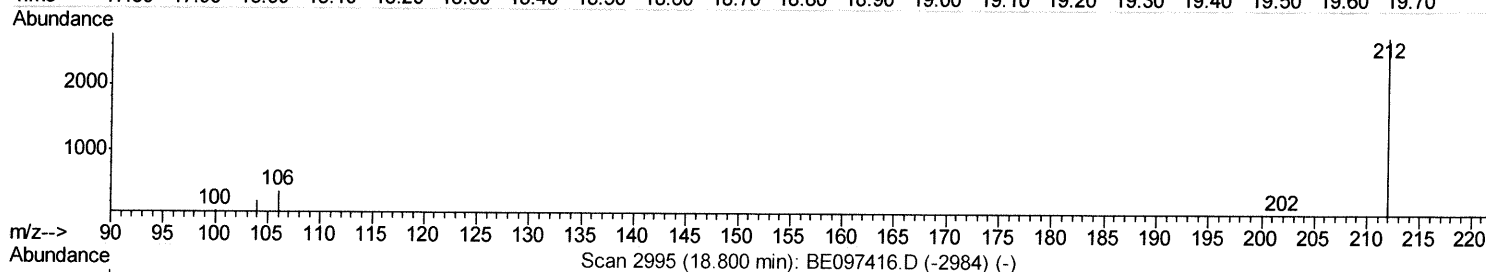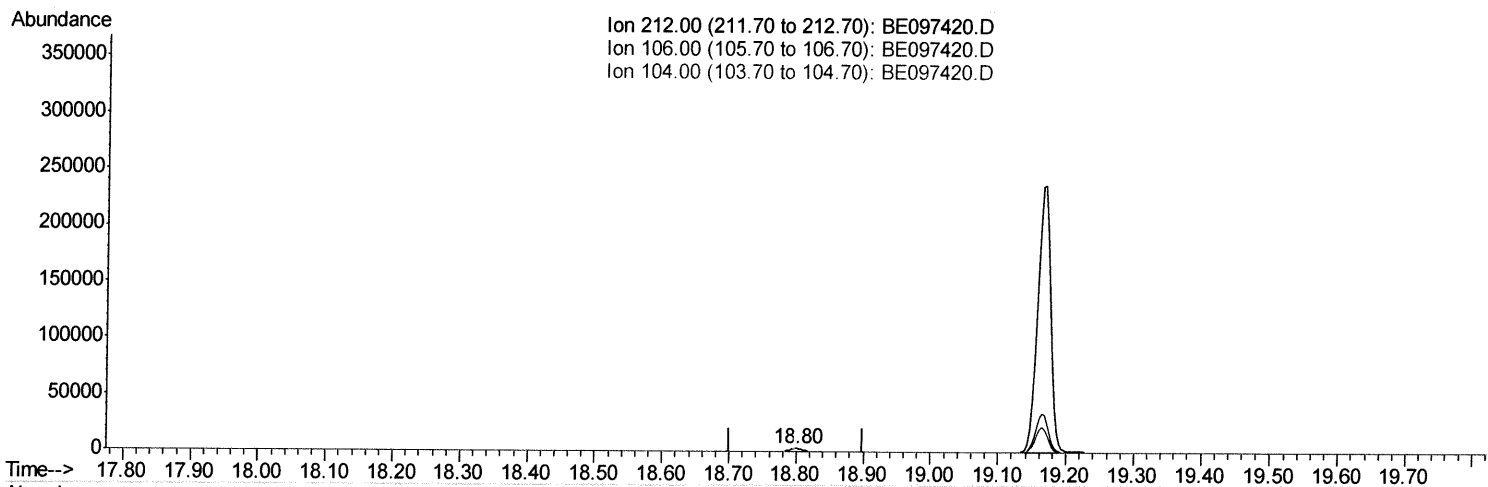

(14) Fluoranthene-d10 (SURR)

18.800min (+0.000) 0.13ng/ul m

response 3660

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090718\
 Data File : BE097420.D
 Acq On : 7 Sep 2018 12:05
 Operator : SJ/JU
 Sample : J4688-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Z17

Manual Integrations
 APPROVED

Sohil
 9/11/2018 2:42:26 PM

Quant Time: Sep 08 00:06:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 07 23:49:56 2018
 Response via : Initial Calibration

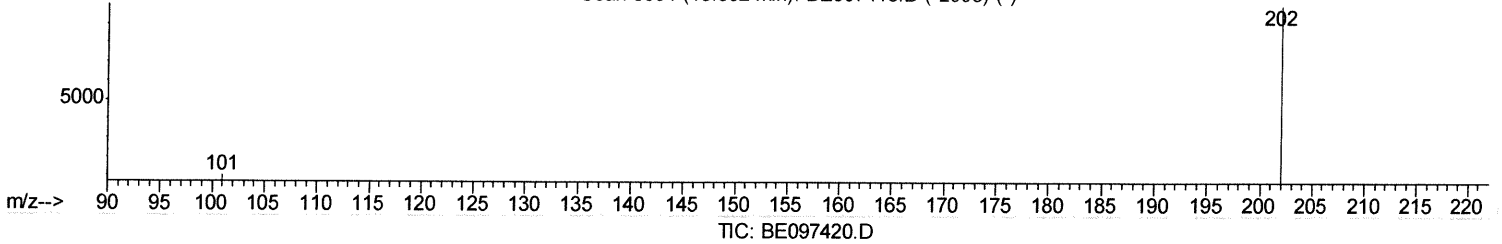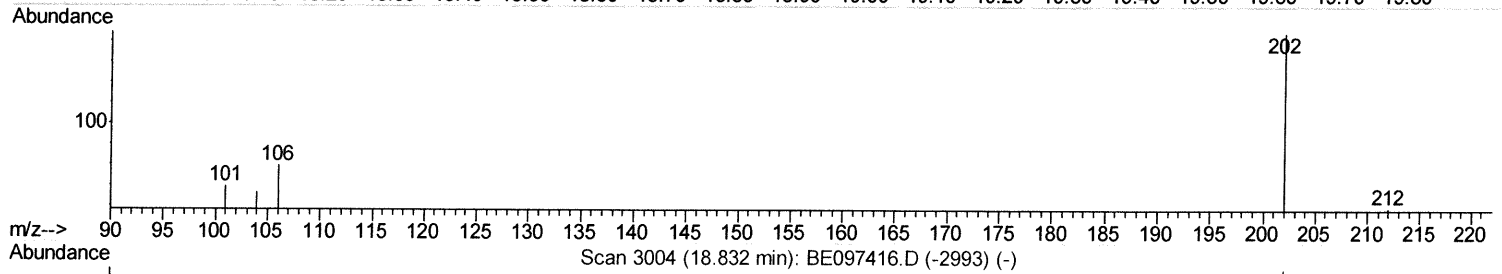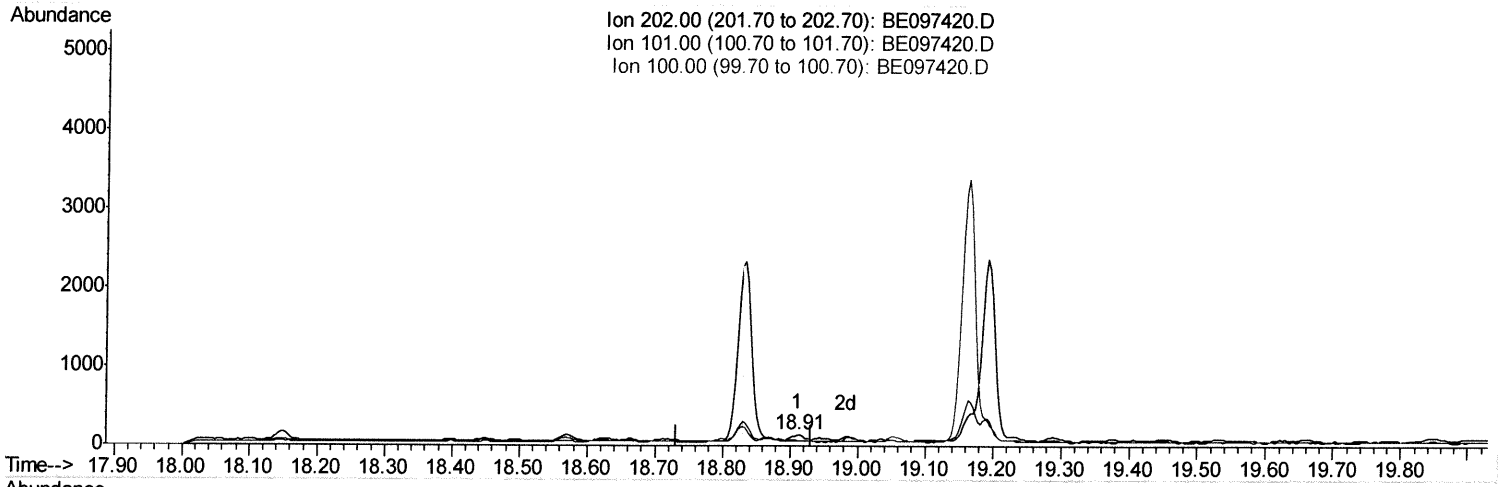

(15) Fluoranthene (C)

18.911min (+0.079) 0.00ng/ul

response 85

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	47.92#
100.00	19.50	40.28#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090718\
 Data File : BE097420.D
 Acq On : 7 Sep 2018 12:05
 Operator : SJ/JU
 Sample : J4688-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Z17

Manual Integrations
 APPROVED

Sohil
 9/11/2018 2:42:26 PM

Quant Time: Sep 08 00:06:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 07 23:49:56 2018
 Response via : Initial Calibration

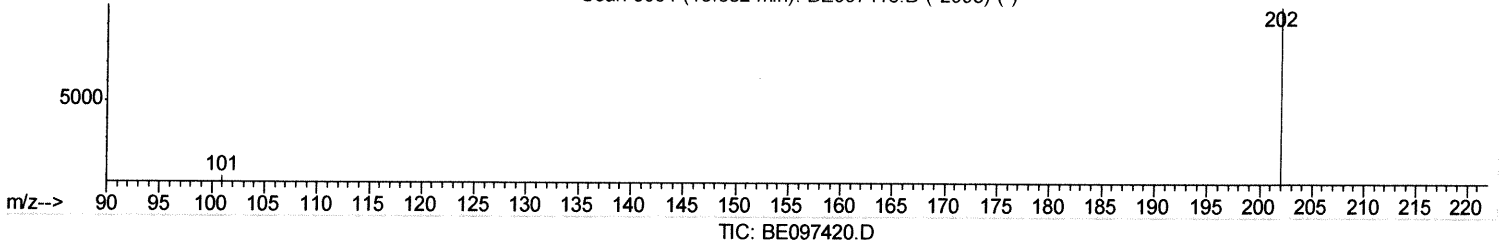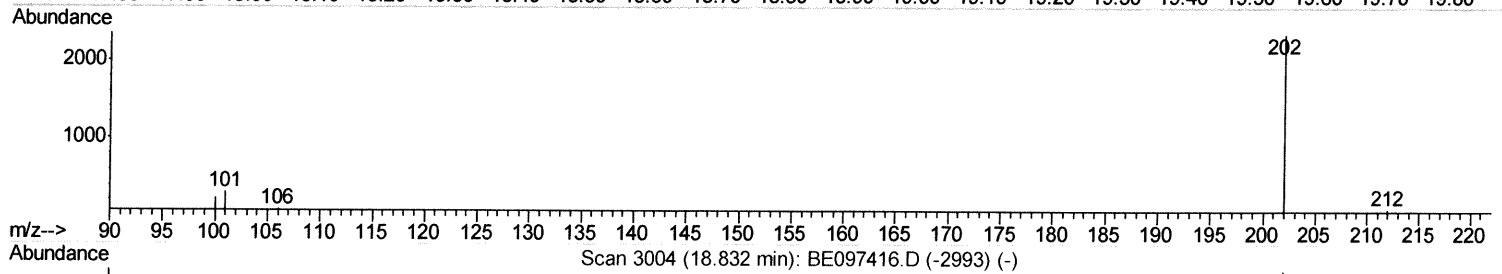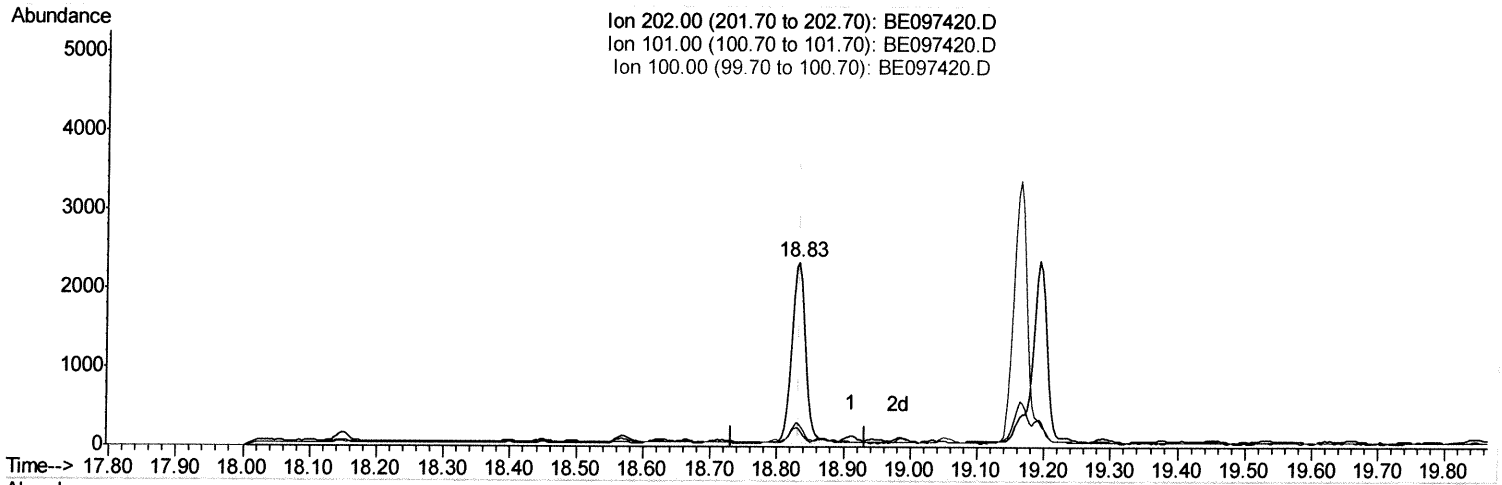

(15) Fluoranthene (C)

18.832min (+0.000) 0.12ng/ul m

response 3211

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	12.60
100.00	19.50	9.78
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090718\
 Data File : BE097420.D
 Acq On : 7 Sep 2018 12:05
 Operator : SJ/JU
 Sample : J4688-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Z17

Manual Integrations
 APPROVED

Sohil
 9/11/2018 2:42:26 PM

Quant Time: Sep 08 00:06:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 07 23:49:56 2018
 Response via : Initial Calibration

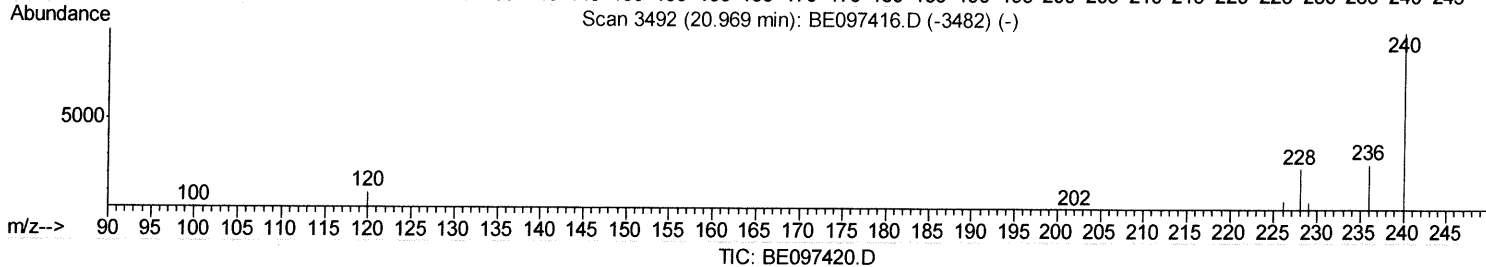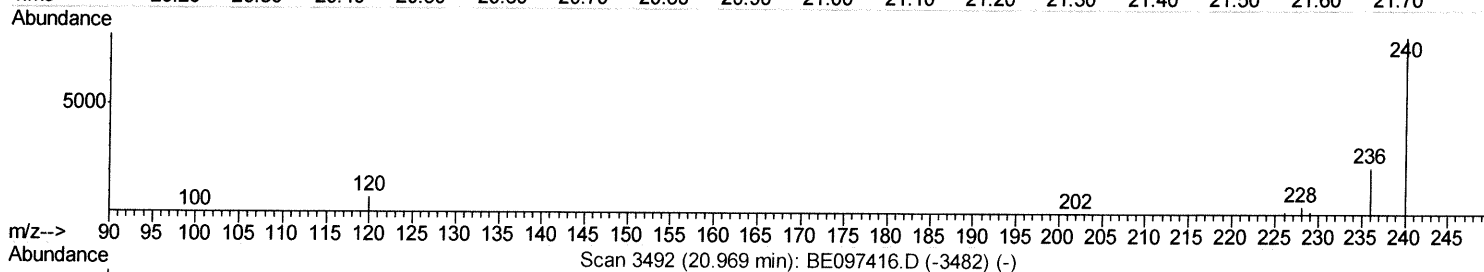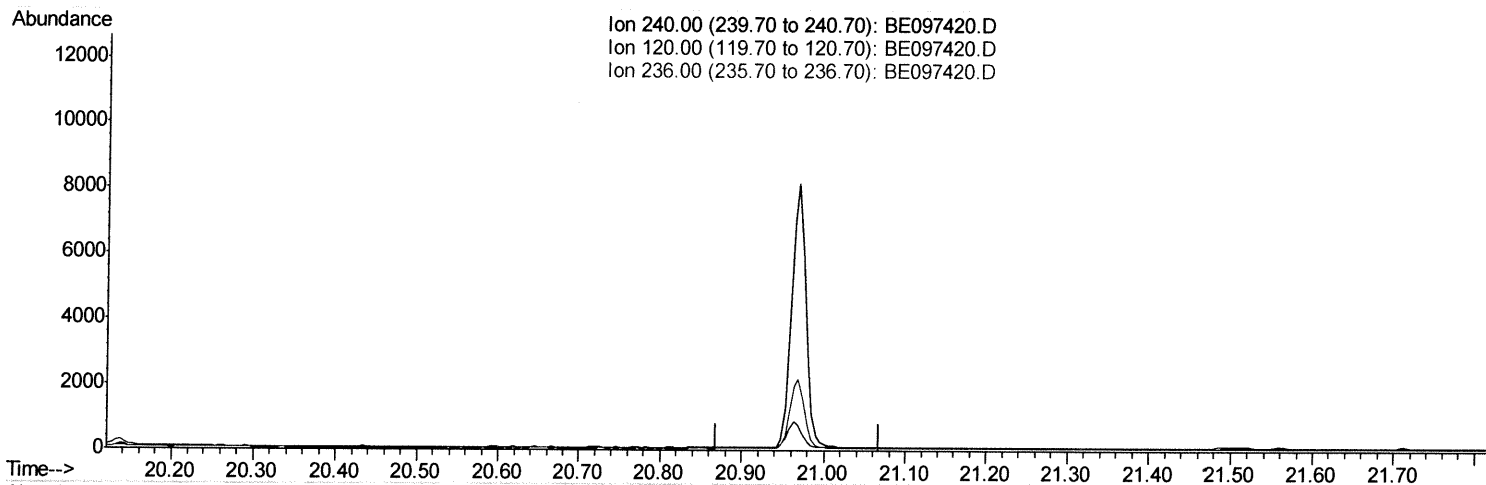

(16) Chrysene-d12 (I)

20.969min (-20.969) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	20.60	0.00#
236.00	34.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090718\
 Data File : BE097420.D
 Acq On : 7 Sep 2018 12:05
 Operator : SJ/JU
 Sample : J4688-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Z17

Manual Integrations
 APPROVED

Sohil
 9/11/2018 2:42:26 PM

Quant Time: Sep 08 00:06:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 07 23:49:56 2018
 Response via : Initial Calibration

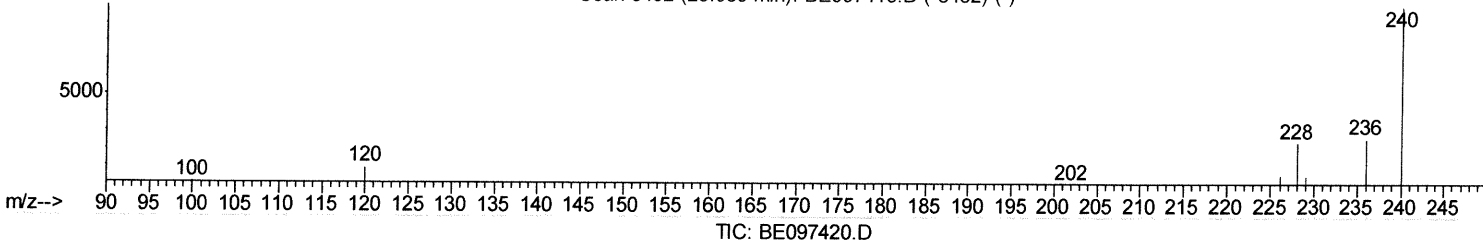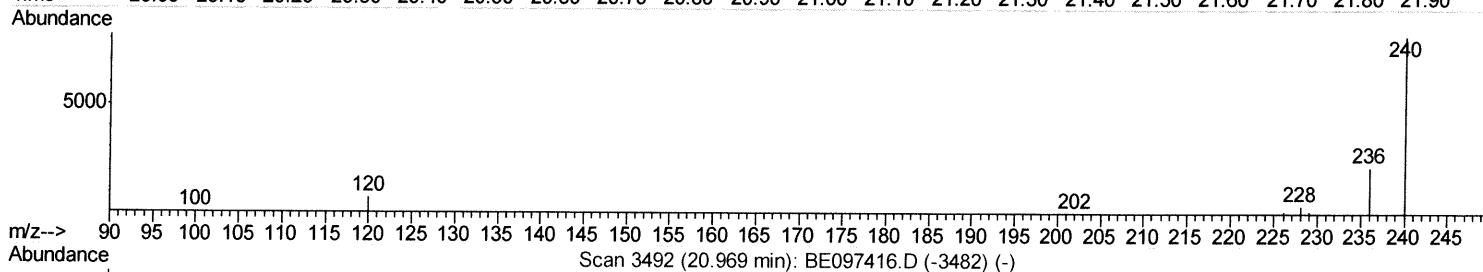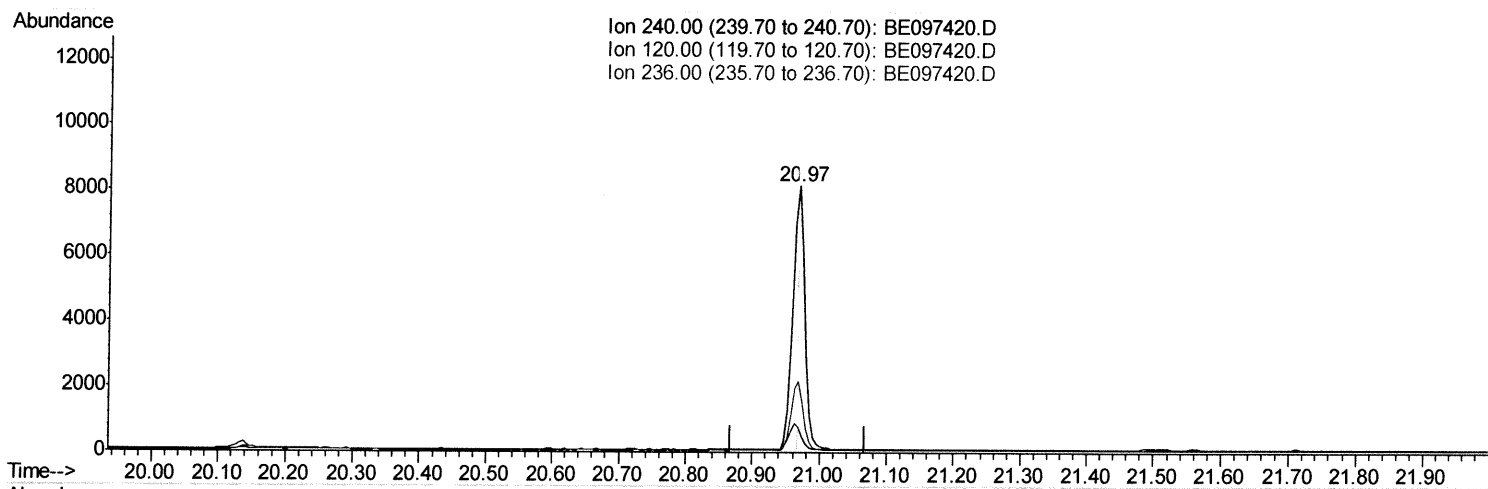

(16) Chrysene-d12 (I)

20.968min (-0.000) 0.40ng/ul m

response 9850

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	9.58#
236.00	34.90	27.06#
0.00	0.00	0.00

Handwritten signature/initials

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090718\
 Data File : BE097420.D
 Acq On : 7 Sep 2018 12:05
 Operator : SJ/JU
 Sample : J4688-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Z17

Manual Integrations
 APPROVED

Sohil
 9/11/2018 2:42:26 PM

Quant Time: Sep 08 00:08:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 07 23:49:56 2018
 Response via : Initial Calibration

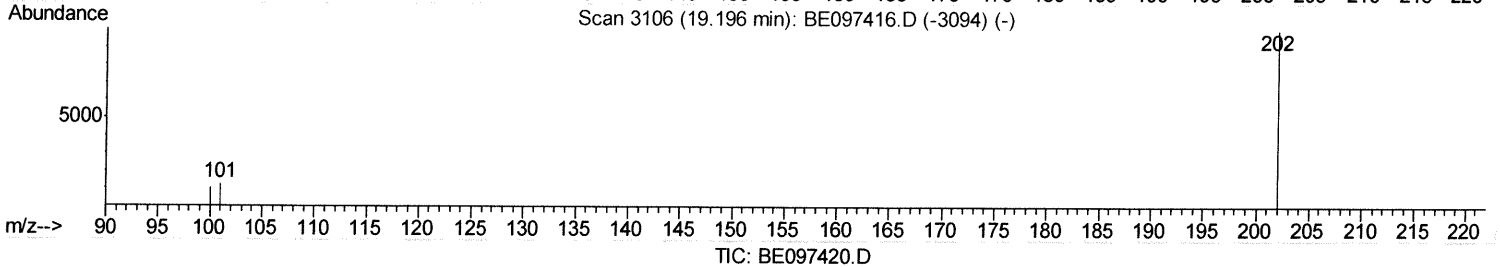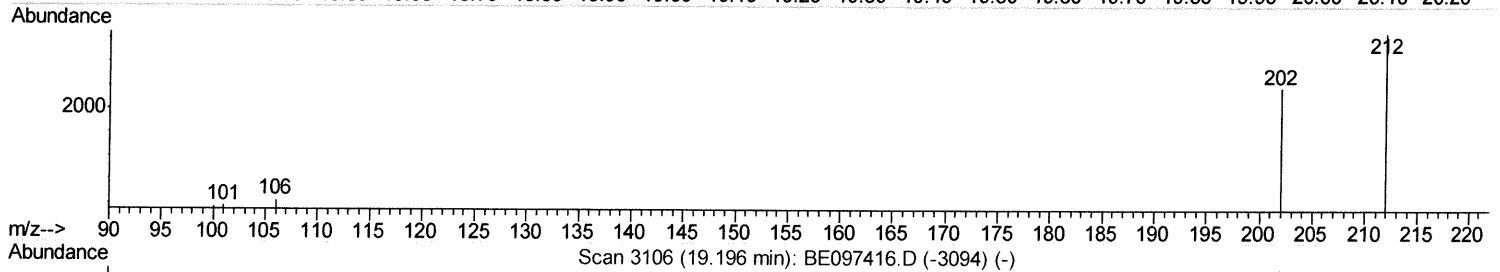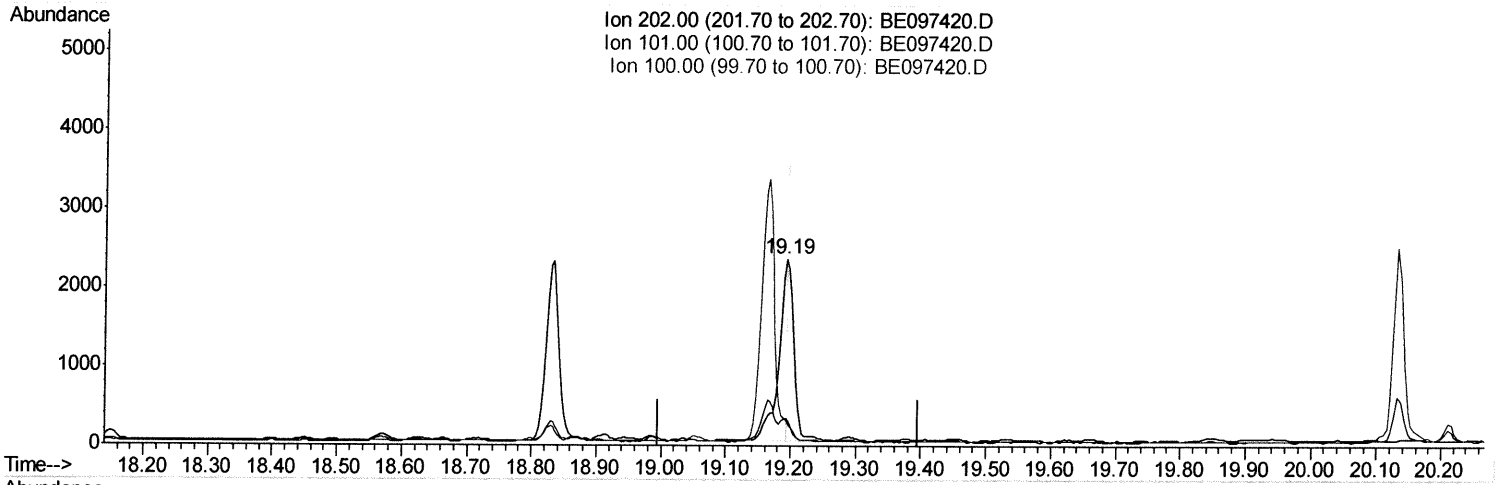

(17) Pyrene

19.193min (-0.004) 0.13ng/ul

response 3532

Ion	Exp%	Act%
202.00	100	100
101.00	22.80	14.64#
100.00	19.50	13.45#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090718\
 Data File : BE097420.D
 Acq On : 7 Sep 2018 12:05
 Operator : SJ/JU
 Sample : J4688-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Z17

Manual Integrations
 APPROVED

Sohil
 9/11/2018 2:42:26 PM

Quant Time: Sep 08 00:08:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 07 23:49:56 2018
 Response via : Initial Calibration

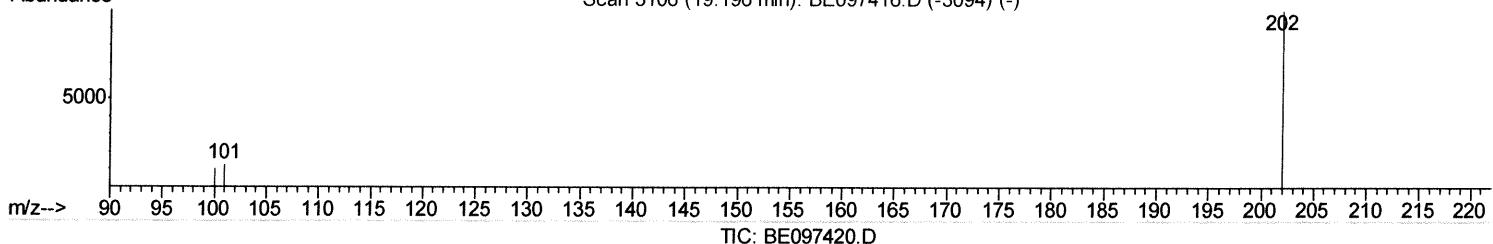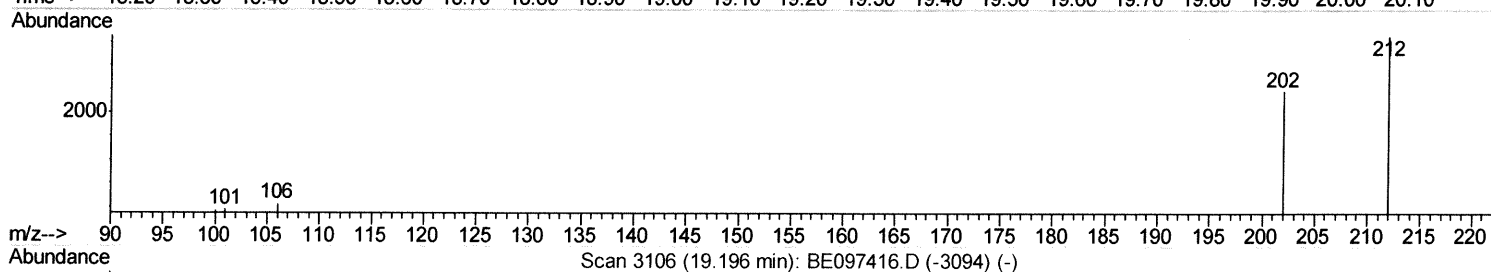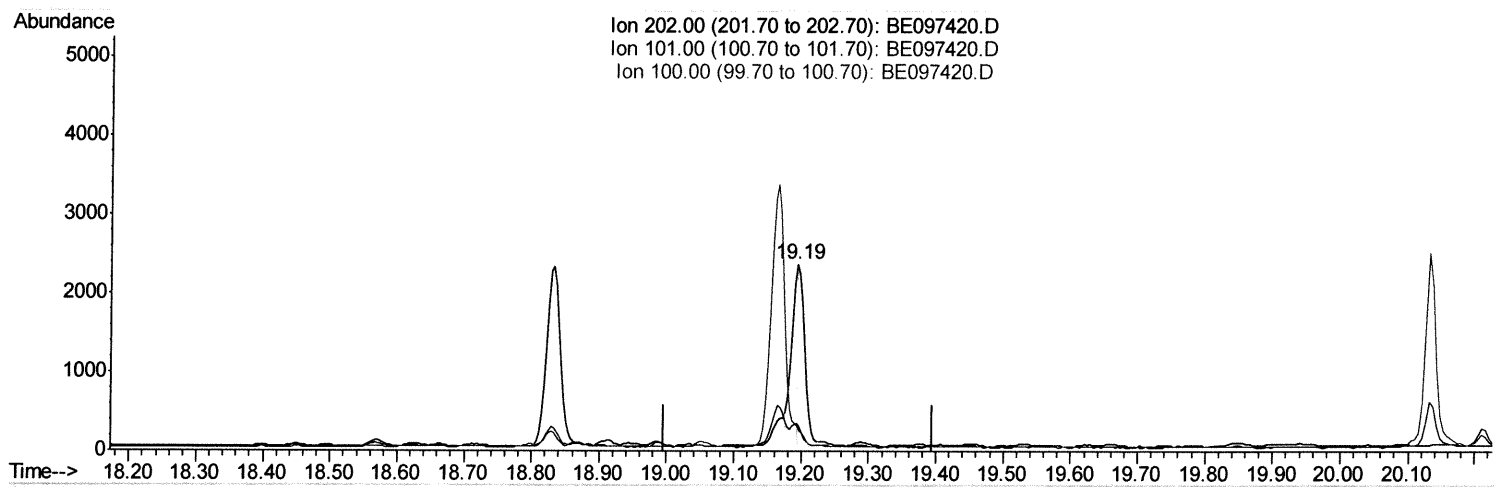

(17) Pyrene

19.193min (-0.004) 0.12ng/ul m

response 3057

Ion	Exp%	Act%
202.00	100	100
101.00	22.80	14.64#
100.00	19.50	13.45#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090718\
Data File : BE097420.D
Acq On : 7 Sep 2018 12:05
Operator : SJ/JU
Sample : J4688-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Z17


Manual Integrations
APPROVED

Sohil
9/11/2018 2:42:26 PM

Quant Time: Sep 08 00:08:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 07 23:49:56 2018
Response via : Initial Calibration

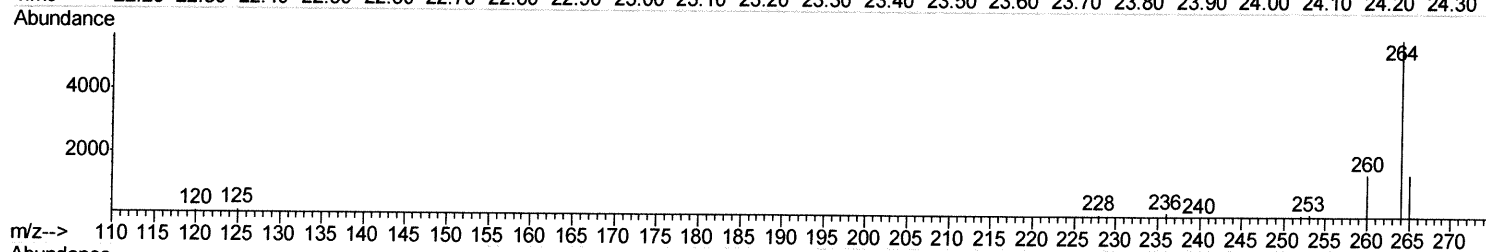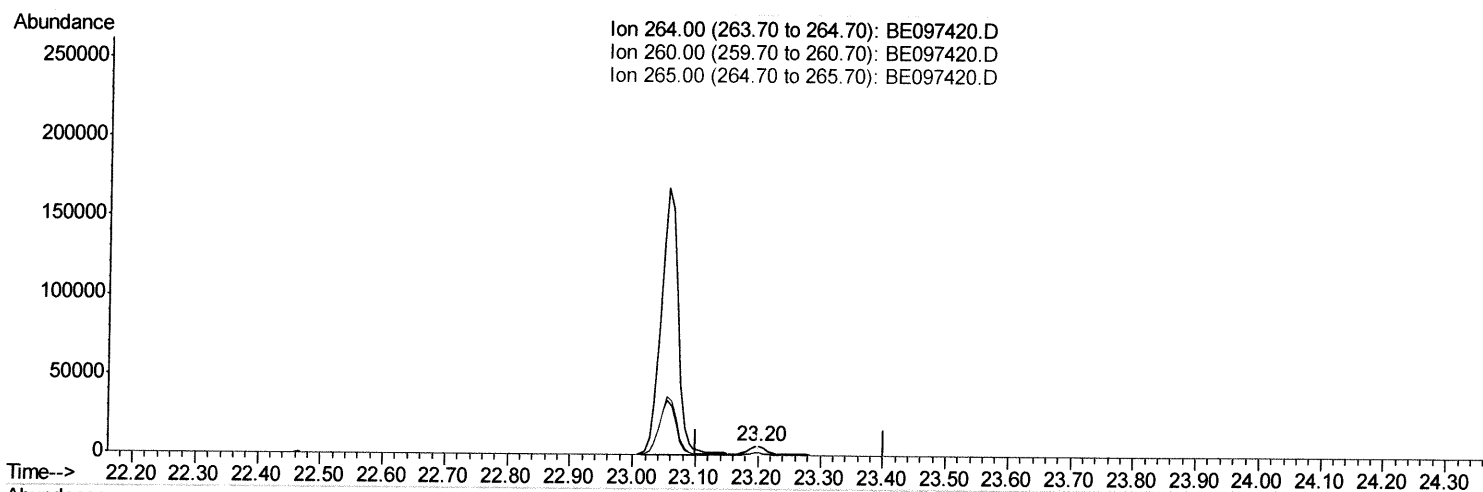

Scan 3826 (23.202 min): BE097416.D (-3817) (-)

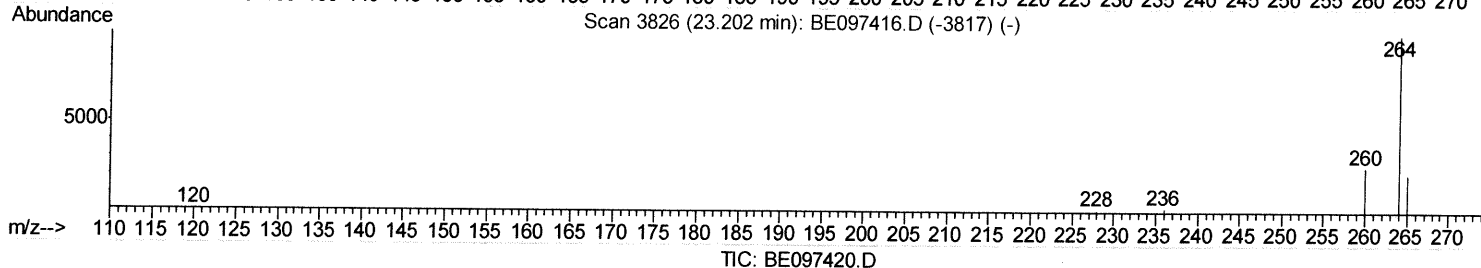

(20) Perylene-d12 (I)

23.202min (+0.000) 0.40ng/ul

response 12342

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.77
265.00	103.50	25.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090718\
 Data File : BE097420.D
 Acq On : 7 Sep 2018 12:05
 Operator : SJ/JU
 Sample : J4688-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Z17

Manual Integrations
 APPROVED

Sohil
 9/11/2018 2:42:26 PM

Quant Time: Sep 08 00:08:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 07 23:49:56 2018
 Response via : Initial Calibration

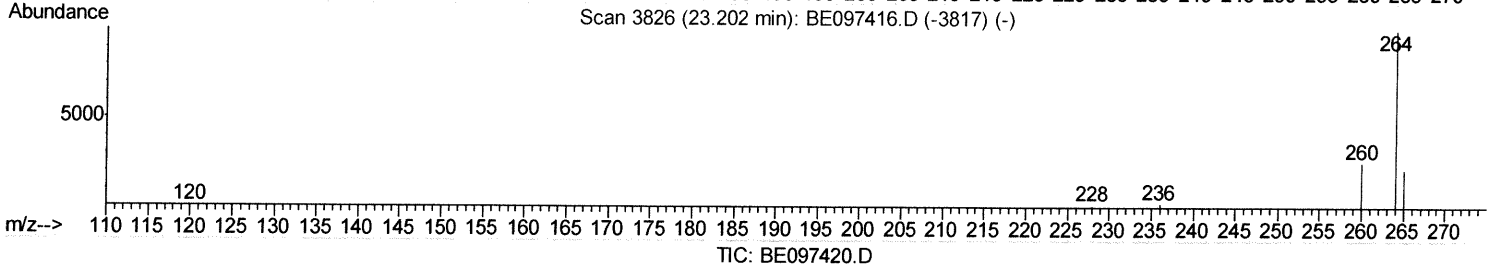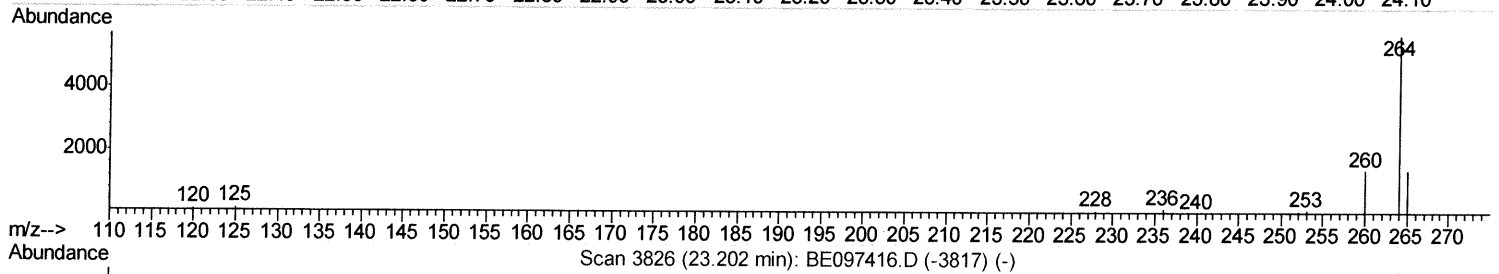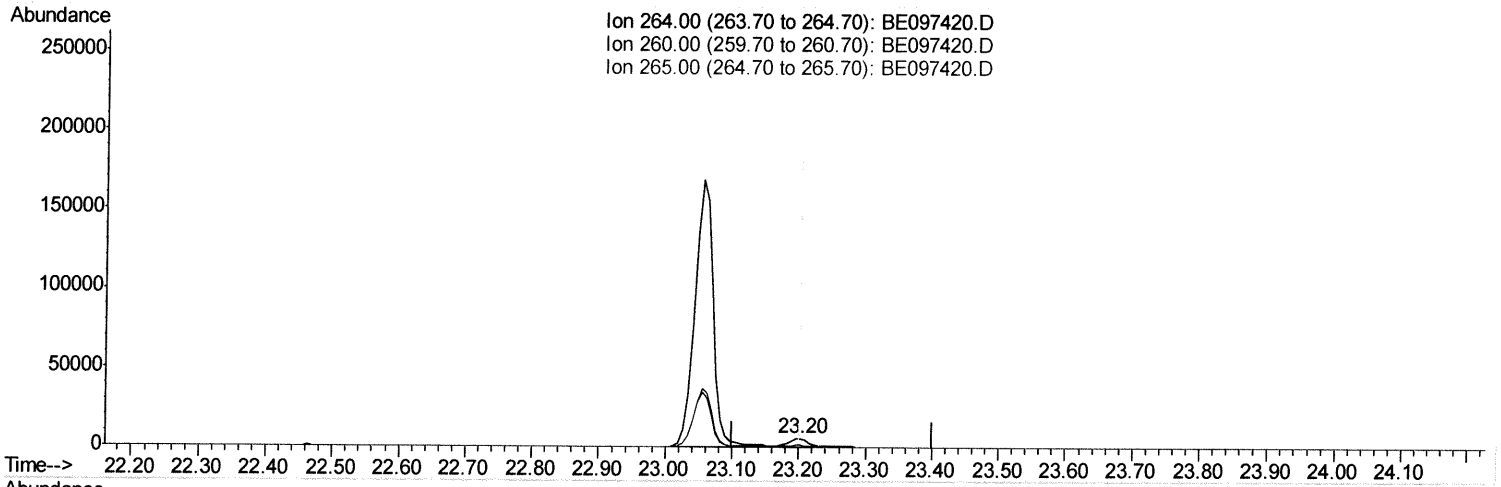

(20) Perylene-d12 (I)

23.202min (+0.000) 0.40ng/ul m

response 8815

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.77
265.00	103.50	25.00#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090718\
Data File : BE097420.D
Acq On : 7 Sep 2018 12:05
Operator : SJ/JU
Sample : J4688-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Z17

Manual Integrations
APPROVED

Sohil
9/11/2018 2:42:26 PM

Quant Time: Sep 08 00:08:57 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 07 23:49:56 2018
Response via : Initial Calibration

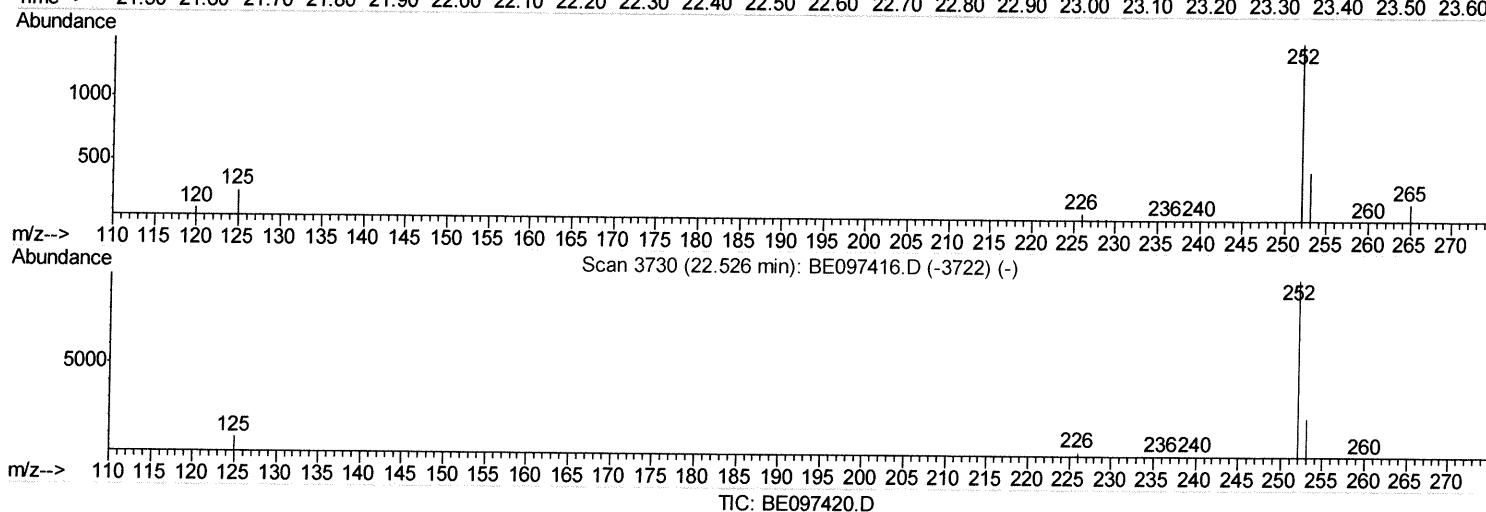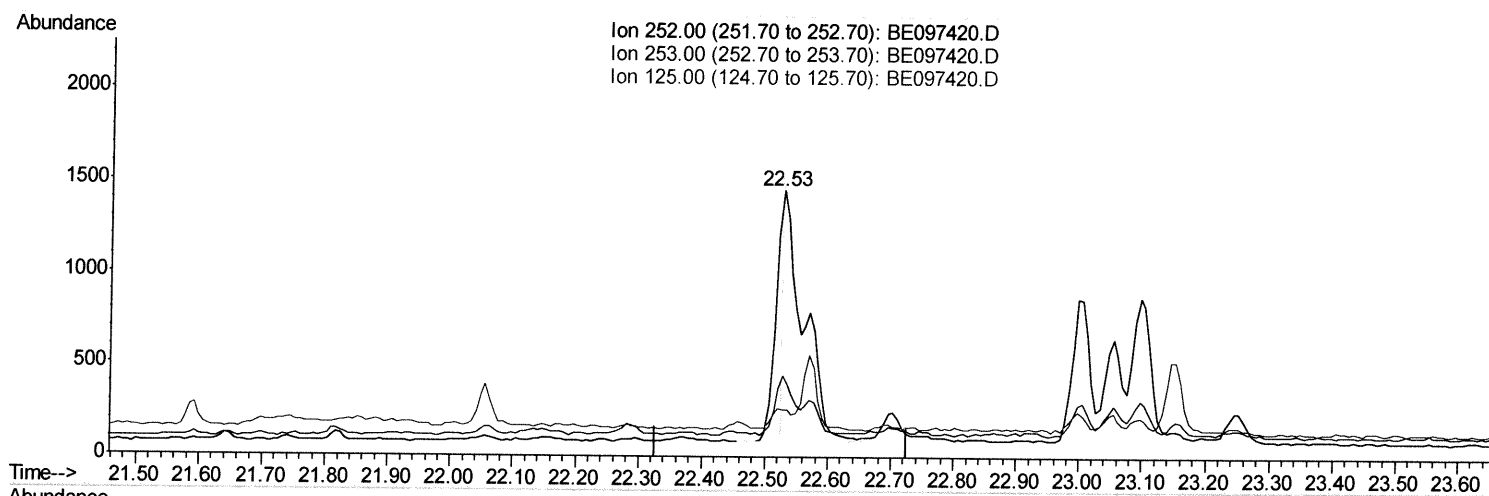

(21) Benzo(b)fluoranthene

22.527min (+0.000) 0.17ng/ul

response 4085

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	30.26
125.00	17.50	17.54
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090718\
 Data File : BE097420.D
 Acq On : 7 Sep 2018 12:05
 Operator : SJ/JU
 Sample : J4688-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Z17

Manual Integrations
 APPROVED

Sohil
 9/11/2018 2:42:26 PM

Quant Time: Sep 08 00:08:57 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 07 23:49:56 2018
 Response via : Initial Calibration

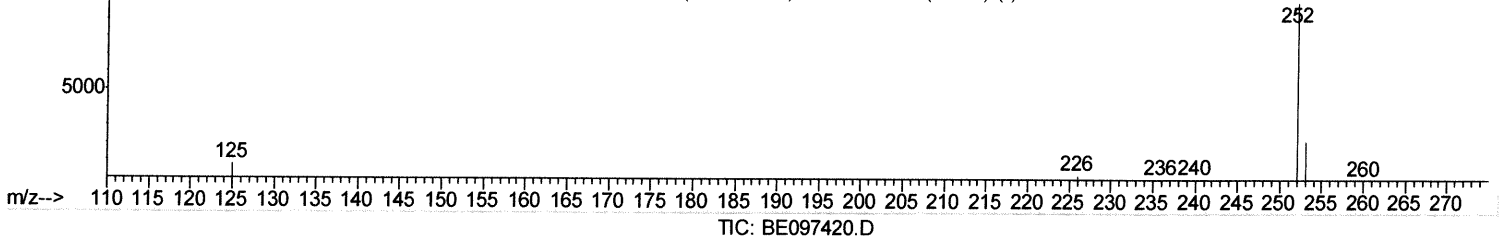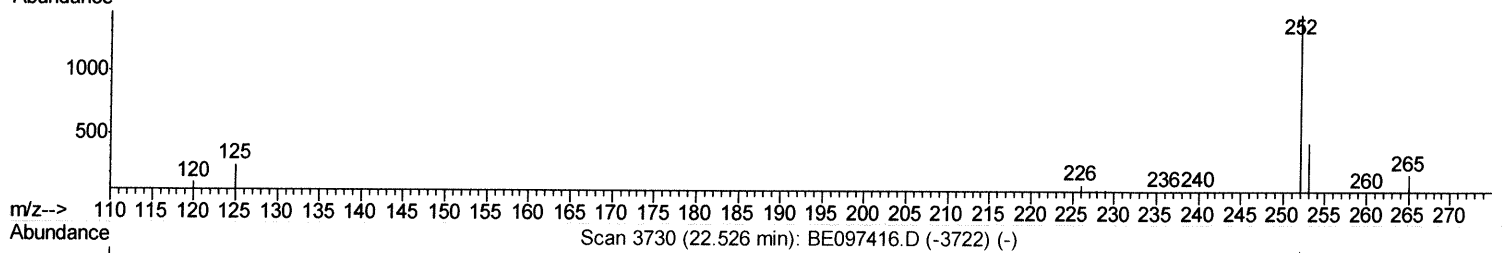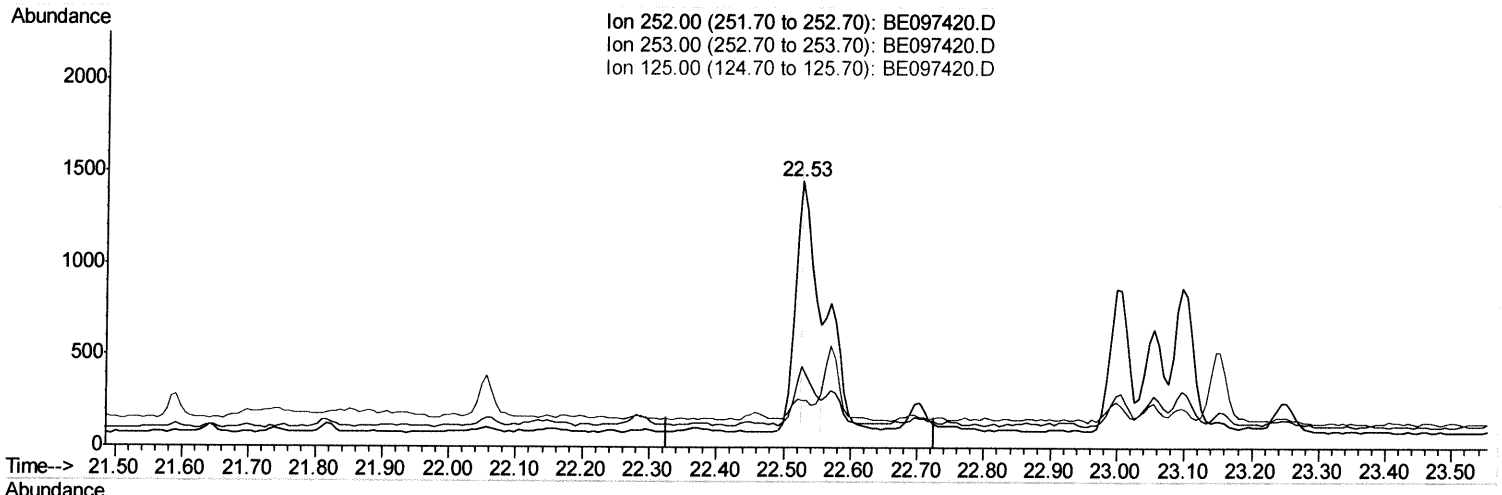

(21) Benzo(b)fluoranthene

22.527min (+0.000) 0.12ng/ul m

response 2854

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	30.26
125.00	17.50	17.54
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090718\
Data File : BE097420.D
Acq On : 7 Sep 2018 12:05
Operator : SJ/JU
Sample : J4688-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Z17

Manual Integrations
APPROVED

Sohil
9/11/2018 2:42:26 PM

Quant Time: Sep 08 00:08:57 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 07 23:49:56 2018
Response via : Initial Calibration

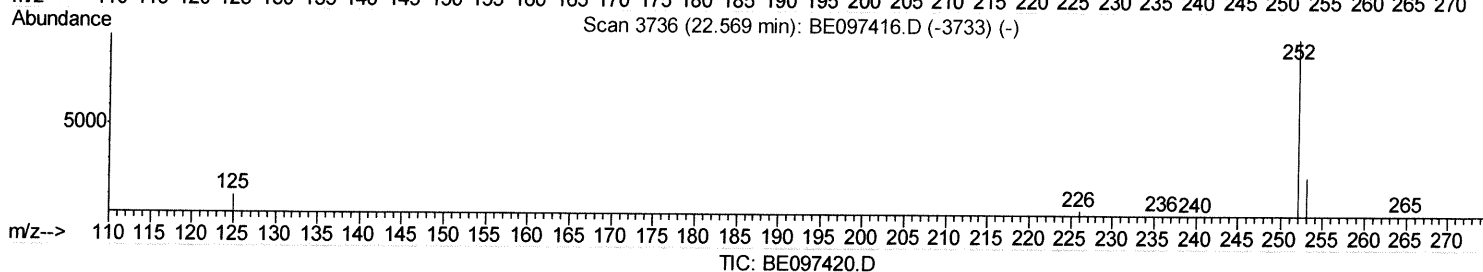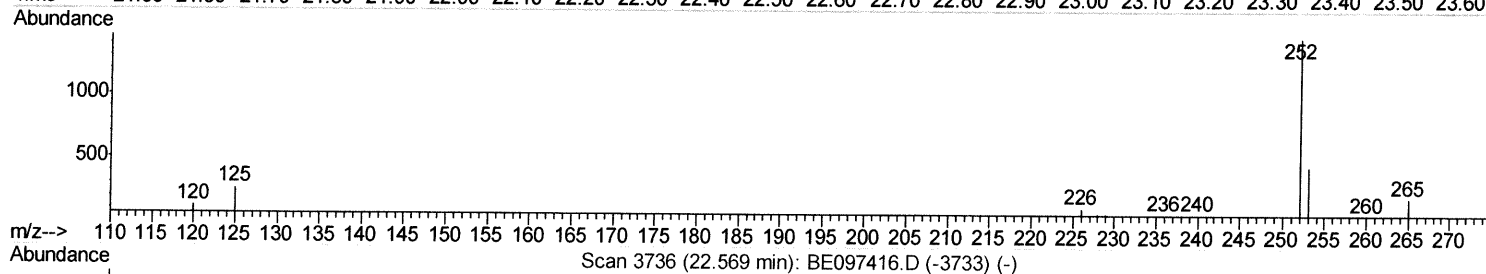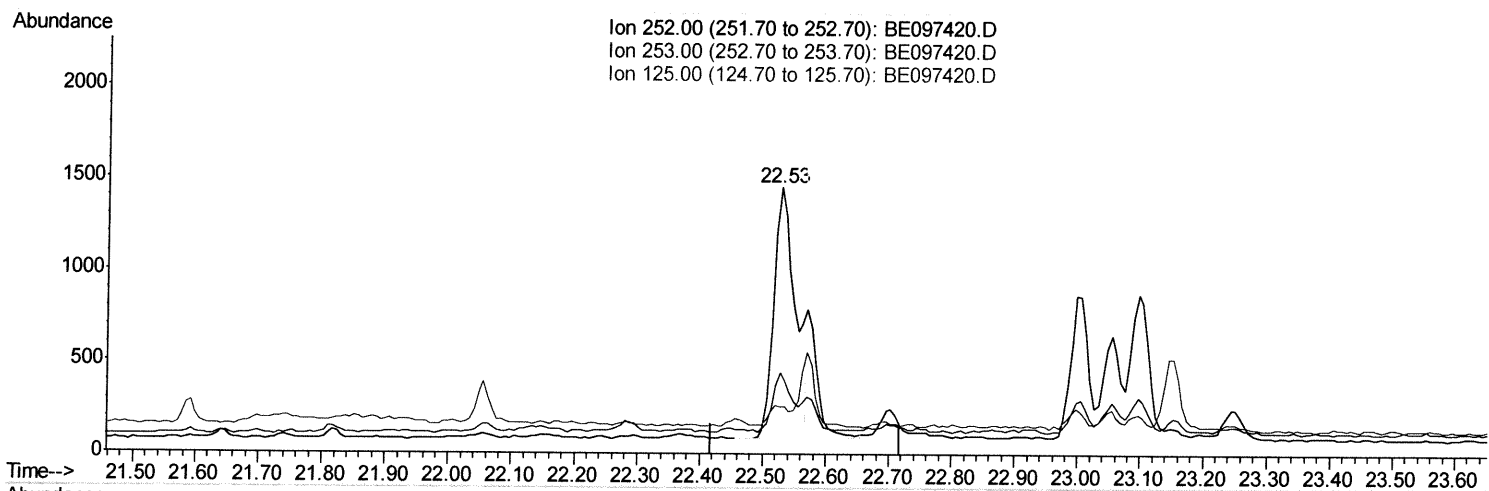

(22) Benzo(k)fluoranthene

22.527min (-0.042) 0.16ng/ul

response 4085

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	30.26
125.00	17.10	17.54
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090718\
 Data File : BE097420.D
 Acq On : 7 Sep 2018 12:05
 Operator : SJ/JU
 Sample : J4688-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Z17

Manual Integrations
 APPROVED

Sohil
 9/11/2018 2:42:26 PM

Quant Time: Sep 08 00:08:57 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 07 23:49:56 2018
 Response via : Initial Calibration

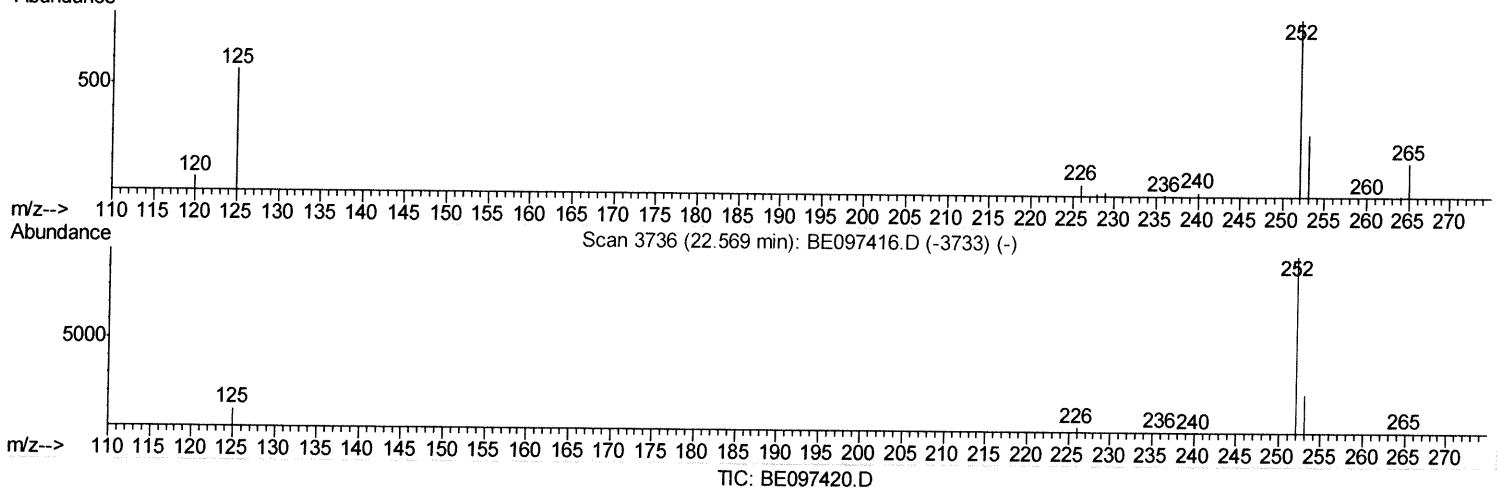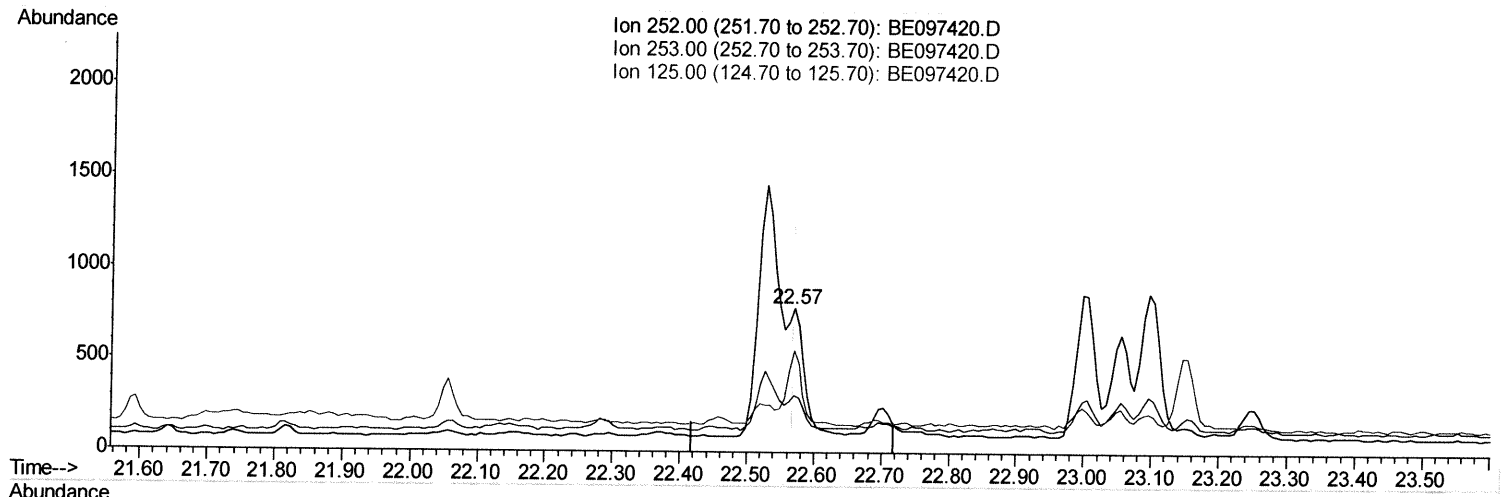

(22) Benzo(k)fluoranthene

22.569min (+0.000) 0.04ng/ul m

response 1098

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	39.82#
125.00	17.10	70.61#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE090718\
 Data File : BE097420.D
 Acq On : 7 Sep 2018 12:05
 Operator : SJ/JU
 Sample : J4688-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Z17

Manual Integrations
 APPROVED

Sohil
 9/11/2018 2:42:26 PM

Quant Time: Sep 08 00:10:54 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 07 23:49:56 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	972	0.40	ng/ul	0.00
2) Naphthalene-d8	10.12	136	5009	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.01	164	3098	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.76	188	8323m	0.40	ng/ul	0.00
16) Chrysene-d12	20.97	240	9850m	0.40	ng/ul	0.00
20) Perylene-d12	23.20	264	8815m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.72	152	1008	0.13	ng/ul	0.00
14) Fluoranthene-d10	18.80	212	3660m	0.13	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.17	128	338	0.028	ng/ul#	67
5) 2-Methylnaphthalene	11.80	142	272	0.035	ng/ul	96
12) Phenanthrene	16.80	178	1914m	0.089	ng/ul	
15) Fluoranthene	18.83	202	3211m	0.117	ng/ul	
17) Pyrene	19.19	202	3057m	0.115	ng/ul	
18) Benzo(a)anthracene	20.95	228	1572	0.062	ng/ul#	88
19) Chrysene	21.00	228	3036	0.104	ng/ul#	91
21) Benzo(b)fluoranthene	22.53	252	2854m	0.121	ng/ul	
22) Benzo(k)fluoranthene	22.57	252	1098m	0.042	ng/ul	
23) Benzo(a)pyrene	23.10	252	1496	0.069	ng/ul	98
24) Indeno(1,2,3-cd)pyrene	25.49	276	1267	0.045	ng/ul#	84
26) Benzo(a,h,i)perylene	26.19	276	1264	0.052	ng/ul#	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed