


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE091018\
 Data File : BE097439.D
 Acq On : 10 Sep 2018 8:14
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE082218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 22 18:07:26 2018

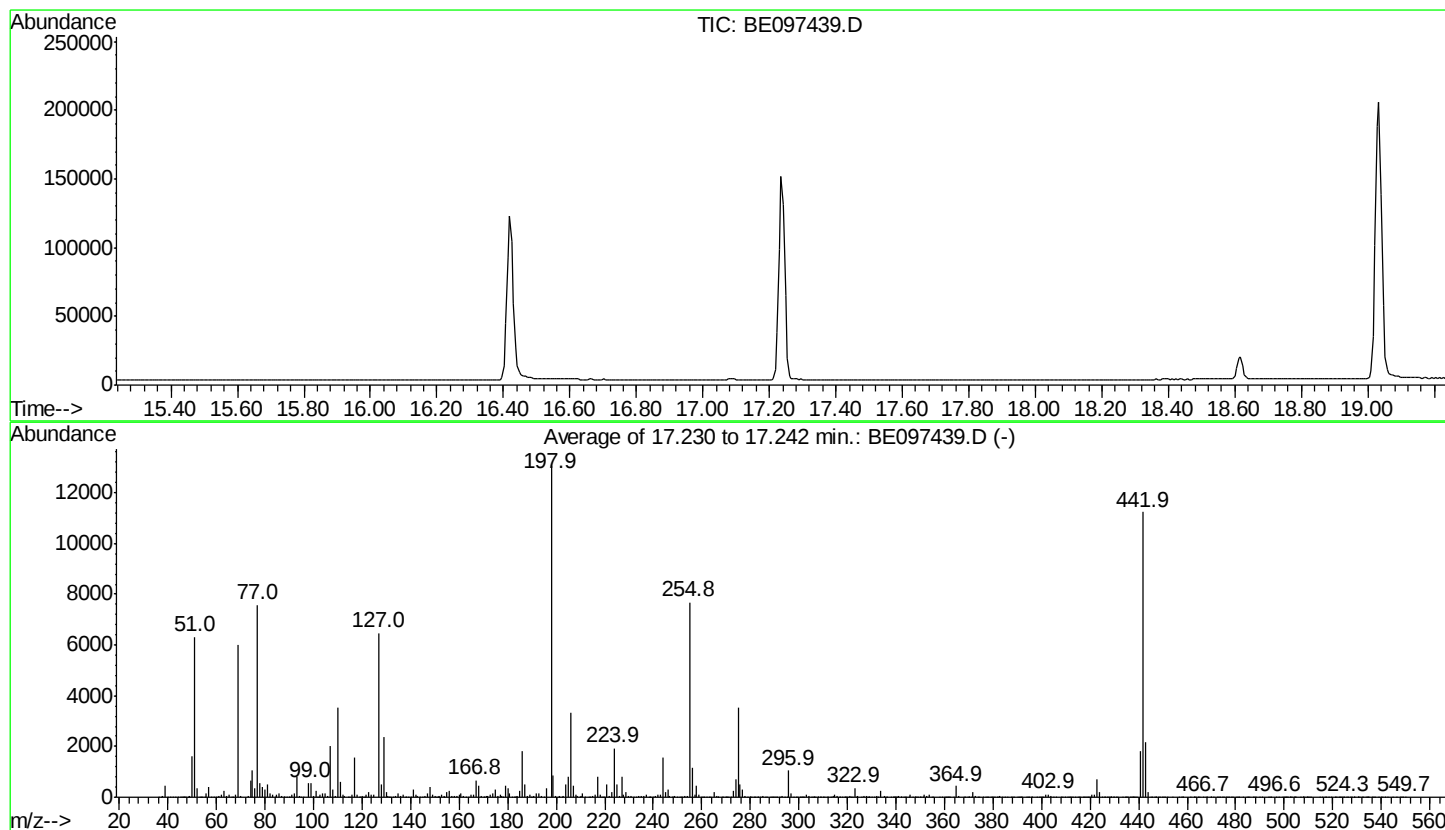

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.3	6308	PASS
68	69	0.00	2	2.0	122	PASS
69	198	0.00	100	46.0	6011	PASS
70	69	0.00	2	0.8	46	PASS
127	198	10	80	49.5	6464	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	13069	PASS
199	198	5	9	6.6	868	PASS
275	198	10	60	26.9	3518	PASS
365	198	1	100	3.4	445	PASS
441	198	0.01	100	14.0	1834	PASS
442	198	50	100	86.0	11240	PASS
443	442	15	24	19.4	2186	PASS