

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE091718\
 Data File : BE097525.D
 Acq On : 18 Sep 2018 10:00
 Operator : SJ/JU
 Sample : J4913-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BP-TT-AOC22-MW09-20180911

Quant Time: Sep 18 10:47:15 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE091718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 17 18:57:11 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	947	0.40	ng	0.00
7) Naphthalene-d8	10.13	136	4339	0.40	ng	0.00
13) Acenaphthene-d10	14.00	164	2612	0.40	ng	0.00
19) Phenanthrene-d10	16.75	188	7236	0.40	ng	-0.01
27) Chrysene-d12	20.97	240	8844	0.40	ng	0.00
34) Perylene-d12	23.20	264	8901	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.06	112	527	0.16	ng	0.00
5) Phenol-d6	6.60	99	448	0.11	ng	0.00
8) Nitrobenzene-d5	8.53	82	1502	0.43	ng	0.00
11) 2-Methylnaphthalene-d10	11.72	152	2610	0.42	ng	0.00
14) 2,4,6-Tribromophenol	15.52	330	536	0.39	ng	-0.01
15) 2-Fluorobiphenyl	12.62	172	5013	0.55	ng	0.00
25) Fluoranthene-d10	18.80	212	37372	0.43	ng	0.00
29) Terphenyl-d14	19.41	244	8362	0.49	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.09	88	133	0.081	ng	Qvalue # 16
22) Pentachlorophenol	16.45	266	23	0.091	ng	95
32) Bis(2-ethylhexyl)phthalate	20.91	149	5574	0.113	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE091718\
Data File : BE097525.D
Acq On : 18 Sep 2018 10:00
Operator : SJ/JU
Sample : J4913-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-TT-AOC22-MW09-20180911

Quant Time: Sep 18 10:47:15 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE091718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 17 18:57:11 2018
Response via : Initial Calibration

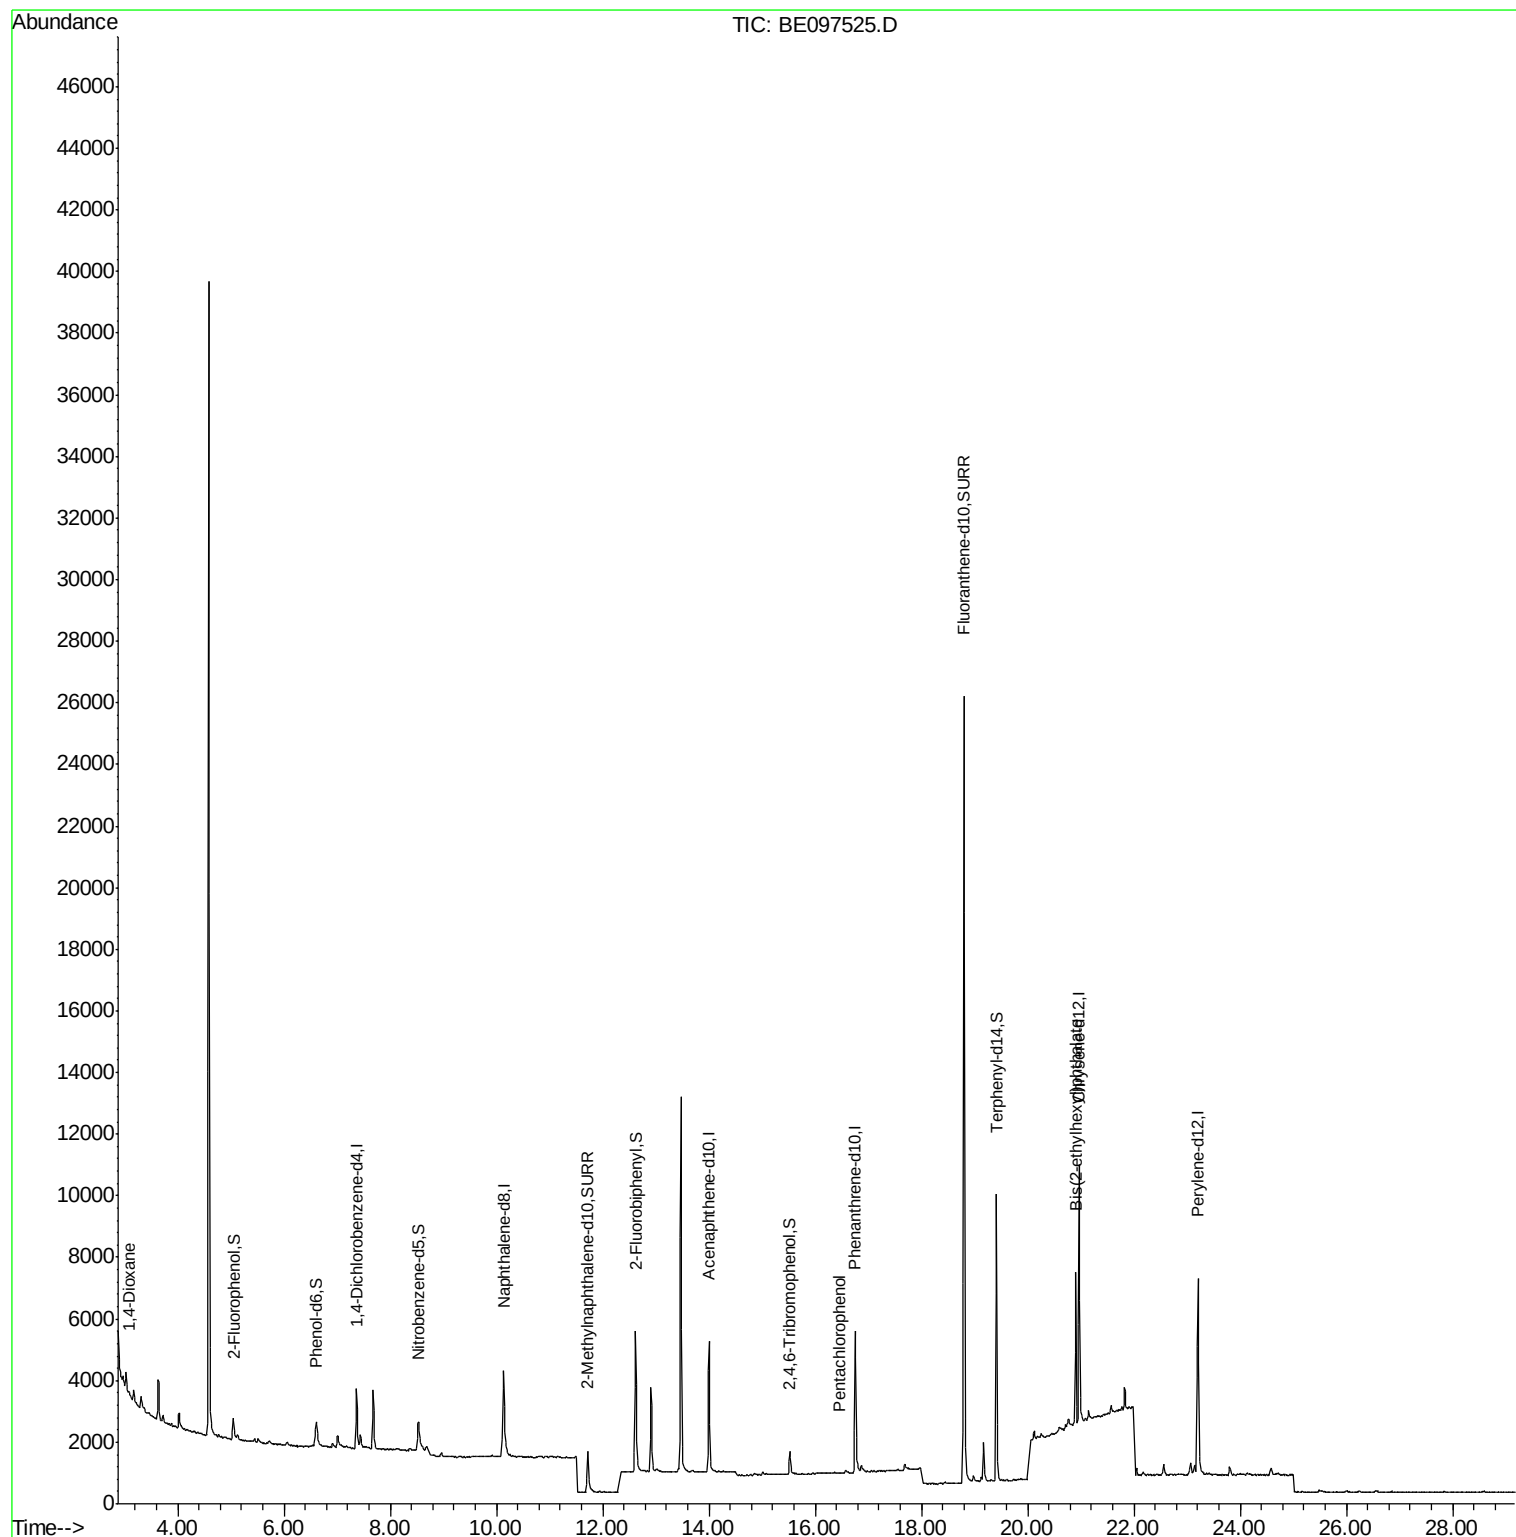

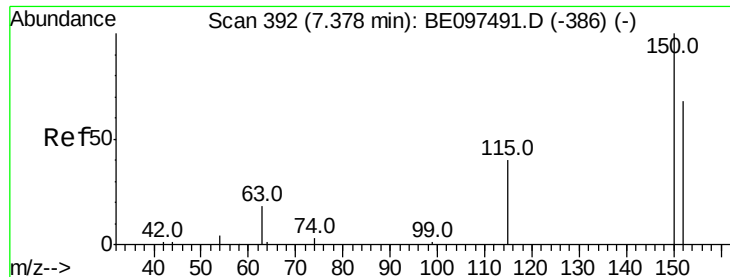


#1




1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.37 min Scan# 391
 Delta R.T. -0.01 min
 Lab File: BE097525.D
 Acq: 18 Sep 2018 10:00

Instrument :
 BNA_E
 ClientSampleId :
 BP-TT-AOC22-MW09-20180911

Tot Ion:152 Resp: 947
 Ion Ratio Lower Upper
 152 100
 150 148.9 117.2 175.8
 115 71.1 57.0 85.6

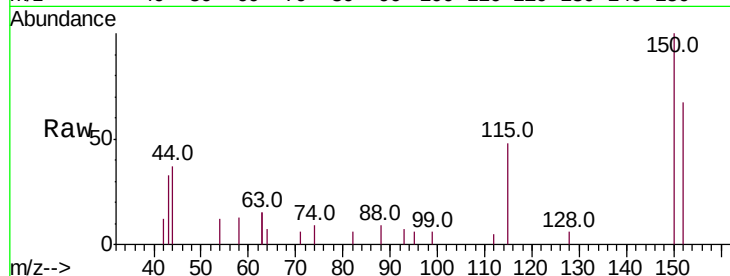


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

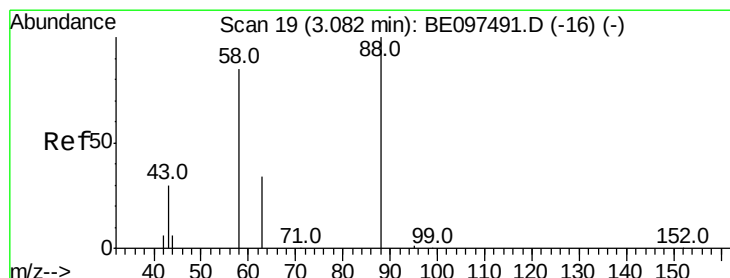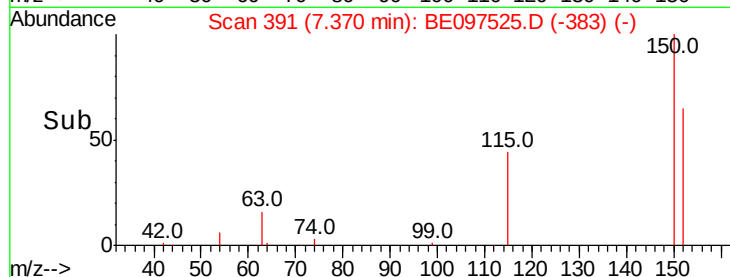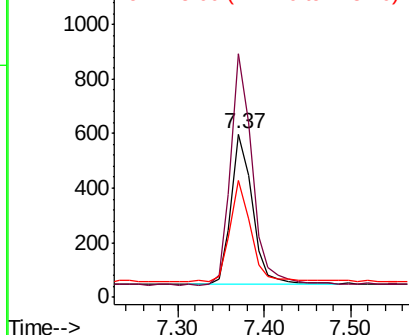



#2


1,4-Dioxane
 Concen: 0.081 ng
 RT: 3.09 min Scan# 19
 Delta R.T. 0.00 min
 Lab File: BE097525.D
 Acq: 18 Sep 2018 10:00

Tgt Ion: 88 Resp: 133
 Ion Ratio Lower Upper
 88 100
 58 0.0 63.2 94.8#
 43 0.0 41.2 61.8#

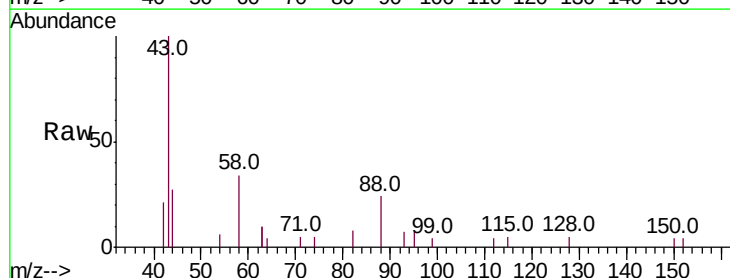

Abundance Ion 88.00 (87.70 to 88.70): BE0
 Ion 58.00 (57.70 to 58.70): BE0
 Ion 43.00 (42.70 to 43.70): BE0

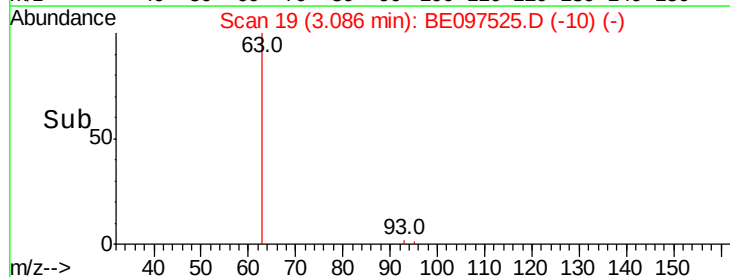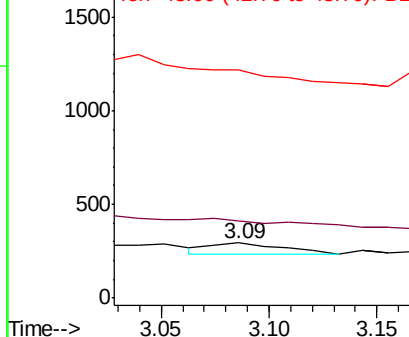



#4

2-Fluorophenol

Concen: 0.164 ng

RT: 5.06 min Scan# 190

Delta R.T. 0.00 min

Lab File: BE097525.D

Acq: 18 Sep 2018 10:00

Instrument :

BNA_E

ClientSampleId :

BP-TT-AOC22-MW09-20180911


Tot Ion: 112 Resp: 527

Ion Ratio Lower Upper

112 100

64 70.2 60.1 90.1




63 136.1 116.8 175.2

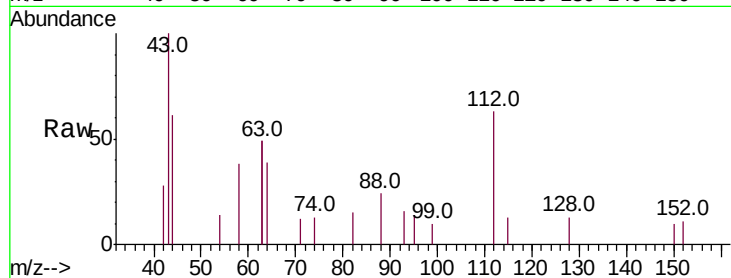

Abundance Ion 112.00 (111.70 to 112.70): BE0

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

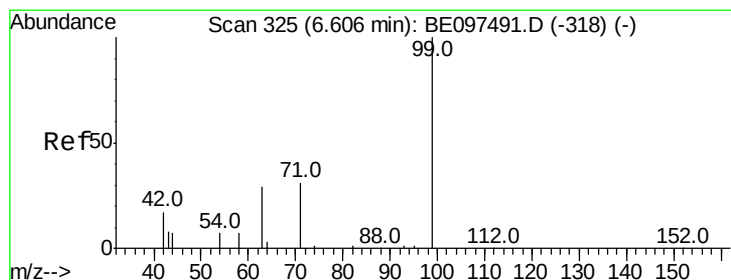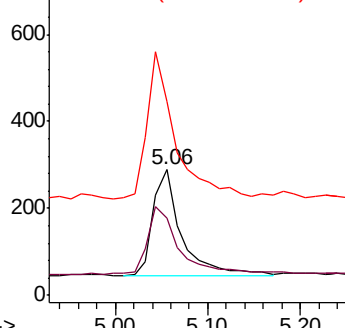

#5

Phenol-d6

Concen: 0.110 ng

RT: 6.60 min Scan# 324

Delta R.T. -0.01 min

Lab File: BE097525.D

Acq: 18 Sep 2018 10:00


Tgt Ion: 99 Resp: 448

Ion Ratio Lower Upper

99 100

42 23.7 20.2 30.2



71 34.8 28.4 42.6

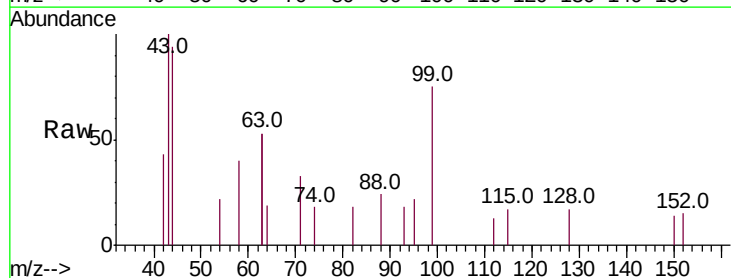


Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

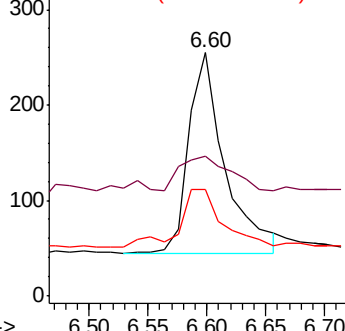



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.13 min Scan# 612

Delta R.T. 0.00 min

Lab File: BE097525.D

Acq: 18 Sep 2018 10:00

Instrument :

BNA_E

ClientSampleId :

BP-TT-AOC22-MW09-20180911

Tot Ion:136 Resp: 4339


Ion Ratio Lower Upper

136 100

137 12.9 9.5 14.3

54 40.1 29.1 43.7

68 8.8 6.2 9.2



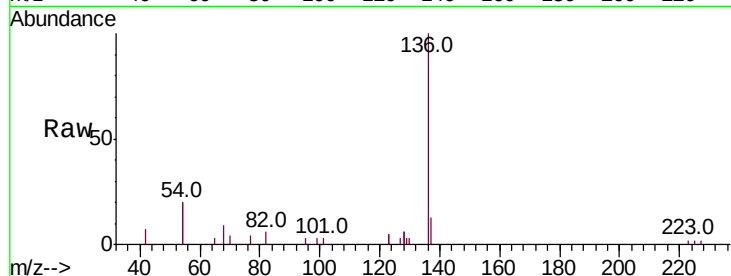


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

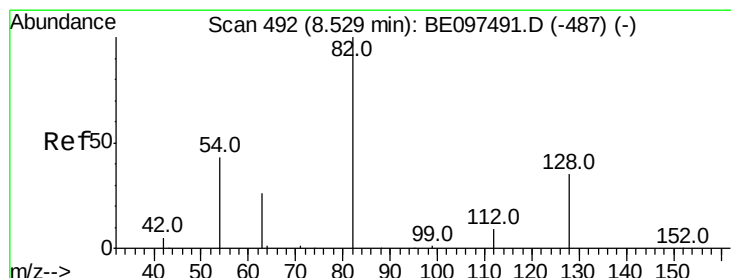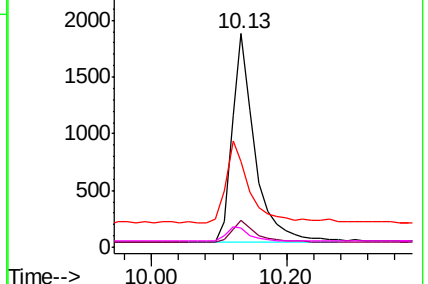

#8

Nitrobenzene-d5

Concen: 0.430 ng

RT: 8.53 min Scan# 492

Delta R.T. 0.00 min

Lab File: BE097525.D

Acq: 18 Sep 2018 10:00


Tgt Ion: 82 Resp: 1502

Ion Ratio Lower Upper

82 100

128 39.9 24.0 36.0#



54 52.0 40.0 60.0

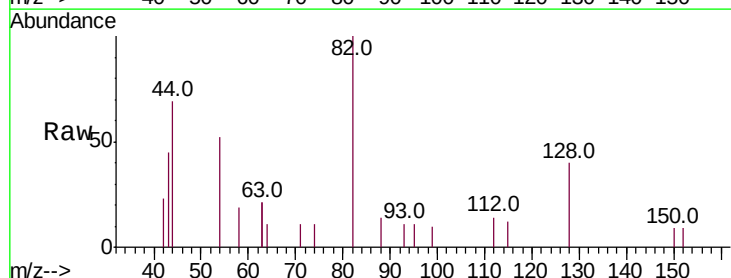


Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0

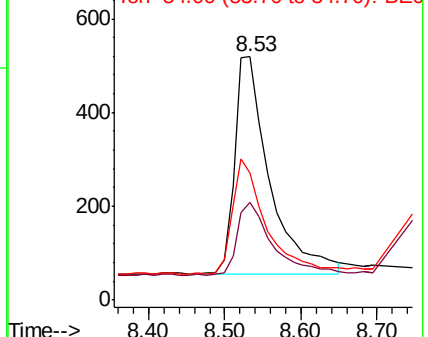

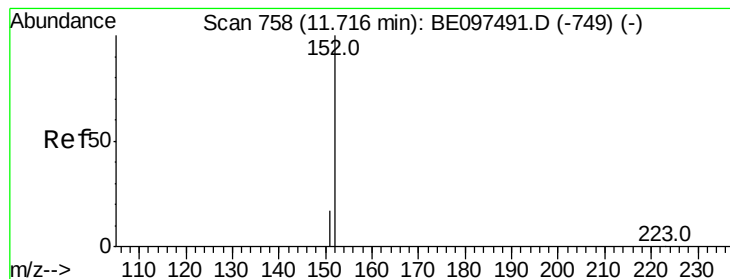

#11

2-Methylnaphthalene-d10

Concen: 0.421 ng

RT: 11.72 min Scan# 759

Delta R.T. 0.00 min

Lab File: BE097525.D

Acq: 18 Sep 2018 10:00

Instrument :

BNA_E

ClientSampleId :


BP-TT-AOC22-MW09-20180911

Tot Ion:152 Resp: 2610

Ion Ratio Lower Upper

152 100

151 18.8 15.4 23.0

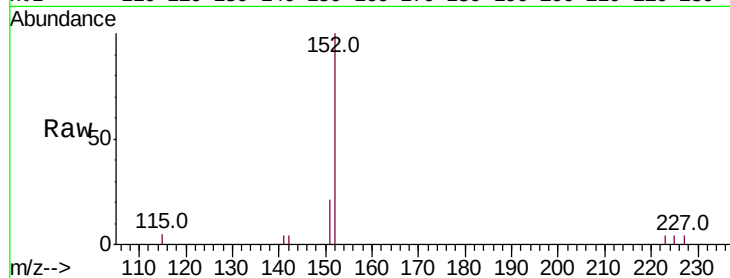

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E



11.72

1000

500

0

Time--> 11.60 11.70 11.80 11.90

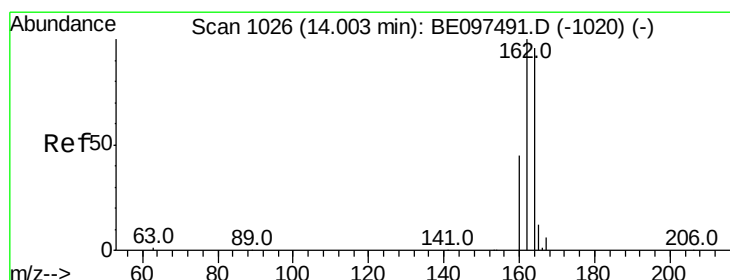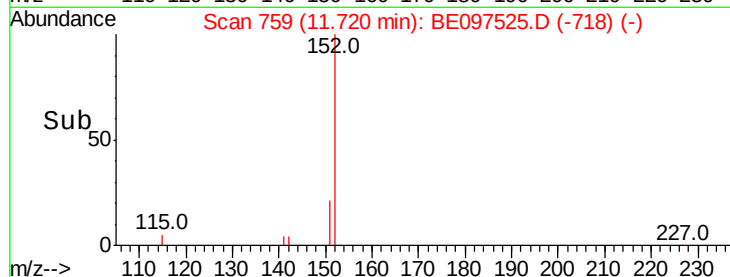

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.00 min Scan# 1026

Delta R.T. -0.00 min

Lab File: BE097525.D

Acq: 18 Sep 2018 10:00


Tgt Ion:164 Resp: 2612

Ion Ratio Lower Upper

164 100

162 104.0 83.1 124.7

160 49.7 37.1 55.7

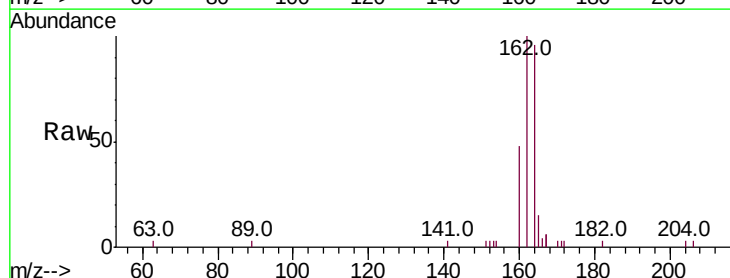

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

14.00

2000


1500


1000

500

0

Time--> 13.90 14.00 14.10 14.20

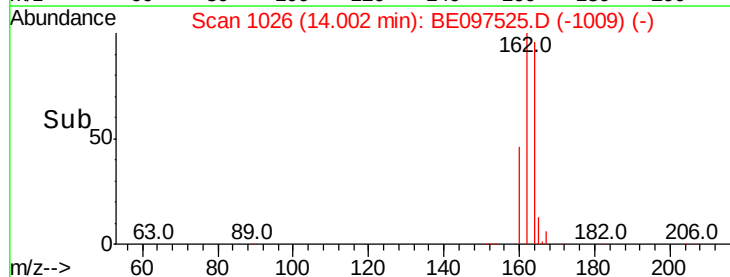



#14

2,4,6-Tribromophenol

Concen: 0.389 ng

RT: 15.52 min Scan# 1153

Delta R.T. -0.01 min

Lab File: BE097525.D

Acq: 18 Sep 2018 10:00

Instrument :

BNA_E

ClientSampleId :

BP-TT-AOC22-MW09-20180911


Tot Ion:330 Resp: 536

Ion Ratio Lower Upper

330 100

332 96.1 152.7 229.1#




141 35.3 33.7 50.5

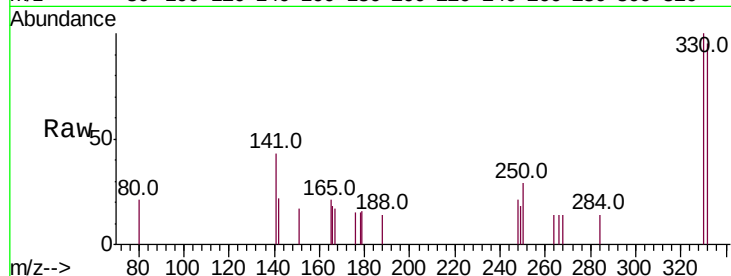

Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

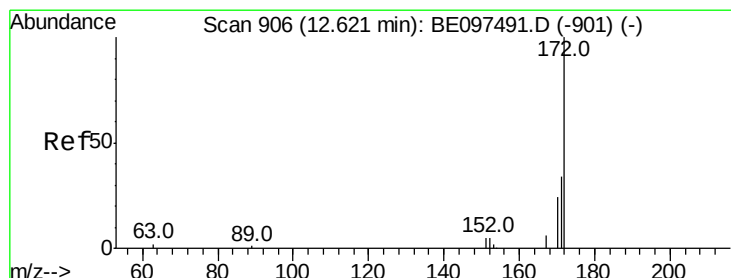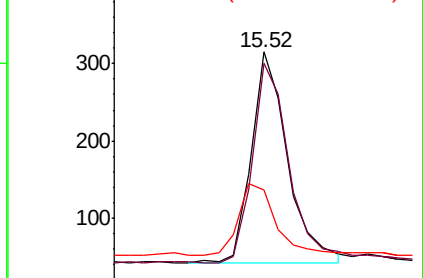

#15

2-Fluorobiphenyl

Concen: 0.550 ng

RT: 12.62 min Scan# 906

Delta R.T. -0.00 min

Lab File: BE097525.D

Acq: 18 Sep 2018 10:00


Tgt Ion:172 Resp: 5013

Ion Ratio Lower Upper

172 100

171 35.3 29.9 44.9



170 24.6 21.8 32.8

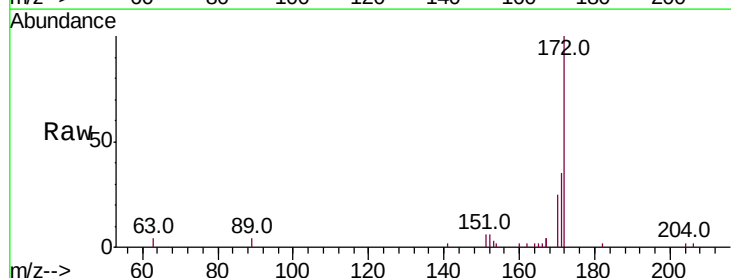


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

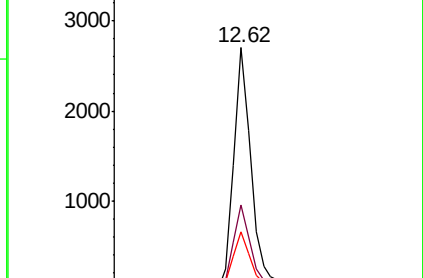

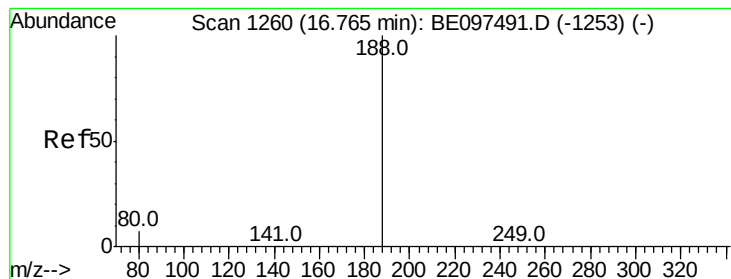

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.75 min Scan# 1259

Delta R.T. -0.01 min

Lab File: BE097525.D

Acq: 18 Sep 2018 10:00

Instrument :

BNA_E

ClientSampleId :

BP-TT-AOC22-MW09-20180911


Tot Ion:188 Resp: 7236

Ion Ratio Lower Upper

188 100

94 0.0 3.9 5.9#




80 14.1 3.6 5.4#

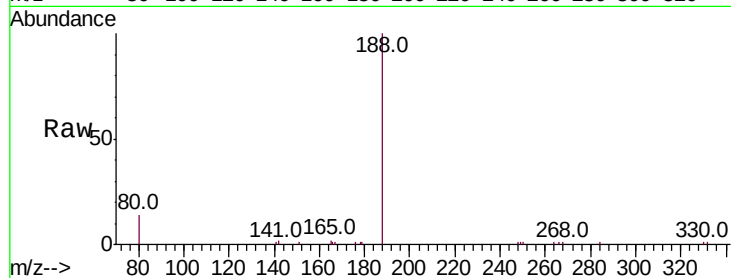

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

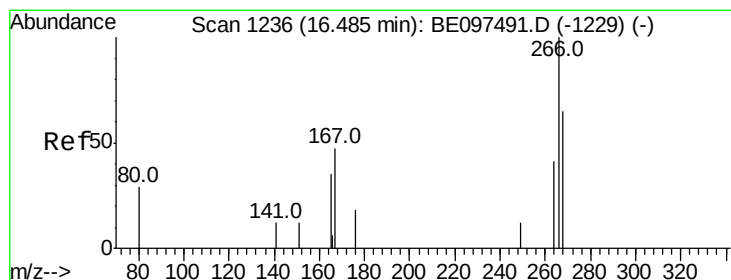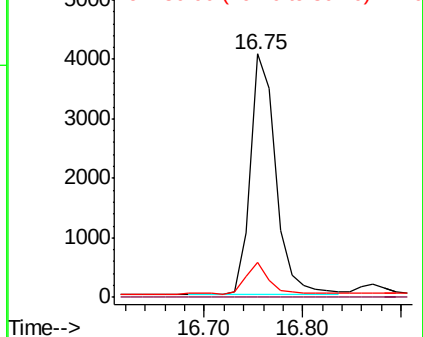

#22

Pentachlorophenol

Concen: 0.091 ng

RT: 16.45 min Scan# 1233

Delta R.T. -0.03 min

Lab File: BE097525.D

Acq: 18 Sep 2018 10:00


Tgt Ion:266 Resp: 23

Ion Ratio Lower Upper

266 100

264 95.8 72.5 108.7



268 95.8 73.8 110.6

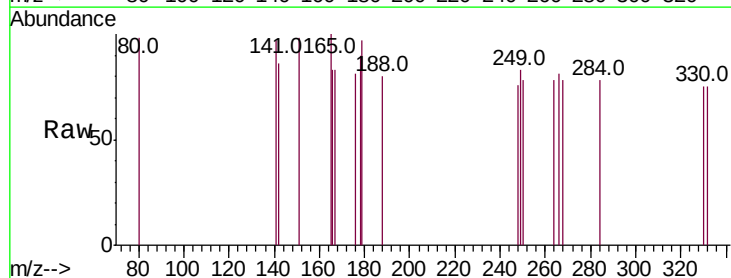


Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

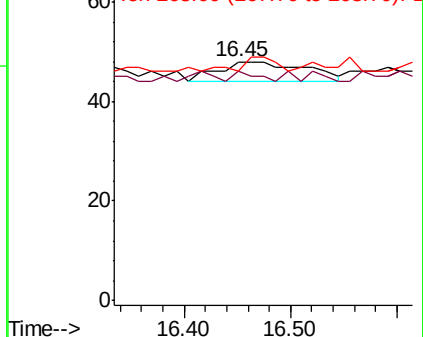

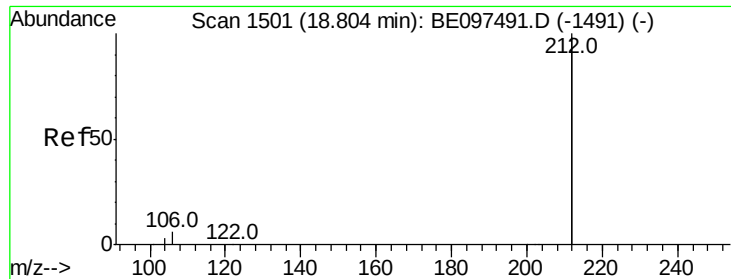

#25

Fluoranthene-d10

Concen: 0.430 ng

RT: 18.80 min Scan# 1500

Delta R.T. -0.00 min

Lab File: BE097525.D

Acq: 18 Sep 2018 10:00

Instrument :

BNA_E

ClientSampleId :

BP-TT-AOC22-MW09-20180911


Tot Ion:212 Resp: 37372

Ion Ratio Lower Upper

212 100

106 3.1 2.8 4.2




104 1.9 1.6 2.4

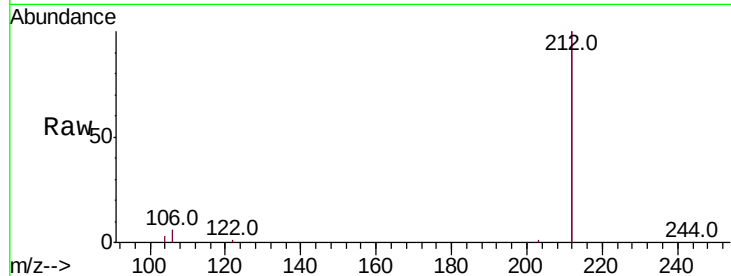

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

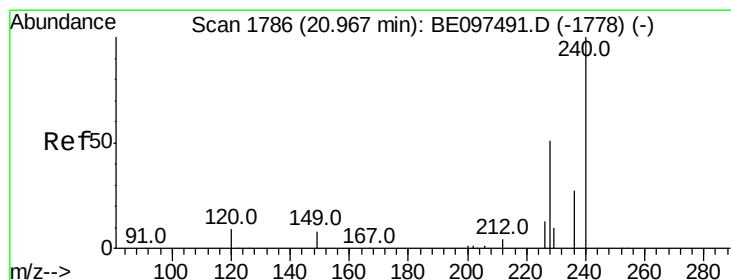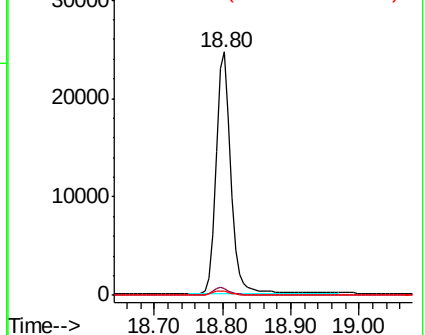

#27

Chrysene-d12

Concen: 0.400 ng

RT: 20.97 min Scan# 1785

Delta R.T. 0.00 min

Lab File: BE097525.D

Acq: 18 Sep 2018 10:00


Tgt Ion:240 Resp: 8844

Ion Ratio Lower Upper

240 100

120 9.0 5.5 8.3#



236 27.6 20.7 31.1

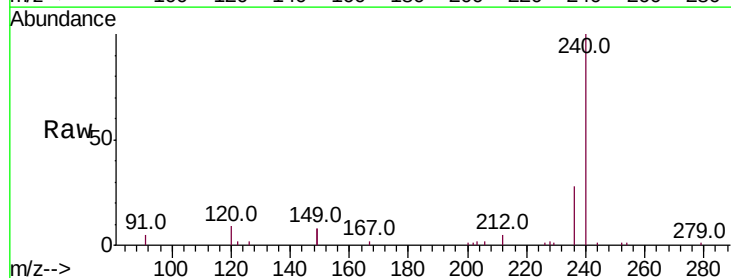


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

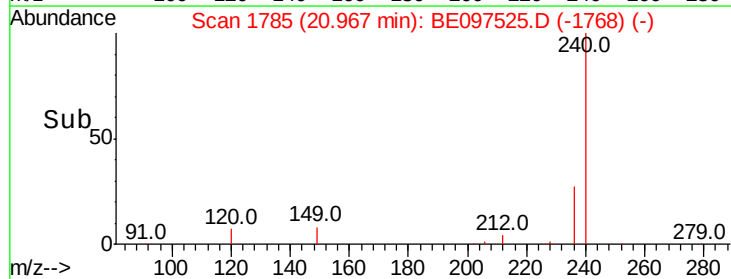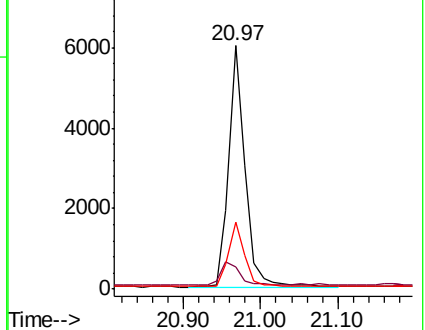

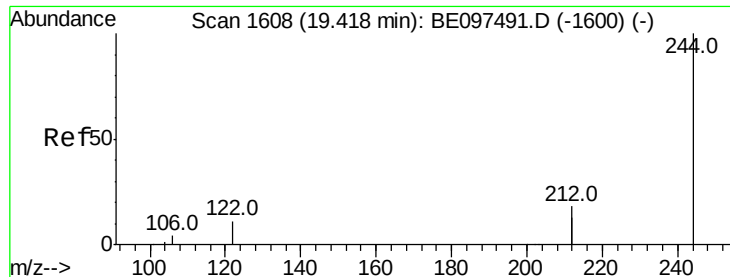

#29

Terphenyl-d14

Concen: 0.494 ng

RT: 19.41 min Scan# 1606

Delta R.T. -0.01 min

Lab File: BE097525.D

Acq: 18 Sep 2018 10:00

Instrument :

BNA_E

ClientSampleId :

BP-TT-AOC22-MW09-20180911





Tot Ion:244 Resp: 8362

Ion Ratio Lower Upper

244 100

212 33.8 25.4 38.0

122 12.5 8.1 12.1#

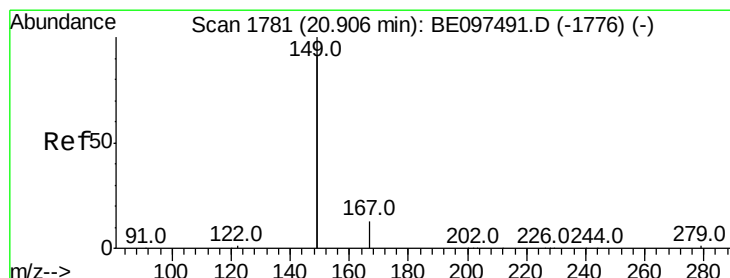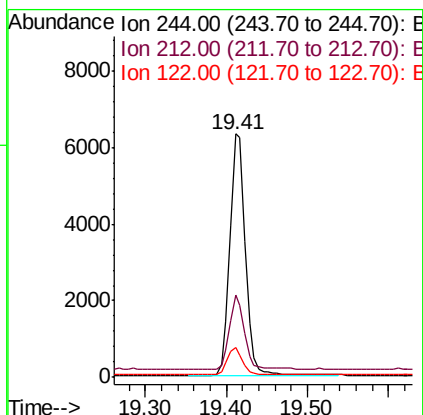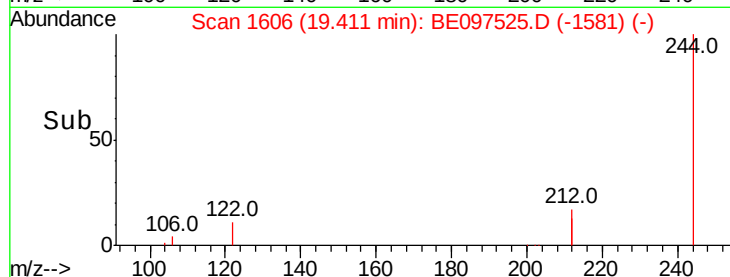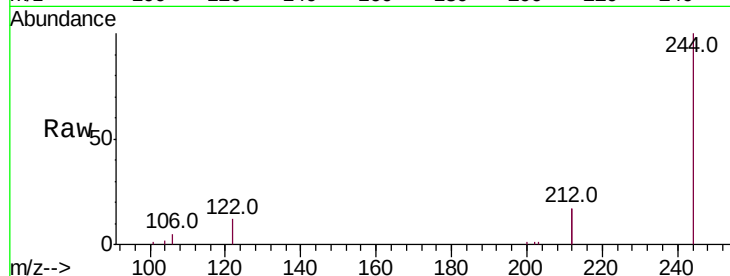

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.113 ng

RT: 20.91 min Scan# 1780

Delta R.T. 0.00 min

Lab File: BE097525.D

Acq: 18 Sep 2018 10:00




Tgt Ion:149 Resp: 5574




Ion Ratio Lower Upper

149 100

167 6.6 5.4 8.0

279 1.1 0.7 1.1

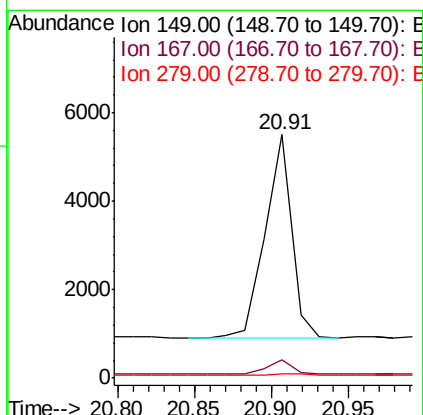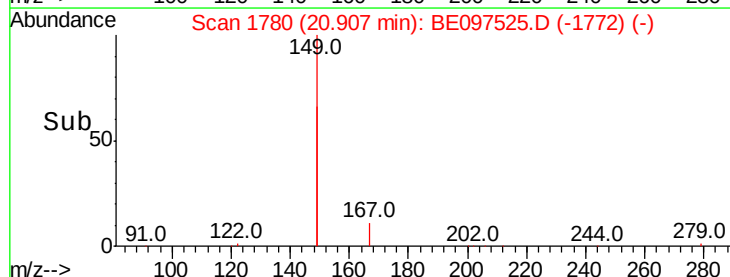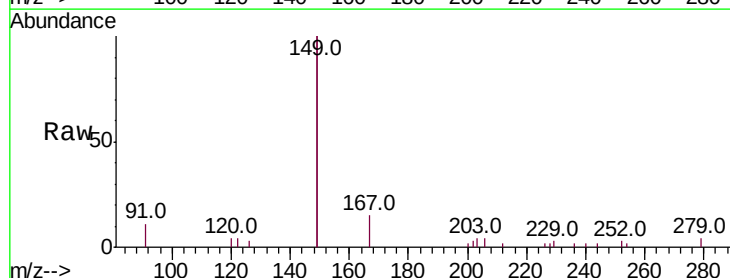

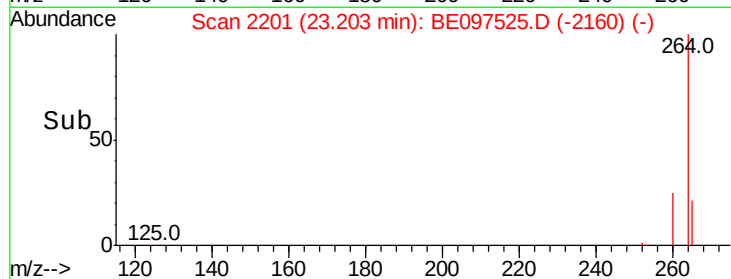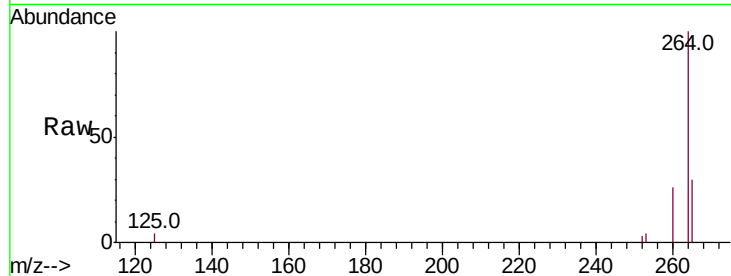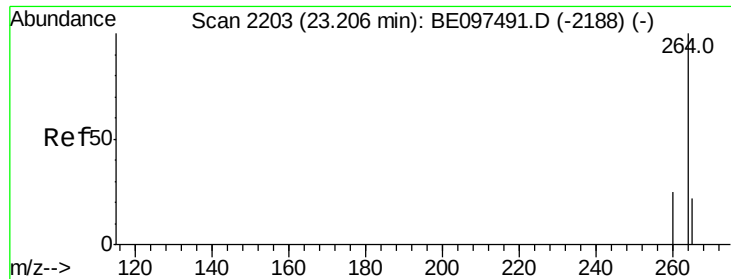

#34
 Pervlene-d12
 Concen: 0.400 ng
 RT: 23.20 min Scan# 2201
 Delta R.T. -0.00 min
 Lab File: BE097525.D
 Acq: 18 Sep 2018 10:00

Instrument :
 BNA_E
 ClientSampleId :
 BP-TT-AOC22-MW09-20180911

Tot Ion:	264	Resp:	8901
Ion	Ratio	Lower	Upper
264	100		
260	25.8	20.5	30.7
265	30.0	22.8	34.2

