

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE091718\
 Data File : BE097529.D
 Acq On : 18 Sep 2018 12:29
 Operator : SJ/JU
 Sample : J4913-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BP-DUP01-20180912

Quant Time: Sep 18 13:12:55 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE091718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 17 18:57:11 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	991	0.40	ng	0.00
7) Naphthalene-d8	10.13	136	4609	0.40	ng	0.00
13) Acenaphthene-d10	14.00	164	2729	0.40	ng	0.00
19) Phenanthrene-d10	16.75	188	7416	0.40	ng	-0.01
27) Chrysene-d12	20.97	240	8615	0.40	ng	0.00
34) Perylene-d12	23.21	264	8702	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.05	112	519	0.15	ng	0.00
5) Phenol-d6	6.62	99	296	0.07	ng	0.01
8) Nitrobenzene-d5	8.54	82	1392	0.38	ng	0.01
11) 2-Methylnaphthalene-d10	11.72	152	2631	0.40	ng	0.00
14) 2,4,6-Tribromophenol	15.53	330	538	0.37	ng	0.00
15) 2-Fluorobiphenyl	12.62	172	4860	0.51	ng	0.00
25) Fluoranthene-d10	18.80	212	35611	0.40	ng	0.00
29) Terphenyl-d14	19.41	244	7955	0.48	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.08	88	870	0.508	ng	94
22) Pentachlorophenol	16.45	266	14	0.070	ng	96
32) Bis(2-ethylhexyl)phthalate	20.91	149	1954	0.041	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE091718\
Data File : BE097529.D
Acq On : 18 Sep 2018 12:29
Operator : SJ/JU
Sample : J4913-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-DUP01-20180912

Quant Time: Sep 18 13:12:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE091718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 17 18:57:11 2018
Response via : Initial Calibration

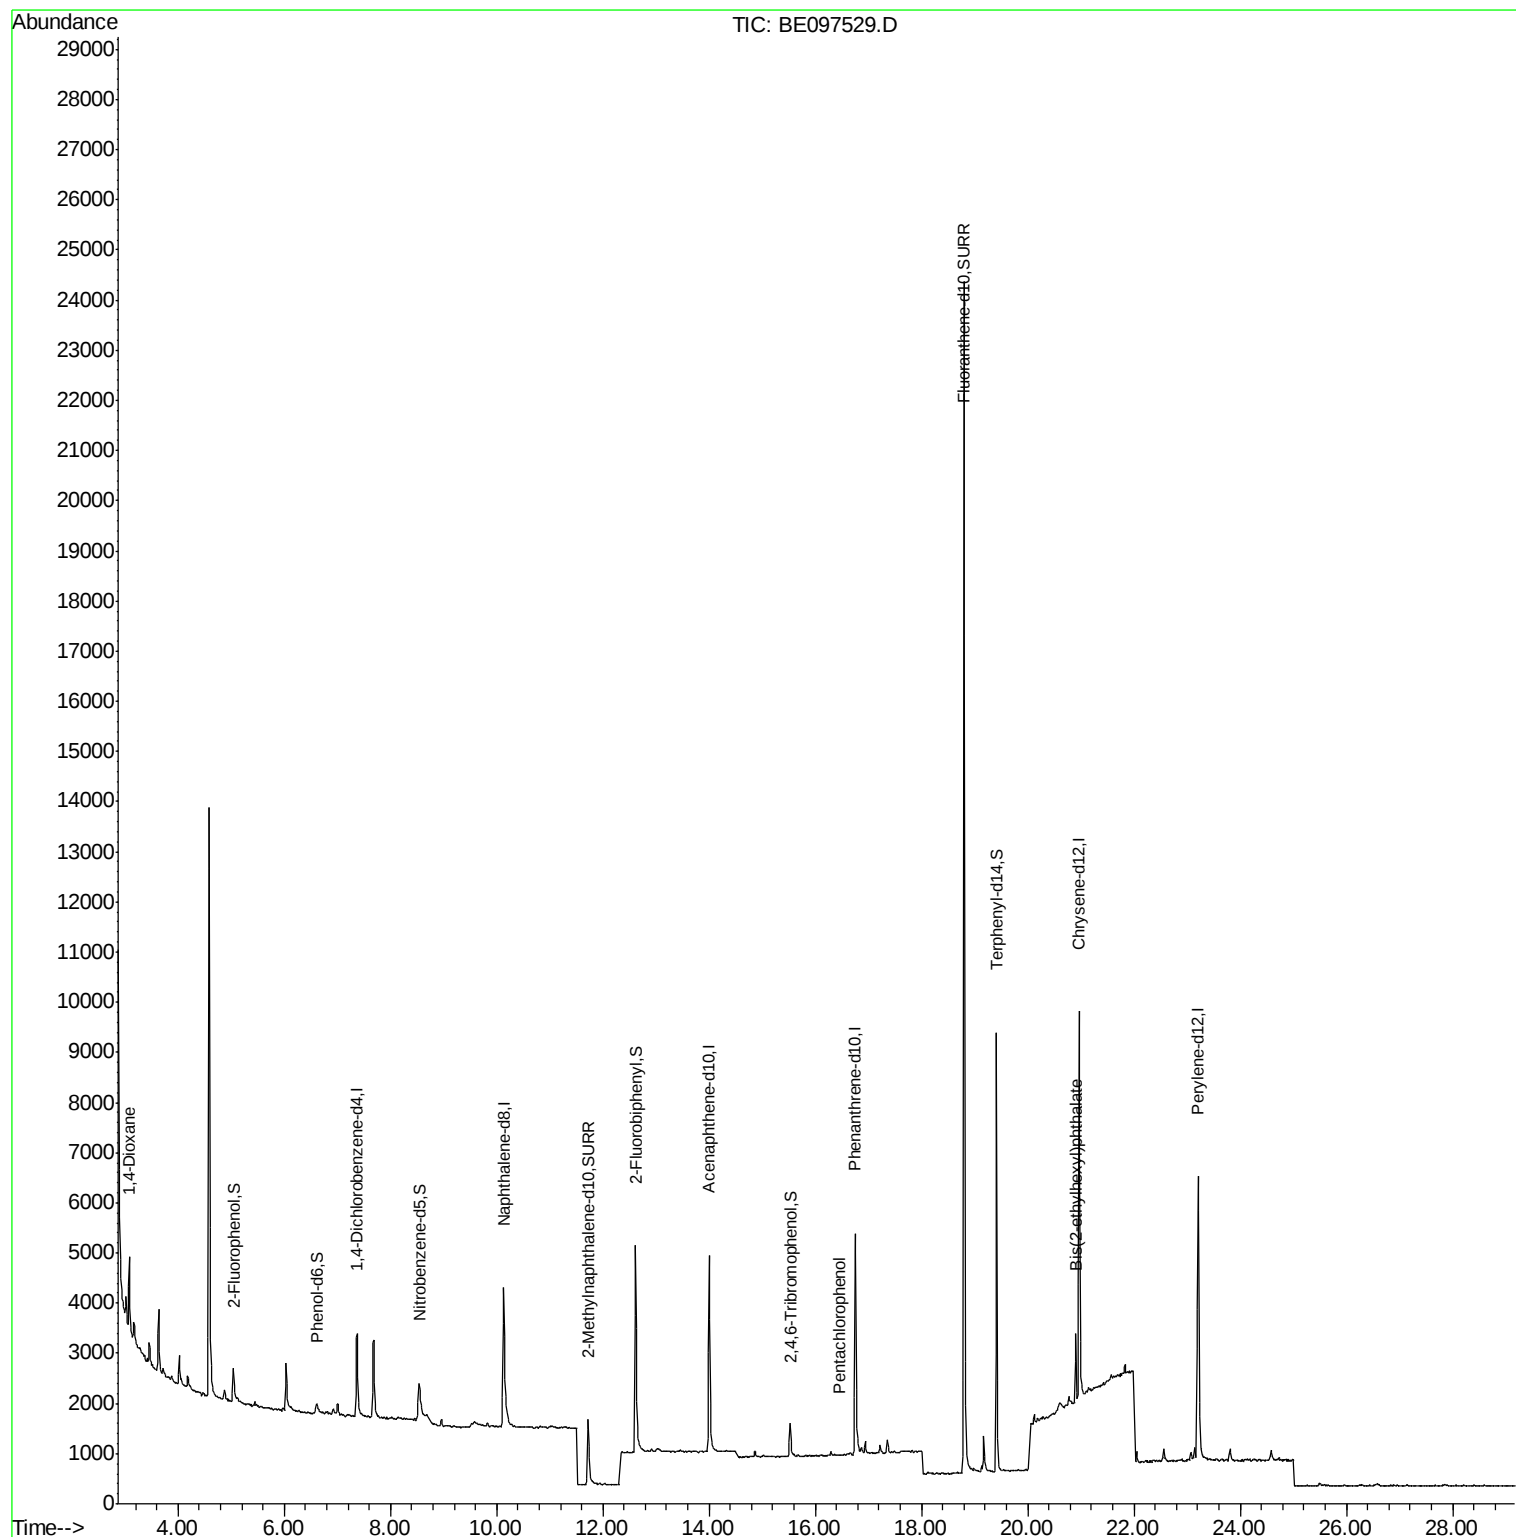



#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.38 min Scan# 392

Delta R.T. -0.00 min

Lab File: BE097529.D

Acq: 18 Sep 2018 12:29

Instrument :

BNA_E

ClientSampleId :

BP-DUP01-20180912


Tot Ion:152 Resp: 991

Ion Ratio Lower Upper

152 100

150 156.0 117.2 175.8




115 70.1 57.0 85.6

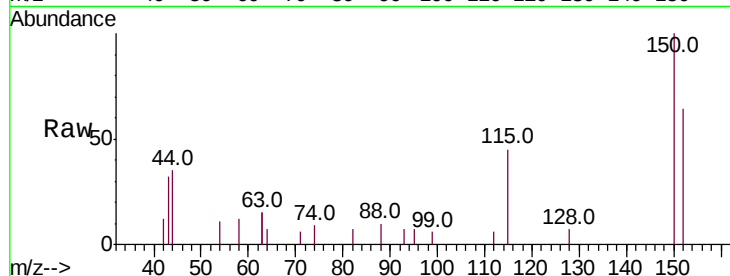

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

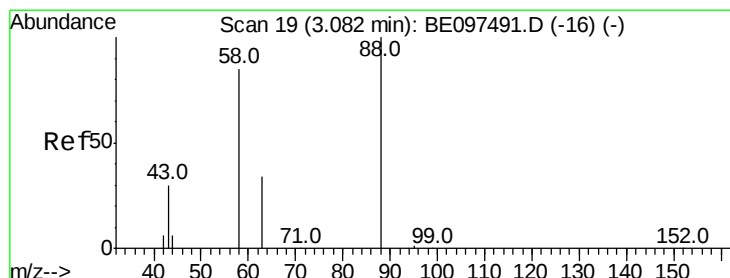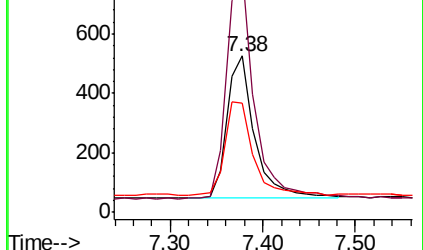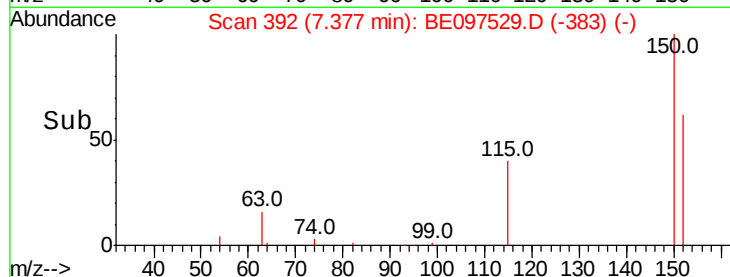

#2

1,4-Dioxane

Concen: 0.508 ng

RT: 3.08 min Scan# 19

Delta R.T. -0.00 min

Lab File: BE097529.D

Acq: 18 Sep 2018 12:29


Tgt Ion: 88 Resp: 870

Ion Ratio Lower Upper

88 100

58 83.6 63.2 94.8



43 57.1 41.2 61.8

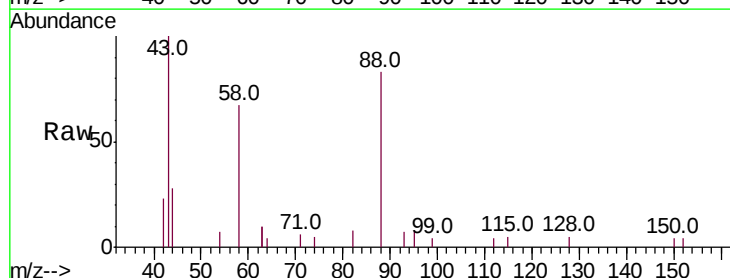


Abundance Ion 88.00 (87.70 to 88.70): BE0

Ion 58.00 (57.70 to 58.70): BE0

Ion 43.00 (42.70 to 43.70): BE0

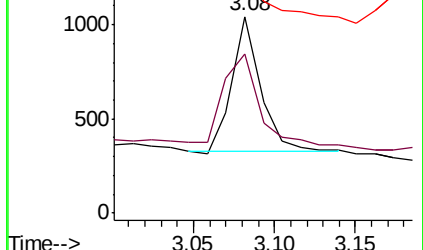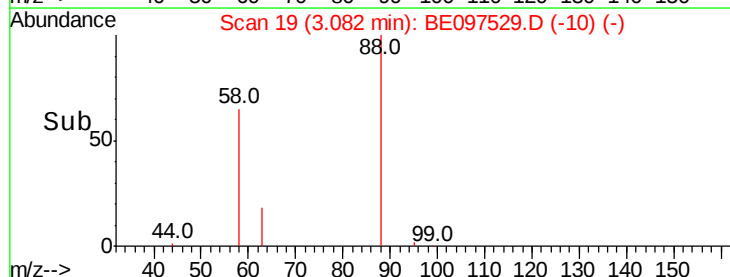

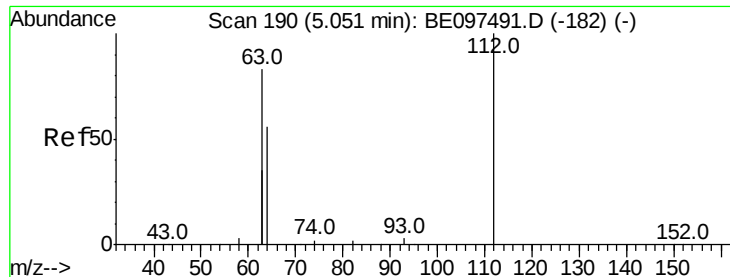

#4

2-Fluorophenol

Concen: 0.155 ng

RT: 5.05 min Scan# 190

Delta R.T. -0.00 min

Lab File: BE097529.D

Acq: 18 Sep 2018 12:29

Instrument :

BNA_E

ClientSampleId :

BP-DUP01-20180912


Tot Ion: 112 Resp: 519

Ion Ratio Lower Upper

112 100

64 69.2 60.1 90.1




63 140.7 116.8 175.2

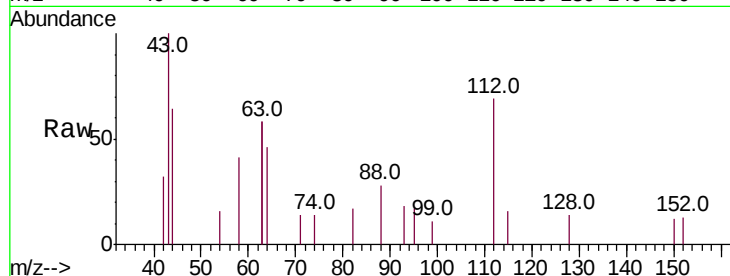

Abundance Ion 112.00 (111.70 to 112.70): BE0

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

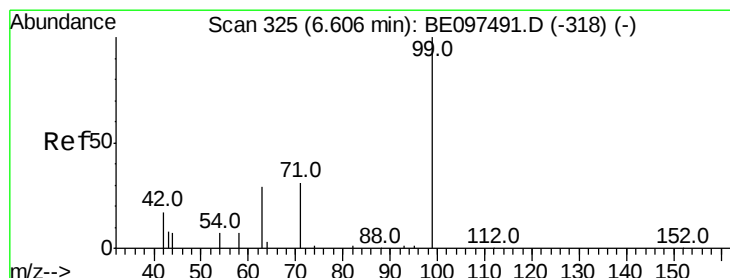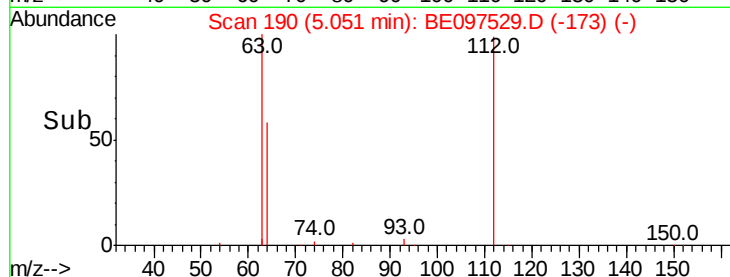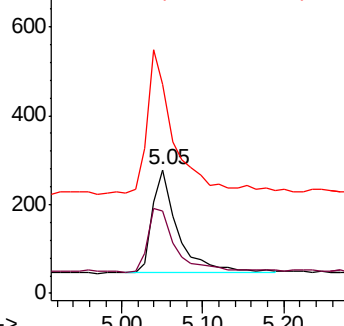

#5

Phenol-d6

Concen: 0.069 ng

RT: 6.62 min Scan# 326

Delta R.T. 0.01 min

Lab File: BE097529.D

Acq: 18 Sep 2018 12:29


Tgt Ion: 99 Resp: 296

Ion Ratio Lower Upper

99 100

42 25.7 20.2 30.2



71 29.4 28.4 42.6

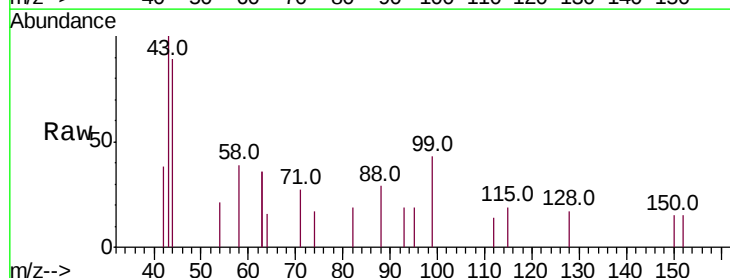


Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

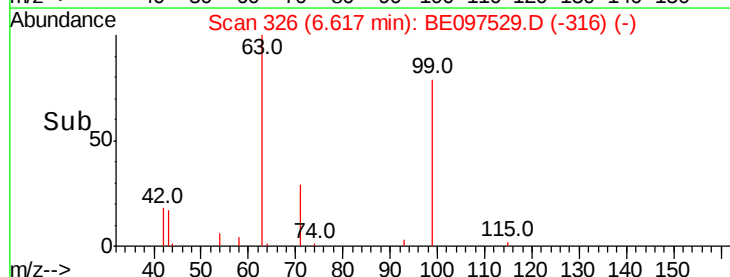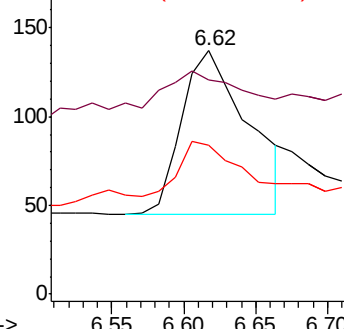

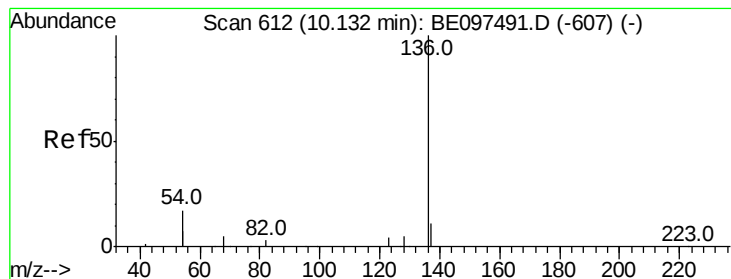

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.13 min Scan# 613

Delta R.T. 0.00 min

Lab File: BE097529.D

Acq: 18 Sep 2018 12:29

Instrument :

BNA_E

ClientSampleId :

BP-DUP01-20180912

Tot Ion:136 Resp: 4609



Ion Ratio Lower Upper

136 100

137 13.2 9.5 14.3

54 42.0 29.1 43.7

68 8.9 6.2 9.2


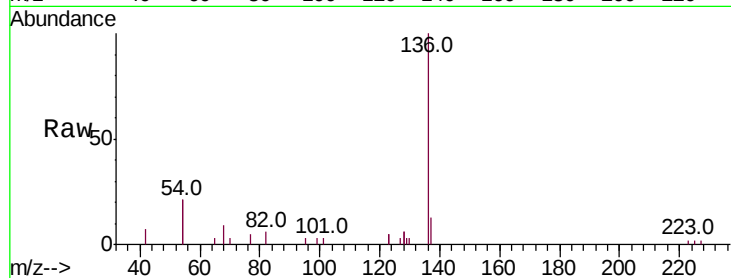


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

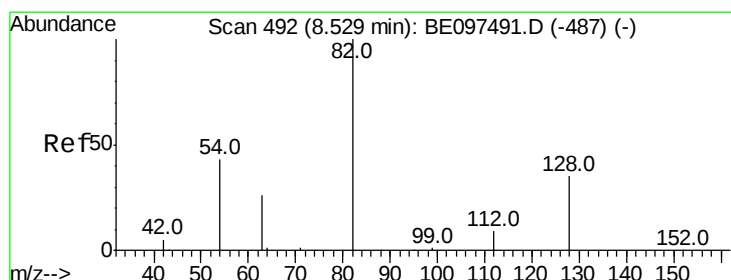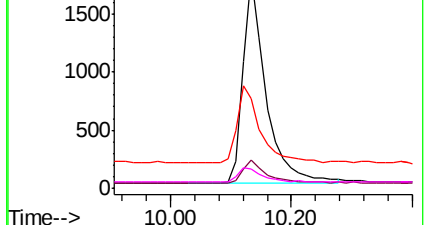

#8

Nitrobenzene-d5

Concen: 0.375 ng

RT: 8.54 min Scan# 493

Delta R.T. 0.01 min

Lab File: BE097529.D

Acq: 18 Sep 2018 12:29



Tgt Ion: 82 Resp: 1392

Ion Ratio Lower Upper

82 100

128 41.8 24.0 36.0#


54 51.7 40.0 60.0

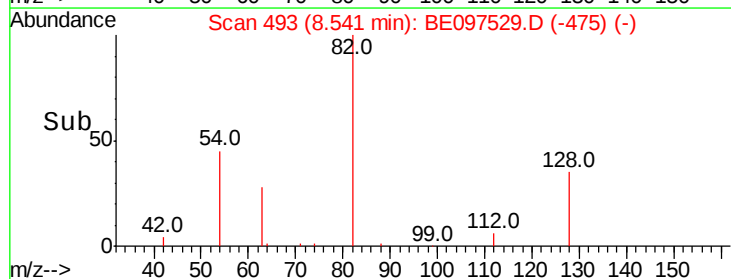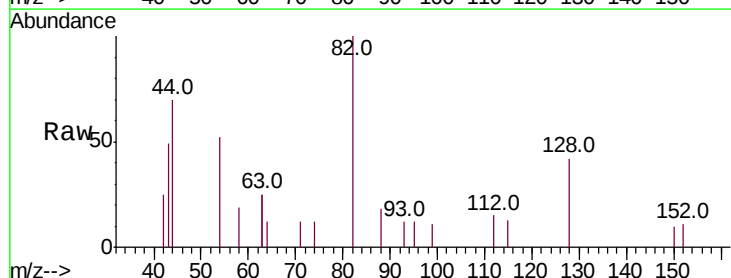


Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0

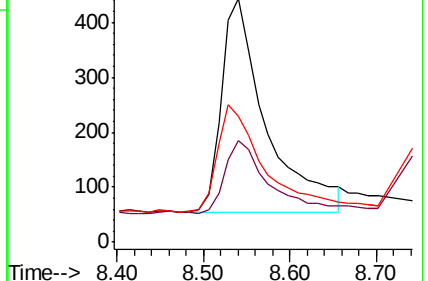

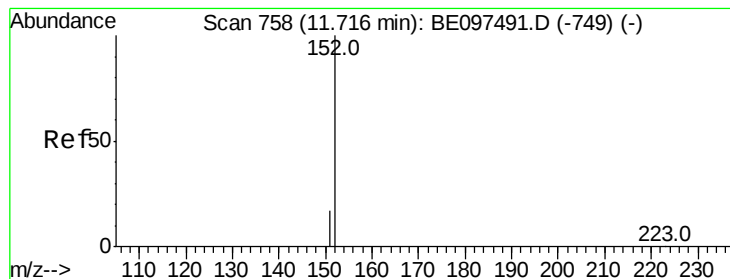

#11

2-Methylnaphthalene-d10

Concen: 0.399 ng

RT: 11.72 min Scan# 760

Delta R.T. 0.00 min

Lab File: BE097529.D

Acq: 18 Sep 2018 12:29

Instrument :

BNA_E

ClientSampleId :


BP-DUP01-20180912

Tot Ion:152 Resp: 2631

Ion Ratio Lower Upper

152 100

151 18.6 15.4 23.0

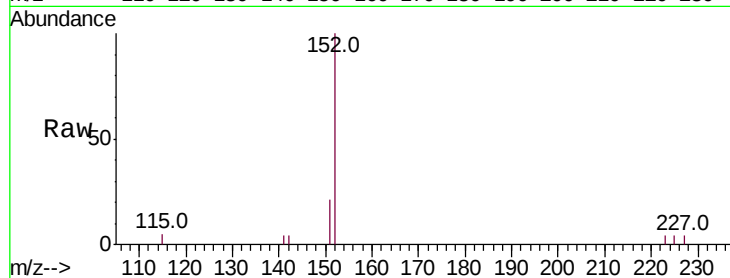

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E



11.72

1000

500

0

Time--> 11.60 11.70 11.80 11.90

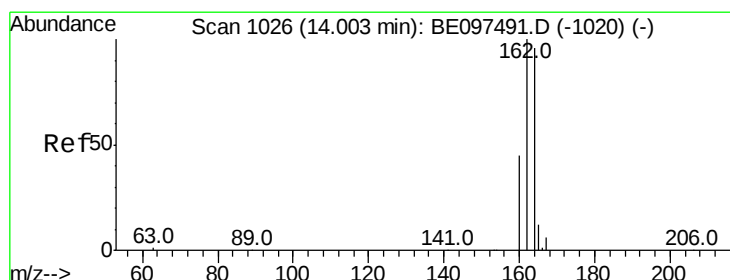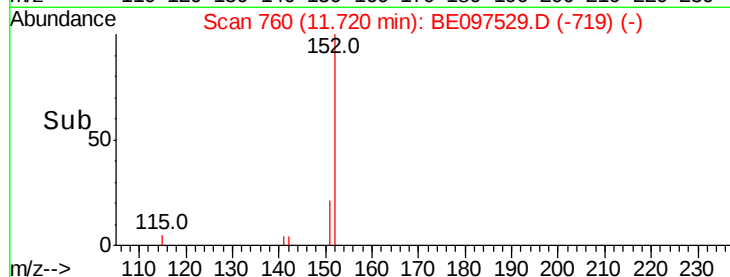

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.00 min Scan# 1028

Delta R.T. 0.00 min

Lab File: BE097529.D

Acq: 18 Sep 2018 12:29


Tgt Ion:164 Resp: 2729

Ion Ratio Lower Upper

164 100

162 102.8 83.1 124.7

160 50.4 37.1 55.7

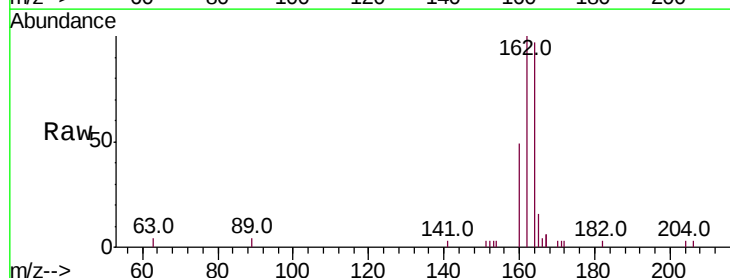

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

14.00

2000


1500


1000

500

0

Time--> 13.90 14.00 14.10 14.20

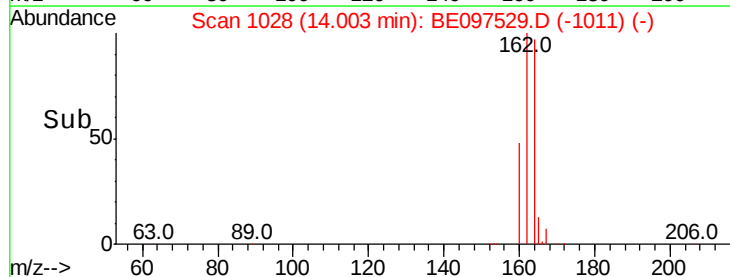




#14
 2,4,6-Tribromophenol
 Concen: 0.373 ng
 RT: 15.53 min Scan# 1156
 Delta R.T. 0.00 min
 Lab File: BE097529.D
 Acq: 18 Sep 2018 12:29




Instrument :
 BNA_E
 ClientSampleId :
 BP-DUP01-20180912

Tot Ion:330 Resp: 538
 Ion Ratio Lower Upper
 330 100
 332 96.1 152.7 229.1#
 141 36.1 33.7 50.5

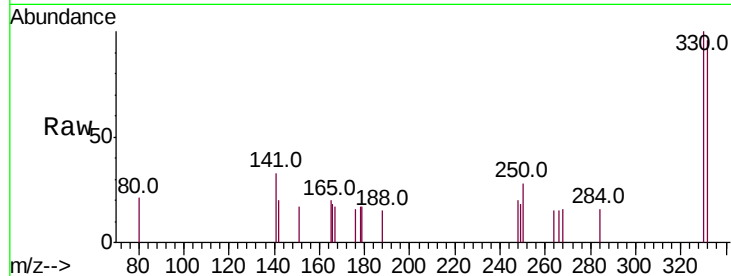


Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

15.53

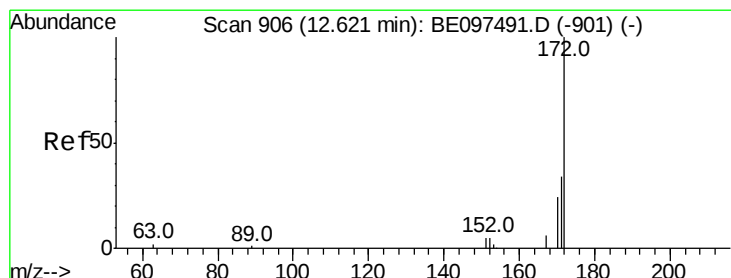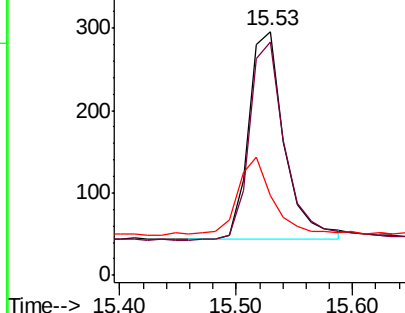



#15
 2-Fluorobiphenyl
 Concen: 0.510 ng
 RT: 12.62 min Scan# 908
 Delta R.T. 0.00 min
 Lab File: BE097529.D
 Acq: 18 Sep 2018 12:29


Tgt Ion:172 Resp: 4860
 Ion Ratio Lower Upper
 172 100
 171 35.5 29.9 44.9
 170 25.6 21.8 32.8

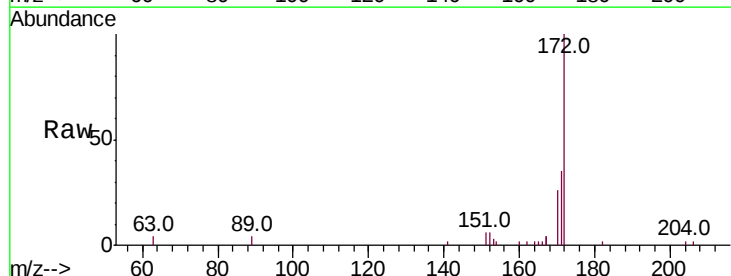

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

12.62

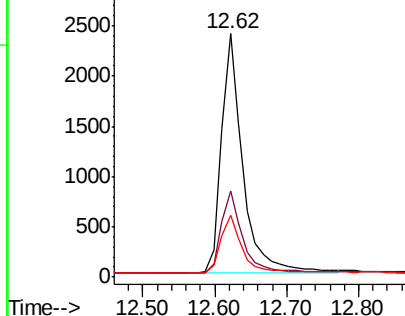



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.75 min Scan# 1261

Delta R.T. -0.01 min

Lab File: BE097529.D

Acq: 18 Sep 2018 12:29

Instrument :

BNA_E

ClientSampleId :

BP-DUP01-20180912



Tot Ion:188 Resp: 7416

Ion Ratio Lower Upper

188 100

94 0.0 3.9 5.9#



80 14.7 3.6 5.4#

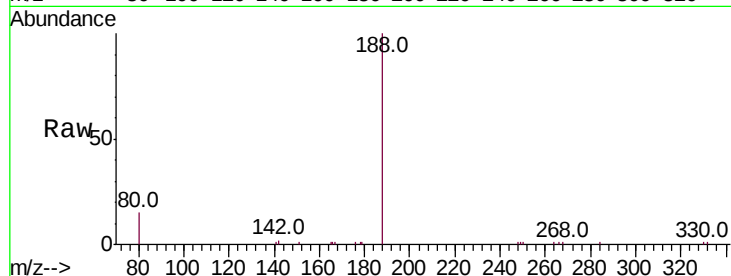

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

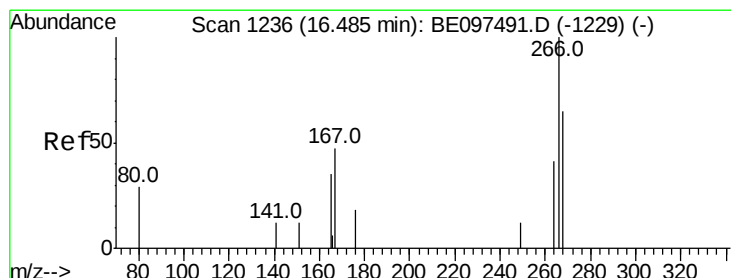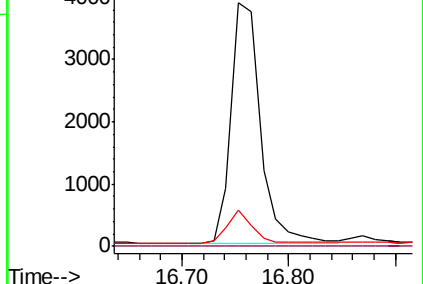

#22

Pentachlorophenol

Concen: 0.070 ng

RT: 16.45 min Scan# 1235

Delta R.T. -0.03 min

Lab File: BE097529.D

Acq: 18 Sep 2018 12:29



Tgt Ion:266 Resp: 14

Ion Ratio Lower Upper

266 100

264 93.9 72.5 108.7


268 95.9 73.8 110.6

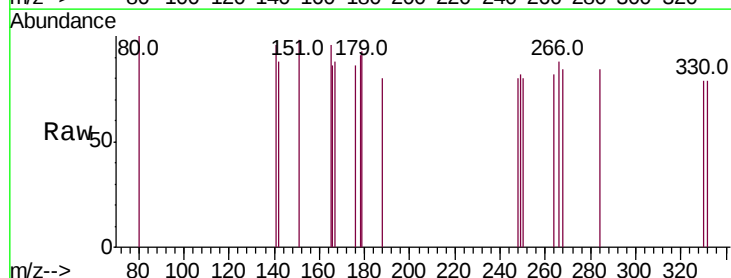


Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

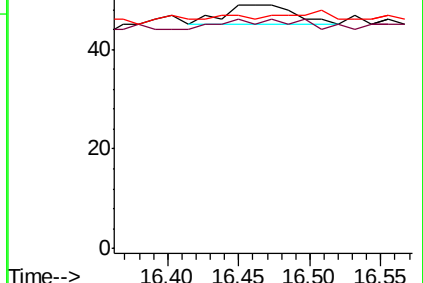

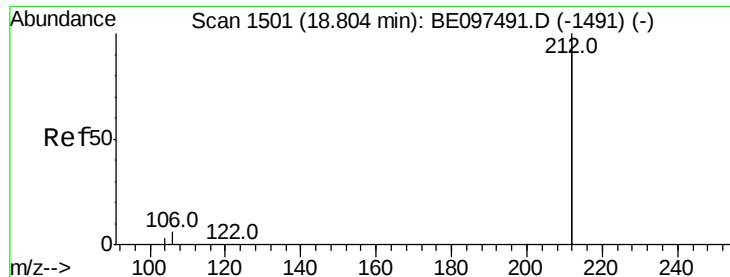

#25

Fluoranthene-d10

Concen: 0.400 ng

RT: 18.80 min Scan# 1503

Delta R.T. -0.00 min

Lab File: BE097529.D

Acq: 18 Sep 2018 12:29

Instrument :

BNA_E

ClientSampleId :

BP-DUP01-20180912


Tot Ion:212 Resp: 35611

Ion Ratio Lower Upper

212 100

106 3.1 2.8 4.2




104 1.7 1.6 2.4

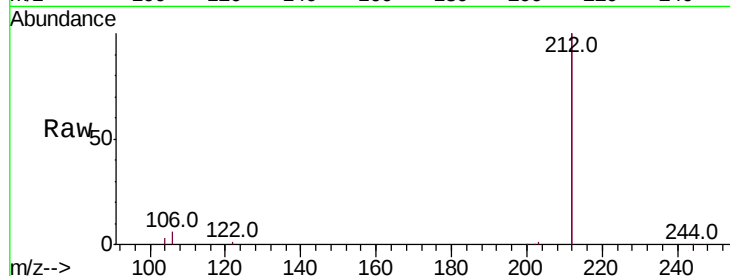

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

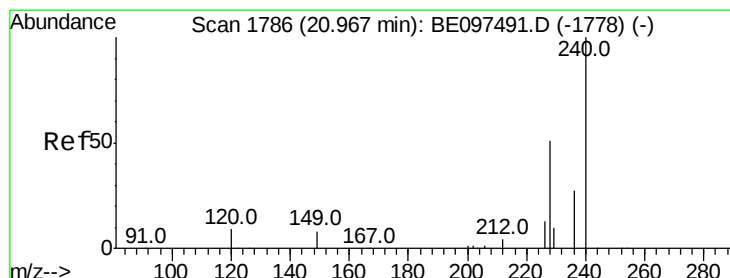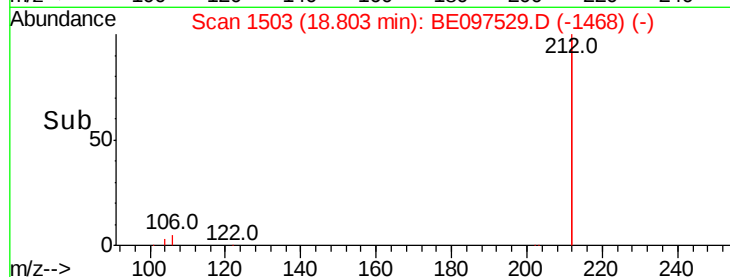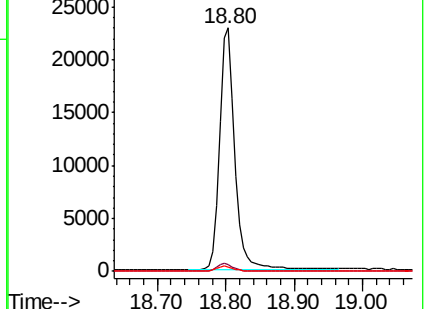

#27

Chrysene-d12

Concen: 0.400 ng

RT: 20.97 min Scan# 1788

Delta R.T. 0.00 min

Lab File: BE097529.D

Acq: 18 Sep 2018 12:29


Tgt Ion:240 Resp: 8615

Ion Ratio Lower Upper

240 100

120 10.4 5.5 8.3#



236 27.0 20.7 31.1

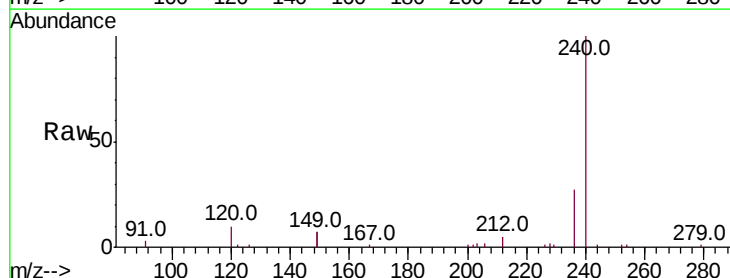


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

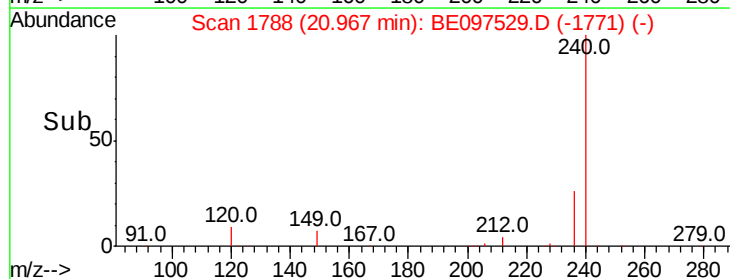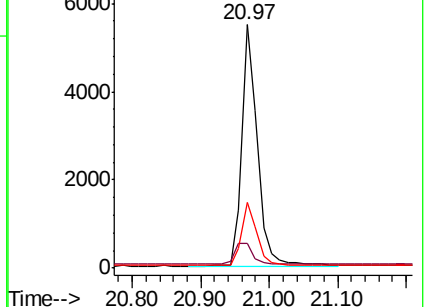



#29

Terphenyl-d14

Concen: 0.483 ng

RT: 19.41 min Scan# 1609

Delta R.T. -0.01 min

Lab File: BE097529.D

Acq: 18 Sep 2018 12:29

Instrument :

BNA_E

ClientSampleId :

BP-DUP01-20180912


Tot Ion:244 Resp: 7955

Ion Ratio Lower Upper

244 100

212 33.6 25.4 38.0




122 12.1 8.1 12.1

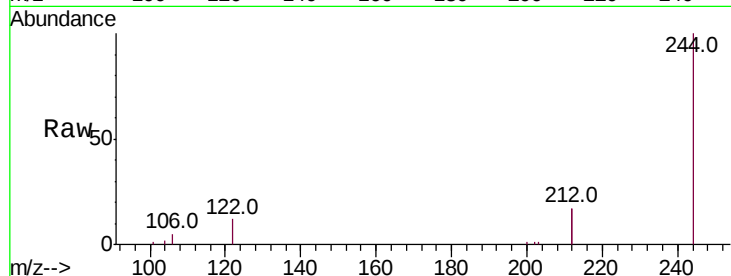

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

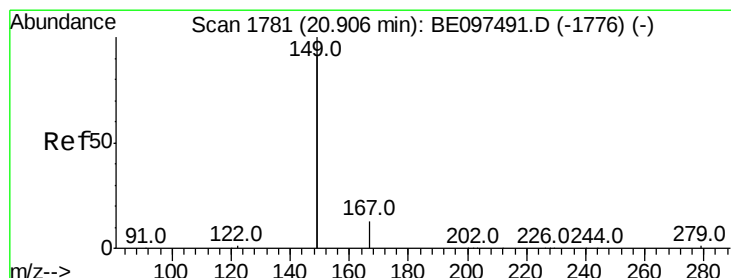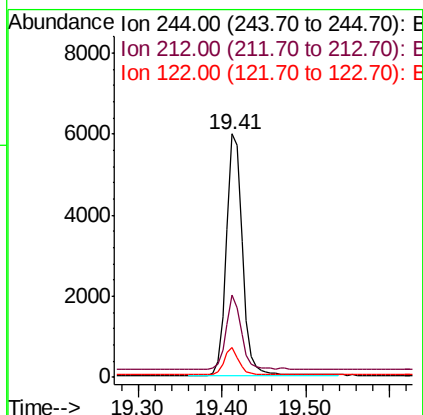

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.041 ng

RT: 20.91 min Scan# 1783

Delta R.T. 0.00 min

Lab File: BE097529.D

Acq: 18 Sep 2018 12:29


Tgt Ion:149 Resp: 1954

Ion Ratio Lower Upper

149 100

167 6.2 5.4 8.0



279 1.1 0.7 1.1



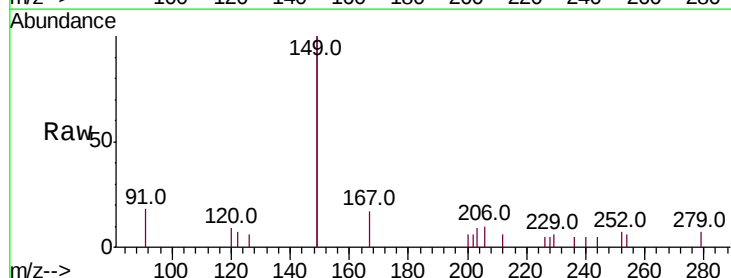


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

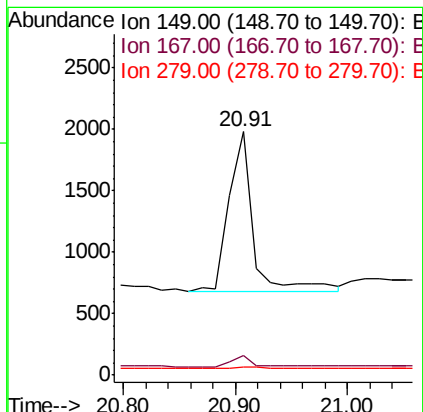

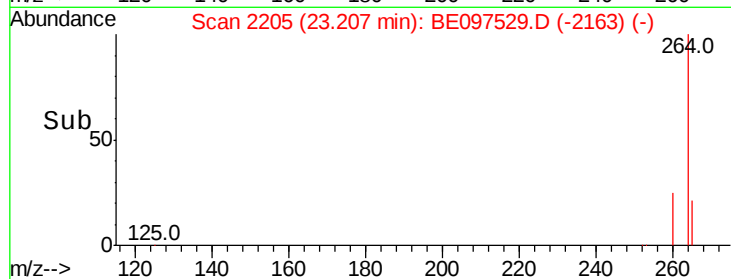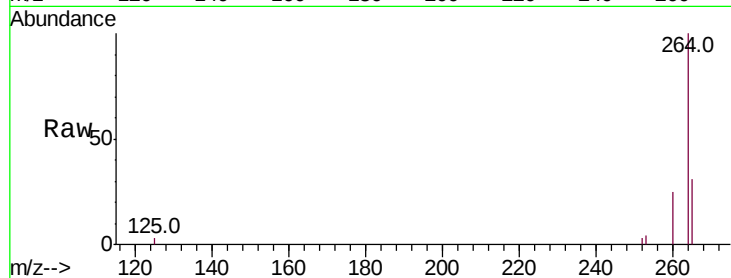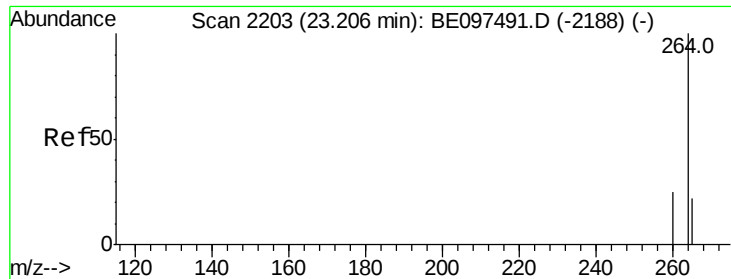

#34

Pervlene-d12

Concen: 0.400 ng

RT: 23.21 min Scan# 2205

Delta R.T. 0.00 min

Lab File: BE097529.D

Acq: 18 Sep 2018 12:29

Instrument :

BNA_E

ClientSampleId :

BP-DUP01-20180912

Tot Ion: 264 Resp: 8702

Ion Ratio Lower Upper

264 100

260 25.5 20.5 30.7

265 30.8 22.8 34.2

