
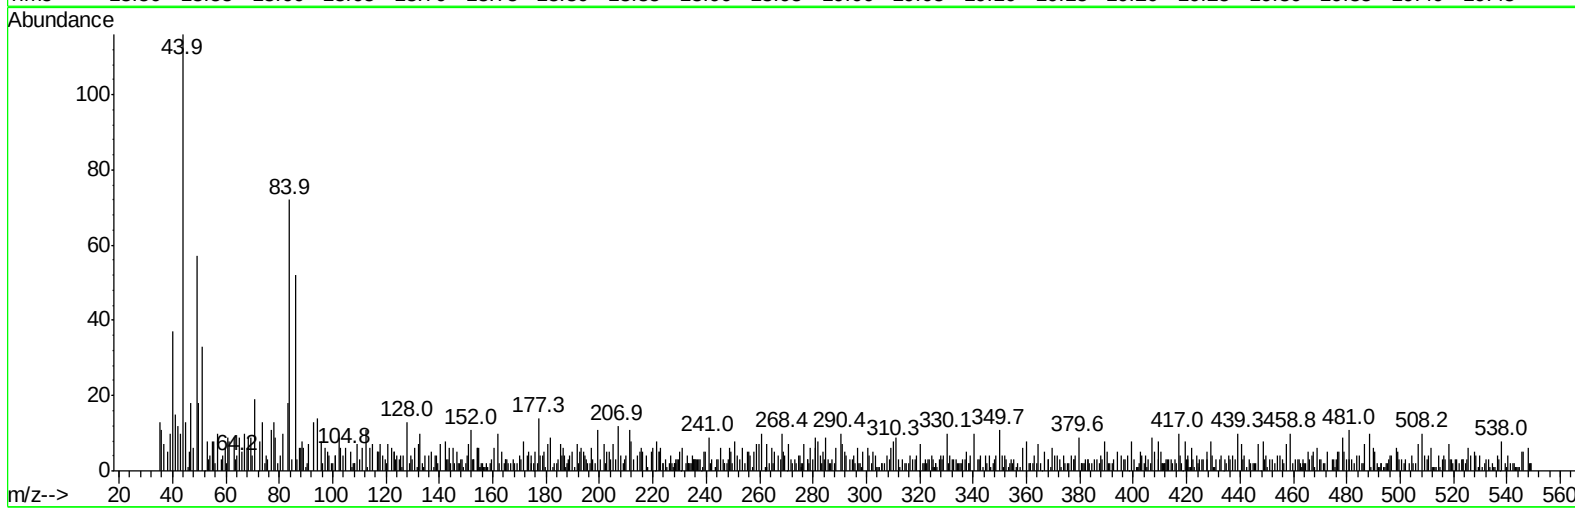


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE091718\
Data File : BE097496.D
Acq On : 17 Sep 2018 15:13
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 07:49:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF090518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 05 18:03:31 2018
Response via : Initial Calibration

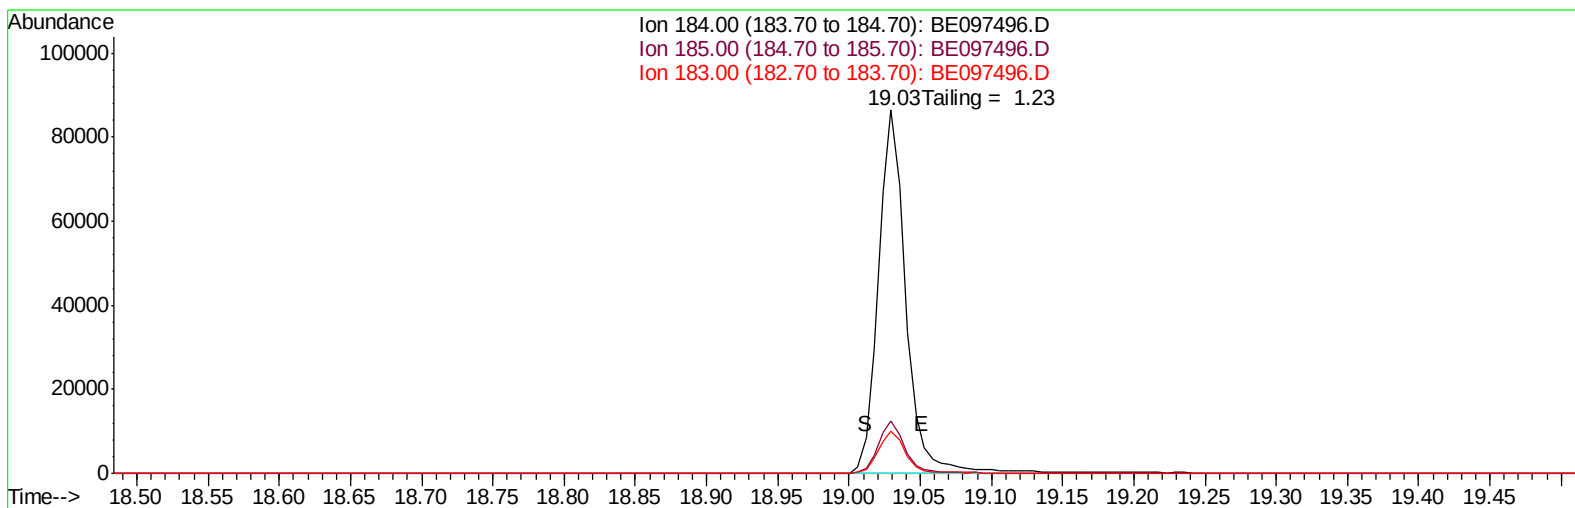

TIC: BE097496.D

(76) Benzidine



12.537min (-0.029) 9.04ng

response 3

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	140.00#
183.00	11.60	60.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE091718\
Data File : BE097496.D
Acq On : 17 Sep 2018 15:13
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 07:49:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF090518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 05 18:03:31 2018
Response via : Initial Calibration

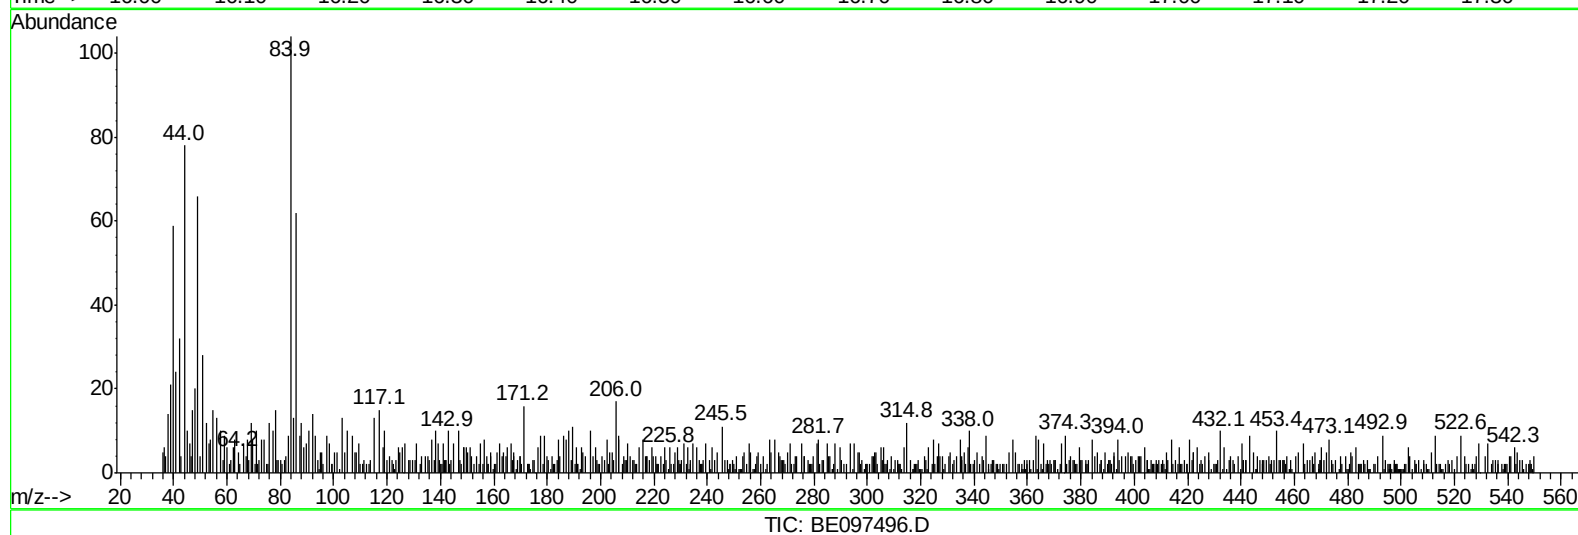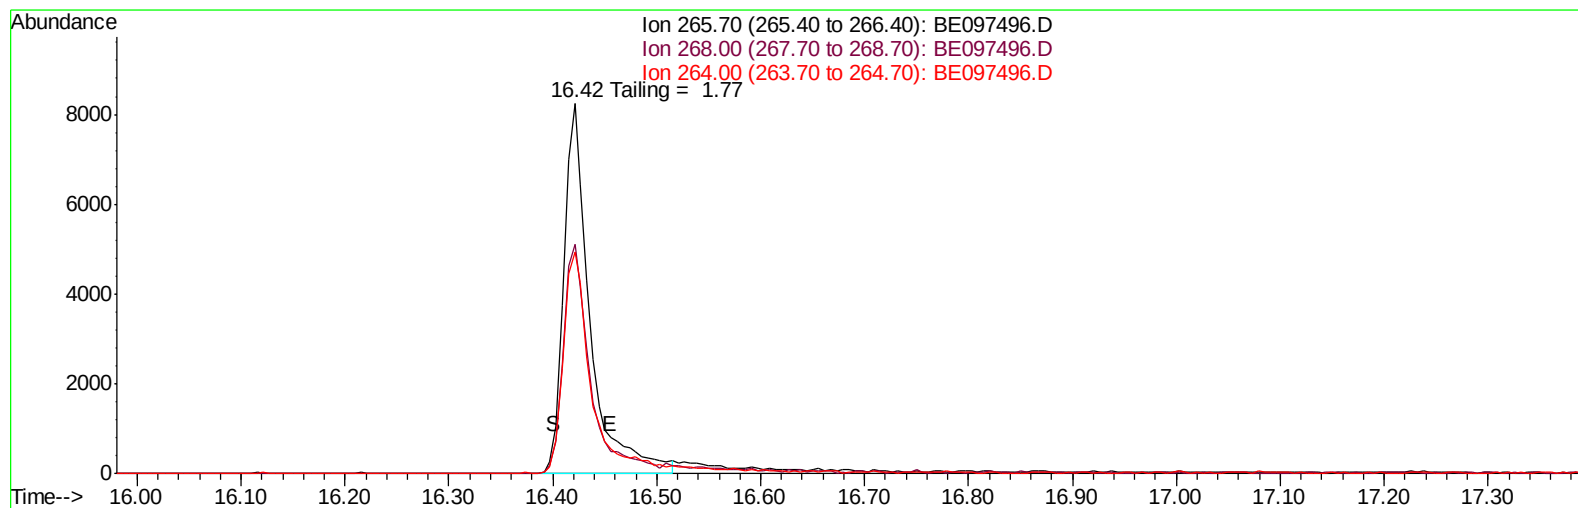

(69) Pentachlorophenol (C)

11.139min (+0.091) 123.33ng

response 10

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	75.00
264.00	61.90	62.50
0.00	0.00	0.00