
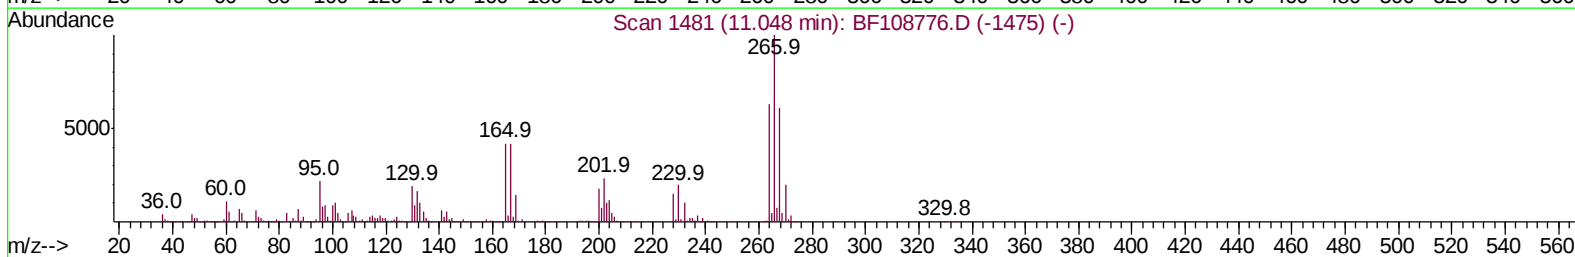
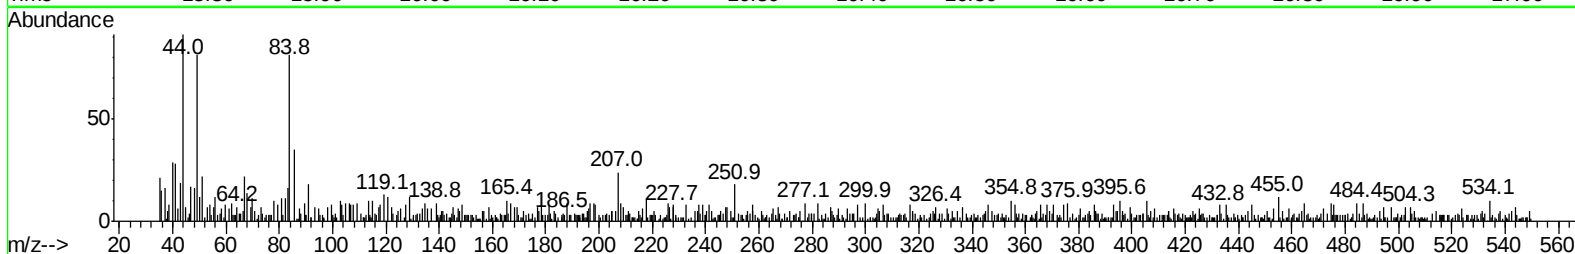


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE091718\  
Data File : BE097515.D  
Acq On : 18 Sep 2018 3:44  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 07:50:29 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF090518.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Sep 05 18:03:31 2018  
Response via : Initial Calibration

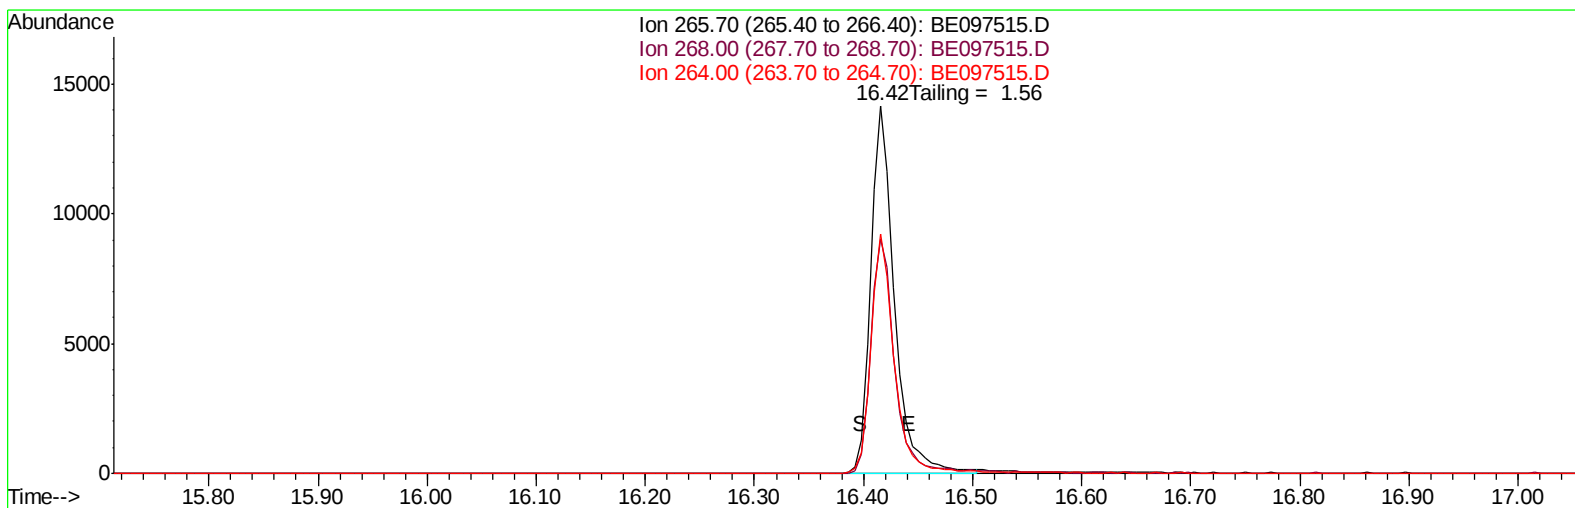

TIC: BE097515.D

(69) Pentachlorophenol (C)




11.215min (+0.167) 58.14ng

response 9

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 55.56 |
| 264.00 | 61.90 | 66.67 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE091718\  
 Data File : BE097515.D  
 Acq On : 18 Sep 2018 3:44  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 07:50:29 2018  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF090518.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Sep 05 18:03:31 2018  
 Response via : Initial Calibration

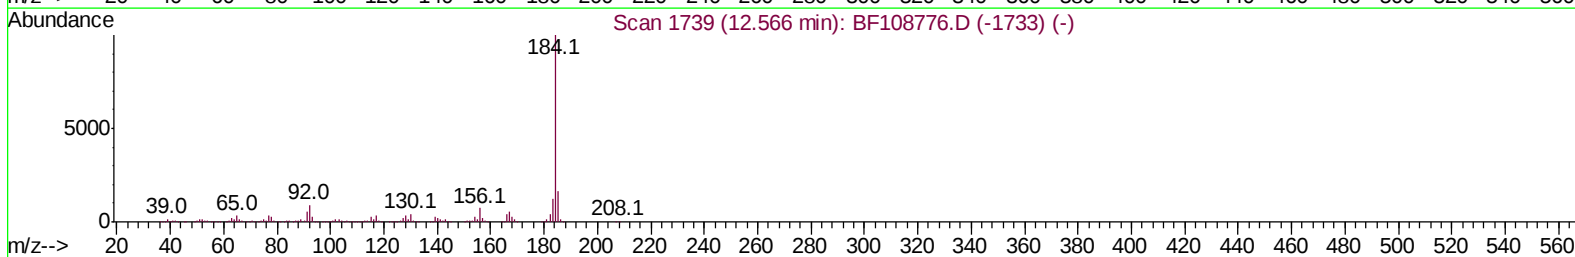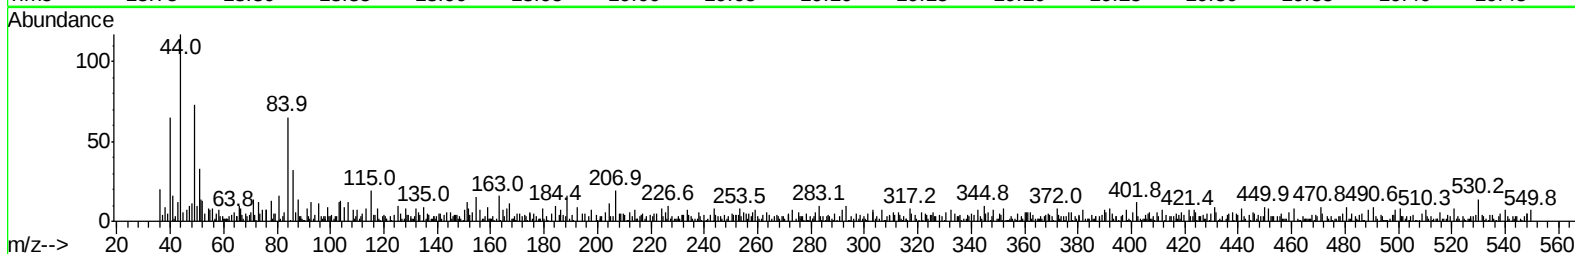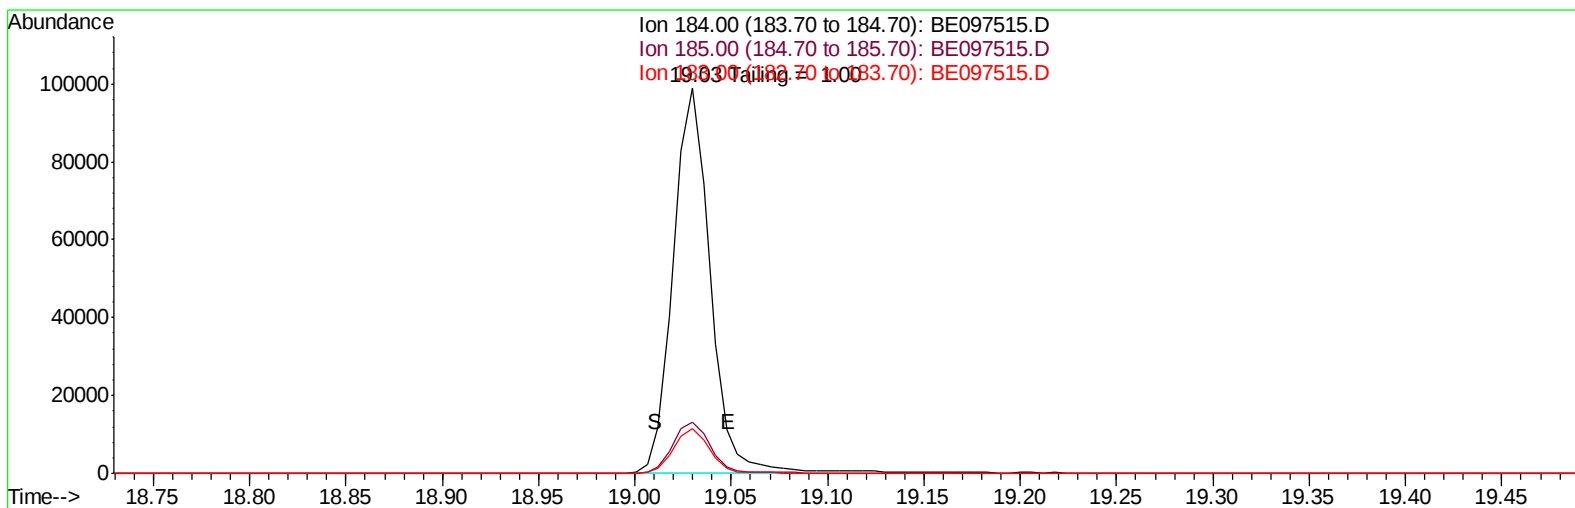

TIC: BE097515.D

(76) Benzidine

12.514min (-0.052) 36.17ng

response 12

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 184.00 | 100   | 100    |
| 185.00 | 15.70 | 40.00# |
| 183.00 | 11.60 | 50.00# |
| 0.00   | 0.00  | 0.00   |