

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE091718\
 Data File : BE097506.D
 Acq On : 17 Sep 2018 21:28
 Operator : SJ/JU
 Sample : J4892-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 PR-MW-05-091218

Manual Integrations
 APPROVED

Sohil
 9/18/2018 5:56:11 PM

Quant Time: Sep 18 14:34:05 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091718.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Sep 17 18:57:11 2018

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	1139	0.40	ng	0.00
7) Naphthalene-d8	10.12	136	5850	0.40	ng	-0.01
13) Acenaphthene-d10	14.00	164	4955m	0.40	ng	0.00
19) Phenanthrene-d10	16.75	188	8490	0.40	ng	-0.01
27) Chrysene-d12	20.97	240	9680	0.40	ng	0.00
34) Perylene-d12	23.20	264	9782	0.40	ng	0.00

System Monitoring Compounds

4) 2-Fluorophenol	5.05	112	1858m	0.48	ng	0.00
5) Phenol-d6	6.62	99	926m	0.19	ng	0.01
8) Nitrobenzene-d5	8.49	82	10694	2.27	ng	-0.03
11) 2-Methylnaphthalene-d10	11.71	152	3833	0.46	ng	-0.01
14) 2,4,6-Tribromophenol	15.51	330	914	0.35	ng	-0.02
15) 2-Fluorobiphenyl	12.61	172	6691	0.39	ng	-0.01
25) Fluoranthene-d10	18.80	212	46444	0.46	ng	0.00
29) Terphenyl-d14	19.41	244	8848	0.48	ng	0.00

Target Compounds

						Qvalue
9) Naphthalene	10.17	128	8547385	160.943	ng	99
12) 2-Methylnaphthalene	11.78	142	524547	61.751	ng	98
17) Acenaphthene	14.06	154	2388	0.180	ng	# 78
18) Fluorene	15.05	166	7478	0.441	ng	# 78
22) Pentachlorophenol	16.43	266	94m	0.212	ng	
23) Phenanthrene	16.79	178	2996	0.150	ng	# 87
26) Fluoranthene	18.83	202	705	0.027	ng	99
28) Pyrene	19.19	202	640	0.026	ng	# 90
32) Bis(2-ethylhexyl)phthalate	20.91	149	11952	0.221	ng	# 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE091718\
Data File : BE097506.D
Acq On : 17 Sep 2018 21:28
Operator : SJ/JU
Sample : J4892-12
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
PR-MW-05-091218

Manual Integrations
APPROVED

Sohil
9/18/2018 5:56:11 PM

Quant Time: Sep 18 14:34:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 17 18:57:11 2018
Response via : Initial Calibration

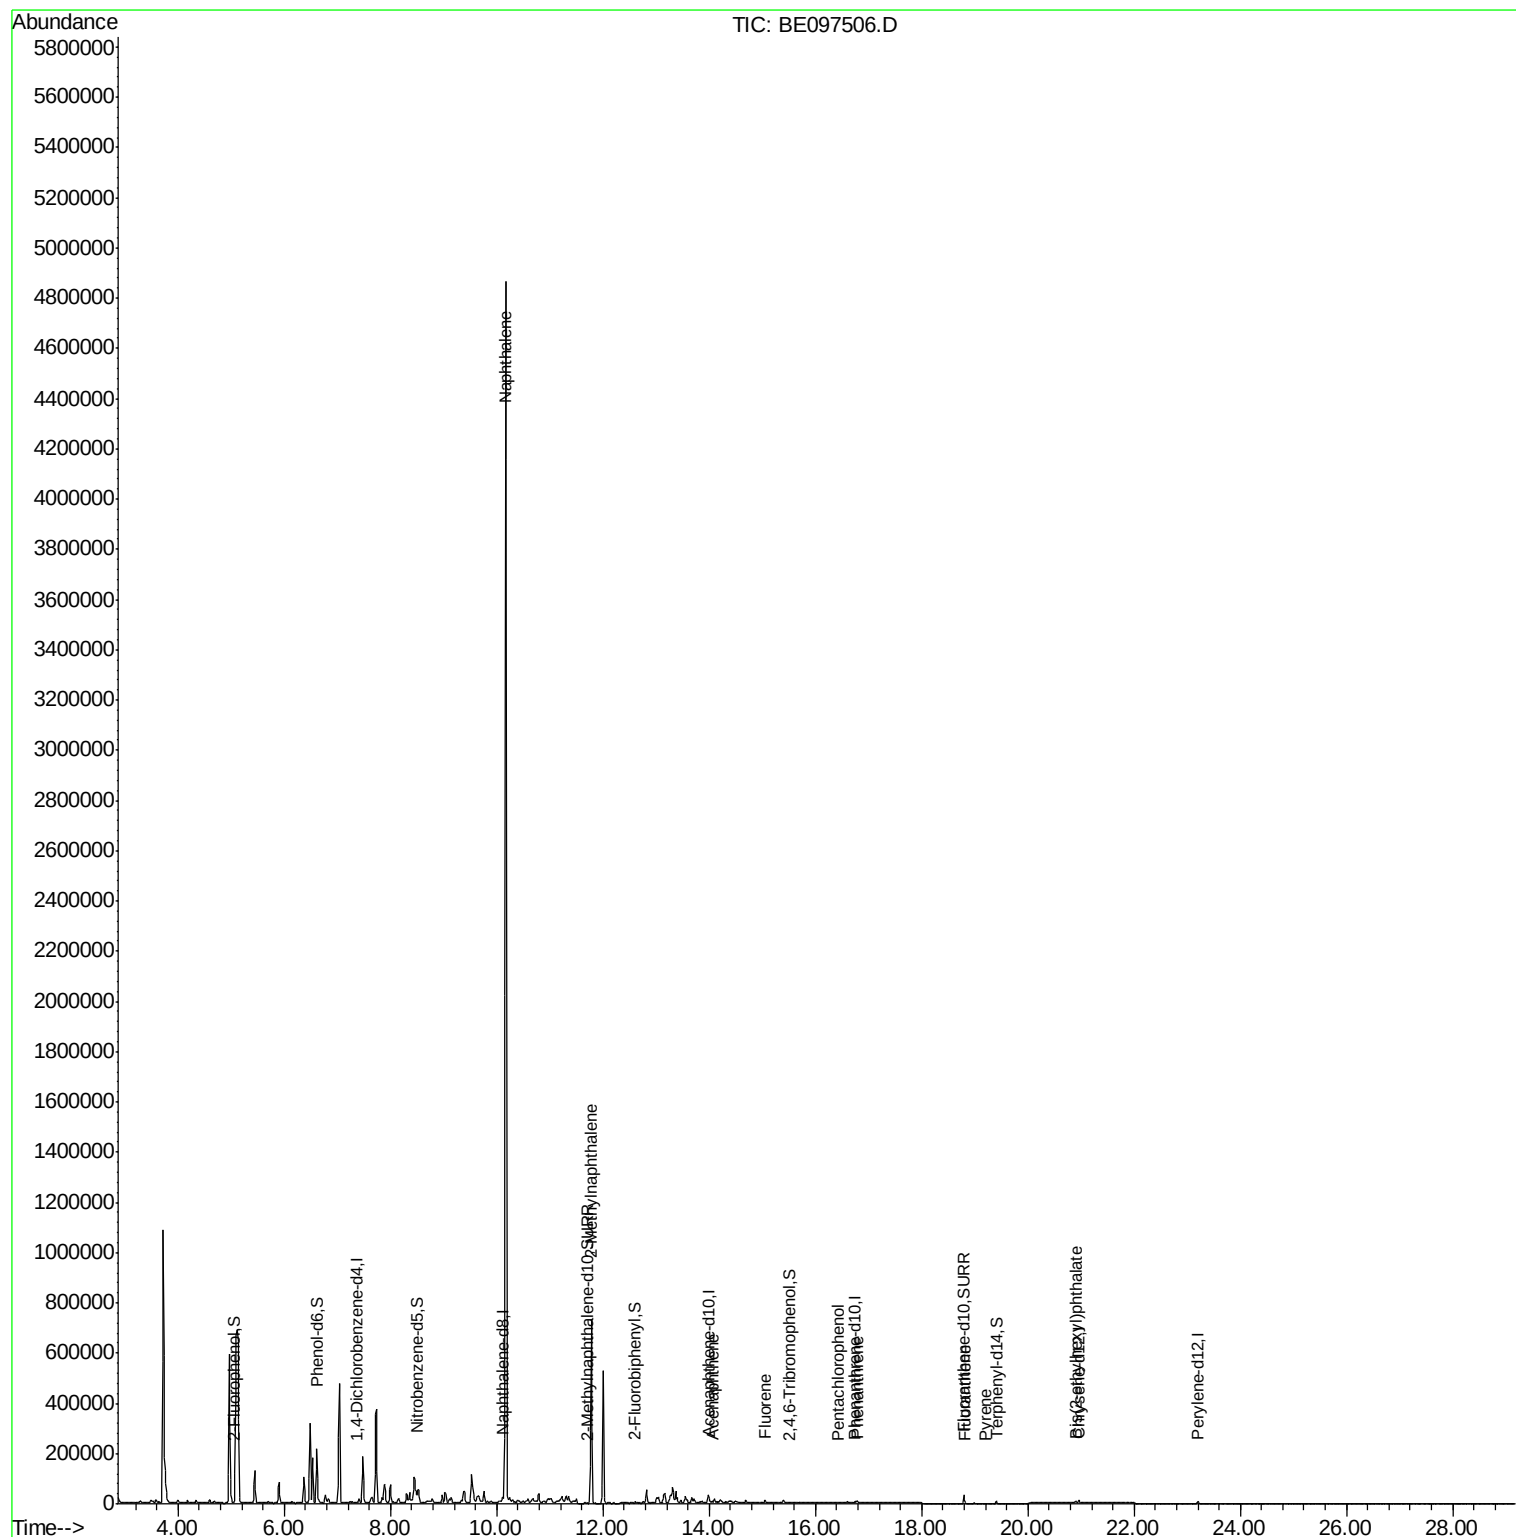


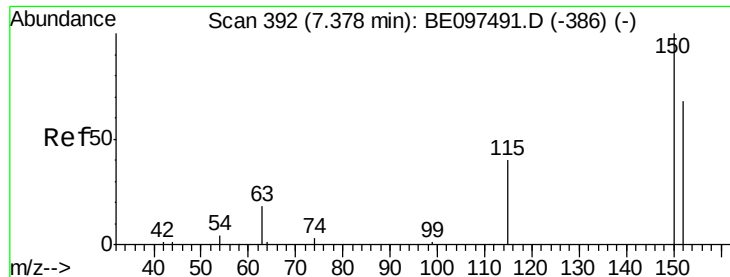

#1

1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.38 min Scan# 392
Delta R.T. 0.00 min
Lab File: BE097506.D
Acq: 17 Sep 2018 21:28




Instrument :
BNA_E
ClientSampleId :
PR-MW-05-091218

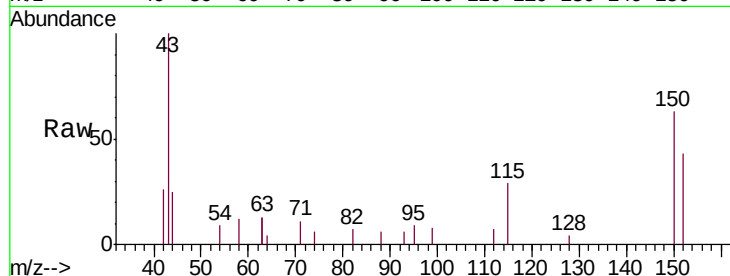

Tgt Ion	Ratio	Lower	Upper
152	100		
150	145.8	117.2	175.8
115	68.0	57.0	85.6


Manual Integrations
APPROVED

Sohil
9/18/2018 5:56:11 PM

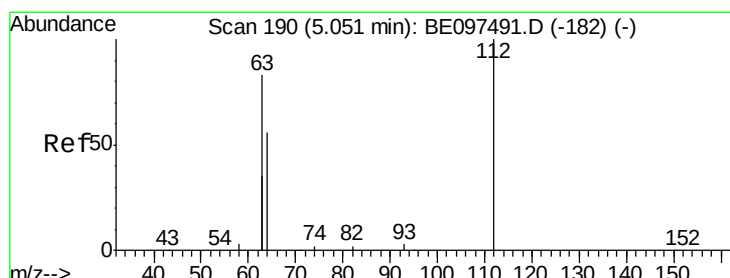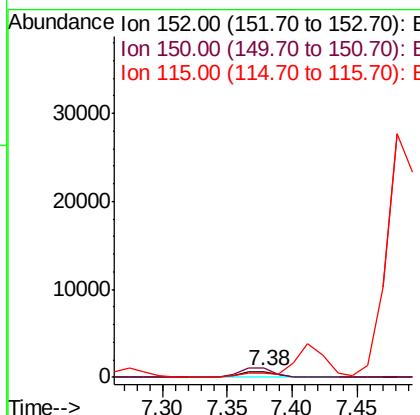
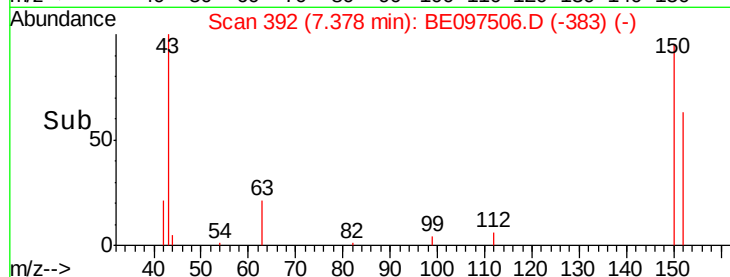





#4

2-Fluorophenol
Concen: 0.482 ng m
RT: 5.05 min Scan# 190
Delta R.T. 0.00 min
Lab File: BE097506.D
Acq: 17 Sep 2018 21:28

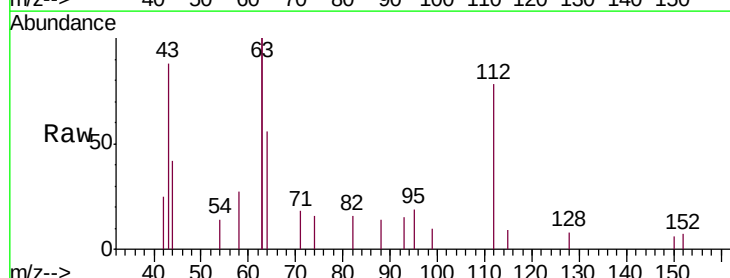

Tgt Ion	Ratio	Lower	Upper
112	100		
64	0.0	60.1	90.1#
63	0.0	116.8	175.2#

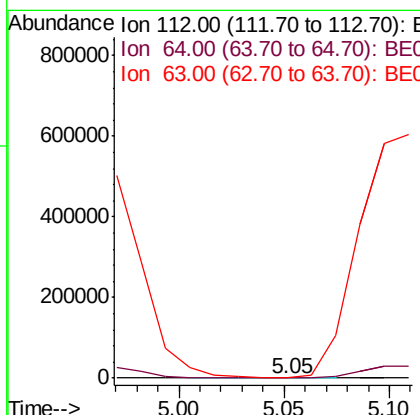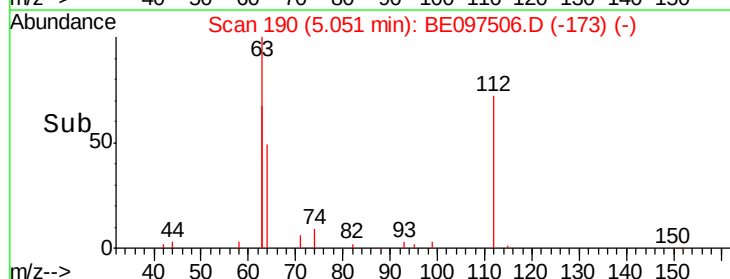

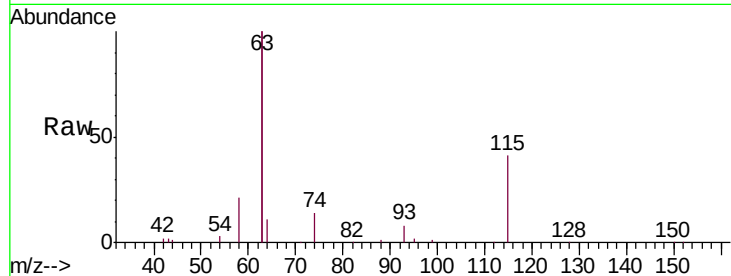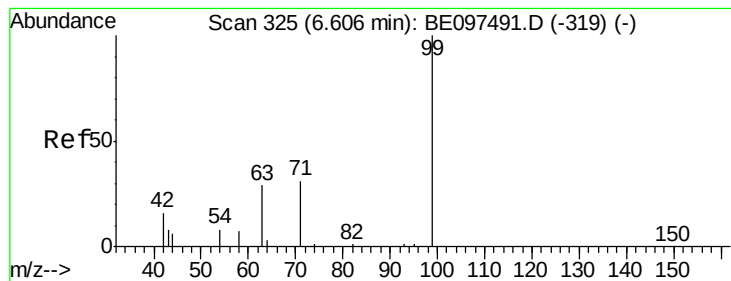

#5

Phenol-d6

Concen: 0.189 ng m

RT: 6.62 min Scan# 326

Delta R.T. 0.01 min

Lab File: BE097506.D

Acq: 17 Sep 2018 21:28

Tgt Ion:	99	Resp:	926
Ion Ratio	Lower	Upper	
99	100		
42	0.0	20.2	30.2#
71	0.0	28.4	42.6#

Instrument :





BNA_E

ClientSampleId :

PR-MW-05-091218

Manual Integrations
APPROVED

Sohil
9/18/2018 5:56:11 PM

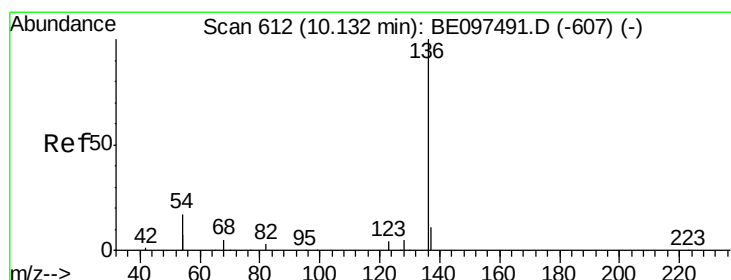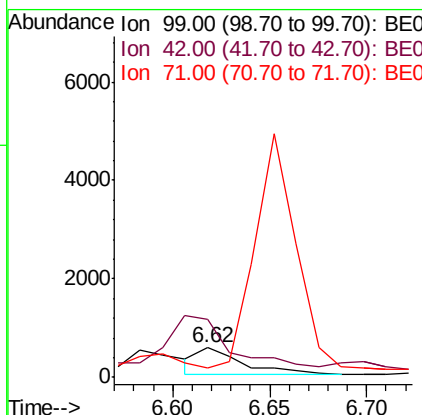

#7

Naphthalene-d8

Concen: 0.400 ng


RT: 10.12 min Scan# 611


Delta R.T. -0.01 min

Lab File: BE097506.D

Acq: 17 Sep 2018 21:28

Tgt Ion:	136	Resp:	5850
Ion Ratio	Lower	Upper	
136	100		
137	12.8	9.5	14.3
54	74.3	29.1	43.7#
68	16.5	6.2	9.2#

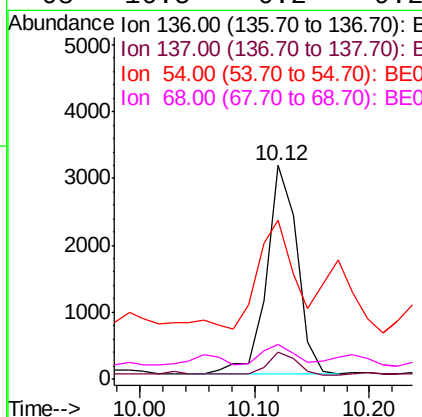







#8
 Nitrobenzene-d5
 Concen: 2.272 ng
 RT: 8.49 min Scan# 489
 Delta R.T. -0.03 min
 Lab File: BE097506.D
 Acq: 17 Sep 2018 21:28

Instrument :
 BNA_E
 ClientSampleId :
 PR-MW-05-091218

Tgt Ion	Ratio	Lower	Upper
82	100		
128	11.6	24.0	36.0#
54	45.5	40.0	60.0




Manual Integrations
 APPROVED


Sohil
 9/18/2018 5:56:11 PM

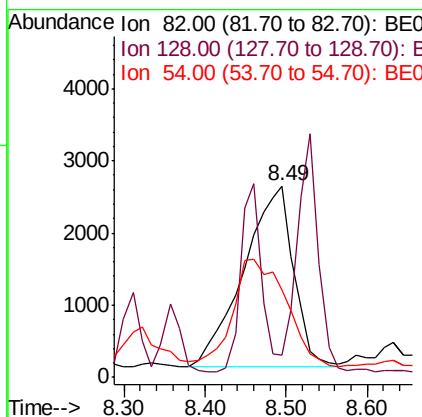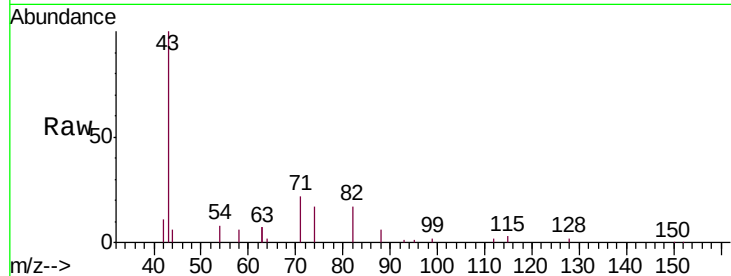

#9
 Naphthalene
 Concen: 160.943 ng
 RT: 10.17 min Scan# 615
 Delta R.T. 0.00 min
 Lab File: BE097506.D
 Acq: 17 Sep 2018 21:28

Tgt Ion	Ratio	Lower	Upper
128	100		
129	2.9	2.6	3.8
127	3.5	2.8	4.2

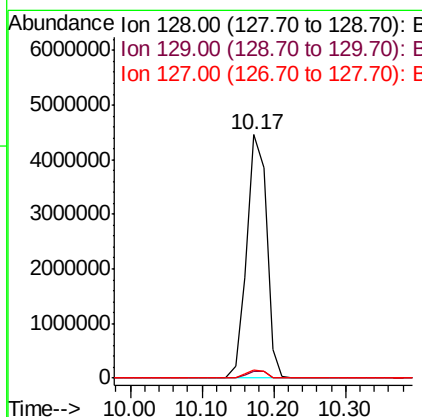

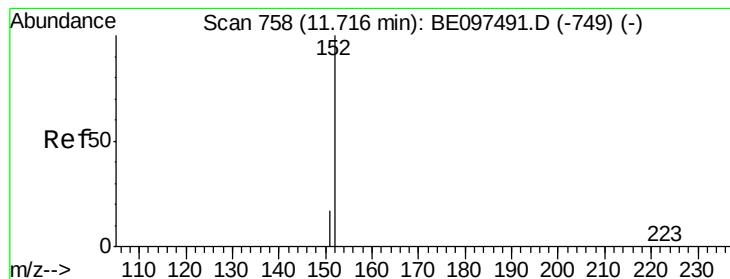

#11

2-Methylnaphthalene-d10

Concen: 0.459 ng

RT: 11.71 min Scan# 756

Delta R.T. -0.01 min

Lab File: BE097506.D

Acq: 17 Sep 2018 21:28

Instrument :

BNA_E

ClientSampleId :

PR-MW-05-091218

Tgt Ion:152 Resp: 3833

Ion Ratio Lower Upper


152 100

151 31.1 15.4 23.0#

Manual Integrations
APPROVED




Sohil

9/18/2018 5:56:11 PM

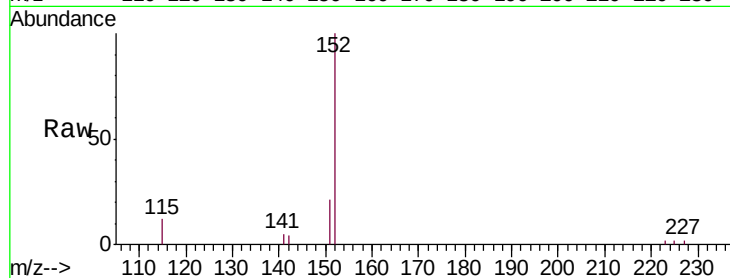

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

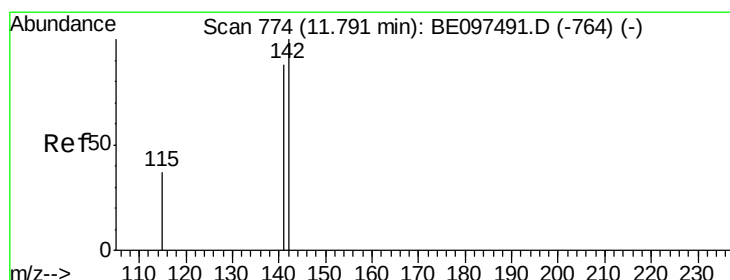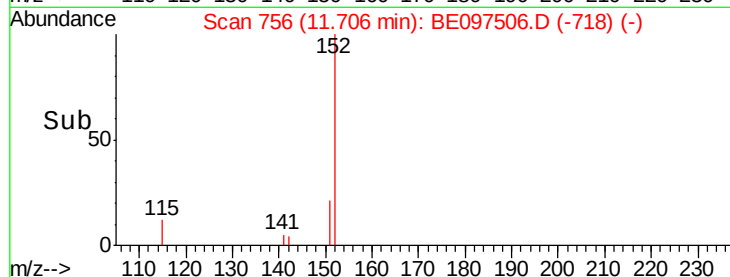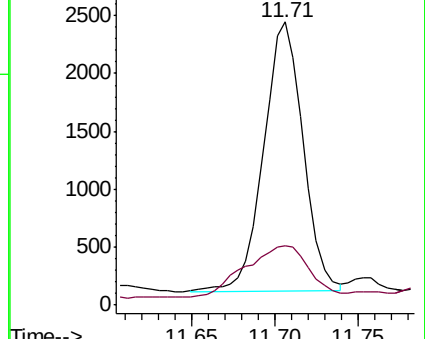

#12

2-Methylnaphthalene

Concen: 61.751 ng

RT: 11.78 min Scan# 772

Delta R.T. -0.01 min

Lab File: BE097506.D

Acq: 17 Sep 2018 21:28


Tgt Ion:142 Resp: 524547

Ion Ratio Lower Upper

142 100

141 89.3 70.4 105.6



115 37.4 31.7 47.5

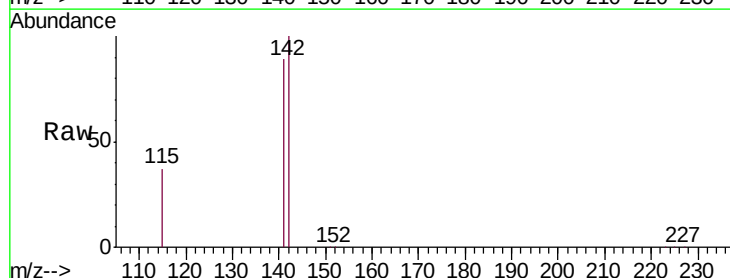


Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 115.00 (114.70 to 115.70): E

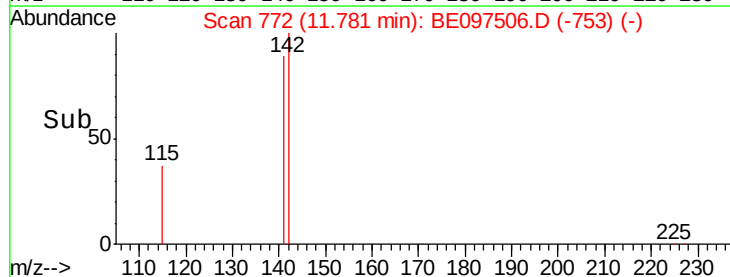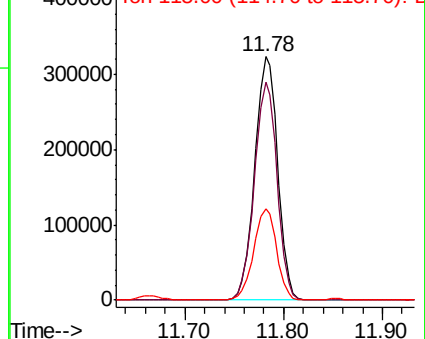



#13

Acenaphthene-d10

Concen: 0.400 ng m

RT: 14.00 min Scan# 1027

Delta R.T. -0.00 min

Lab File: BE097506.D

Acq: 17 Sep 2018 21:28

Instrument :

BNA_E





ClientSampleId :

PR-MW-05-091218

Tgt Ion	Ratio	Resp	Lower	Upper
164	100	4955		
162	90.1	83.1	124.7	
160	122.8	37.1	55.7#	

Manual Integrations
APPROVED

Sohil
9/18/2018 5:56:11 PM

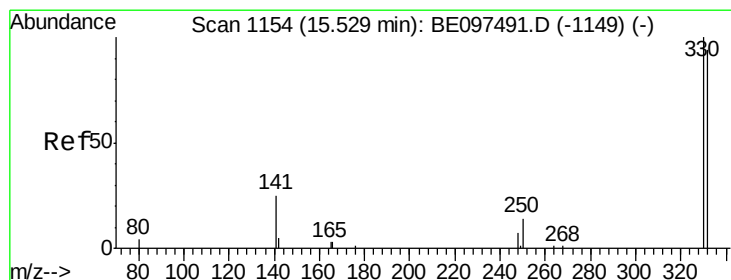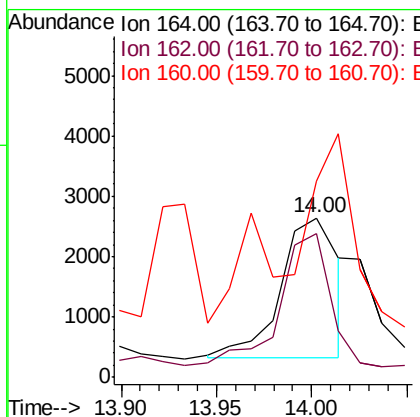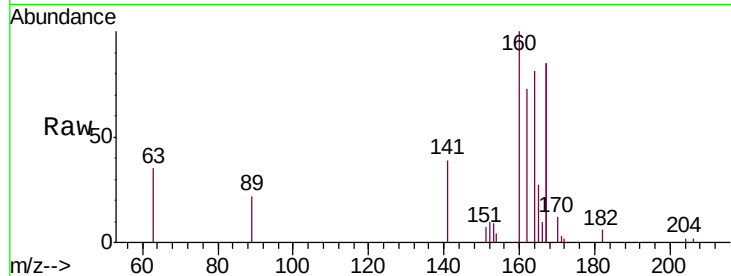

#14

2,4,6-Tribromophenol

Concen: 0.349 ng




RT: 15.51 min Scan# 1153


Delta R.T. -0.02 min

Lab File: BE097506.D

Acq: 17 Sep 2018 21:28

Tgt Ion	Ratio	Resp	Lower	Upper
330	100	914		
332	98.0	152.7	229.1#	
141	57.3	33.7	50.5#	

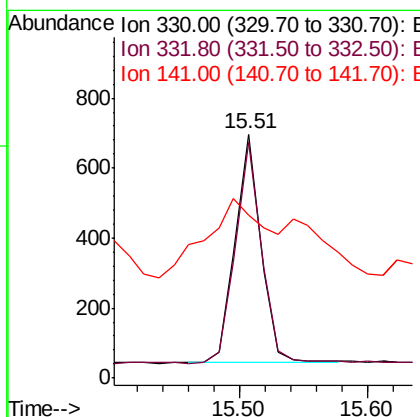

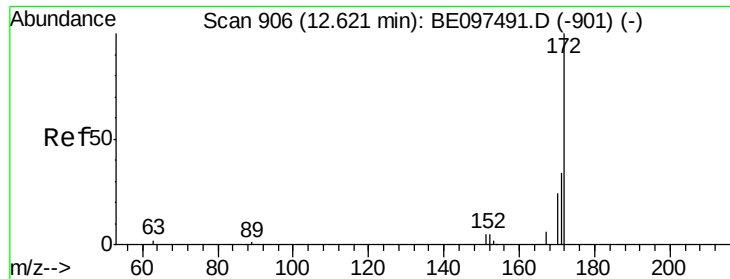





#15
2-Fluorobiphenyl
Concen: 0.387 ng
RT: 12.61 min Scan# 906
Delta R.T. -0.01 min
Lab File: BE097506.D
Acq: 17 Sep 2018 21:28

Instrument :
BNA_E
ClientSampleId :
PR-MW-05-091218

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.2	29.9	44.9
170	25.2	21.8	32.8




Manual Integrations
APPROVED


Sohil
9/18/2018 5:56:11 PM

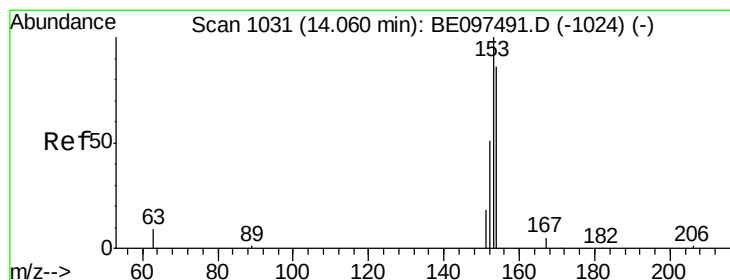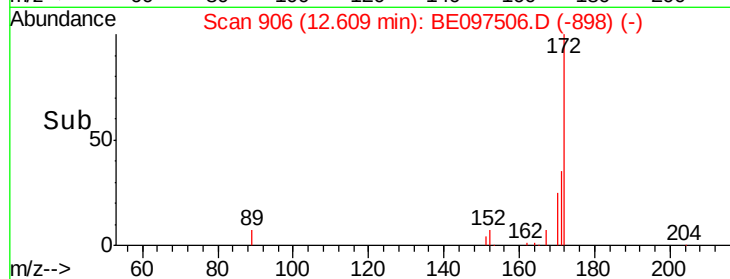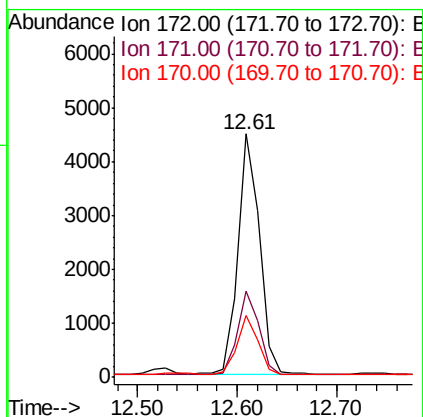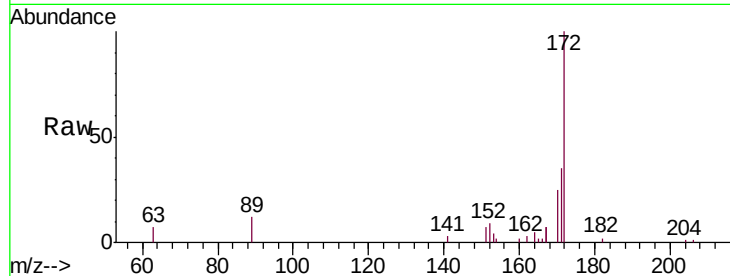

#17
Acenaphthene
Concen: 0.180 ng
RT: 14.06 min Scan# 1032
Delta R.T. -0.00 min
Lab File: BE097506.D
Acq: 17 Sep 2018 21:28

Tgt Ion	Ratio	Lower	Upper
154	100		
153	145.4	89.2	133.8#
152	51.9	42.0	63.0

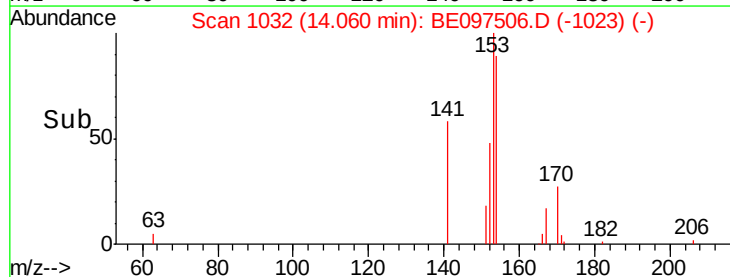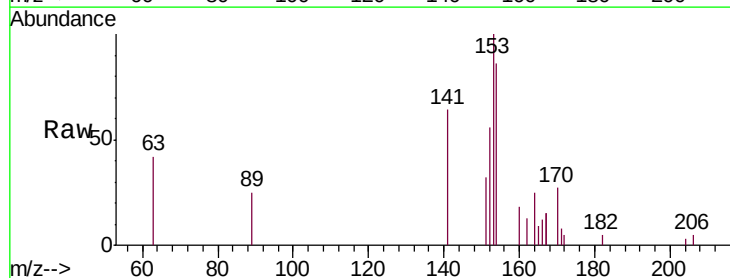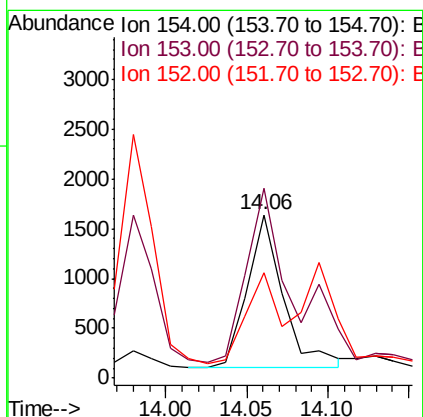







#18
Fluorene
 Concen: 0.441 ng
 RT: 15.05 min Scan# 1114
 Delta R.T. -0.01 min
 Lab File: BE097506.D
 Acq: 17 Sep 2018 21:28

Instrument :
 BNA_E
 ClientSampleId :
 PR-MW-05-091218

Tgt Ion	Ratio	Lower	Upper
166	100		
165	101.6	77.8	116.6
167	15.1	42.4	63.6#




Manual Integrations
 APPROVED


Sohil
 9/18/2018 5:56:11 PM

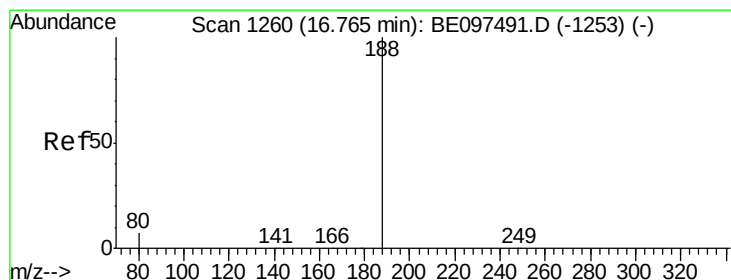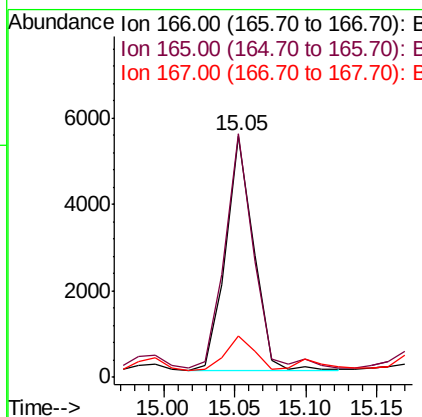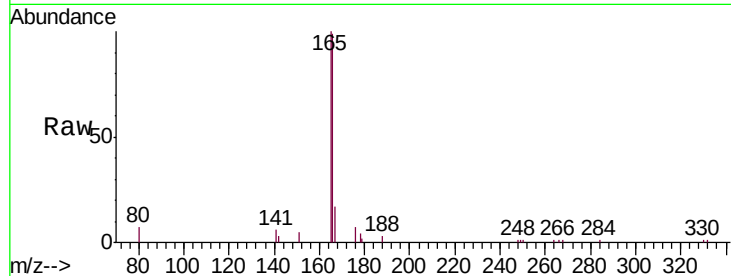

#19
Phenanthrene-d10
 Concen: 0.400 ng
 RT: 16.75 min Scan# 1260
 Delta R.T. -0.01 min
 Lab File: BE097506.D
 Acq: 17 Sep 2018 21:28

Tgt Ion	Ratio	Lower	Upper
188	100		
94	0.0	3.9	5.9#
80	15.7	3.6	5.4#

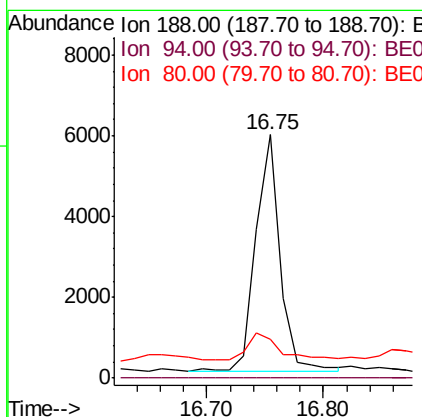



#22

Pentachlorophenol

Concen: 0.212 ng m

RT: 16.43 min Scan# 1232

Delta R.T. -0.06 min

Lab File: BE097506.D

Acq: 17 Sep 2018 21:28

Instrument :

BNA_E

ClientSampleId :


PR-MW-05-091218

Tgt Ion:	266	Resp:	94
Ion	Ratio	Lower	Upper
266	100		
264	74.5	72.5	108.7
268	82.4	73.8	110.6


Manual Integrations
APPROVED

Sohil



9/18/2018 5:56:11 PM

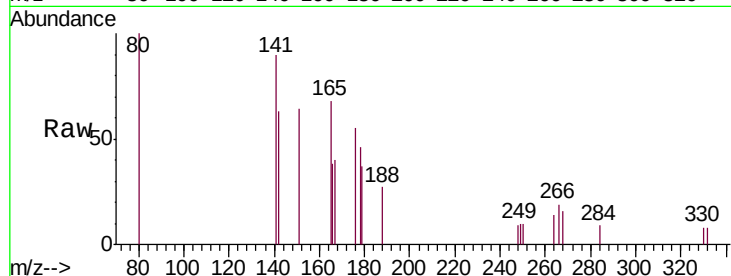

Abundance Ion 266.00 (265.70 to 266.70): E
Ion 264.00 (263.70 to 264.70): E
Ion 268.00 (267.70 to 268.70): E

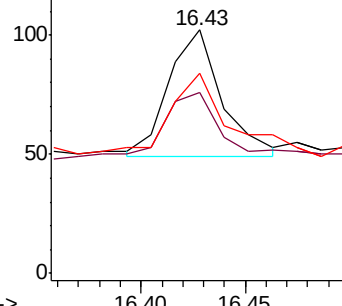

Time-->



#23

Phenanthrene

Concen: 0.150 ng

RT: 16.79 min Scan# 1263


Delta R.T. -0.01 min

Lab File: BE097506.D



Acq: 17 Sep 2018 21:28


Tgt Ion:	178	Resp:	2996
Ion	Ratio	Lower	Upper
178	100		
176	23.5	15.1	22.7#
179	21.2	11.8	17.6#

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

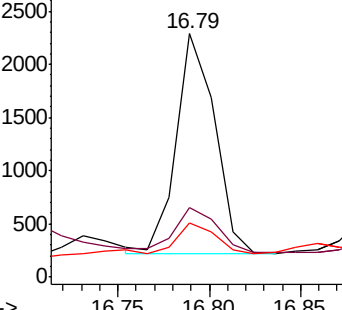

Time-->





#25

Fluoranthene-d10

Concen: 0.455 ng

RT: 18.80 min Scan# 1500

Delta R.T. -0.01 min

Lab File: BE097506.D

Acq: 17 Sep 2018 21:28

Instrument :

BNA_E





ClientSampleId :

PR-MW-05-091218

Tgt Ion:	212	Resp:	46444
Ion Ratio	Lower	Upper	
212	100		
106	3.4	2.8	4.2
104	1.8	1.6	2.4

Manual Integrations
APPROVED

Sohil
9/18/2018 5:56:11 PM

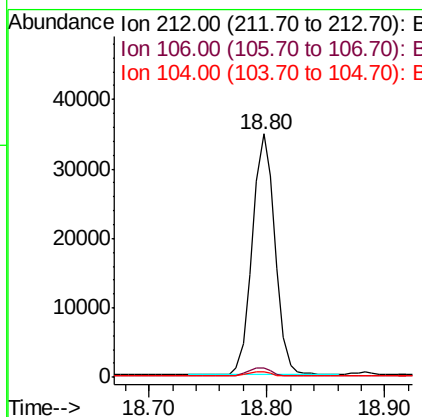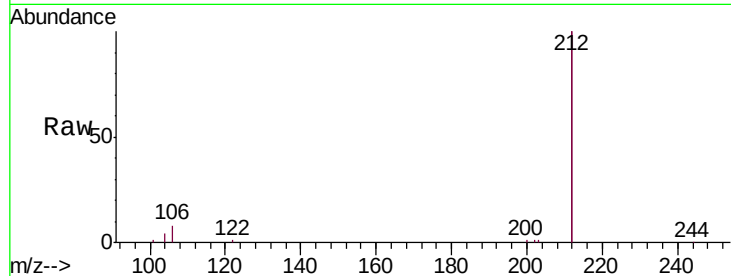

#26

Fluoranthene

Concen: 0.027 ng




RT: 18.83 min Scan# 1505


Delta R.T. -0.01 min

Lab File: BE097506.D

Acq: 17 Sep 2018 21:28

Tgt Ion:	202	Resp:	705
Ion Ratio	Lower	Upper	
202	100		
101	12.5	9.8	14.8
203	17.7	13.7	20.5

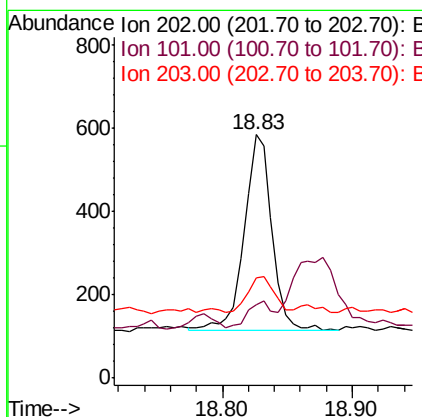



#27

Chrysene-d12

Concen: 0.400 ng

RT: 20.97 min Scan# 1786

Delta R.T. 0.00 min

Lab File: BE097506.D

Acq: 17 Sep 2018 21:28

Instrument :

BNA_E


ClientSampleId :

PR-MW-05-091218




Tgt Ion:	240	Resp:	9680
Ion Ratio	Lower	Upper	
240	100		
120	6.8	5.5	8.3
236	26.4	20.7	31.1

Manual Integrations
APPROVED

Sohil
9/18/2018 5:56:11 PM

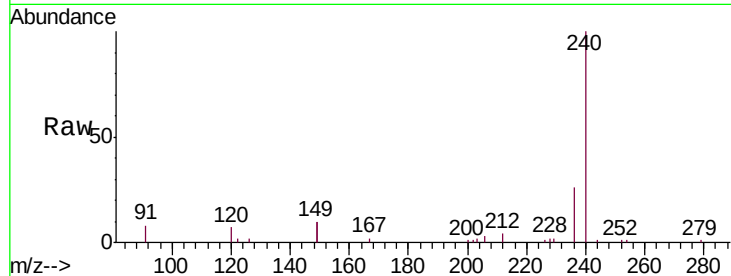

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

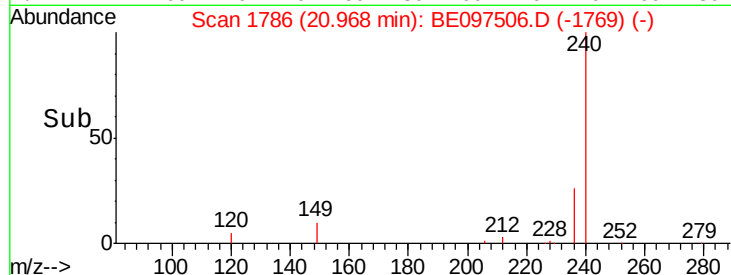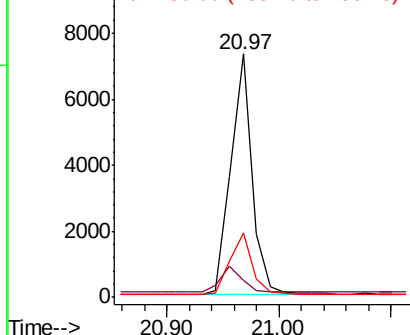

#28

Pyrene

Concen: 0.026 ng


RT: 19.19 min Scan# 1569

Delta R.T. -0.01 min



Lab File: BE097506.D


Acq: 17 Sep 2018 21:28

Tgt Ion:	202	Resp:	640
Ion Ratio	Lower	Upper	
202	100		
200	21.9	16.6	25.0
203	25.6	13.8	20.8#



Abundance Ion 202.00 (201.70 to 202.70): E
Ion 200.00 (199.70 to 200.70): E
Ion 203.00 (202.70 to 203.70): E

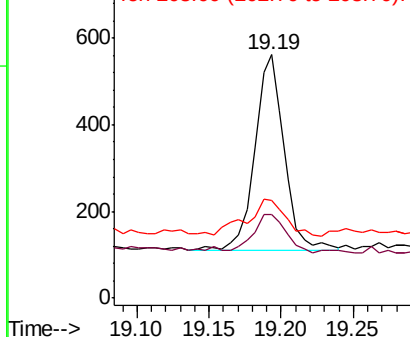







#29
 Terphenyl-d14
 Concen: 0.478 ng
 RT: 19.41 min Scan# 1607
 Delta R.T. -0.01 min
 Lab File: BE097506.D
 Acq: 17 Sep 2018 21:28

Instrument :
 BNA_E
 ClientSampleId :
 PR-MW-05-091218

Tgt Ion	Ratio	Resp	Lower	Upper
244	100	8848		
212	34.3		25.4	38.0
122	12.4		8.1	12.1#




Manual Integrations
 APPROVED




Sohil
 9/18/2018 5:56:11 PM

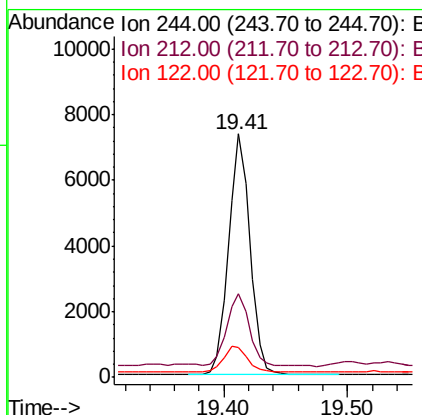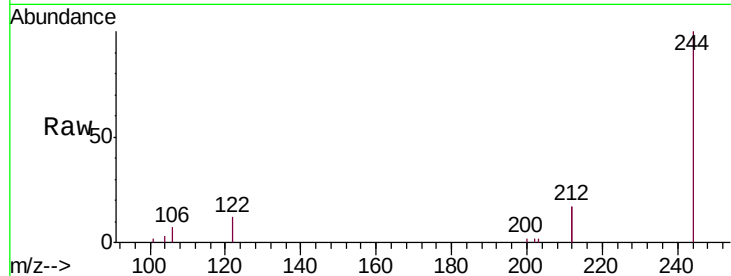

#32
 Bis(2-ethylhexyl)phthalate
 Concen: 0.221 ng
 RT: 20.91 min Scan# 1781
 Delta R.T. 0.00 min
 Lab File: BE097506.D
 Acq: 17 Sep 2018 21:28

Tgt Ion	Ratio	Resp	Lower	Upper
149	100	11952		
167	6.3		5.4	8.0
279	1.1		0.7	1.1#

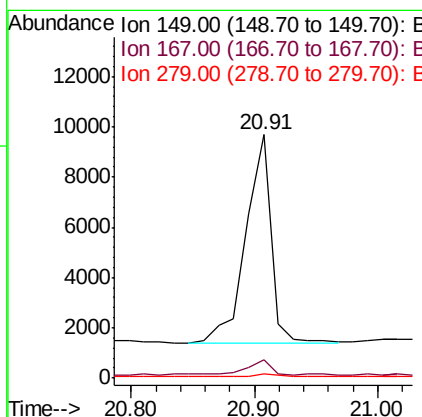

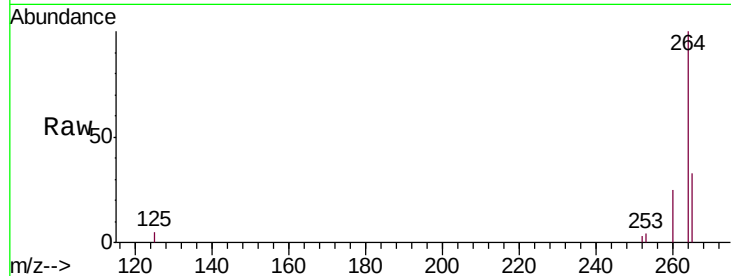

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.20 min Scan# 2202

Delta R.T. -0.00 min

Lab File: BE097506.D

Acq: 17 Sep 2018 21:28

Instrument :

BNA_E

ClientSampleId :

PR-MW-05-091218

Tgt Ion: 264 Resp: 9782

Ion Ratio Lower Upper

264 100

260 25.3 20.5 30.7

265 33.3 22.8 34.2

Manual Integrations
APPROVED

Sohil
9/18/2018 5:56:11 PM

