

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE091718\
 Data File : BE097525.D
 Acq On : 18 Sep 2018 10:00
 Operator : SJ/JU
 Sample : J4913-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BP-TT-AOC22-MW09-20180911

Quant Time: Sep 18 11:02:21 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 17 18:57:11 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	947	0.40	ng	0.00
7) Naphthalene-d8	10.13	136	4339	0.40	ng	0.00
13) Acenaphthene-d10	14.00	164	2612	0.40	ng	0.00
19) Phenanthrene-d10	16.75	188	7236	0.40	ng	-0.01
27) Chrysene-d12	20.97	240	8844	0.40	ng	0.00
34) Perylene-d12	23.20	264	8901	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.06	112	527	0.16	ng	0.00
5) Phenol-d6	6.60	99	448	0.11	ng	0.00
8) Nitrobenzene-d5	8.53	82	1502	0.43	ng	0.00
11) 2-Methylnaphthalene-d10	11.72	152	2610	0.42	ng	0.00
14) 2,4,6-Tribromophenol	15.52	330	536	0.39	ng	-0.01
15) 2-Fluorobiphenyl	12.62	172	5013	0.55	ng	0.00
25) Fluoranthene-d10	18.80	212	37372	0.43	ng	0.00
29) Terphenyl-d14	19.41	244	8362	0.49	ng	0.00
Target Compounds						Qvalue
32) Bis(2-ethylhexyl)phthalate	20.91	149	5574	0.113	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE091718\
Data File : BE097525.D
Acq On : 18 Sep 2018 10:00
Operator : SJ/JU
Sample : J4913-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-TT-AOC22-MW09-20180911

Quant Time: Sep 18 11:02:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 17 18:57:11 2018
Response via : Initial Calibration

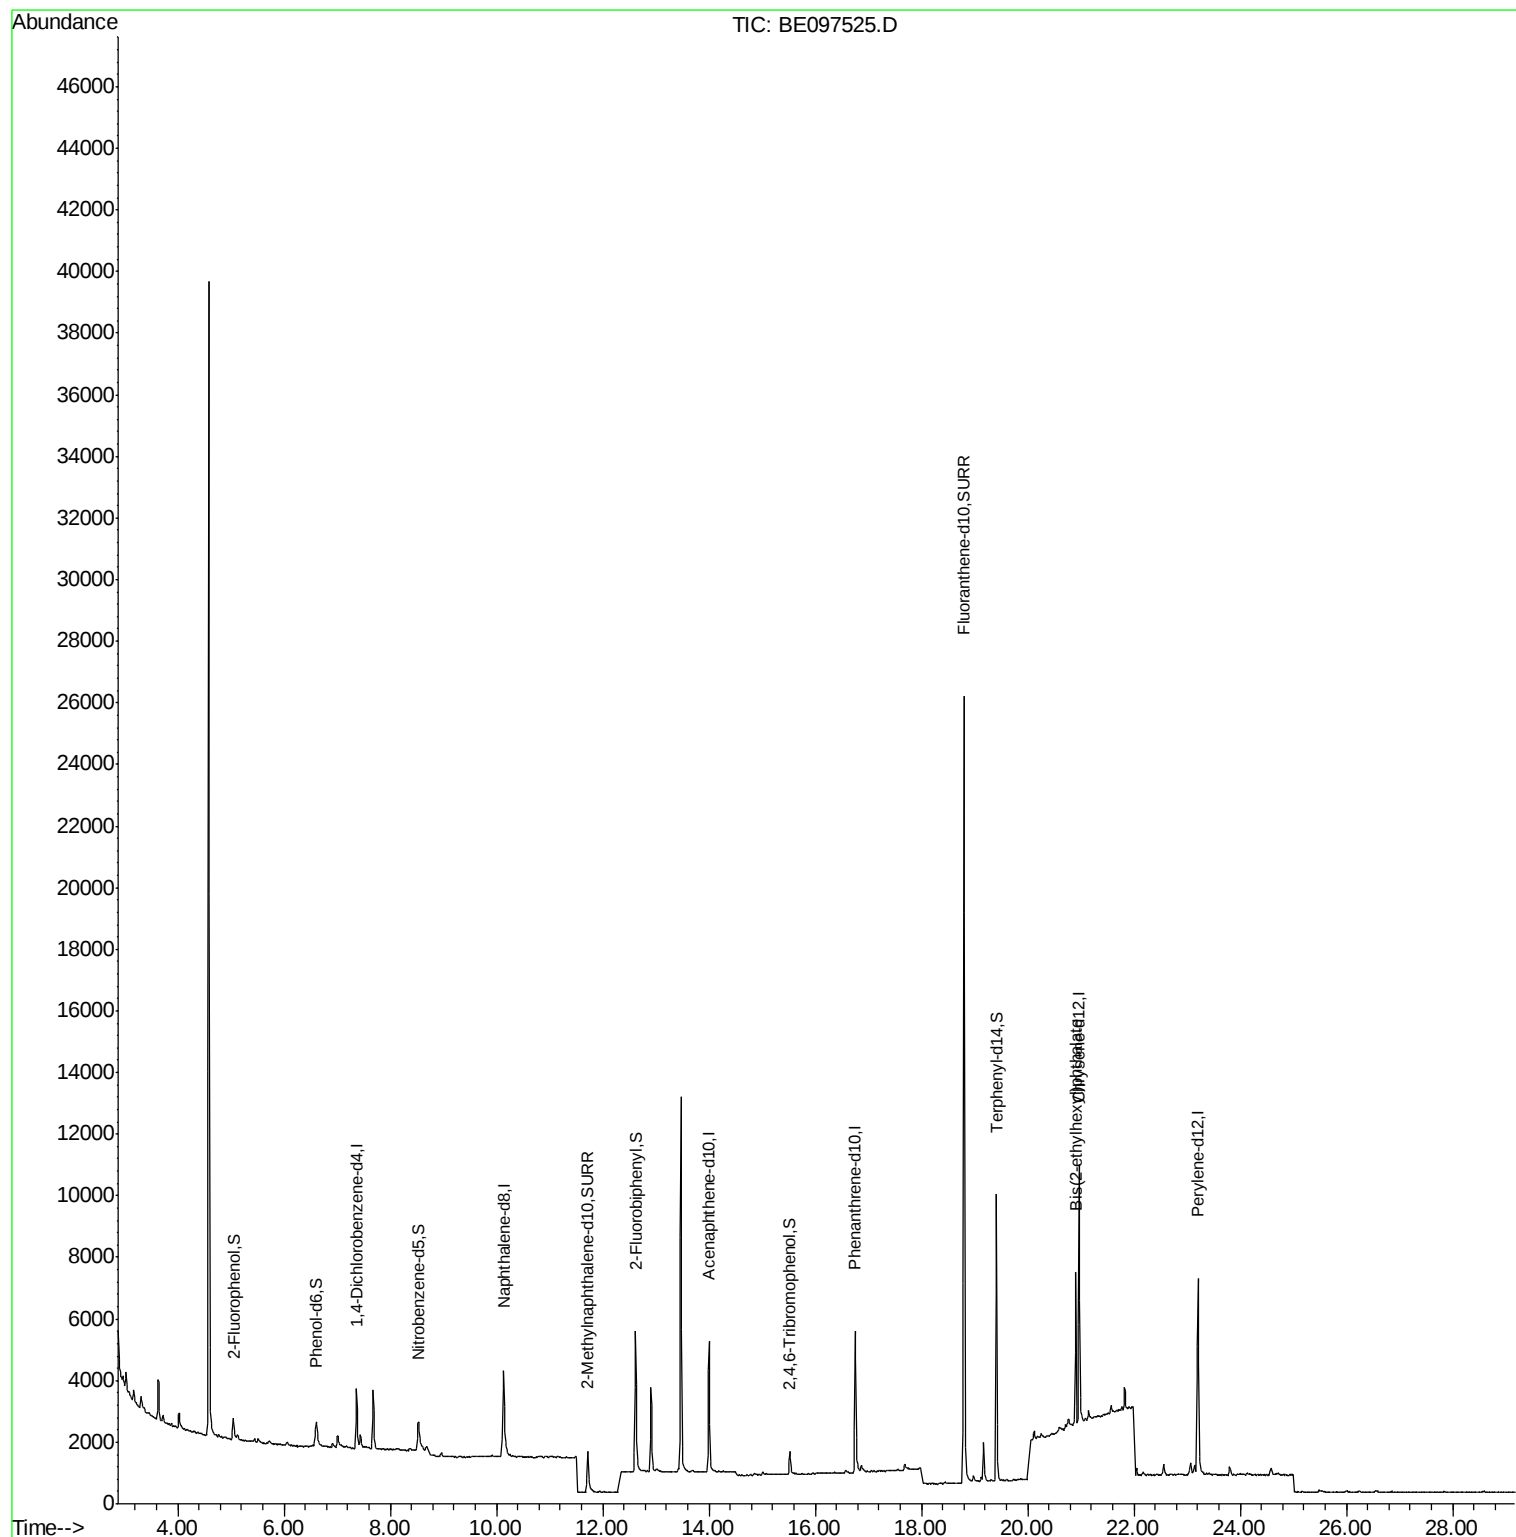


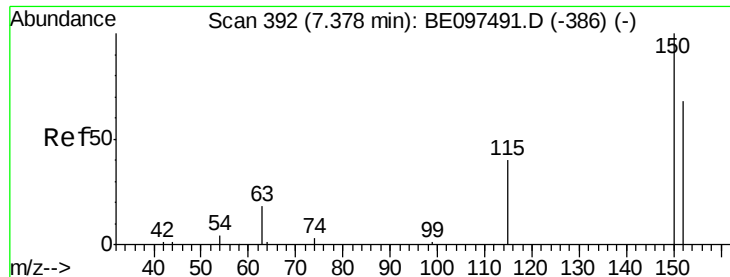




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.37 min Scan# 391
 Delta R.T. -0.01 min
 Lab File: BE097525.D
 Acq: 18 Sep 2018 10:00

Instrument :
 BNA_E
 ClientSampleId :
 BP-TT-AOC22-MW09-20180911

Tgt Ion:152 Resp: 947
 Ion Ratio Lower Upper
 152 100
 150 148.9 117.2 175.8
 115 71.1 57.0 85.6

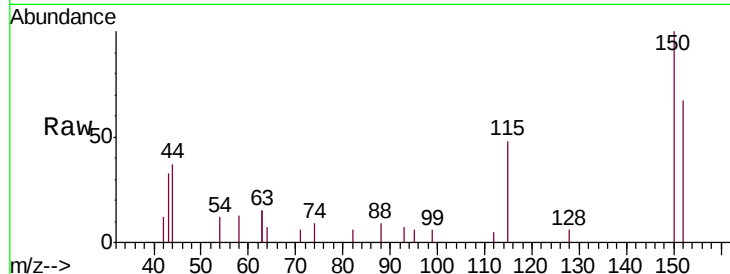


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

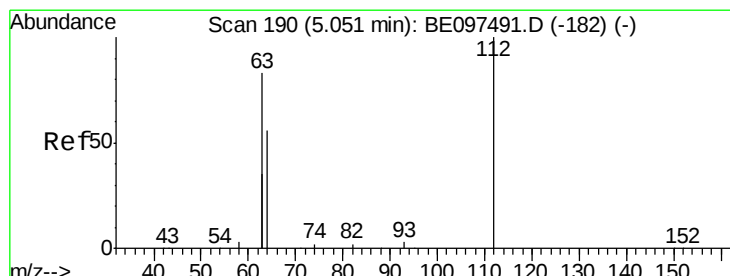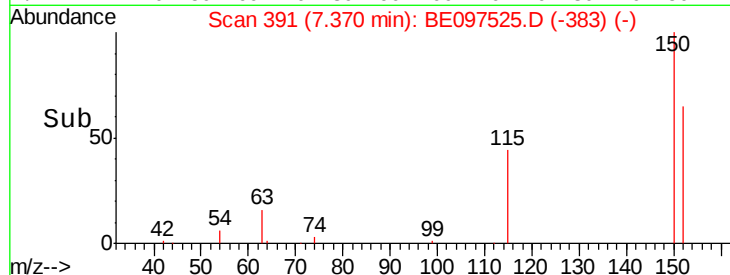
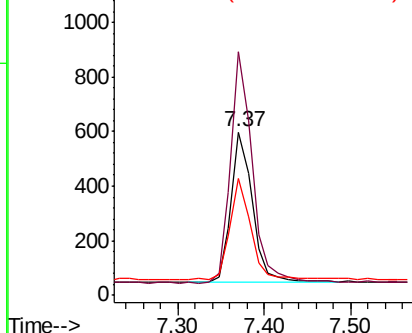



#4
 2-Fluorophenol
 Concen: 0.164 ng
 RT: 5.06 min Scan# 190
 Delta R.T. 0.00 min
 Lab File: BE097525.D
 Acq: 18 Sep 2018 10:00

Tgt Ion:112 Resp: 527
 Ion Ratio Lower Upper
 112 100
 64 70.2 60.1 90.1
 63 136.1 116.8 175.2

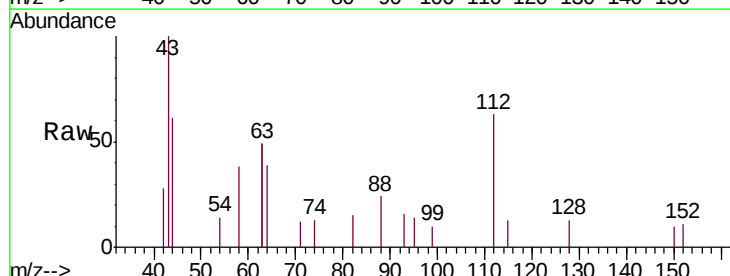

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BE0
 Ion 63.00 (62.70 to 63.70): BE0

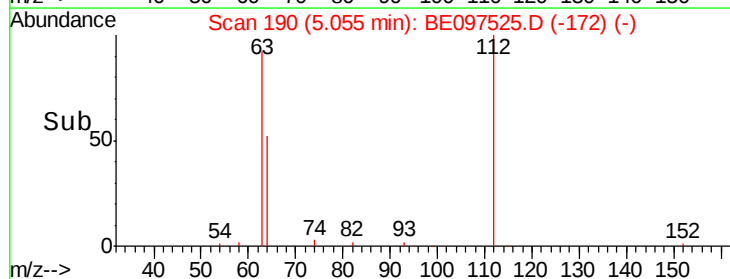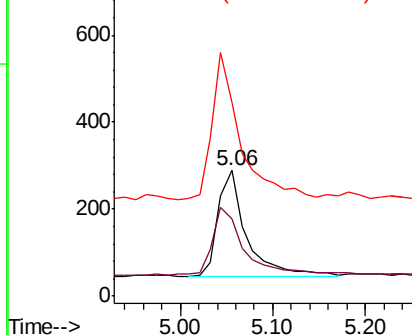

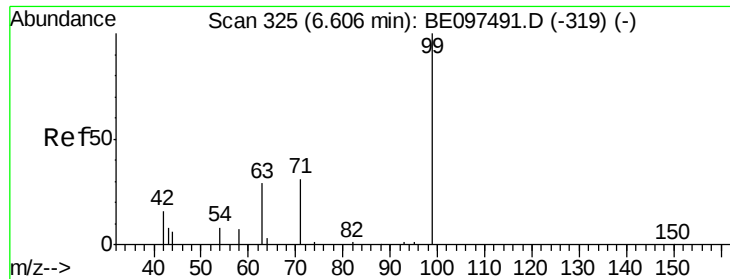

#5

Phenol-d6

Concen: 0.110 ng

RT: 6.60 min Scan# 324

Delta R.T. -0.01 min

Lab File: BE097525.D

Acq: 18 Sep 2018 10:00

Instrument :

BNA_E

ClientSampleId :

BP-TT-AOC22-MW09-20180911


Tgt Ion: 99 Resp: 448

Ion Ratio Lower Upper

99 100

42 23.7 20.2 30.2




71 34.8 28.4 42.6

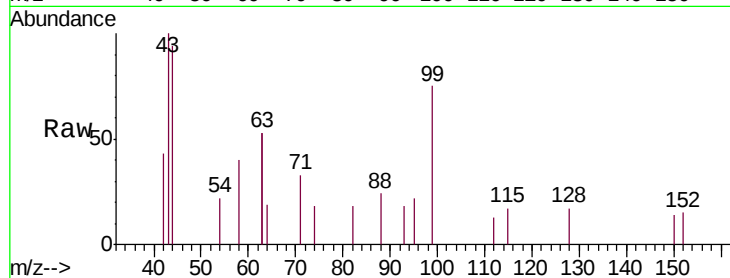

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

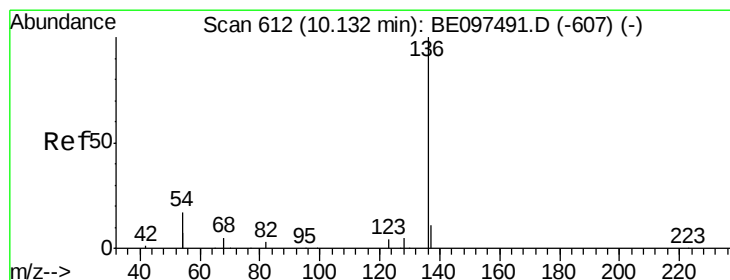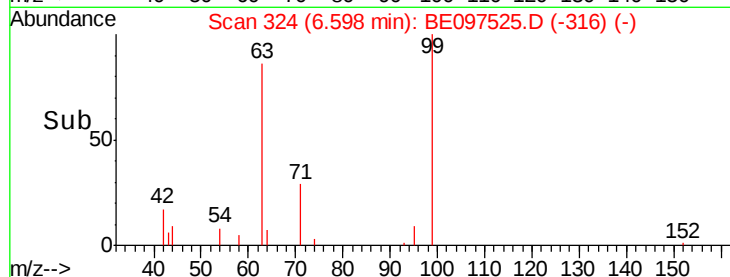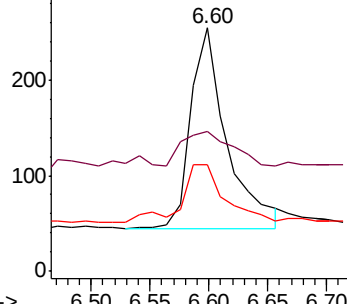

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.13 min Scan# 612

Delta R.T. 0.00 min

Lab File: BE097525.D

Acq: 18 Sep 2018 10:00

Tgt Ion: 136 Resp: 4339


Ion Ratio Lower Upper

136 100

137 12.9 9.5 14.3

54 40.1 29.1 43.7

68 8.8 6.2 9.2


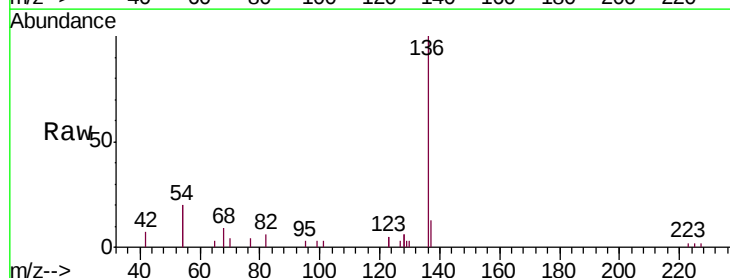



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

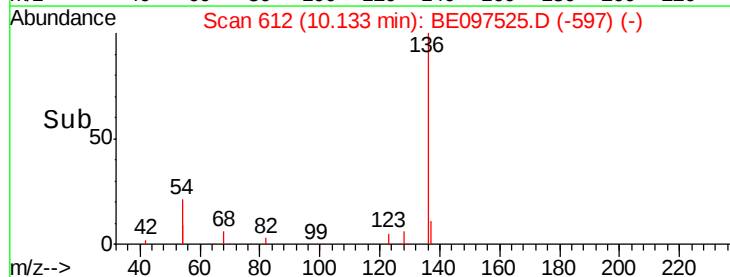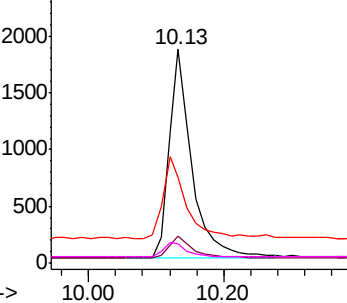

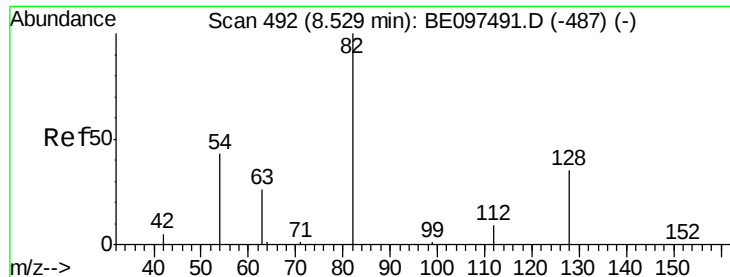

#8

Nitrobenzene-d5

Concen: 0.430 ng

RT: 8.53 min Scan# 492

Delta R.T. 0.00 min

Lab File: BE097525.D

Acq: 18 Sep 2018 10:00

Instrument :

BNA_E

ClientSampleId :

BP-TT-AOC22-MW09-20180911


Tgt Ion: 82 Resp: 1502

Ion Ratio Lower Upper

82 100

128 39.9 24.0 36.0#




54 52.0 40.0 60.0

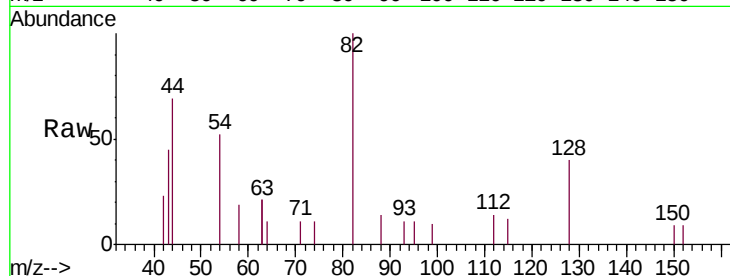

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0

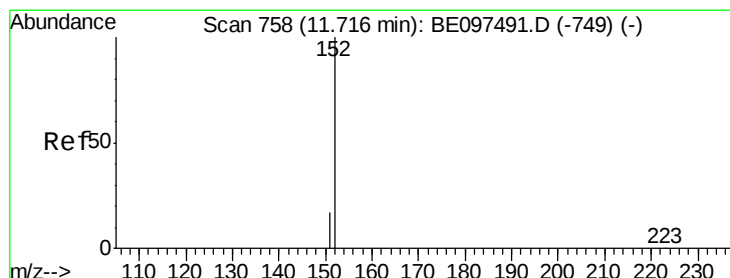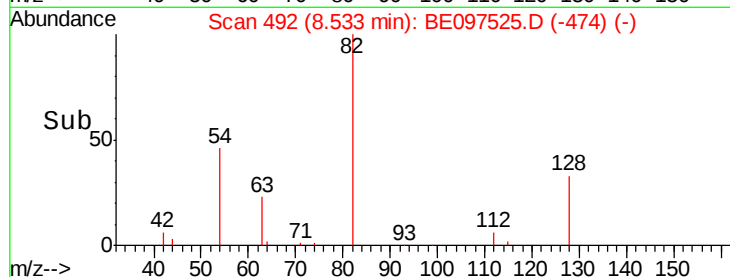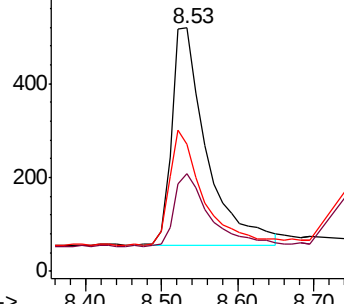

#11

2-Methylnaphthalene-d10

Concen: 0.421 ng

RT: 11.72 min Scan# 759

Delta R.T. 0.00 min

Lab File: BE097525.D


Acq: 18 Sep 2018 10:00

Tgt Ion: 152 Resp: 2610

Ion Ratio Lower Upper



152 100


151 18.8 15.4 23.0

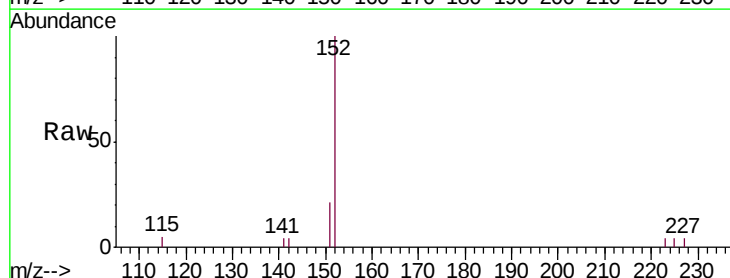

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E



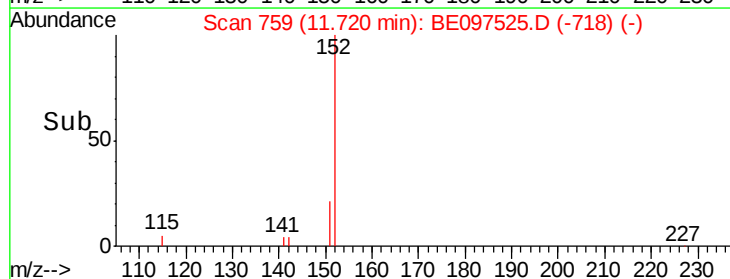
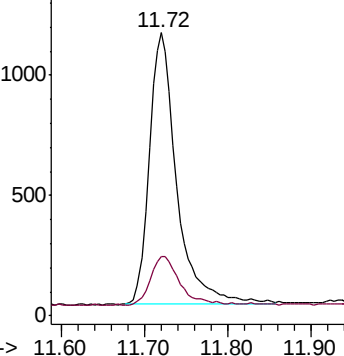


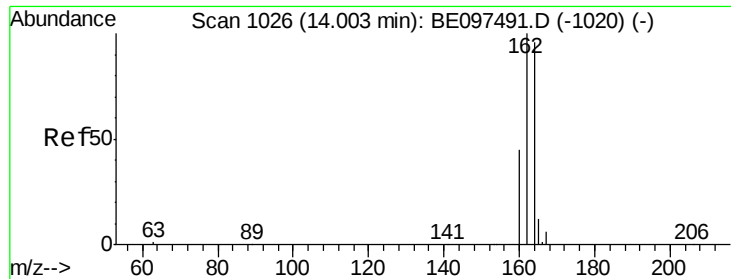

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.00 min Scan# 1026
Delta R.T. -0.00 min
Lab File: BE097525.D
Acq: 18 Sep 2018 10:00




Instrument :
BNA_E
ClientSampleId :
BP-TT-AOC22-MW09-20180911


Tgt Ion:164 Resp: 2612
Ion Ratio Lower Upper
164 100
162 104.0 83.1 124.7
160 49.7 37.1 55.7

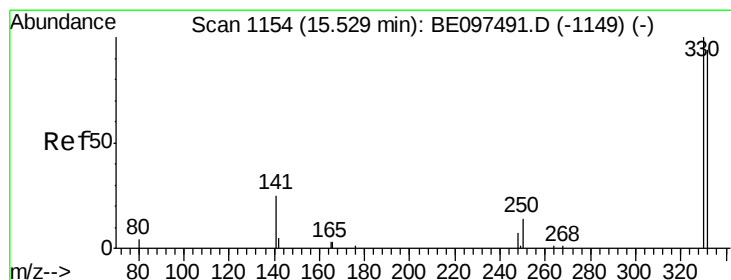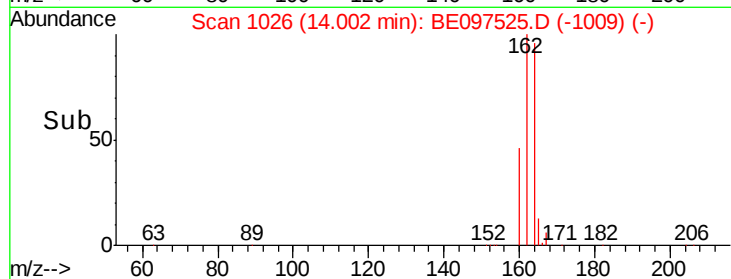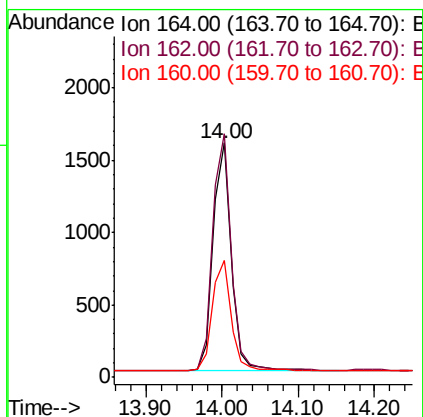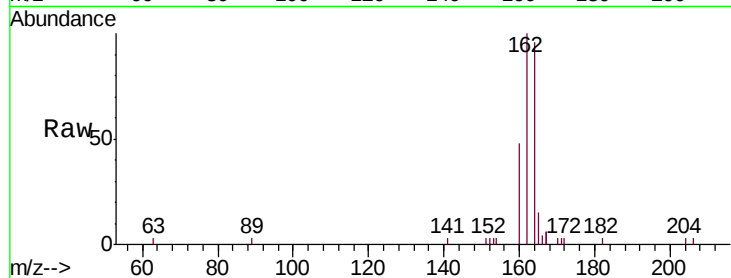

#14
2,4,6-Tribromophenol
Concen: 0.389 ng
RT: 15.52 min Scan# 1153
Delta R.T. -0.01 min
Lab File: BE097525.D
Acq: 18 Sep 2018 10:00

Tgt Ion:330 Resp: 536
Ion Ratio Lower Upper
330 100
332 96.1 152.7 229.1#
141 35.3 33.7 50.5


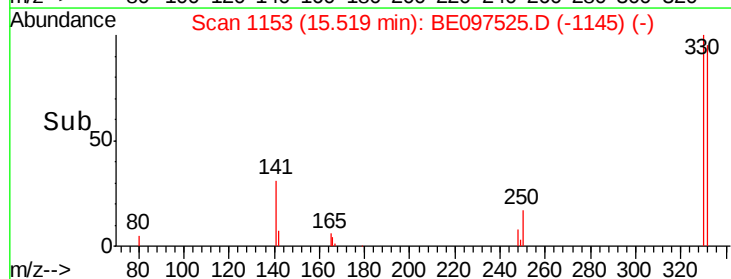
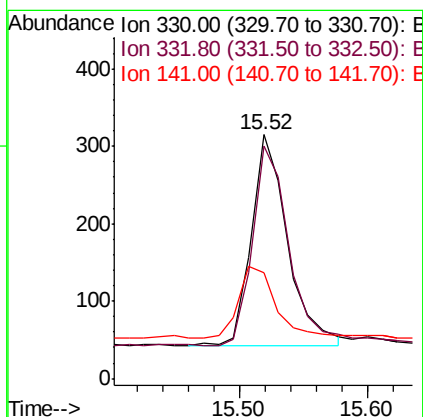
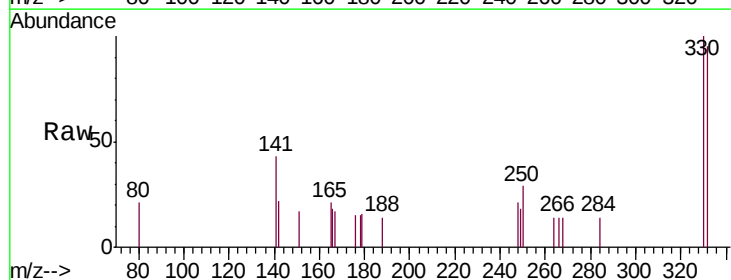


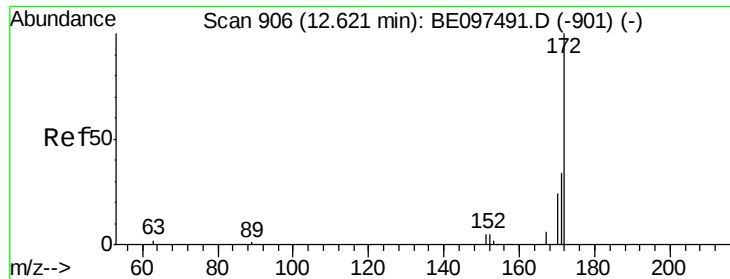

#15
2-Fluorobiphenyl
Concen: 0.550 ng
RT: 12.62 min Scan# 906
Delta R.T. -0.00 min
Lab File: BE097525.D
Acq: 18 Sep 2018 10:00




Instrument :
BNA_E
ClientSampleId :
BP-TT-AOC22-MW09-20180911


Tgt Ion:172 Resp: 5013
Ion Ratio Lower Upper
172 100
171 35.3 29.9 44.9
170 24.6 21.8 32.8

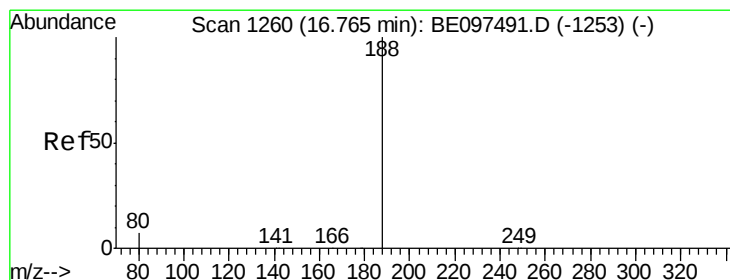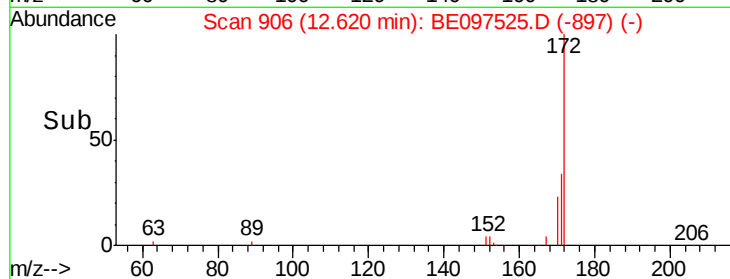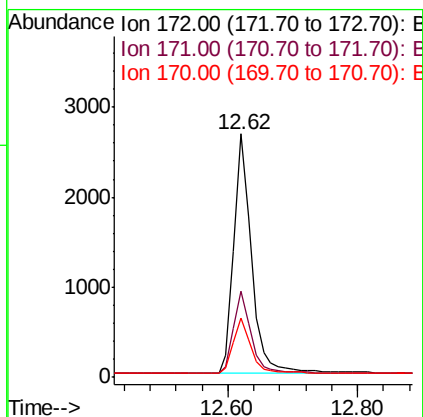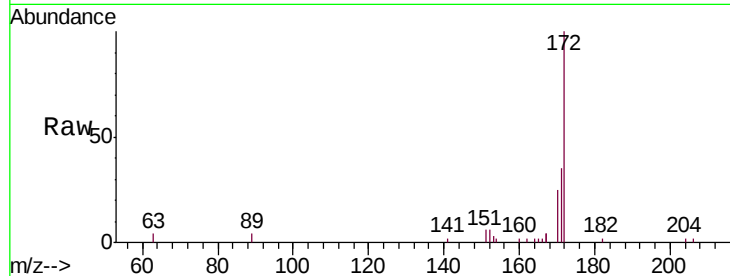

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.75 min Scan# 1259
Delta R.T. -0.01 min
Lab File: BE097525.D
Acq: 18 Sep 2018 10:00

Tgt Ion:188 Resp: 7236
Ion Ratio Lower Upper
188 100
94 0.0 3.9 5.9#
80 14.1 3.6 5.4#

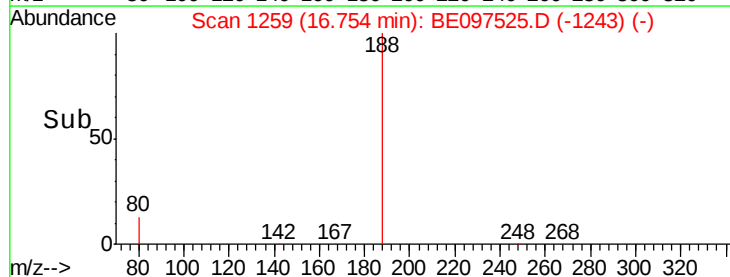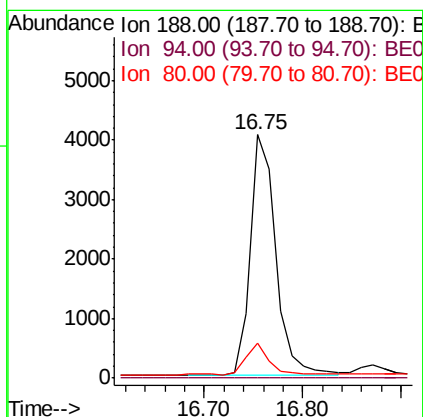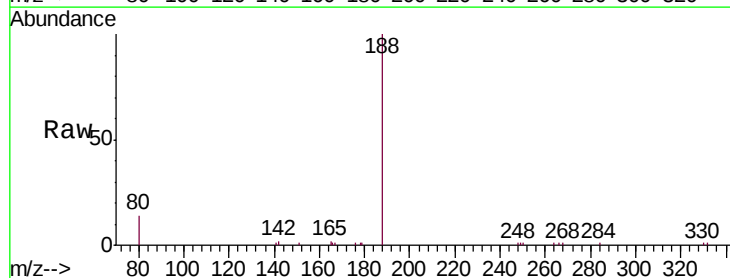

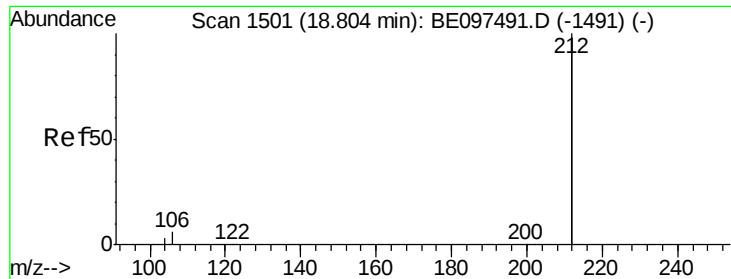

#25

Fluoranthene-d10

Concen: 0.430 ng

RT: 18.80 min Scan# 1500

Delta R.T. -0.00 min

Lab File: BE097525.D

Acq: 18 Sep 2018 10:00

Instrument :

BNA_E

ClientSampleId :

BP-TT-AOC22-MW09-20180911


Tgt Ion:212 Resp: 37372

Ion Ratio Lower Upper

212 100

106 3.1 2.8 4.2




104 1.9 1.6 2.4

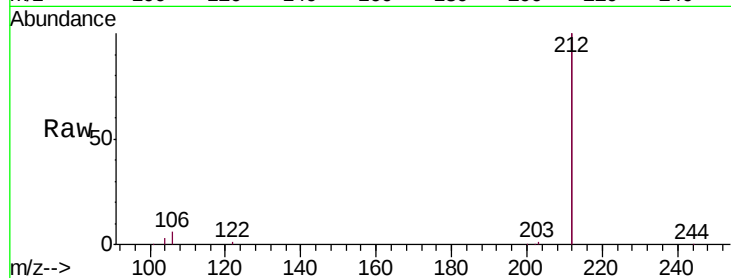

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

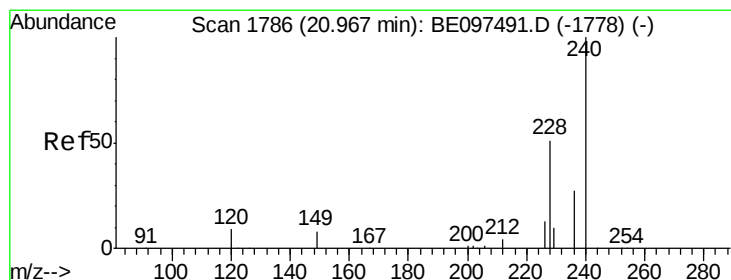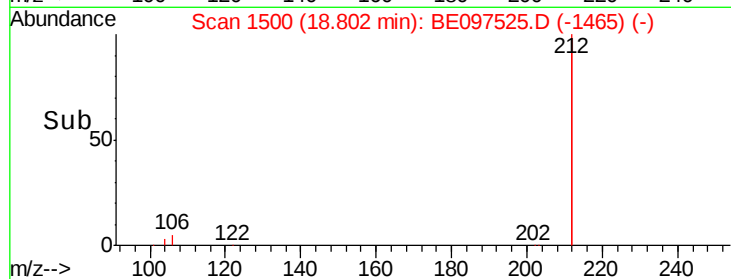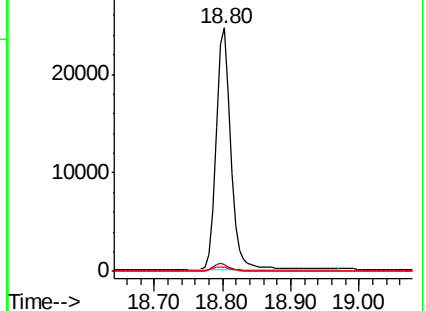

#27

Chrysene-d12

Concen: 0.400 ng

RT: 20.97 min Scan# 1785

Delta R.T. 0.00 min

Lab File: BE097525.D

Acq: 18 Sep 2018 10:00


Tgt Ion:240 Resp: 8844

Ion Ratio Lower Upper

240 100

120 9.0 5.5 8.3#



236 27.6 20.7 31.1

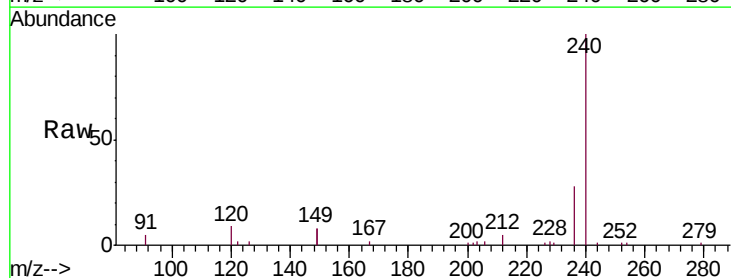


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

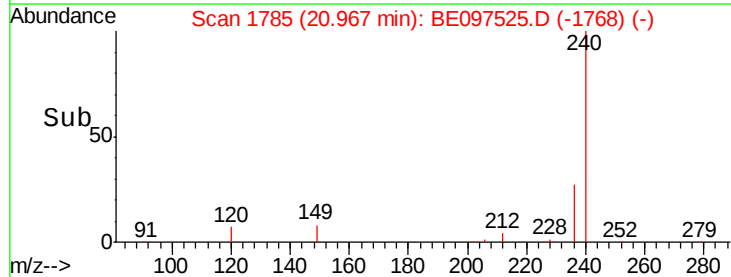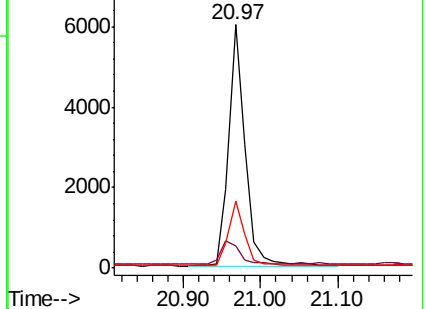

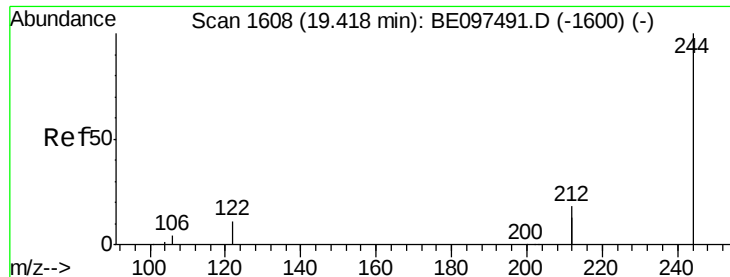

#29

Terphenyl-d14

Concen: 0.494 ng

RT: 19.41 min Scan# 1606

Delta R.T. -0.01 min

Lab File: BE097525.D

Acq: 18 Sep 2018 10:00

Instrument :

BNA_E

ClientSampleId :

BP-TT-AOC22-MW09-20180911


Tgt Ion:244 Resp: 8362

Ion Ratio Lower Upper

244 100

212 33.8 25.4 38.0




122 12.5 8.1 12.1#

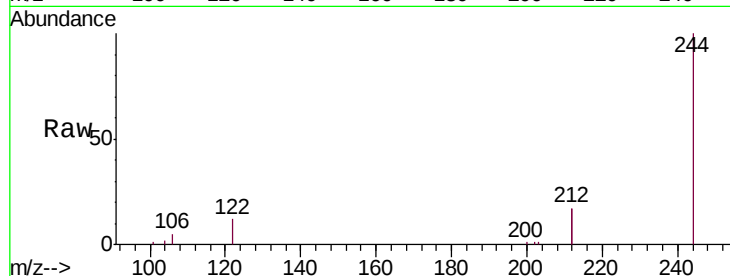

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

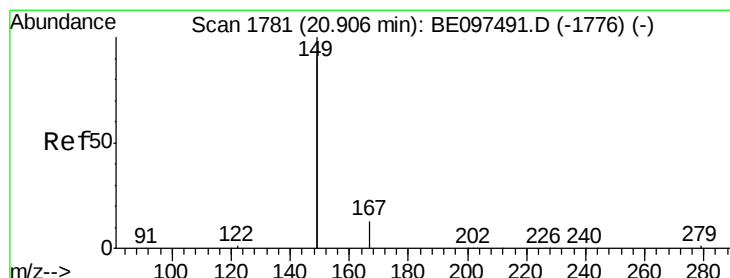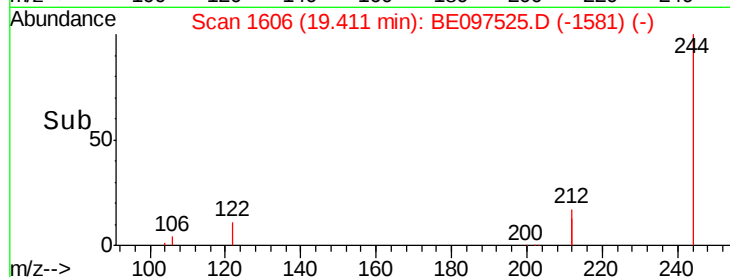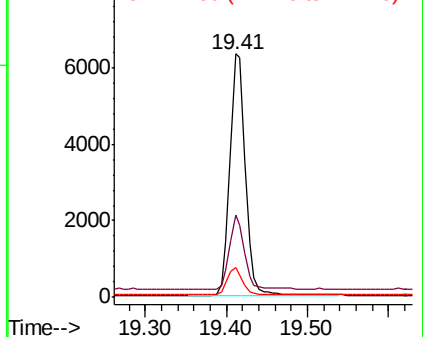

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.113 ng

RT: 20.91 min Scan# 1780

Delta R.T. 0.00 min

Lab File: BE097525.D

Acq: 18 Sep 2018 10:00


Tgt Ion:149 Resp: 5574

Ion Ratio Lower Upper

149 100

167 6.6 5.4 8.0



279 1.1 0.7 1.1



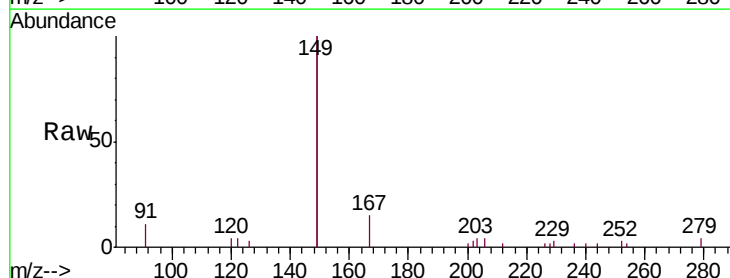


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

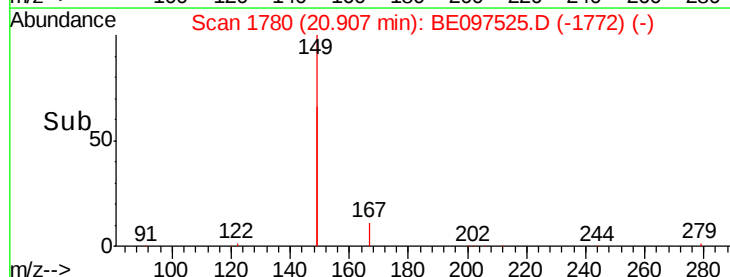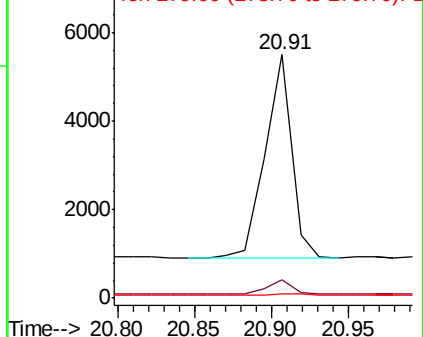

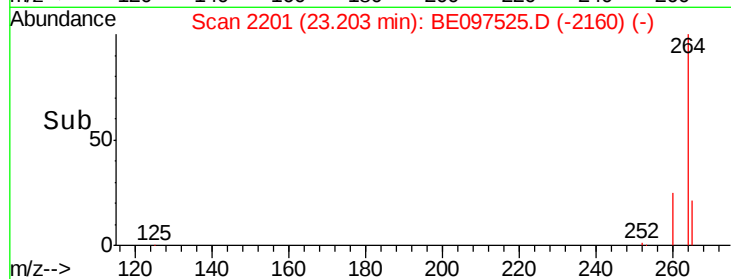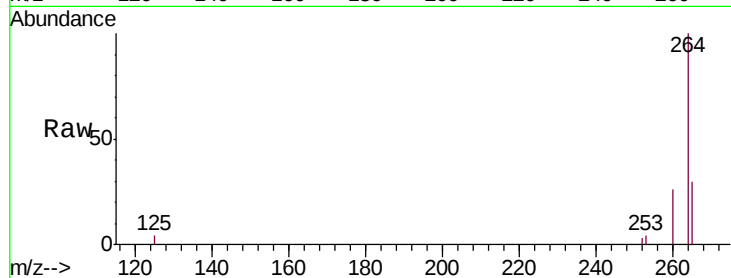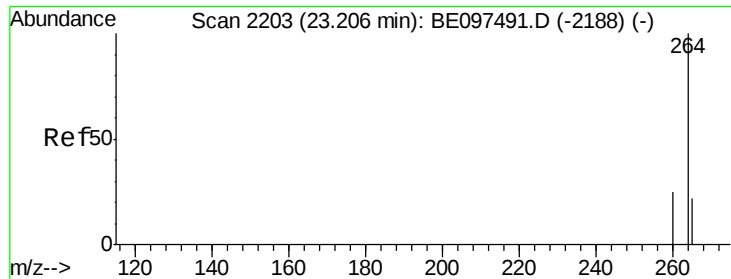

#34
Perylene-d12
Concen: 0.400 ng
RT: 23.20 min Scan# 2201
Delta R.T. -0.00 min
Lab File: BE097525.D
Acq: 18 Sep 2018 10:00

Instrument :
BNA_E
ClientSampleId :
BP-TT-AOC22-MW09-20180911

Tgt Ion: 264 Resp: 8901
Ion Ratio Lower Upper
264 100
260 25.8 20.5 30.7
265 30.0 22.8 34.2

