

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE091718\
 Data File : BE097528.D
 Acq On : 18 Sep 2018 11:50
 Operator : SJ/JU
 Sample : J4913-07
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BPSI-TT-MW303D-20180912

Quant Time: Sep 18 13:15:42 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 17 18:57:11 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	948	0.40	ng	-0.01
7) Naphthalene-d8	10.13	136	4345	0.40	ng	0.00
13) Acenaphthene-d10	14.00	164	2613	0.40	ng	0.00
19) Phenanthrene-d10	16.75	188	7366	0.40	ng	-0.01
27) Chrysene-d12	20.97	240	8900	0.40	ng	0.00
34) Perylene-d12	23.21	264	8851	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.05	112	536	0.17	ng	0.00
5) Phenol-d6	6.59	99	442	0.11	ng	-0.01
8) Nitrobenzene-d5	8.53	82	1517	0.43	ng	0.00
11) 2-Methylnaphthalene-d10	11.72	152	2638	0.42	ng	0.00
14) 2,4,6-Tribromophenol	15.52	330	571	0.41	ng	-0.01
15) 2-Fluorobiphenyl	12.62	172	4841	0.53	ng	0.00
25) Fluoranthene-d10	18.80	212	37705	0.43	ng	0.00
29) Terphenyl-d14	19.41	244	8157	0.48	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.08	88	613	0.374	ng	Qvalue # 89
32) Bis(2-ethylhexyl)phthalate	20.91	149	69800	1.403	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE091718\
Data File : BE097528.D
Acq On : 18 Sep 2018 11:50
Operator : SJ/JU
Sample : J4913-07
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BPSI-TT-MW303D-20180912

Quant Time: Sep 18 13:15:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 17 18:57:11 2018
Response via : Initial Calibration




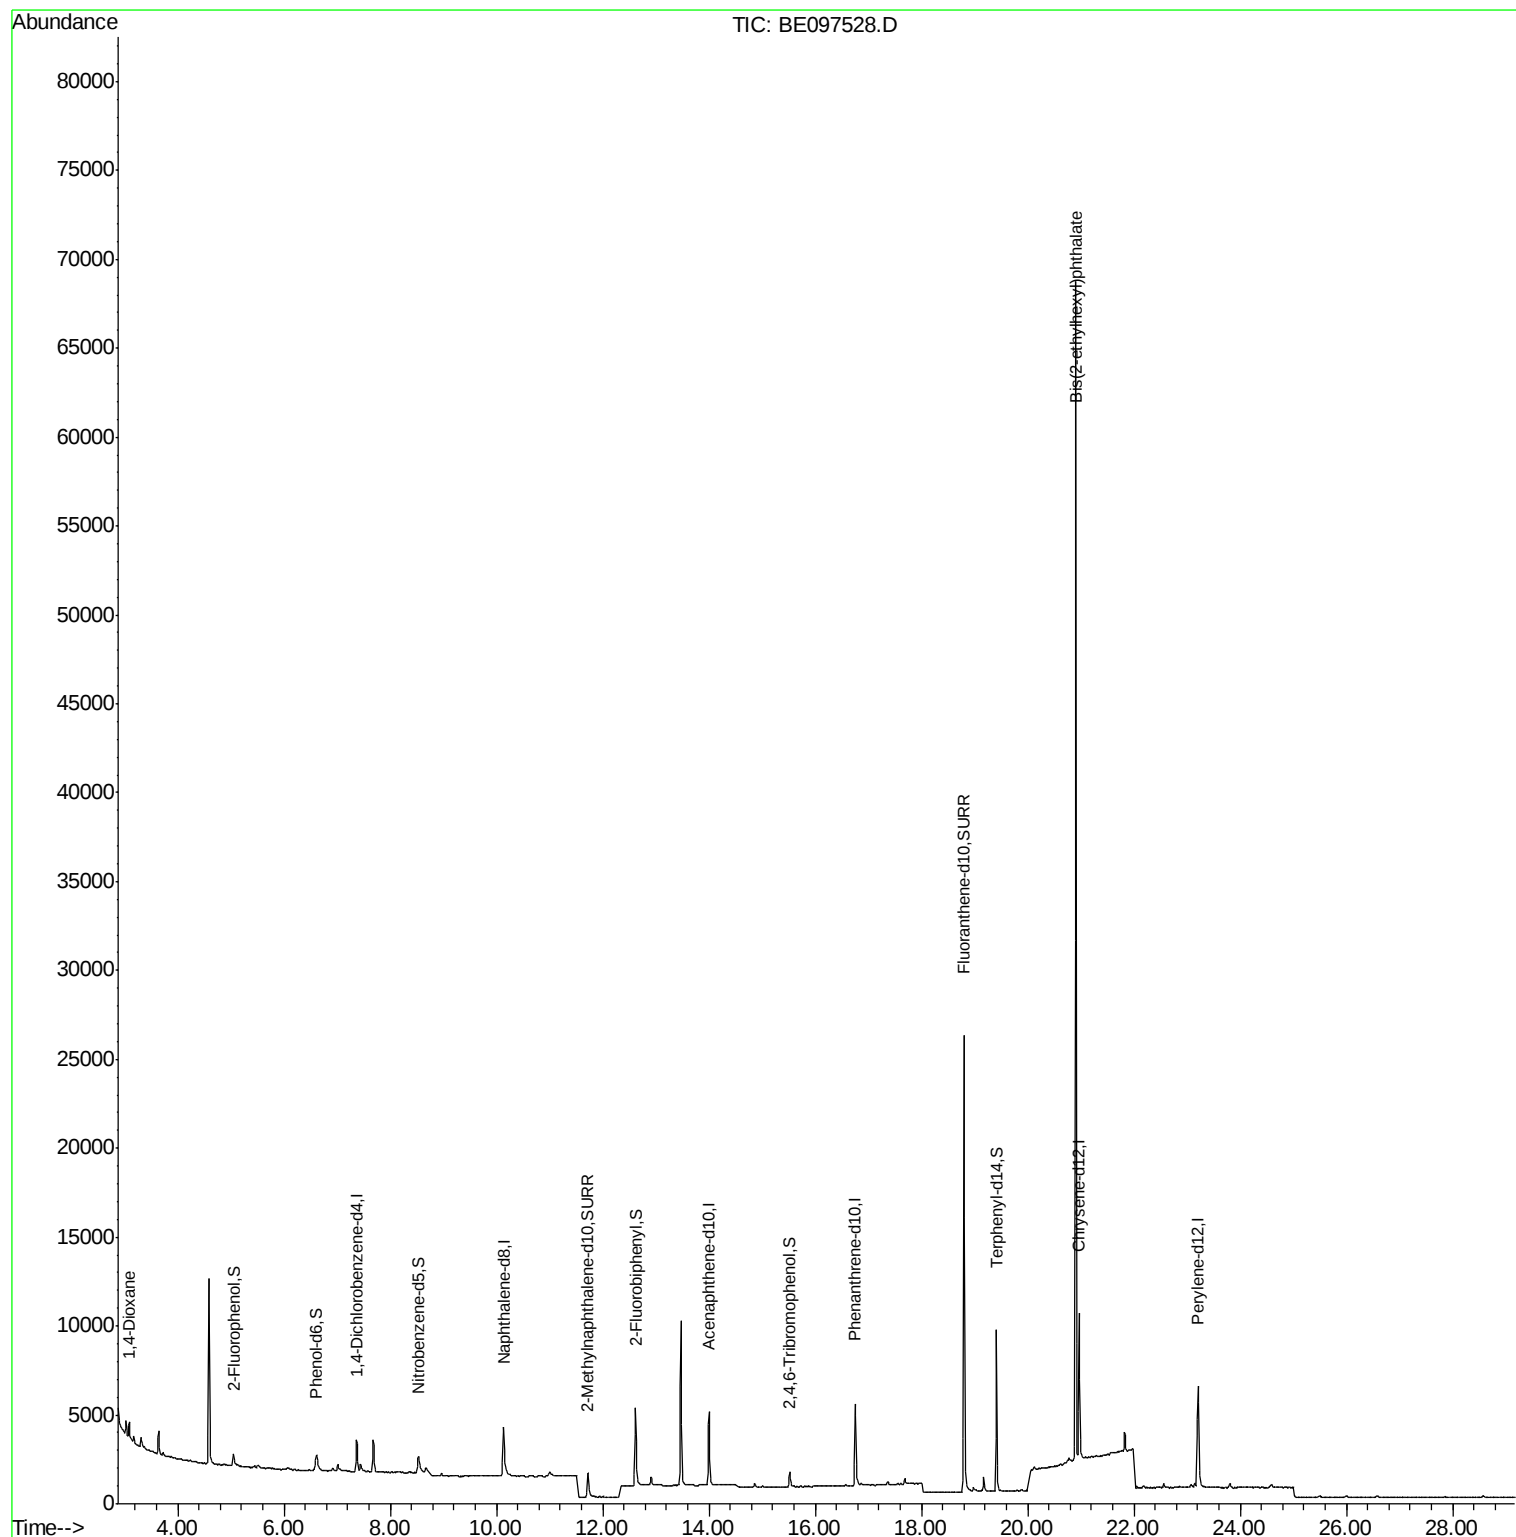


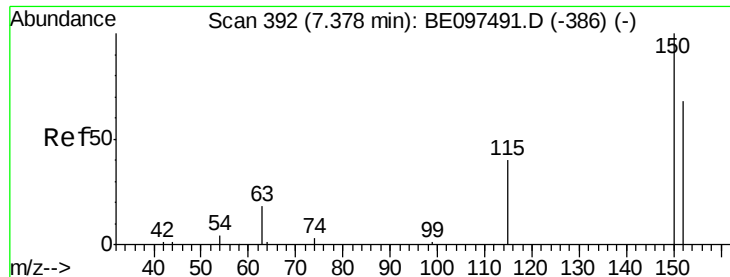

#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.37 min Scan# 391
 Delta R.T. -0.01 min
 Lab File: BE097528.D
 Acq: 18 Sep 2018 11:50




Instrument :
 BNA_E
 ClientSampleId :
 BPSI-TT-MW303D-20180912


Tgt Ion: 152 Resp: 948
 Ion Ratio Lower Upper
 152 100
 150 158.8 117.2 175.8
 115 81.4 57.0 85.6

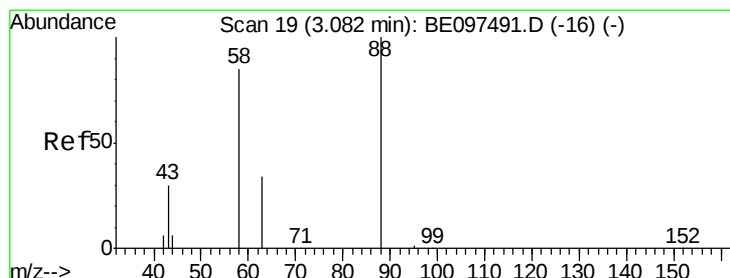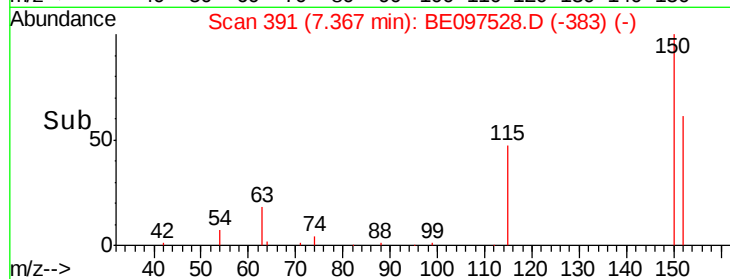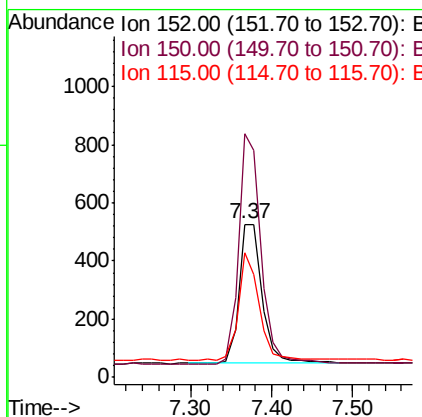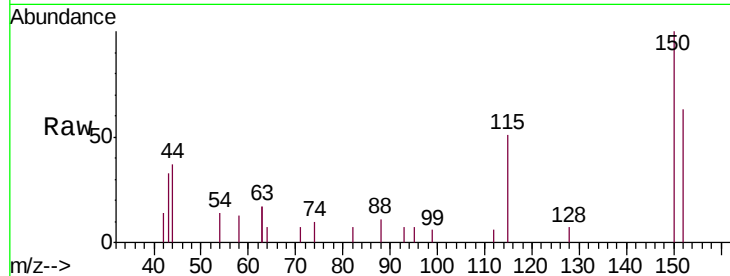

#2
 1,4-Dioxane
 Concen: 0.374 ng
 RT: 3.08 min Scan# 19
 Delta R.T. 0.00 min
 Lab File: BE097528.D
 Acq: 18 Sep 2018 11:50

Tgt Ion: 88 Resp: 613
 Ion Ratio Lower Upper
 88 100
 58 83.0 63.2 94.8
 43 66.1 41.2 61.8#

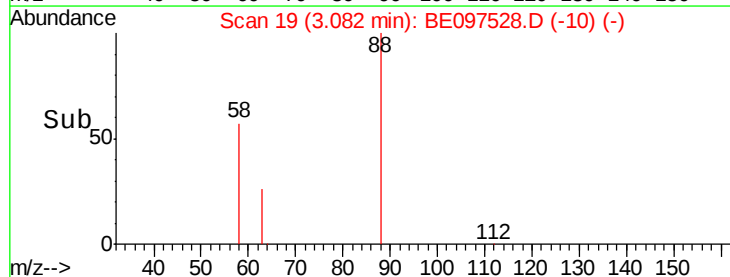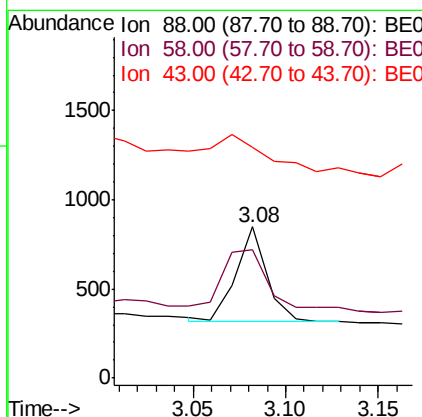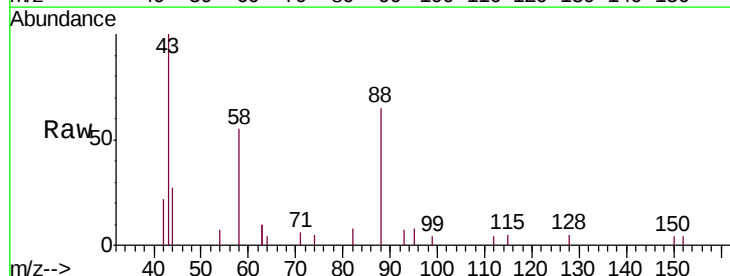

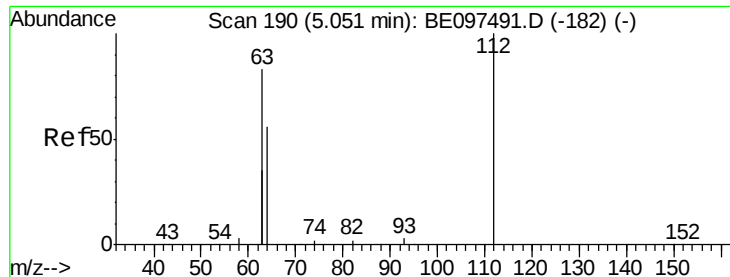

#4

2-Fluorophenol

Concen: 0.167 ng

RT: 5.05 min Scan# 190

Delta R.T. 0.00 min

Lab File: BE097528.D

Acq: 18 Sep 2018 11:50

Instrument :

BNA_E

ClientSampleId :

BPSI-TT-MW303D-20180912


Tgt Ion: 112 Resp: 536

Ion Ratio Lower Upper

112 100

64 68.7 60.1 90.1




63 140.3 116.8 175.2

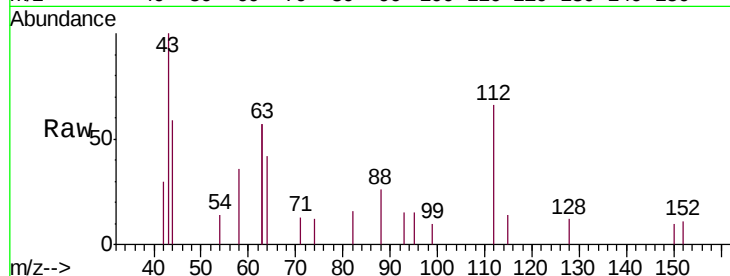

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

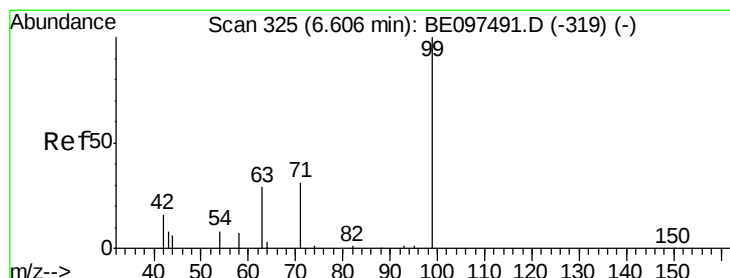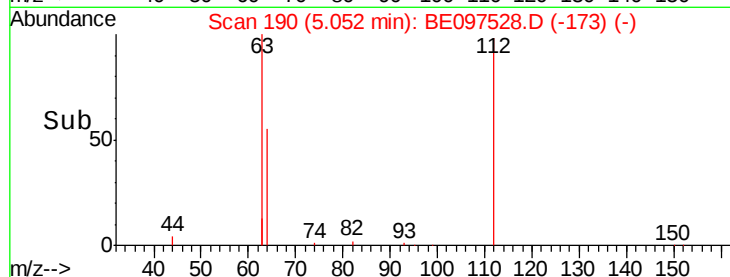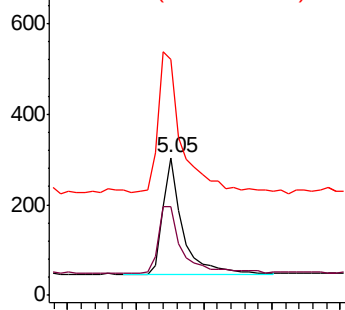

#5

Phenol-d6

Concen: 0.108 ng

RT: 6.59 min Scan# 324

Delta R.T. -0.01 min

Lab File: BE097528.D

Acq: 18 Sep 2018 11:50


Tgt Ion: 99 Resp: 442

Ion Ratio Lower Upper

99 100

42 30.3 20.2 30.2#



71 34.8 28.4 42.6

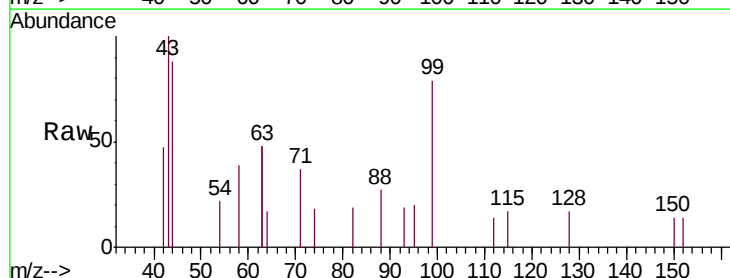


Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

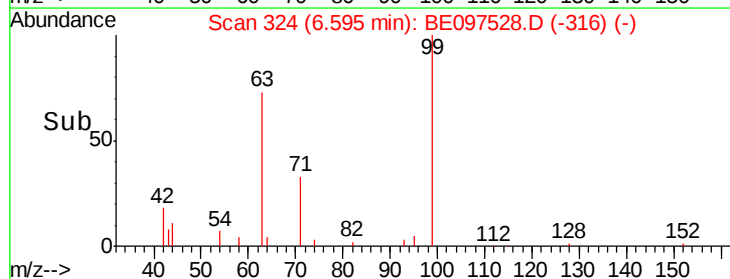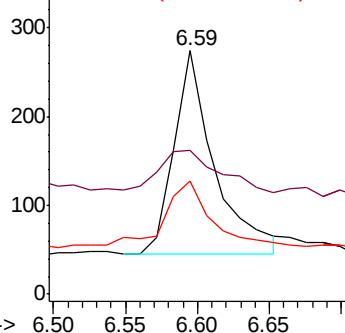

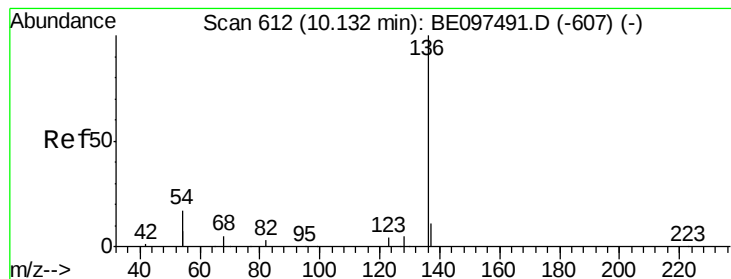

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.13 min Scan# 612

Delta R.T. 0.00 min

Lab File: BE097528.D

Acq: 18 Sep 2018 11:50

Instrument :

BNA_E

ClientSampleId :

BPSI-TT-MW303D-20180912

Tgt Ion: 136 Resp: 4345


Ion Ratio Lower Upper

136 100

137 13.0 9.5 14.3

54 38.2 29.1 43.7

68 8.4 6.2 9.2



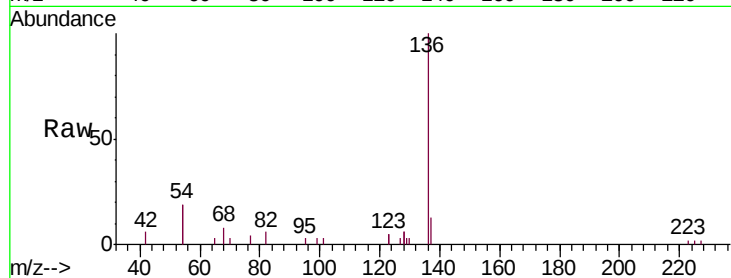


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

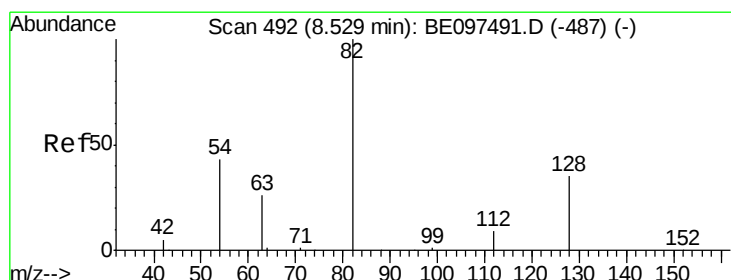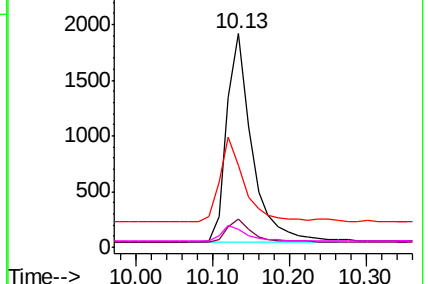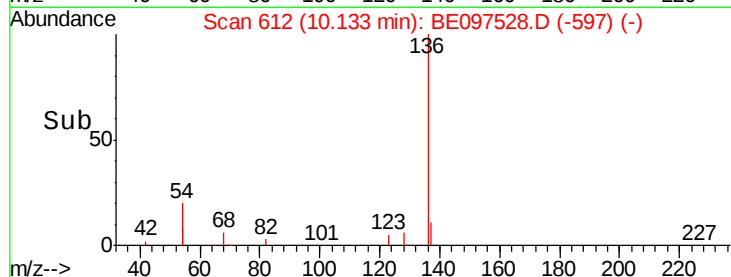

#8

Nitrobenzene-d5

Concen: 0.434 ng

RT: 8.53 min Scan# 492

Delta R.T. 0.00 min

Lab File: BE097528.D

Acq: 18 Sep 2018 11:50


Tgt Ion: 82 Resp: 1517

Ion Ratio Lower Upper

82 100

128 42.1 24.0 36.0#



54 53.1 40.0 60.0

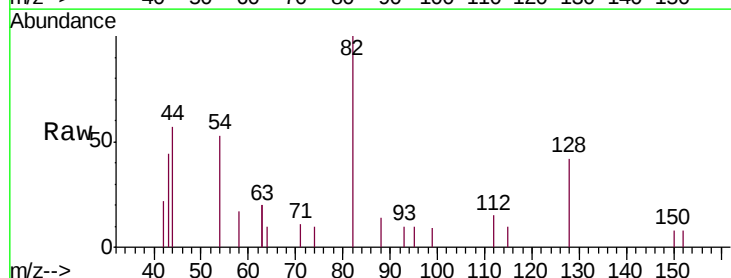


Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0

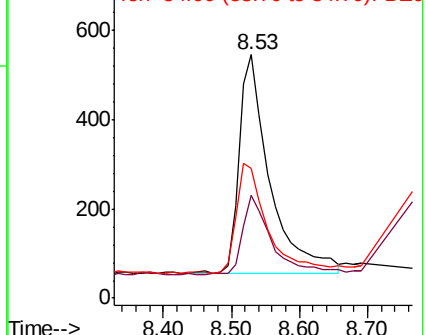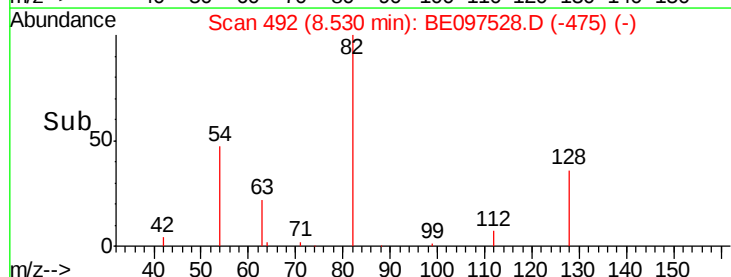

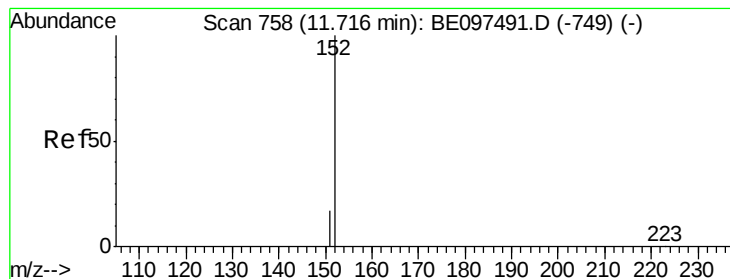

#11

2-Methylnaphthalene-d10

Concen: 0.425 ng

RT: 11.72 min Scan# 758

Delta R.T. 0.00 min

Lab File: BE097528.D

Acq: 18 Sep 2018 11:50

Instrument :

BNA_E

ClientSampleId :


BPSI-TT-MW303D-20180912

Tgt Ion:152 Resp: 2638

Ion Ratio Lower Upper

152 100

151 18.4 15.4 23.0

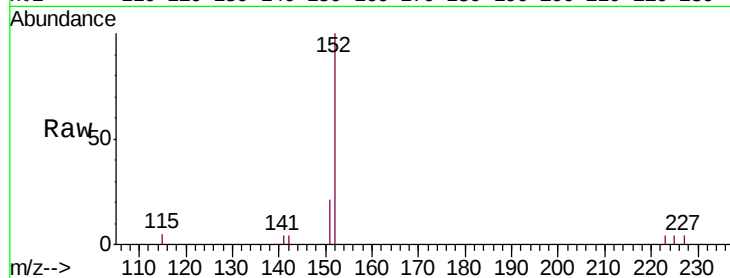

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E



11.72

1000

500

0

Time-->

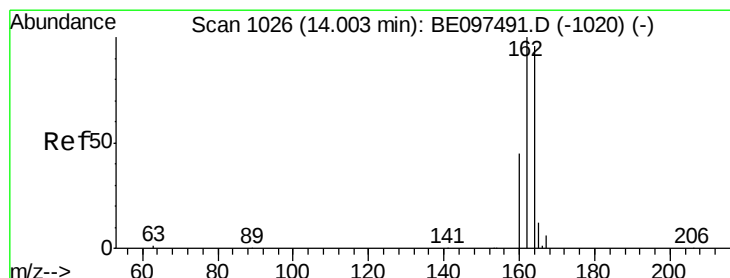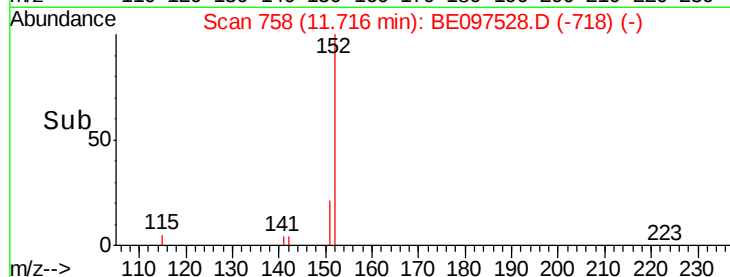

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.00 min Scan# 1026

Delta R.T. -0.00 min

Lab File: BE097528.D

Acq: 18 Sep 2018 11:50


Tgt Ion:164 Resp: 2613

Ion Ratio Lower Upper

164 100

162 104.0 83.1 124.7

160 48.6 37.1 55.7

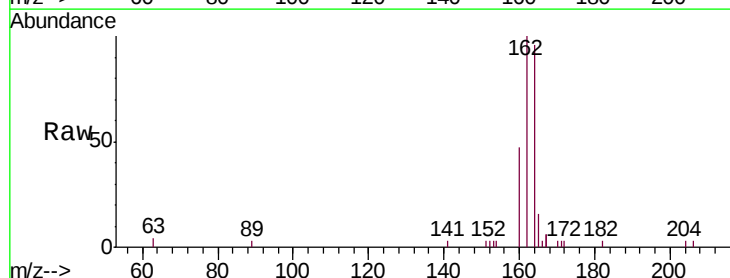

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

14.00

2000


1500


1000

500

0

Time-->




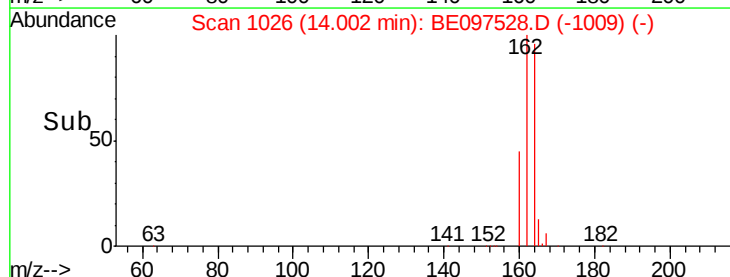


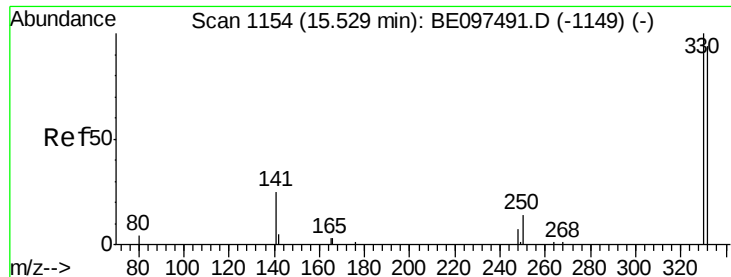

#14
 2,4,6-Tribromophenol
 Concen: 0.414 ng
 RT: 15.52 min Scan# 1153
 Delta R.T. -0.01 min
 Lab File: BE097528.D
 Acq: 18 Sep 2018 11:50




Instrument :
 BNA_E
 ClientSampleId :
 BPSI-TT-MW303D-20180912


Tgt Ion: 330 Resp: 571
 Ion Ratio Lower Upper
 330 100
 332 99.5 152.7 229.1#
 141 35.2 33.7 50.5

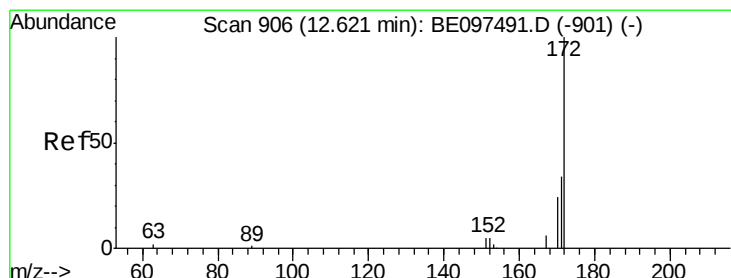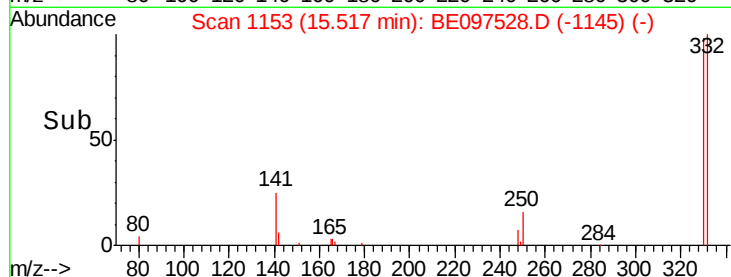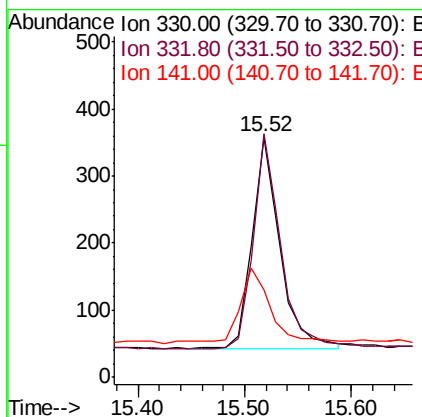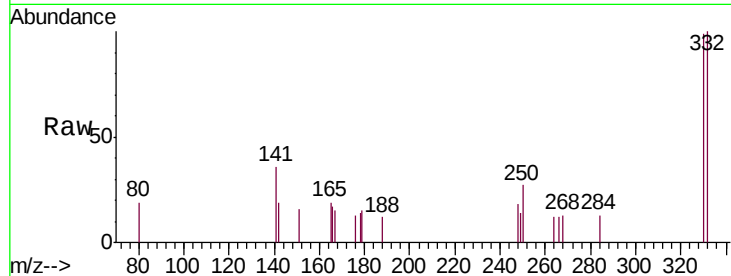

#15
 2-Fluorobiphenyl
 Concen: 0.530 ng
 RT: 12.62 min Scan# 906
 Delta R.T. -0.00 min
 Lab File: BE097528.D
 Acq: 18 Sep 2018 11:50

Tgt Ion: 172 Resp: 4841
 Ion Ratio Lower Upper
 172 100
 171 35.3 29.9 44.9
 170 24.0 21.8 32.8


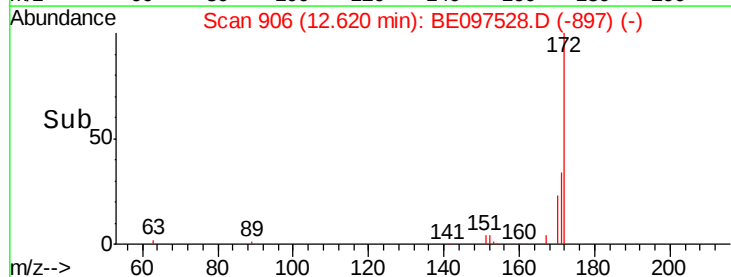
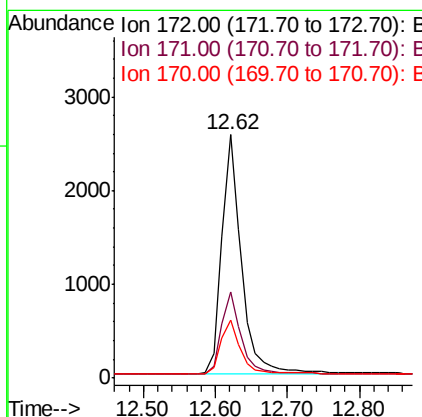
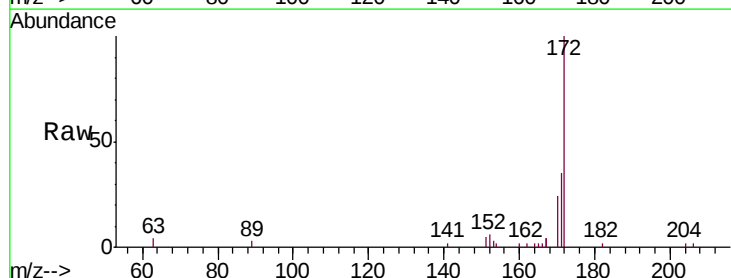


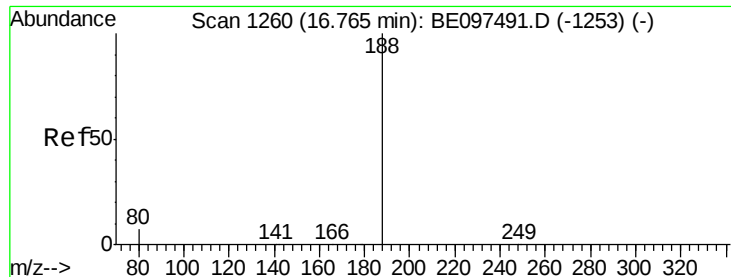

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.75 min Scan# 1259
Delta R.T. -0.01 min
Lab File: BE097528.D
Acq: 18 Sep 2018 11:50




Instrument :
BNA_E
ClientSampleId :
BPSI-TT-MW303D-20180912


Tgt Ion:188 Resp: 7366
Ion Ratio Lower Upper
188 100
94 0.0 3.9 5.9#
80 14.6 3.6 5.4#

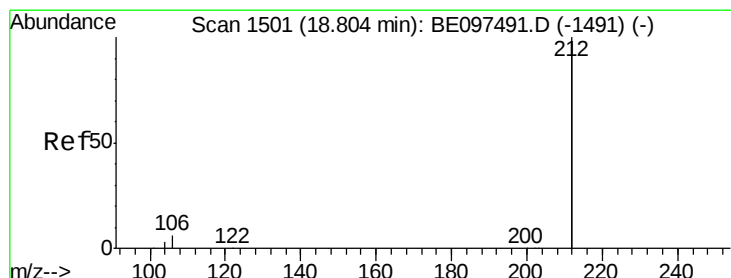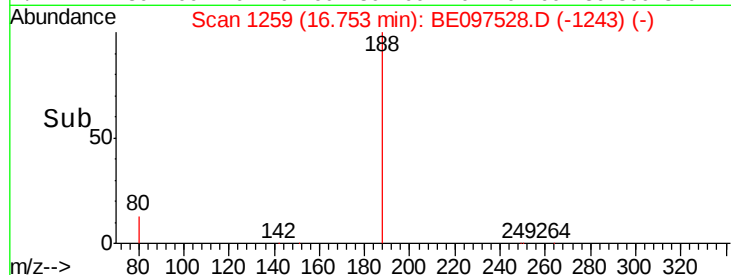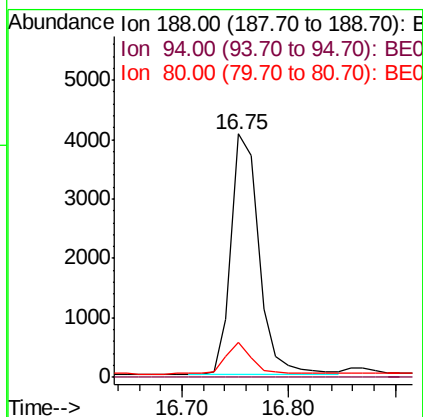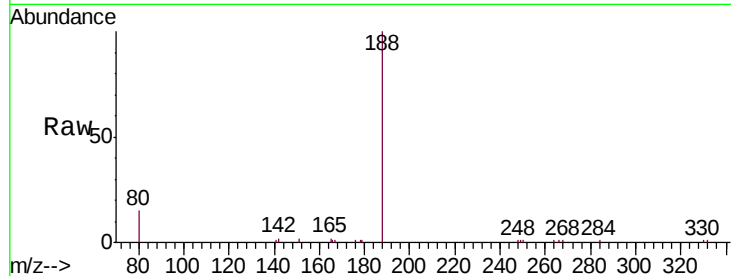

#25
Fluoranthene-d10
Concen: 0.426 ng
RT: 18.80 min Scan# 1500
Delta R.T. -0.01 min
Lab File: BE097528.D
Acq: 18 Sep 2018 11:50

Tgt Ion:212 Resp: 37705
Ion Ratio Lower Upper
212 100
106 3.1 2.8 4.2
104 1.7 1.6 2.4

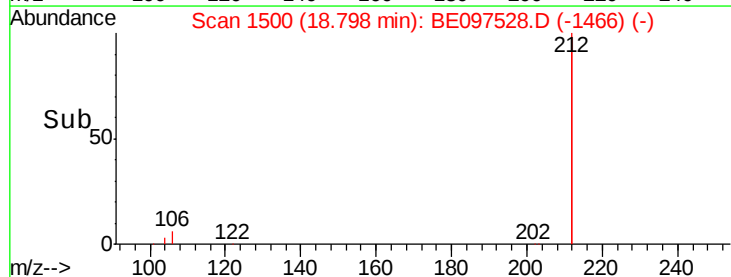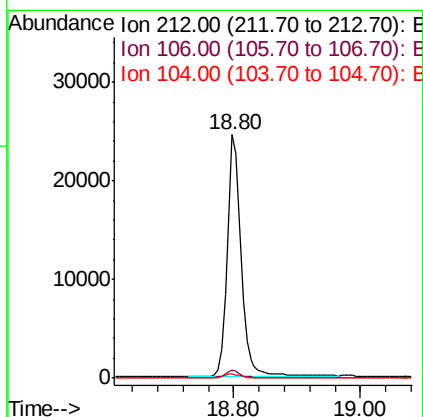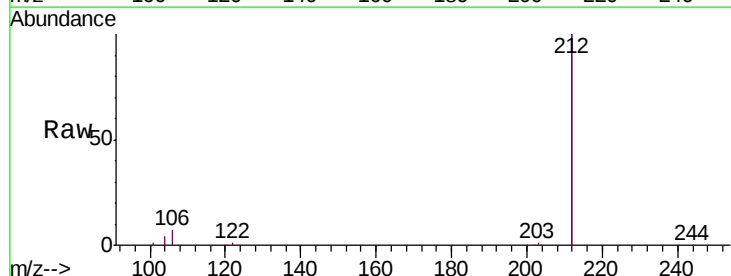

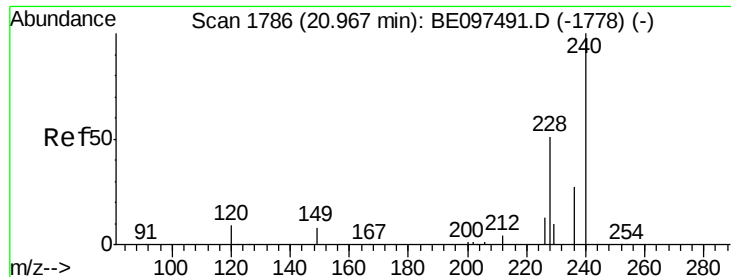

#27

Chrysene-d12

Concen: 0.400 ng

RT: 20.97 min Scan# 1786

Delta R.T. 0.00 min

Lab File: BE097528.D

Acq: 18 Sep 2018 11:50

Instrument :

BNA_E

ClientSampleId :

BPSI-TT-MW303D-20180912


Tgt Ion:240 Resp: 8900

Ion Ratio Lower Upper

240 100

120 10.0 5.5 8.3#




236 28.5 20.7 31.1

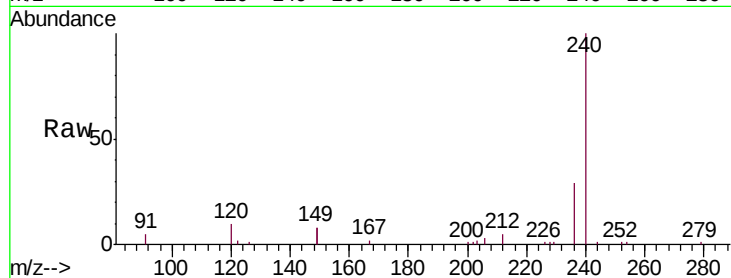

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

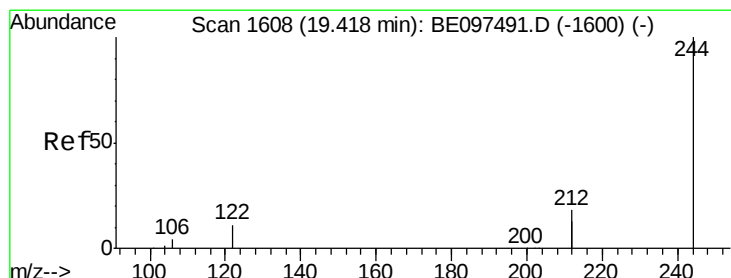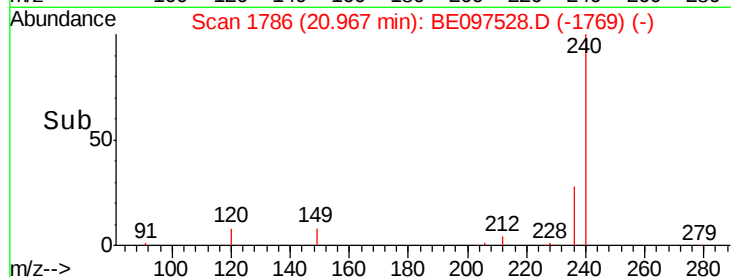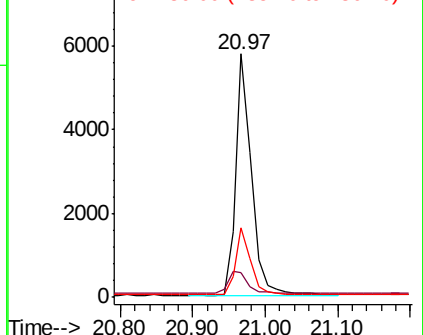

#29

Terphenyl-d14

Concen: 0.479 ng

RT: 19.41 min Scan# 1607

Delta R.T. -0.01 min

Lab File: BE097528.D

Acq: 18 Sep 2018 11:50


Tgt Ion:244 Resp: 8157

Ion Ratio Lower Upper

244 100

212 32.5 25.4 38.0



122 11.3 8.1 12.1

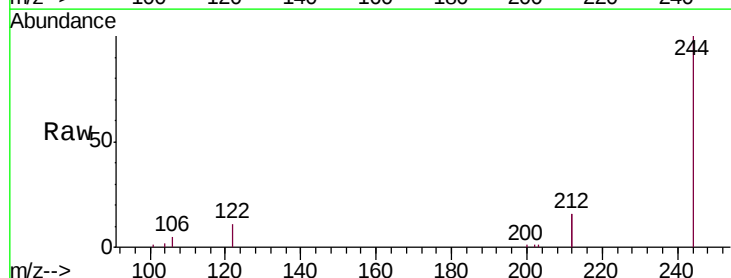


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E



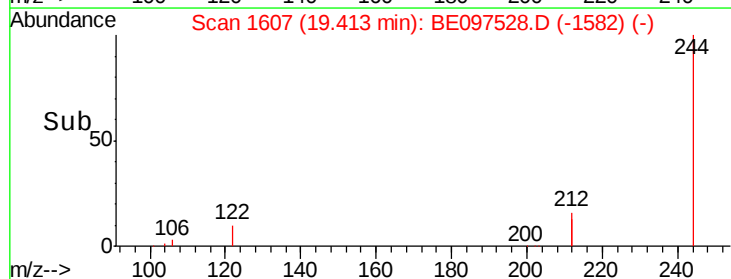
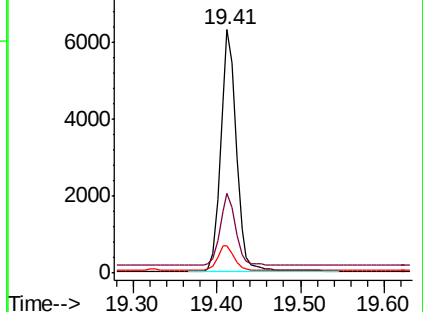


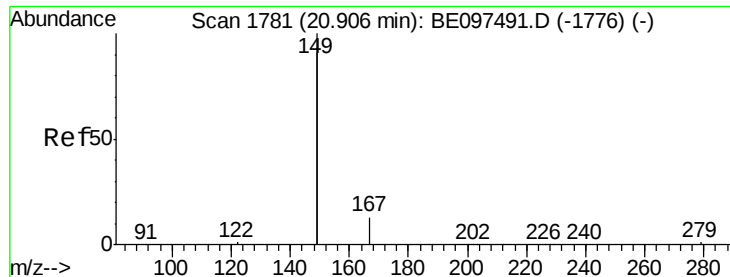

#32
 Bis(2-ethylhexyl)phthalate
 Concen: 1.403 ng
 RT: 20.91 min Scan# 1781
 Delta R.T. 0.00 min
 Lab File: BE097528.D
 Acq: 18 Sep 2018 11:50

Instrument :
 BNA_E
 ClientSampleId :
 BPSI-TT-MW303D-20180912

Tgt Ion:149 Resp: 69800
 Ion Ratio Lower Upper
 149 100
 167 6.8 5.4 8.0
 279 1.1 0.7 1.1

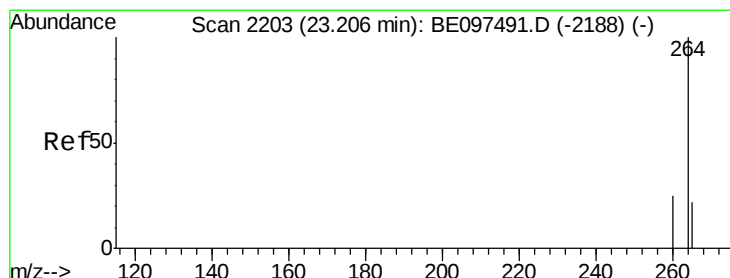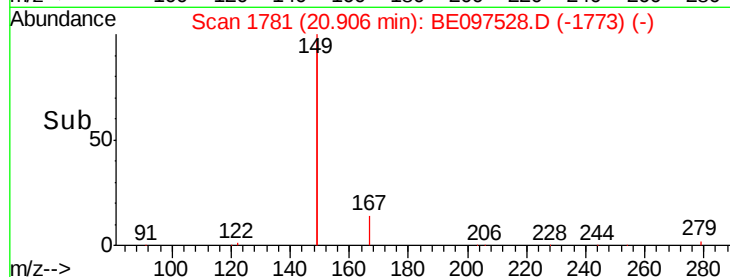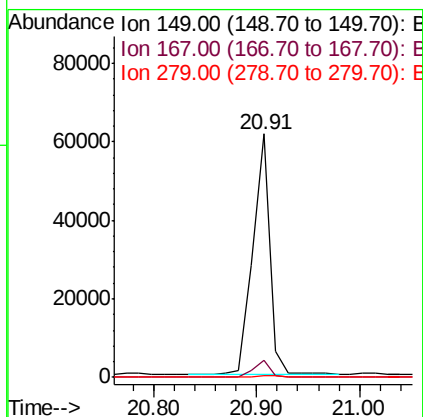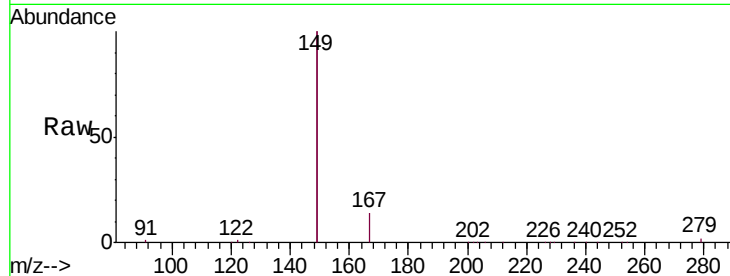

#34
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.21 min Scan# 2203
 Delta R.T. 0.00 min
 Lab File: BE097528.D
 Acq: 18 Sep 2018 11:50

Tgt Ion:264 Resp: 8851
 Ion Ratio Lower Upper
 264 100
 260 25.8 20.5 30.7
 265 31.4 22.8 34.2

