


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE091718\
Data File : BE097488.D
Acq On : 17 Sep 2018 9:27
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091718.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Sep 17 18:57:11 2018

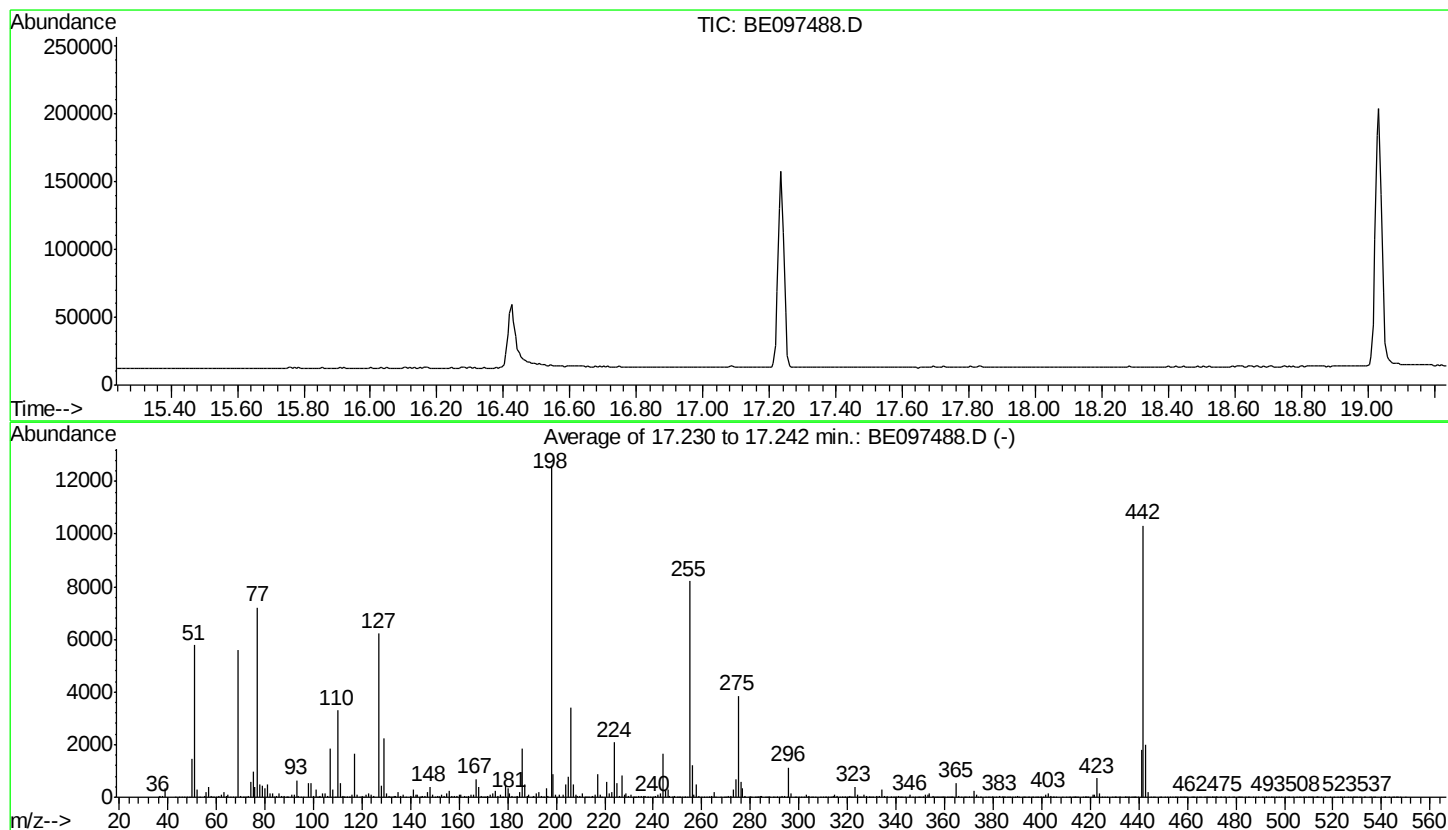

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.9	5787	PASS
68	69	0.00	2	0.4	23	PASS
69	198	0.00	100	44.5	5603	PASS
70	69	0.00	2	0.6	34	PASS
127	198	10	80	49.3	6217	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	12602	PASS
199	198	5	9	7.1	890	PASS
275	198	10	60	30.6	3862	PASS
365	198	1	100	4.3	544	PASS
441	198	0.01	100	14.4	1809	PASS
442	198	50	100	81.9	10327	PASS
443	442	15	24	19.2	1984	PASS