


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE091718\
 Data File : BE097496.D
 Acq On : 17 Sep 2018 15:13
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 17 18:57:11 2018

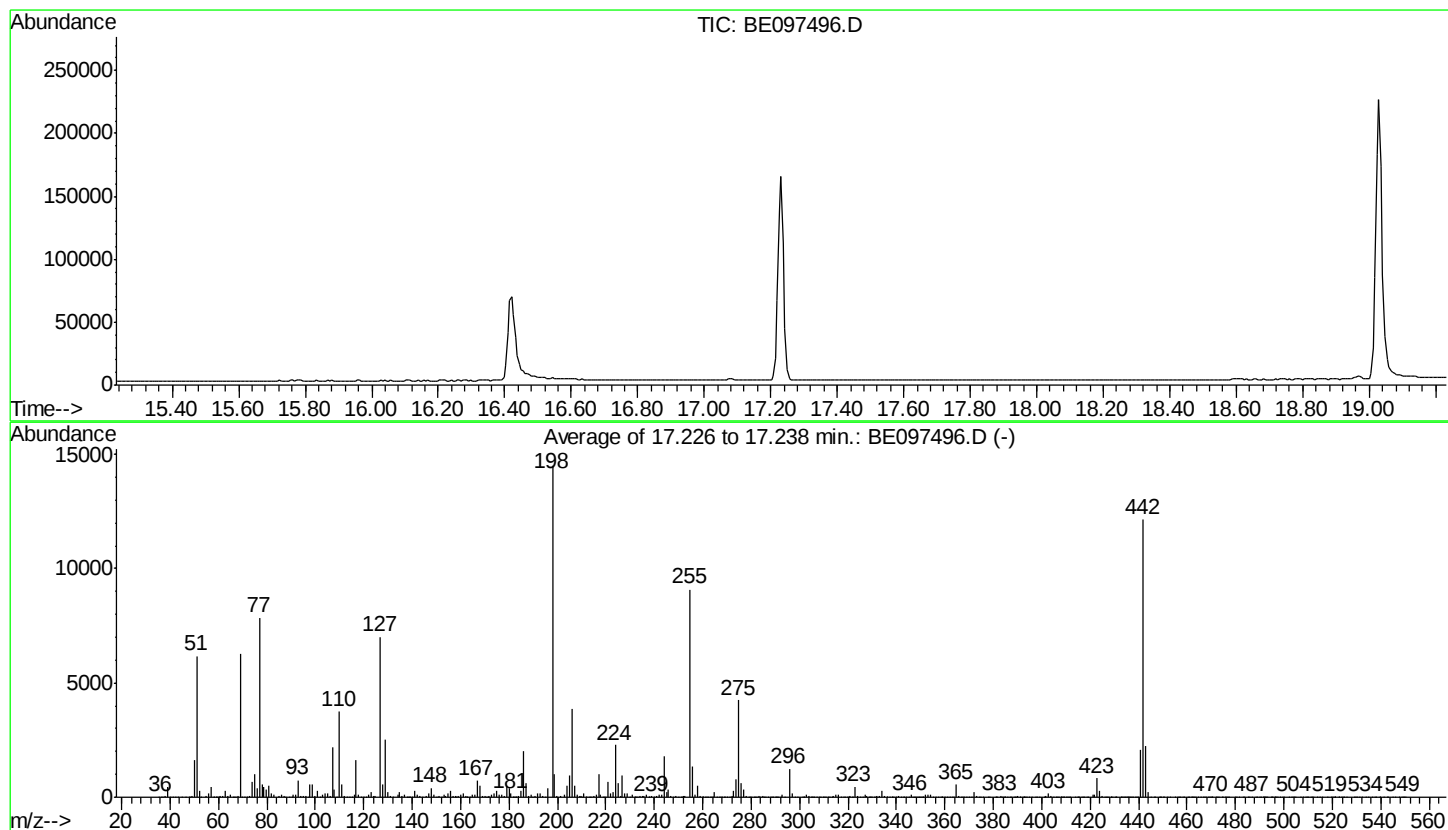

AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	6179	PASS
68	69	0.00	2	1.2	74	PASS
69	198	0.00	100	43.4	6296	PASS
70	69	0.00	2	0.5	29	PASS
127	198	10	80	48.3	7004	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	14501	PASS
199	198	5	9	6.9	1003	PASS
275	198	10	60	29.2	4234	PASS
365	198	1	100	3.8	557	PASS
441	198	0.01	100	14.2	2053	PASS
442	198	50	100	83.7	12138	PASS
443	442	15	24	18.7	2267	PASS