


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE091718\
 Data File : BE097515.D
 Acq On : 18 Sep 2018 3:44
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 17 18:57:11 2018

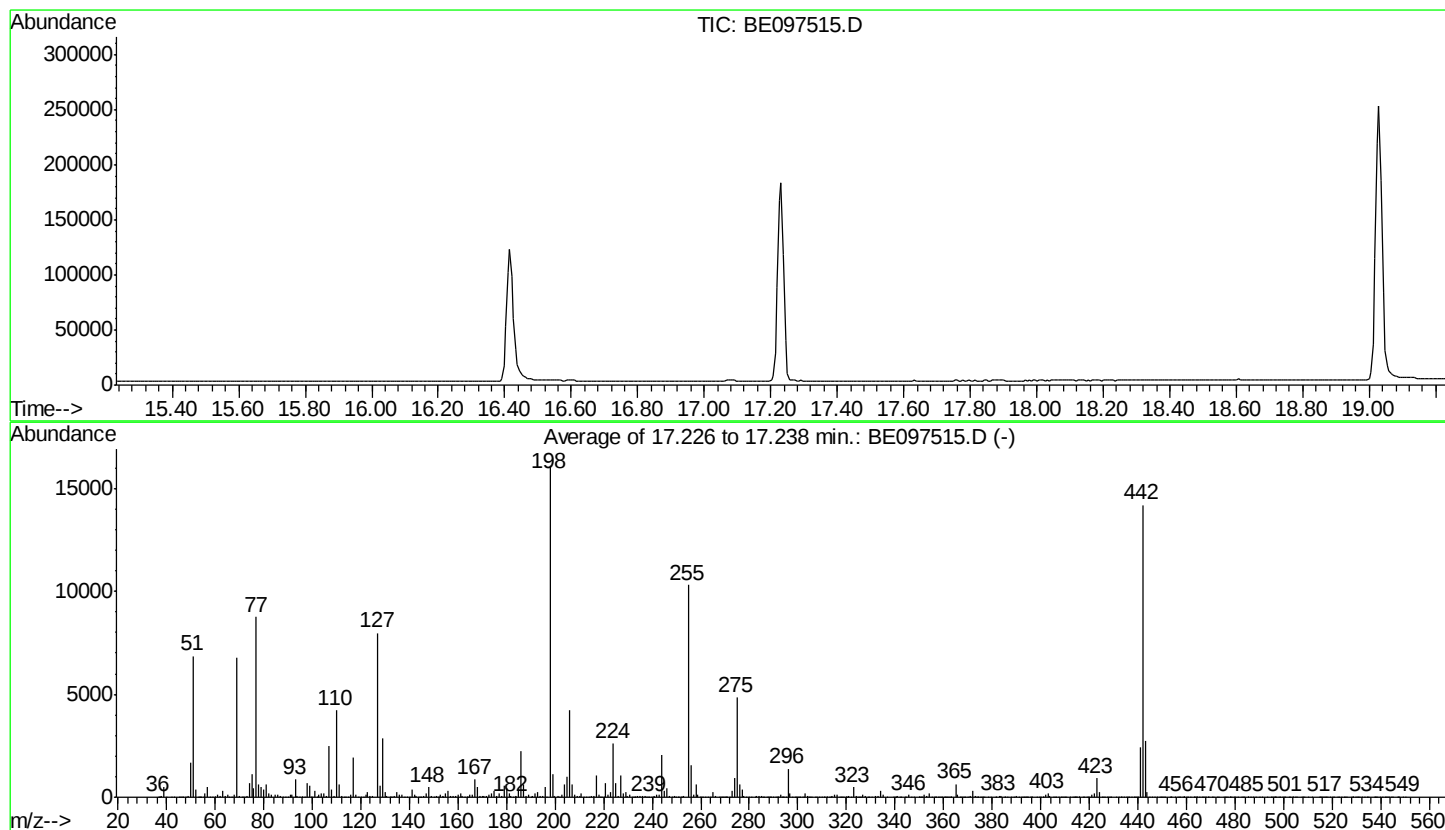

AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.7	6870	PASS
68	69	0.00	2	1.8	120	PASS
69	198	0.00	100	42.3	6805	PASS
70	69	0.00	2	0.6	43	PASS
127	198	10	80	49.5	7966	PASS
197	198	0.00	2	0.2	33	PASS
198	198	100	100	100.0	16103	PASS
199	198	5	9	6.8	1100	PASS
275	198	10	60	30.0	4831	PASS
365	198	1	100	4.0	644	PASS
441	198	0.01	100	15.0	2418	PASS
442	198	50	100	88.2	14201	PASS
443	442	15	24	19.3	2743	PASS