
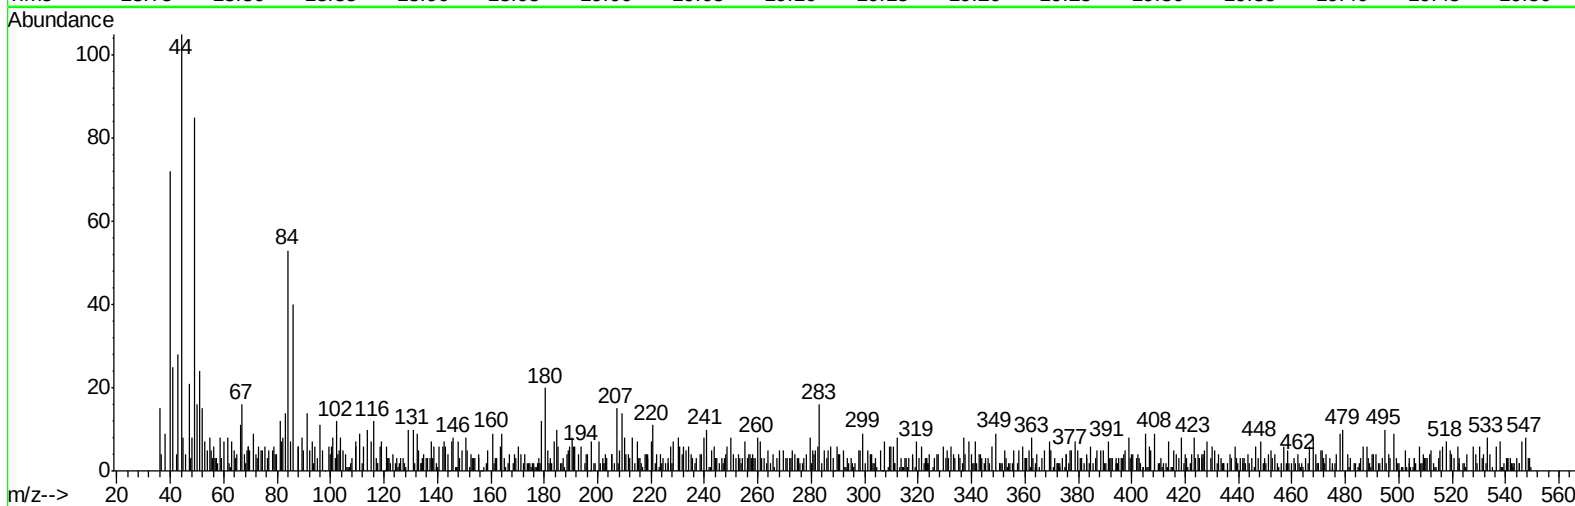


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_E\DATA\BE092018\  
Data File : BE097589.D  
Acq On : 21 Sep 2018 1:10  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 21 07:28:05 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF091418.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Sep 14 13:26:52 2018  
Response via : Initial Calibration

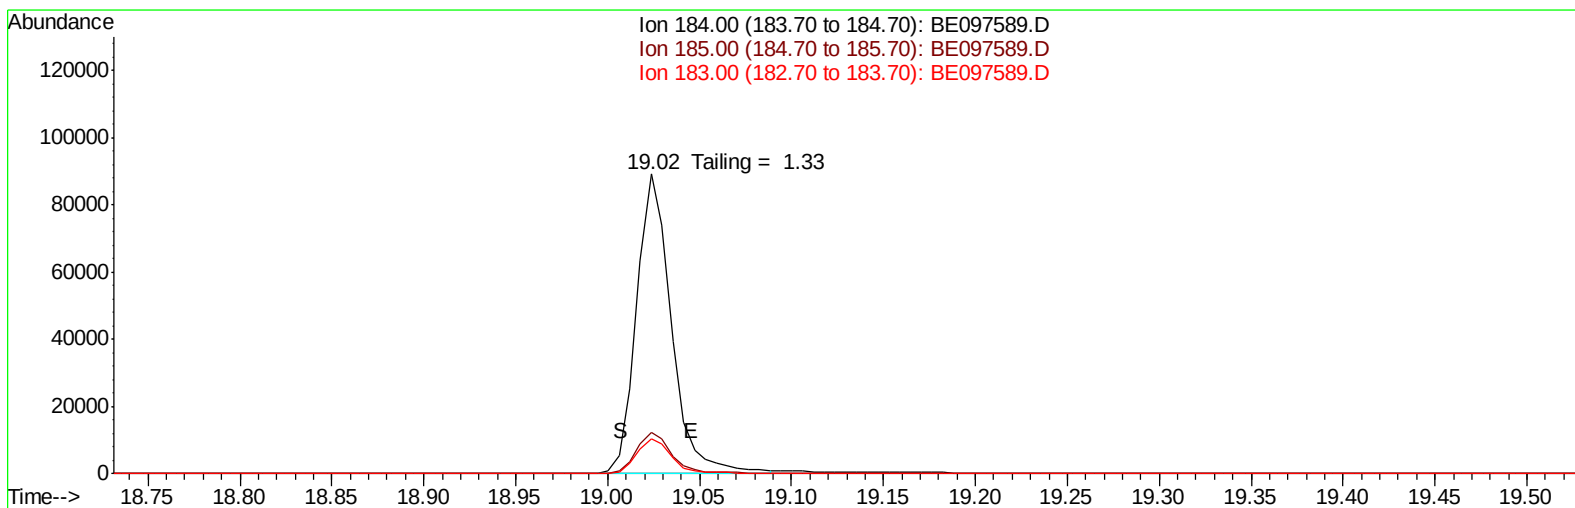

TIC: BE097589.D

(76) Benzidine



12.590min (+0.037) 38.52ng

response 15

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 184.00 | 100   | 100    |
| 185.00 | 15.70 | 35.29# |
| 183.00 | 11.60 | 52.94# |
| 0.00   | 0.00  | 0.00   |

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_E\DATA\BE092018\  
Data File : BE097589.D  
Acq On : 21 Sep 2018 1:10  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 21 07:28:05 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF091418.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Sep 14 13:26:52 2018  
Response via : Initial Calibration

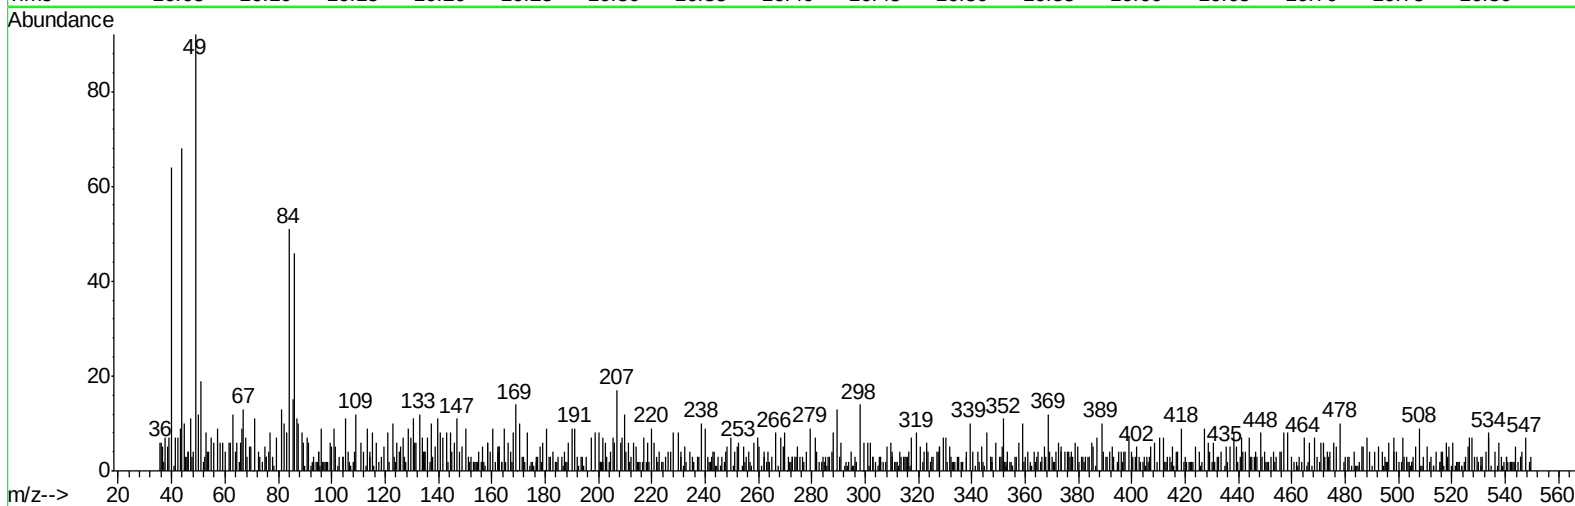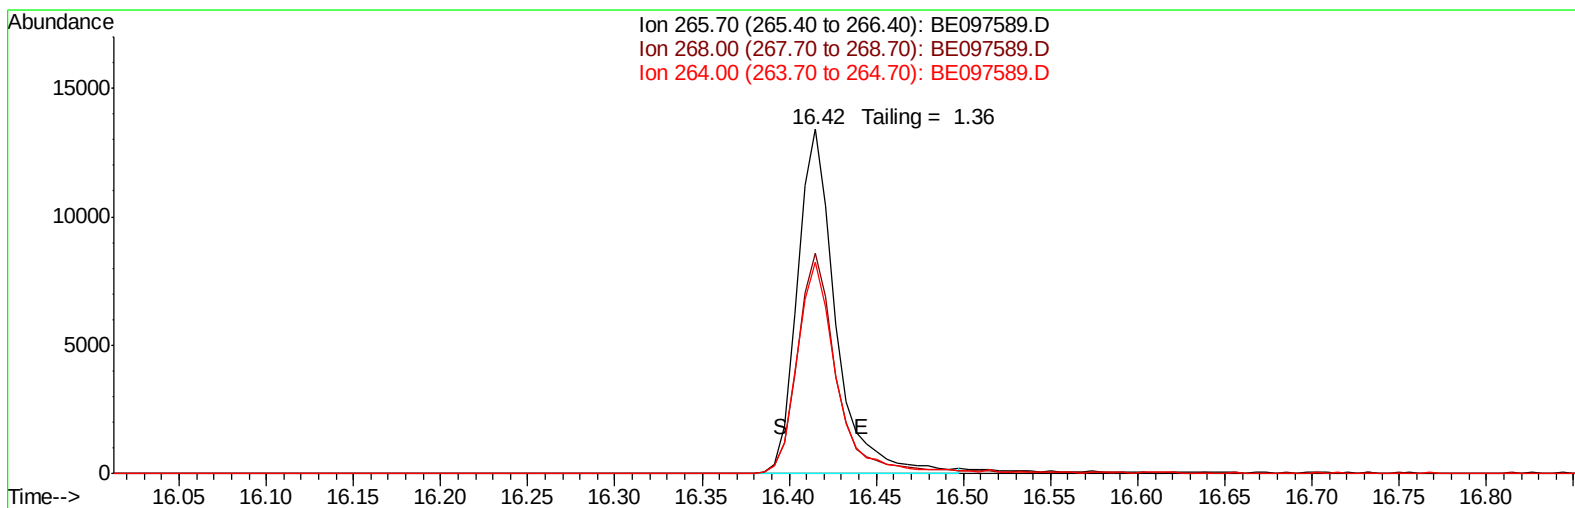

TIC: BE097589.D

(69) Pentachlorophenol (C)

11.045min (+0.003) 194.42ng

response 3

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 265.70 | 100   | 100    |
| 268.00 | 63.90 | 87.50# |
| 264.00 | 61.90 | 50.00  |
| 0.00   | 0.00  | 0.00   |