


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE092018\
Data File : BE097573.D
Acq On : 20 Sep 2018 12:29
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091918.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 20 10:54:43 2018

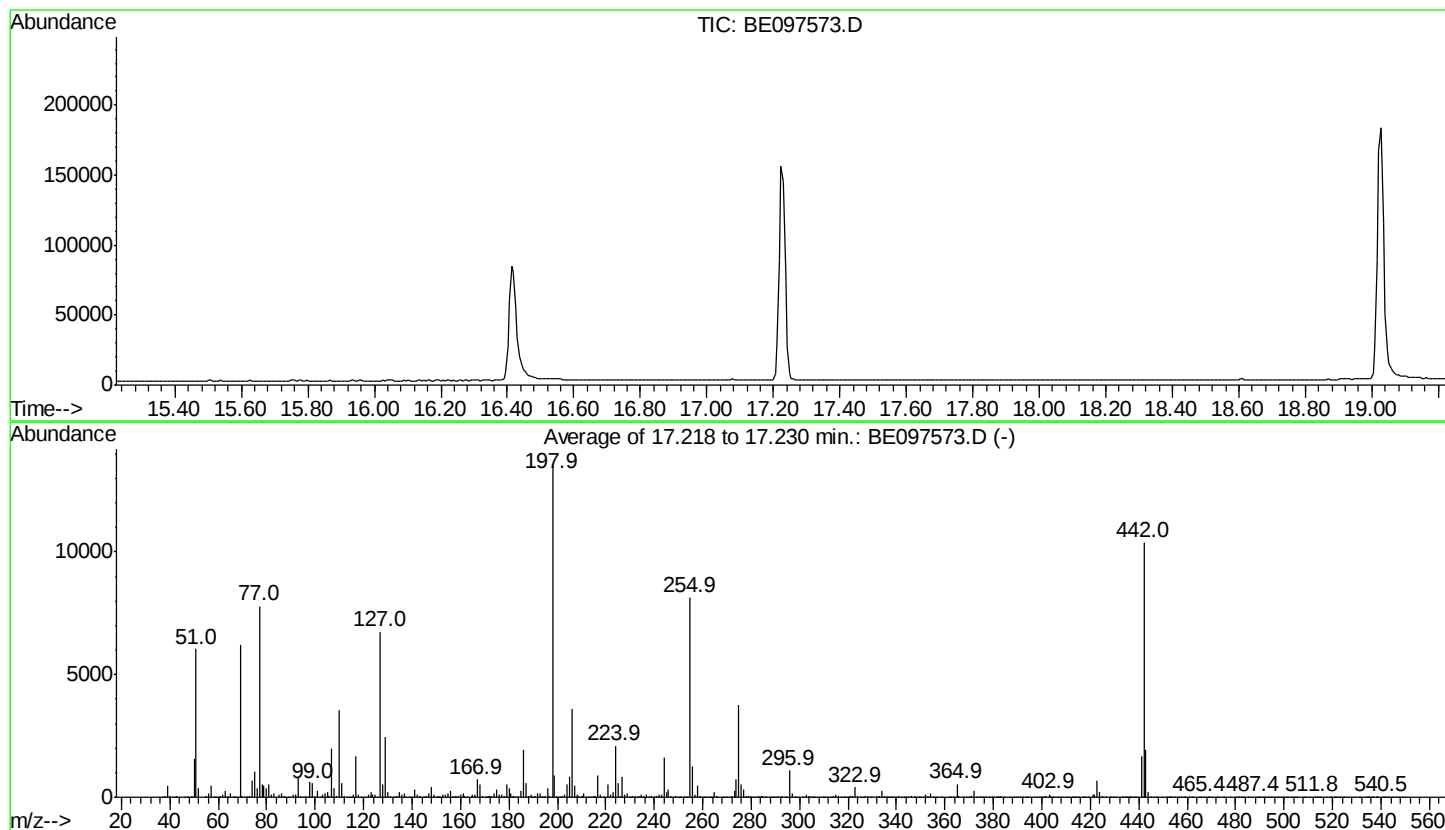

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.8	6050	PASS
68	69	0.00	2	0.4	23	PASS
69	198	0.00	100	45.9	6203	PASS
70	69	0.00	2	0.6	37	PASS
127	198	10	80	50.0	6752	PASS
197	198	0.00	2	0.4	49	PASS
198	198	100	100	100.0	13513	PASS
199	198	5	9	6.8	914	PASS
275	198	10	60	27.8	3762	PASS
365	198	1	100	4.0	541	PASS
441	198	0.01	100	12.5	1684	PASS
442	198	50	100	76.7	10368	PASS
443	442	15	24	18.6	1928	PASS