


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE092018\
 Data File : BE097589.D
 Acq On : 21 Sep 2018 1:10
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 20 10:54:43 2018

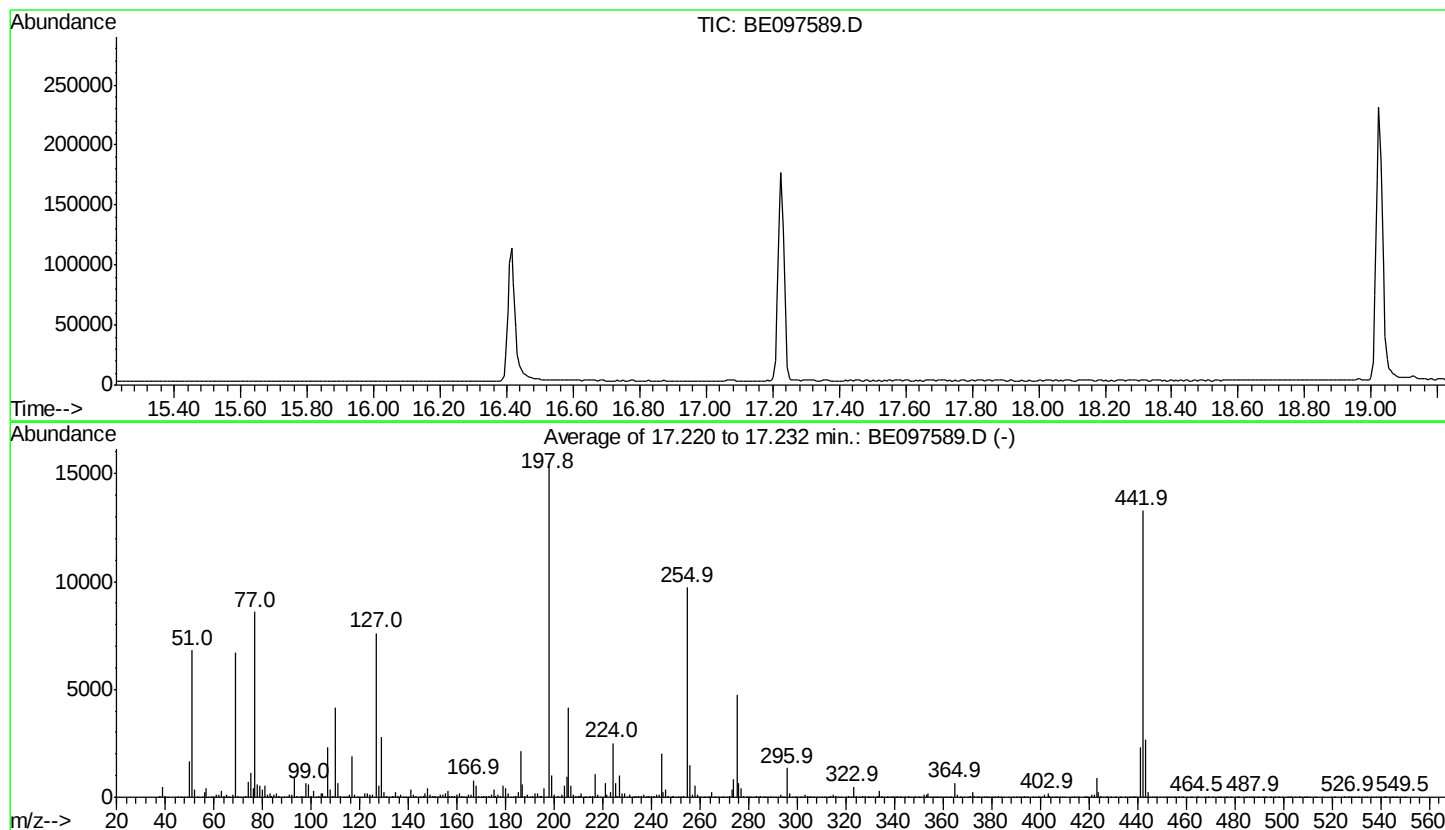

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.4	6822	PASS
68	69	0.00	2	1.5	98	PASS
69	198	0.00	100	43.7	6714	PASS
70	69	0.00	2	0.6	39	PASS
127	198	10	80	49.6	7621	PASS
197	198	0.00	2	0.2	28	PASS
198	198	100	100	100.0	15374	PASS
199	198	5	9	6.7	1023	PASS
275	198	10	60	30.8	4732	PASS
365	198	1	100	4.3	664	PASS
441	198	0.01	100	14.9	2296	PASS
442	198	50	100	86.4	13288	PASS
443	442	15	24	20.2	2684	PASS