


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE092019\
Data File : BE100525.D
Acq On : 20 Sep 2019 13:24
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Sep 20 18:26:17 2019

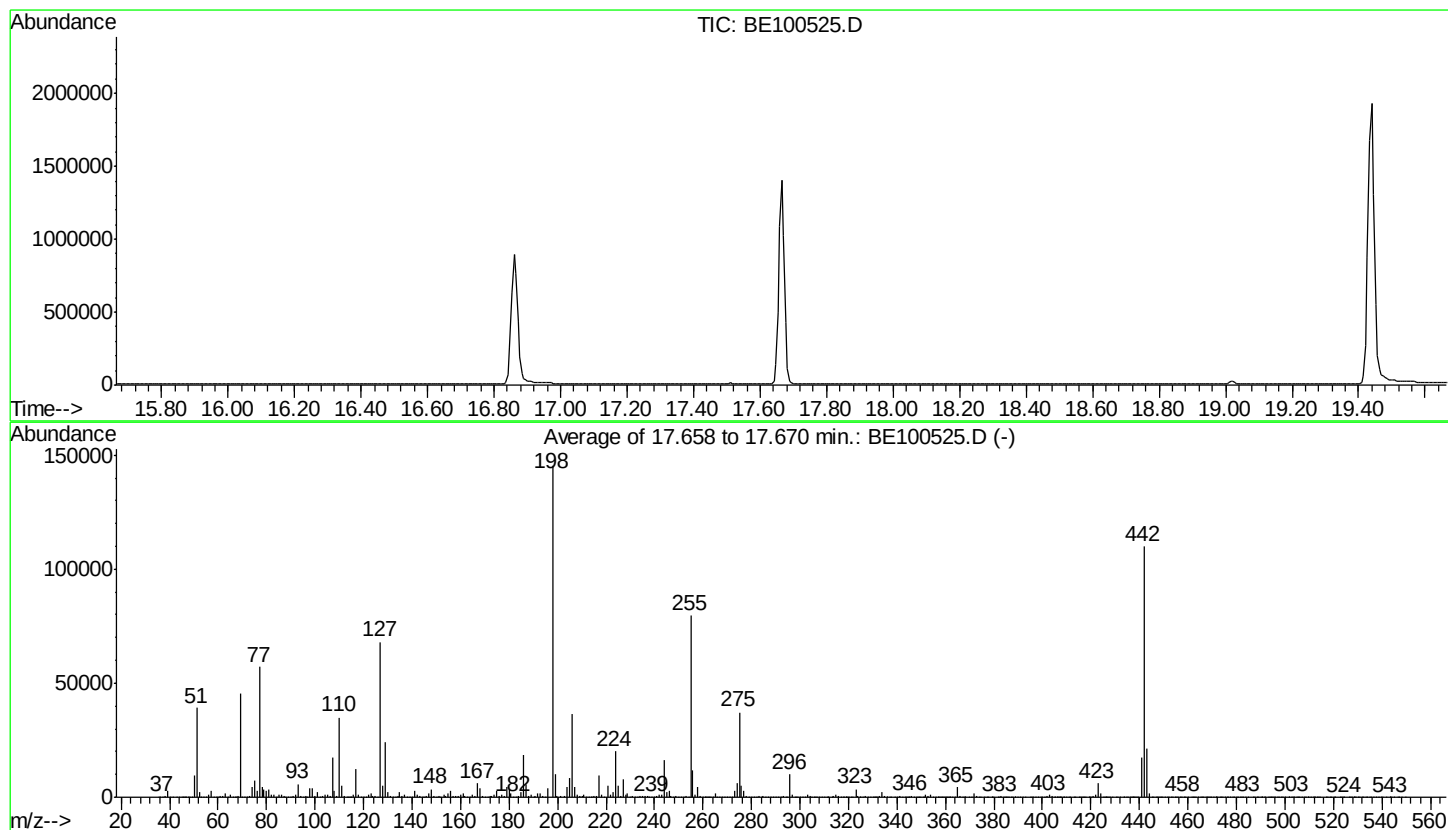

AutoFind: Scans 2565, 2566, 2567; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.9	39134	PASS
68	69	0.00	2	1.6	721	PASS
69	198	0.00	100	31.3	45463	PASS
70	69	0.00	2	0.5	249	PASS
127	198	10	80	46.8	68011	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	145346	PASS
199	198	5	9	7.0	10155	PASS
275	198	10	60	25.7	37313	PASS
365	198	1	100	2.9	4234	PASS
441	198	0.01	100	11.8	17160	PASS
442	198	50	100	75.5	109761	PASS
443	442	15	24	19.4	21347	PASS