


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE092418\
Data File : BE097643.D
Acq On : 24 Sep 2018 13:55
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092418.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Sep 24 18:40:34 2018

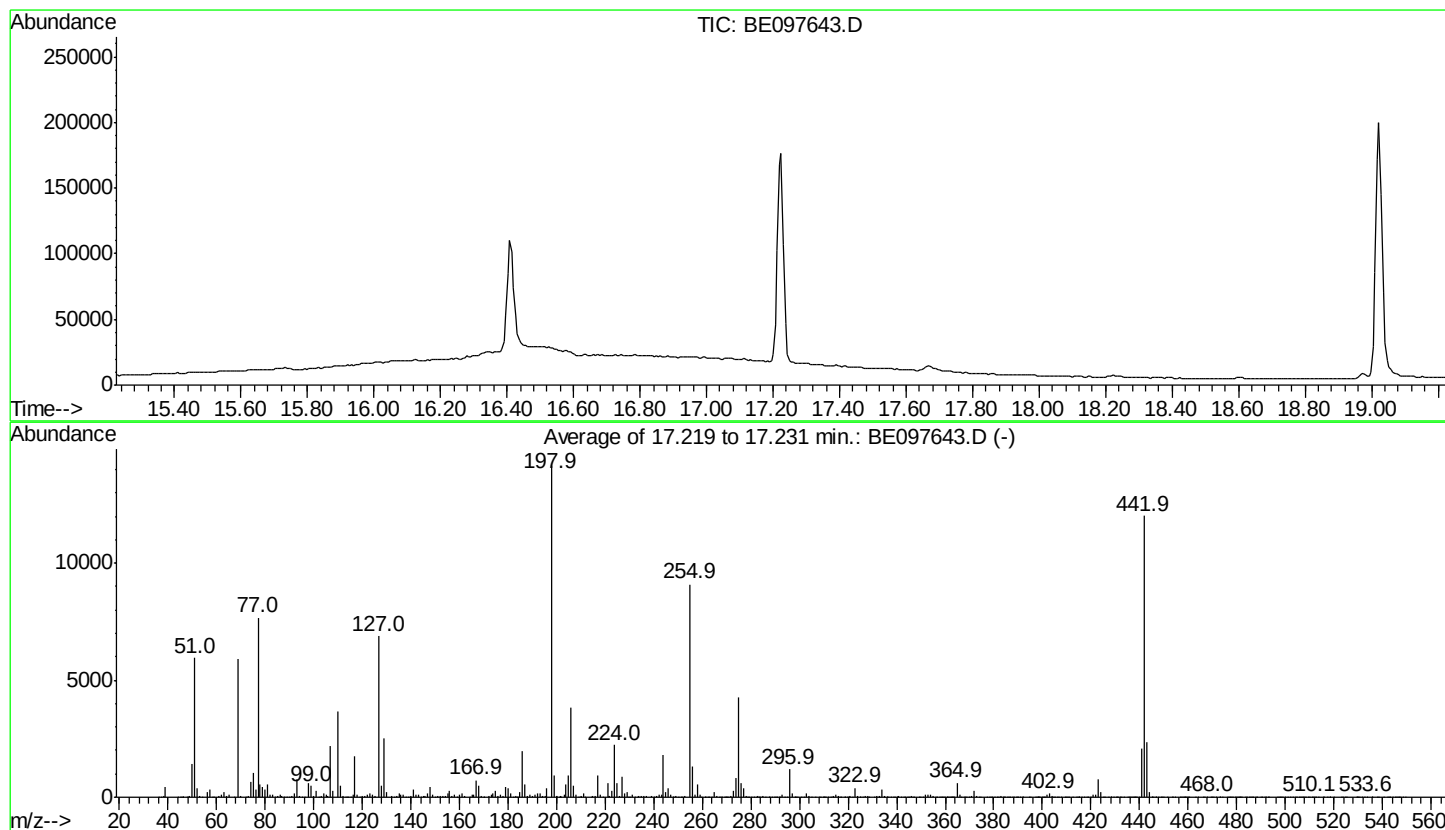

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.9	5939	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.6	5893	PASS
70	69	0.00	2	1.1	62	PASS
127	198	10	80	48.5	6872	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	14167	PASS
199	198	5	9	6.7	947	PASS
275	198	10	60	30.3	4289	PASS
365	198	1	100	4.3	613	PASS
441	198	0.01	100	14.7	2084	PASS
442	198	50	100	84.9	12030	PASS
443	442	15	24	19.6	2358	PASS