
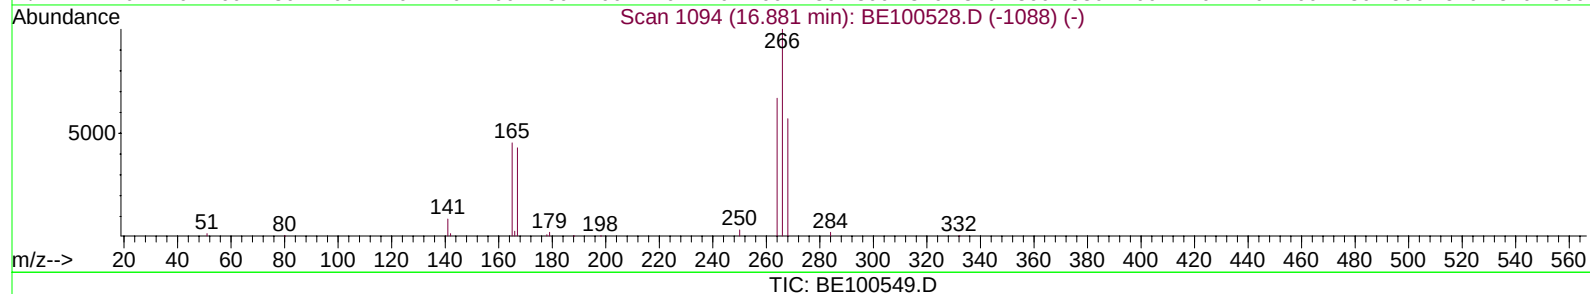
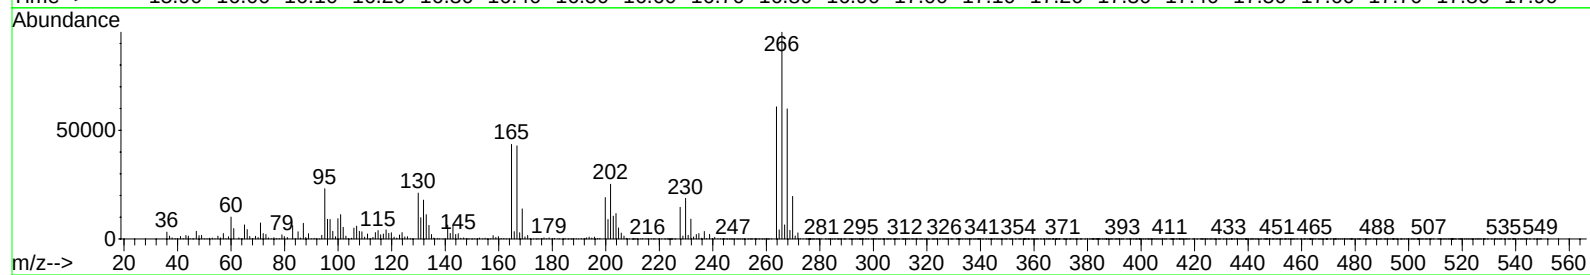


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE092519\
Data File : BE100549.D
Acq On : 25 Sep 2019 8:55
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 25 18:58:24 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE092019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 20 18:26:17 2019
Response via : Initial Calibration

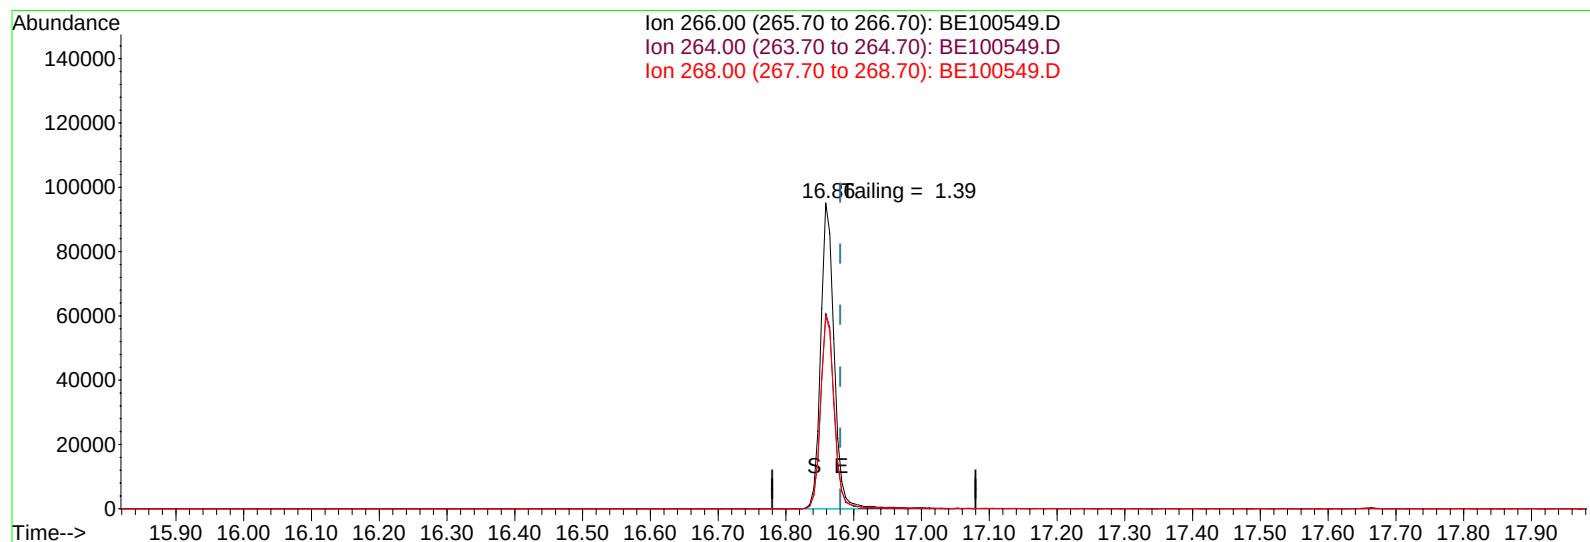

(22) Pentachlorophenol

16.859min (-0.021) 724.08ng

response 131534

Ion	Exp%	Act%
266.00	100	100
264.00	72.00	63.90
268.00	68.90	62.95
0.00	0.00	0.00