


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE092519\
 Data File : BE100549.D
 Acq On : 25 Sep 2019 8:55
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 20 18:26:17 2019

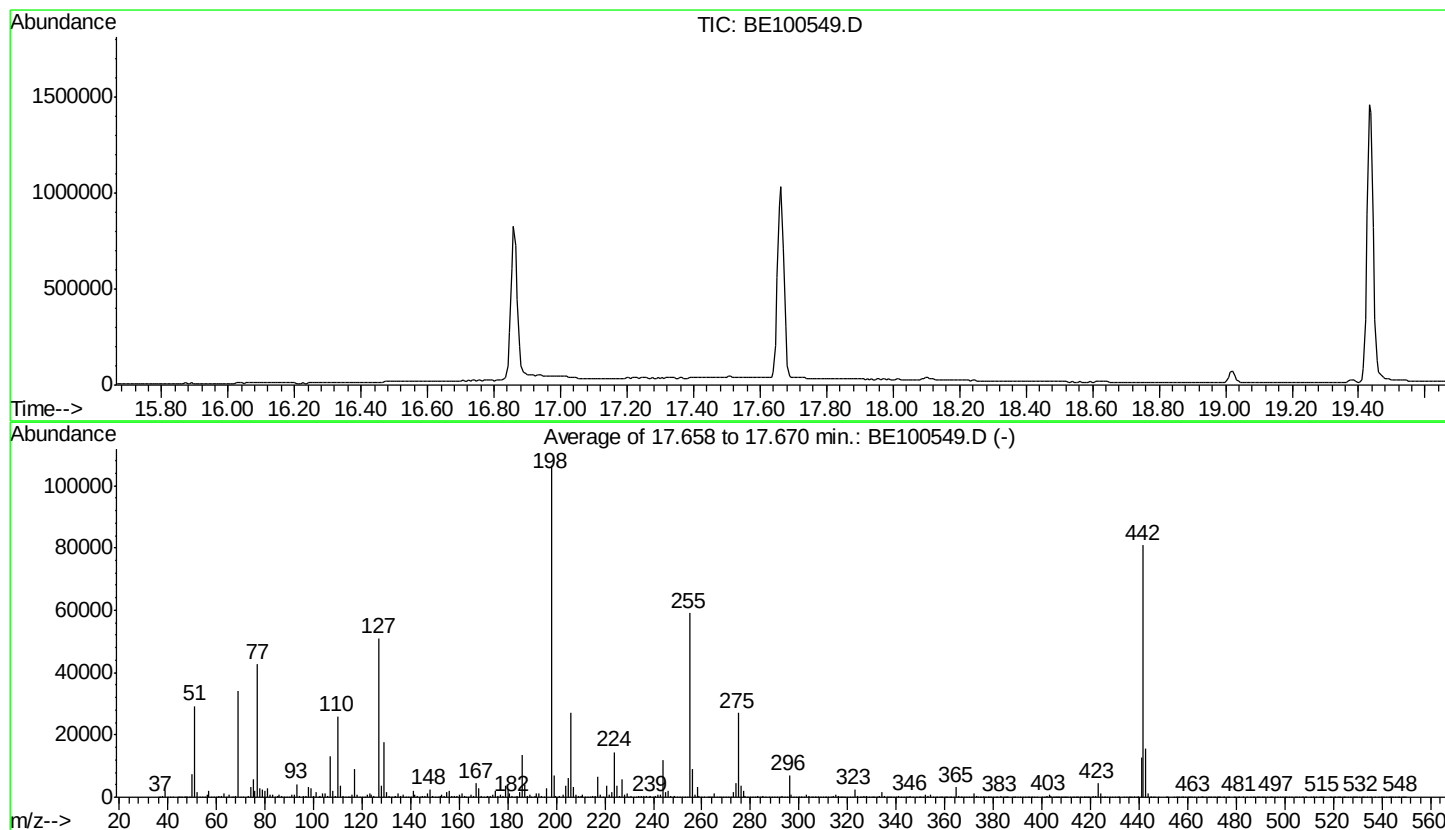

AutoFind: Scans 2565, 2566, 2567; Background Corrected with Scan 2557

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.4	29201	PASS
68	69	0.00	2	1.6	563	PASS
69	198	0.00	100	32.1	34187	PASS
70	69	0.00	2	0.4	120	PASS
127	198	10	80	47.7	50777	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	106393	PASS
199	198	5	9	6.8	7185	PASS
275	198	10	60	25.4	27045	PASS
365	198	1	100	3.1	3270	PASS
441	198	0.01	100	11.9	12616	PASS
442	198	50	100	76.0	80822	PASS
443	442	15	24	19.4	15665	PASS