
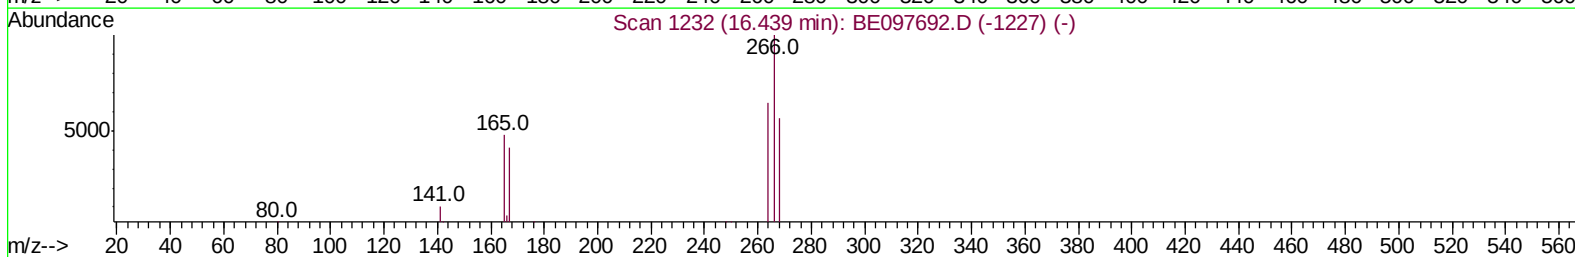
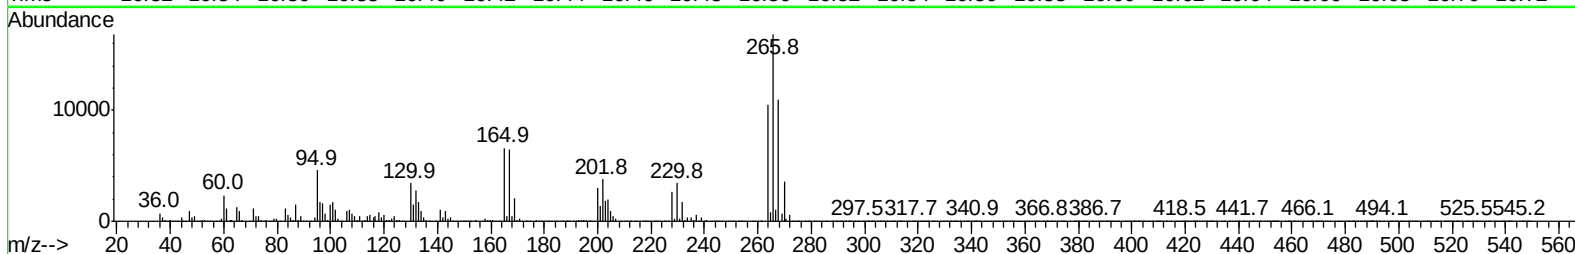


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE092718\
 Data File : BE097689.D
 Acq On : 27 Sep 2018 10:00
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 28 12:07:35 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE092718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 27 15:45:00 2018
 Response via : Initial Calibration

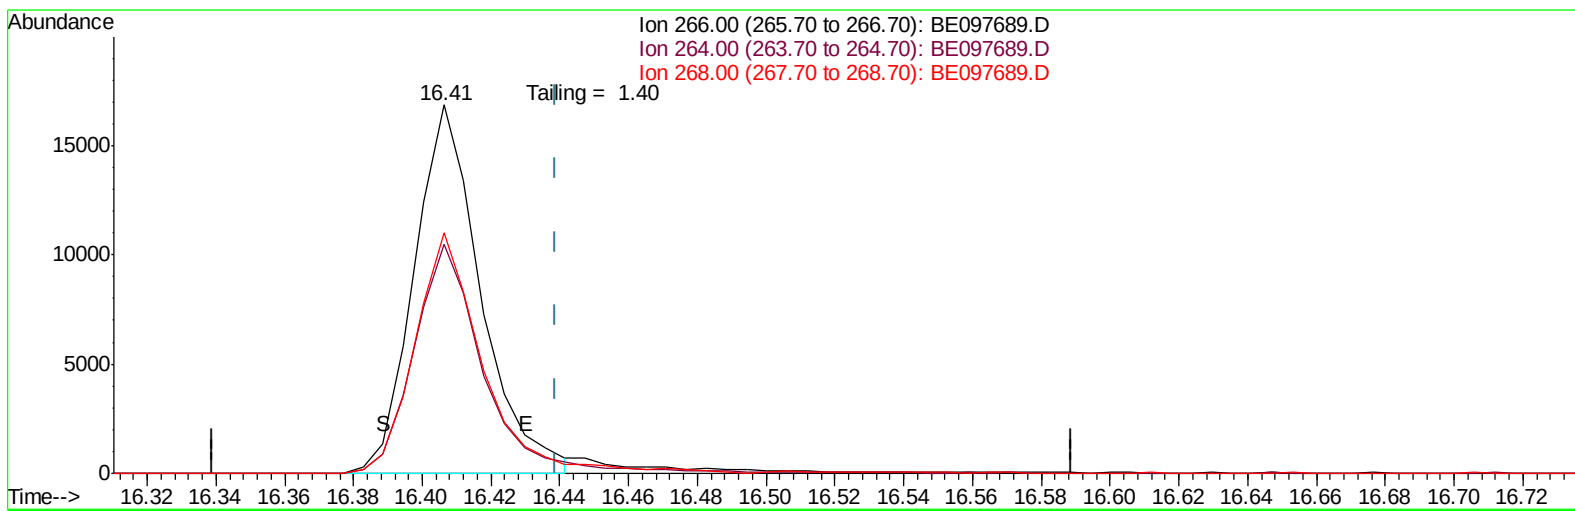

TIC: BE097689.D

(22) Pentachlorophenol

16.406min (-0.033) 36253.47ng

response 23875

Ion	Exp%	Act%
266.00	100	100
264.00	90.60	62.07#
268.00	92.20	65.40#
0.00	0.00	0.00