


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE092718\  
 Data File : BE097689.D  
 Acq On : 27 Sep 2018 10:00  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_E\METHODS\8270-SIM-BE092718.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Sep 27 15:45:00 2018

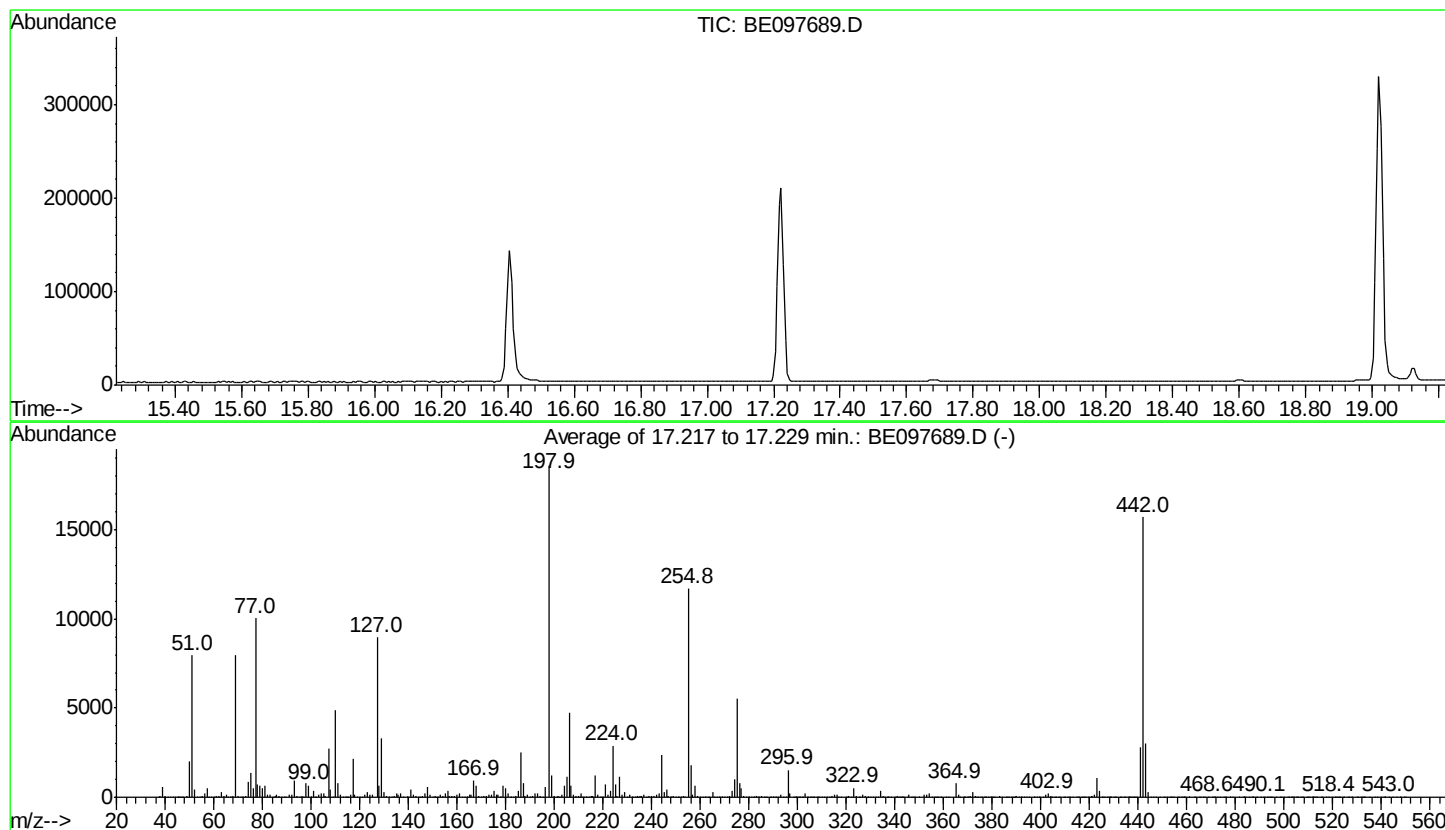

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2481

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 42.8      | 7950    | PASS             |
| 68          | 69           | 0.00         | 2            | 0.6       | 47      | PASS             |
| 69          | 198          | 0.00         | 100          | 42.8      | 7964    | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 49      | PASS             |
| 127         | 198          | 10           | 80           | 48.1      | 8952    | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 18592   | PASS             |
| 199         | 198          | 5            | 9            | 6.5       | 1214    | PASS             |
| 275         | 198          | 10           | 60           | 29.8      | 5535    | PASS             |
| 365         | 198          | 1            | 100          | 4.1       | 767     | PASS             |
| 441         | 198          | 0.01         | 100          | 15.2      | 2828    | PASS             |
| 442         | 198          | 50           | 100          | 84.4      | 15686   | PASS             |
| 443         | 442          | 15           | 24           | 19.2      | 3019    | PASS             |