


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE092719\
 Data File : BE100570.D
 Acq On : 27 Sep 2019 13:29
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 27 18:32:20 2019

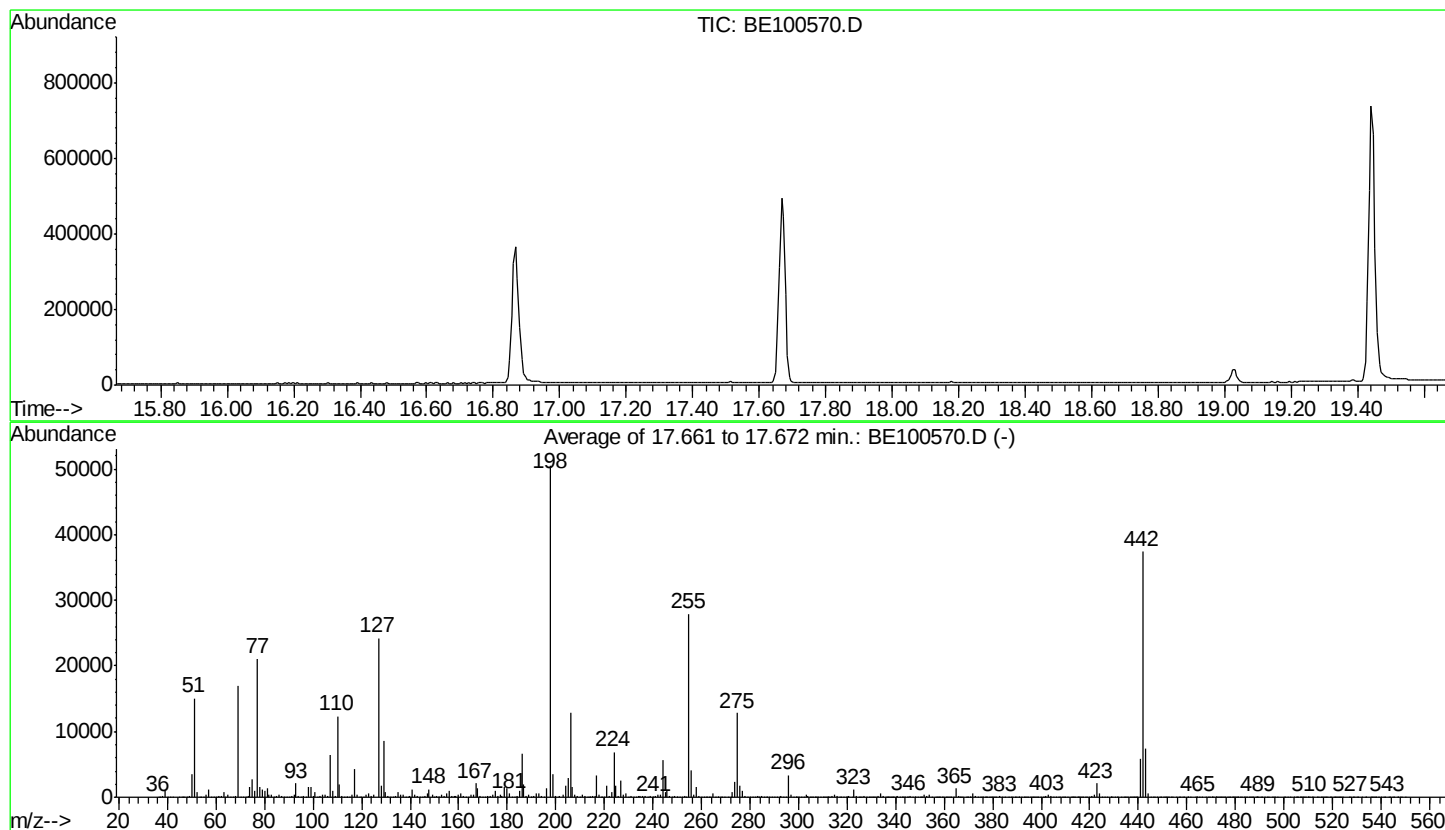

AutoFind: Scans 2565, 2566, 2567; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.8	15060	PASS
68	69	0.00	2	1.7	296	PASS
69	198	0.00	100	33.7	17004	PASS
70	69	0.00	2	0.6	99	PASS
127	198	10	80	48.0	24241	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	50517	PASS
199	198	5	9	7.0	3511	PASS
275	198	10	60	25.3	12805	PASS
365	198	1	100	2.7	1360	PASS
441	198	0.01	100	11.5	5834	PASS
442	198	50	100	74.0	37392	PASS
443	442	15	24	19.6	7338	PASS