


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE092818\
Data File : BE097697.D
Acq On : 28 Sep 2018 8:50
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092718.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 27 15:45:00 2018

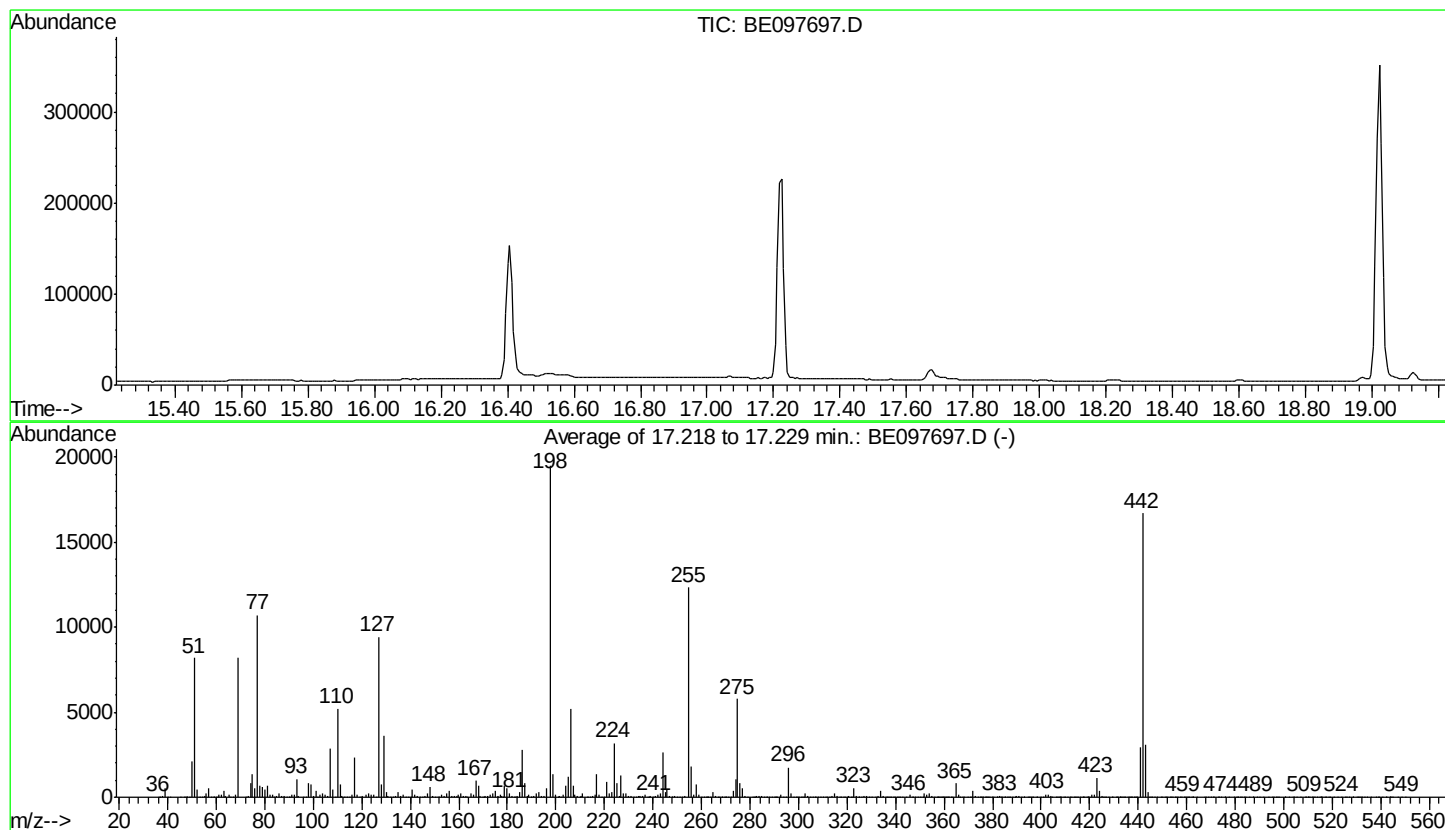

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.9	8181	PASS
68	69	0.00	2	1.7	141	PASS
69	198	0.00	100	42.2	8223	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.3	9414	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	19504	PASS
199	198	5	9	7.0	1370	PASS
275	198	10	60	29.7	5796	PASS
365	198	1	100	4.2	823	PASS
441	198	0.01	100	15.3	2975	PASS
442	198	50	100	85.6	16699	PASS
443	442	15	24	18.7	3121	PASS