


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE093019\
 Data File : BE100579.D
 Acq On : 30 Sep 2019 9:59
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 27 18:32:20 2019

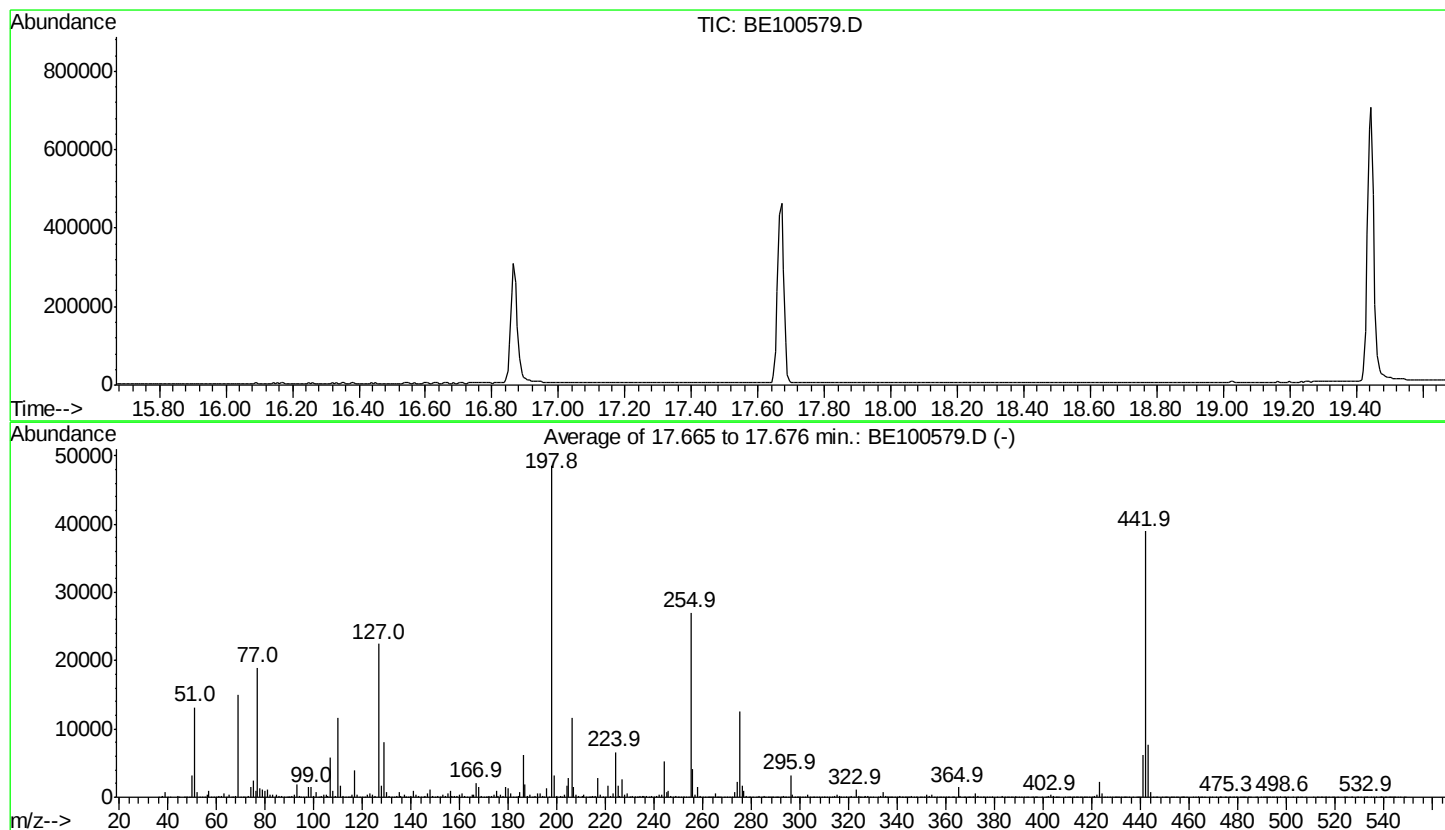

AutoFind: Scans 2566, 2567, 2568; Background Corrected with Scan 2555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.2	13202	PASS
68	69	0.00	2	1.7	258	PASS
69	198	0.00	100	30.9	15000	PASS
70	69	0.00	2	0.4	66	PASS
127	198	10	80	46.2	22425	PASS
197	198	0.00	2	0.1	45	PASS
198	198	100	100	100.0	48570	PASS
199	198	5	9	6.6	3223	PASS
275	198	10	60	26.0	12651	PASS
365	198	1	100	3.0	1455	PASS
441	198	0.01	100	12.6	6113	PASS
442	198	50	100	80.3	38983	PASS
443	442	15	24	19.7	7675	PASS