


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE100318\
Data File : BE097705.D
Acq On : 3 Oct 2018 7:53
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE100318.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 03 12:17:19 2018

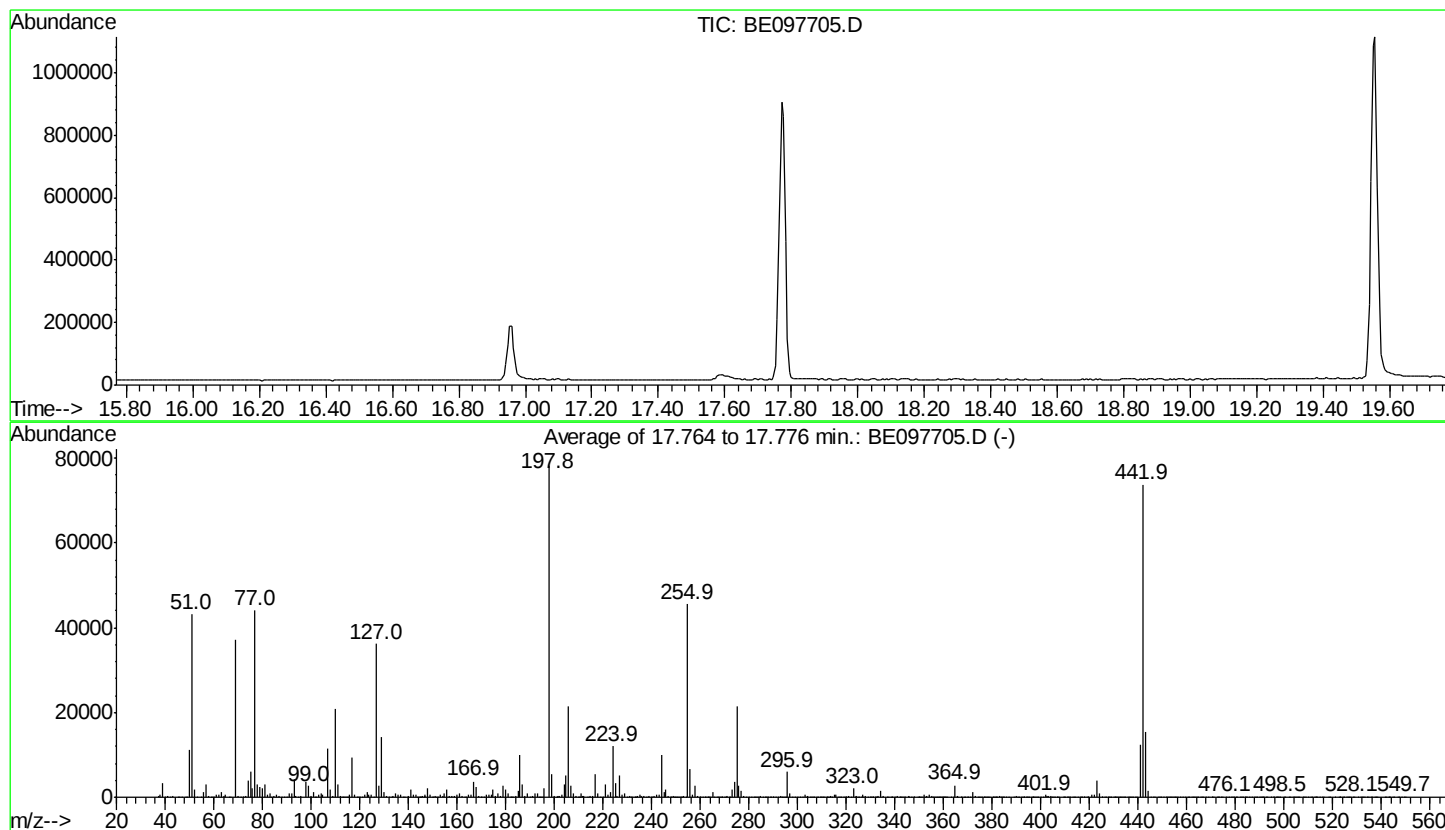

AutoFind: Scans 2583, 2584, 2585; Background Corrected with Scan 2573

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.2	43170	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	47.5	37122	PASS
70	69	0.00	2	0.8	293	PASS
127	198	10	80	46.1	36091	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	78207	PASS
199	198	5	9	6.8	5323	PASS
275	198	10	60	27.4	21438	PASS
365	198	1	100	3.6	2806	PASS
441	198	0.01	100	15.9	12470	PASS
442	198	50	100	94.2	73688	PASS
443	442	15	24	21.1	15553	PASS