


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE100319\
 Data File : BE100593.D
 Acq On : 3 Oct 2019 12:43
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE100319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 04 13:00:50 2019

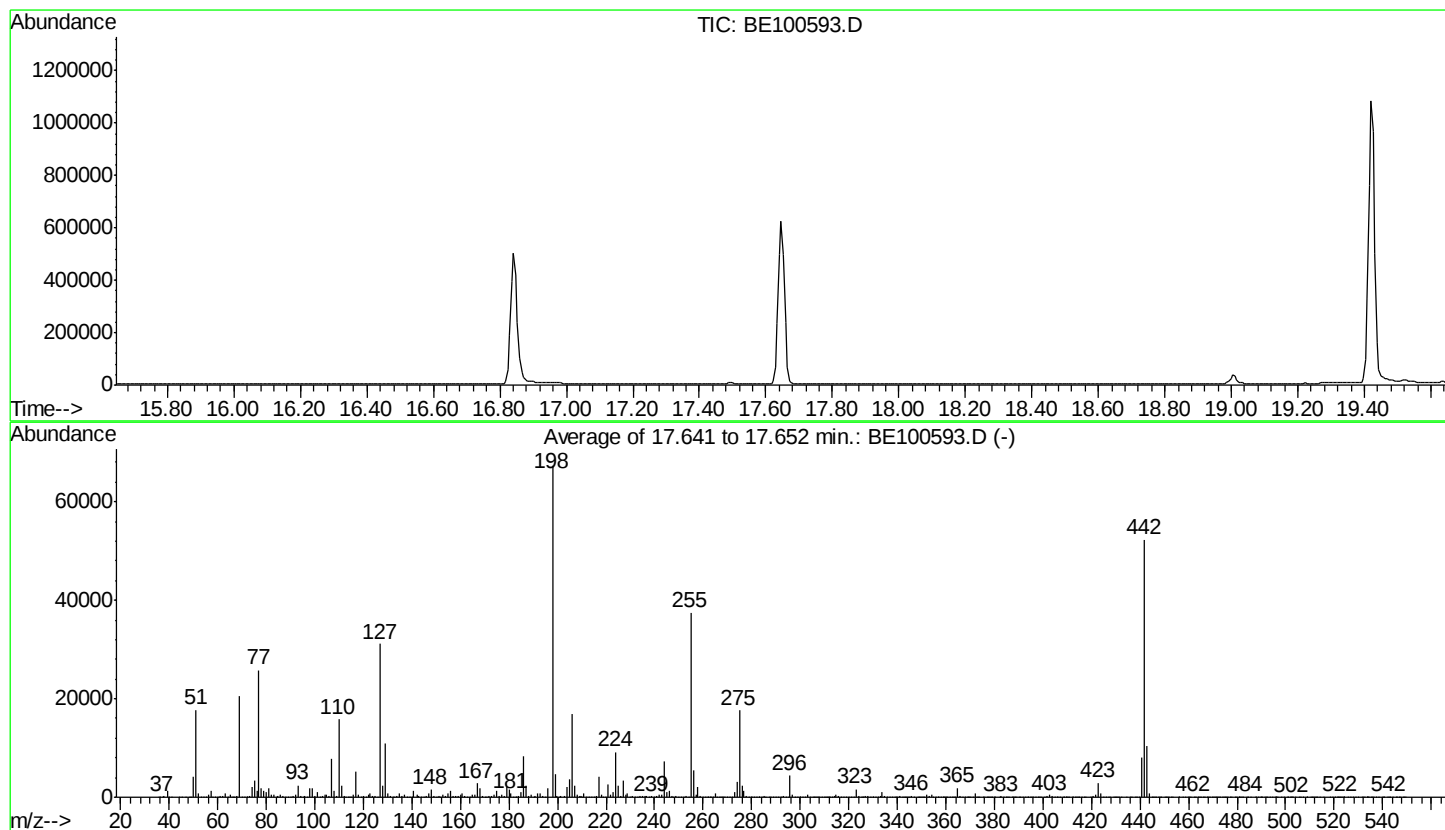

AutoFind: Scans 2562, 2563, 2564; Background Corrected with Scan 2554

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.4	17762	PASS
68	69	0.00	2	1.5	307	PASS
69	198	0.00	100	30.6	20632	PASS
70	69	0.00	2	0.6	126	PASS
127	198	10	80	46.2	31116	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	67333	PASS
199	198	5	9	6.8	4597	PASS
275	198	10	60	26.2	17662	PASS
365	198	1	100	2.8	1868	PASS
441	198	0.01	100	12.1	8145	PASS
442	198	50	100	77.7	52317	PASS
443	442	15	24	19.7	10317	PASS