

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE100518\
 Data File : BE097748.D
 Acq On : 5 Oct 2018 10:36
 Operator : SJ/JU
 Sample : PB113432BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Oct 05 14:04:27 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE100318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 03 12:17:19 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	3550	0.40	ng	0.00
7) Naphthalene-d8	10.69	136	12943	0.40	ng	0.00
13) Acenaphthene-d10	14.56	164	6021	0.40	ng	0.00
19) Phenanthrene-d10	17.30	188	13801	0.40	ng	0.00
27) Chrysene-d12	21.49	240	14703	0.40	ng	0.00
34) Perylene-d12	24.03	264	15485	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.47	112	3013	0.36	ng	0.00
5) Phenol-d6	7.04	99	3702	0.29	ng	0.00
8) Nitrobenzene-d5	9.04	82	2483	0.59	ng	0.00
11) 2-Methylnaphthalene-d10	12.30	152	6688	0.32	ng	0.00
14) 2,4,6-Tribromophenol	16.05	330	359	0.33	ng	0.00
15) 2-Fluorobiphenyl	13.19	172	10203	0.38	ng	0.00
25) Fluoranthene-d10	19.33	212	57773	0.33	ng	0.00
29) Terphenyl-d14	19.93	244	9671	0.32	ng	0.00
Target Compounds						Qvalue
32) Bis(2-ethylhexyl)phthalate	21.41	149	591	0.020	ng	# 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE100518\
Data File : BE097748.D
Acq On : 5 Oct 2018 10:36
Operator : SJ/JU
Sample : PB113432BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Oct 05 14:04:27 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE100318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 03 12:17:19 2018
Response via : Initial Calibration

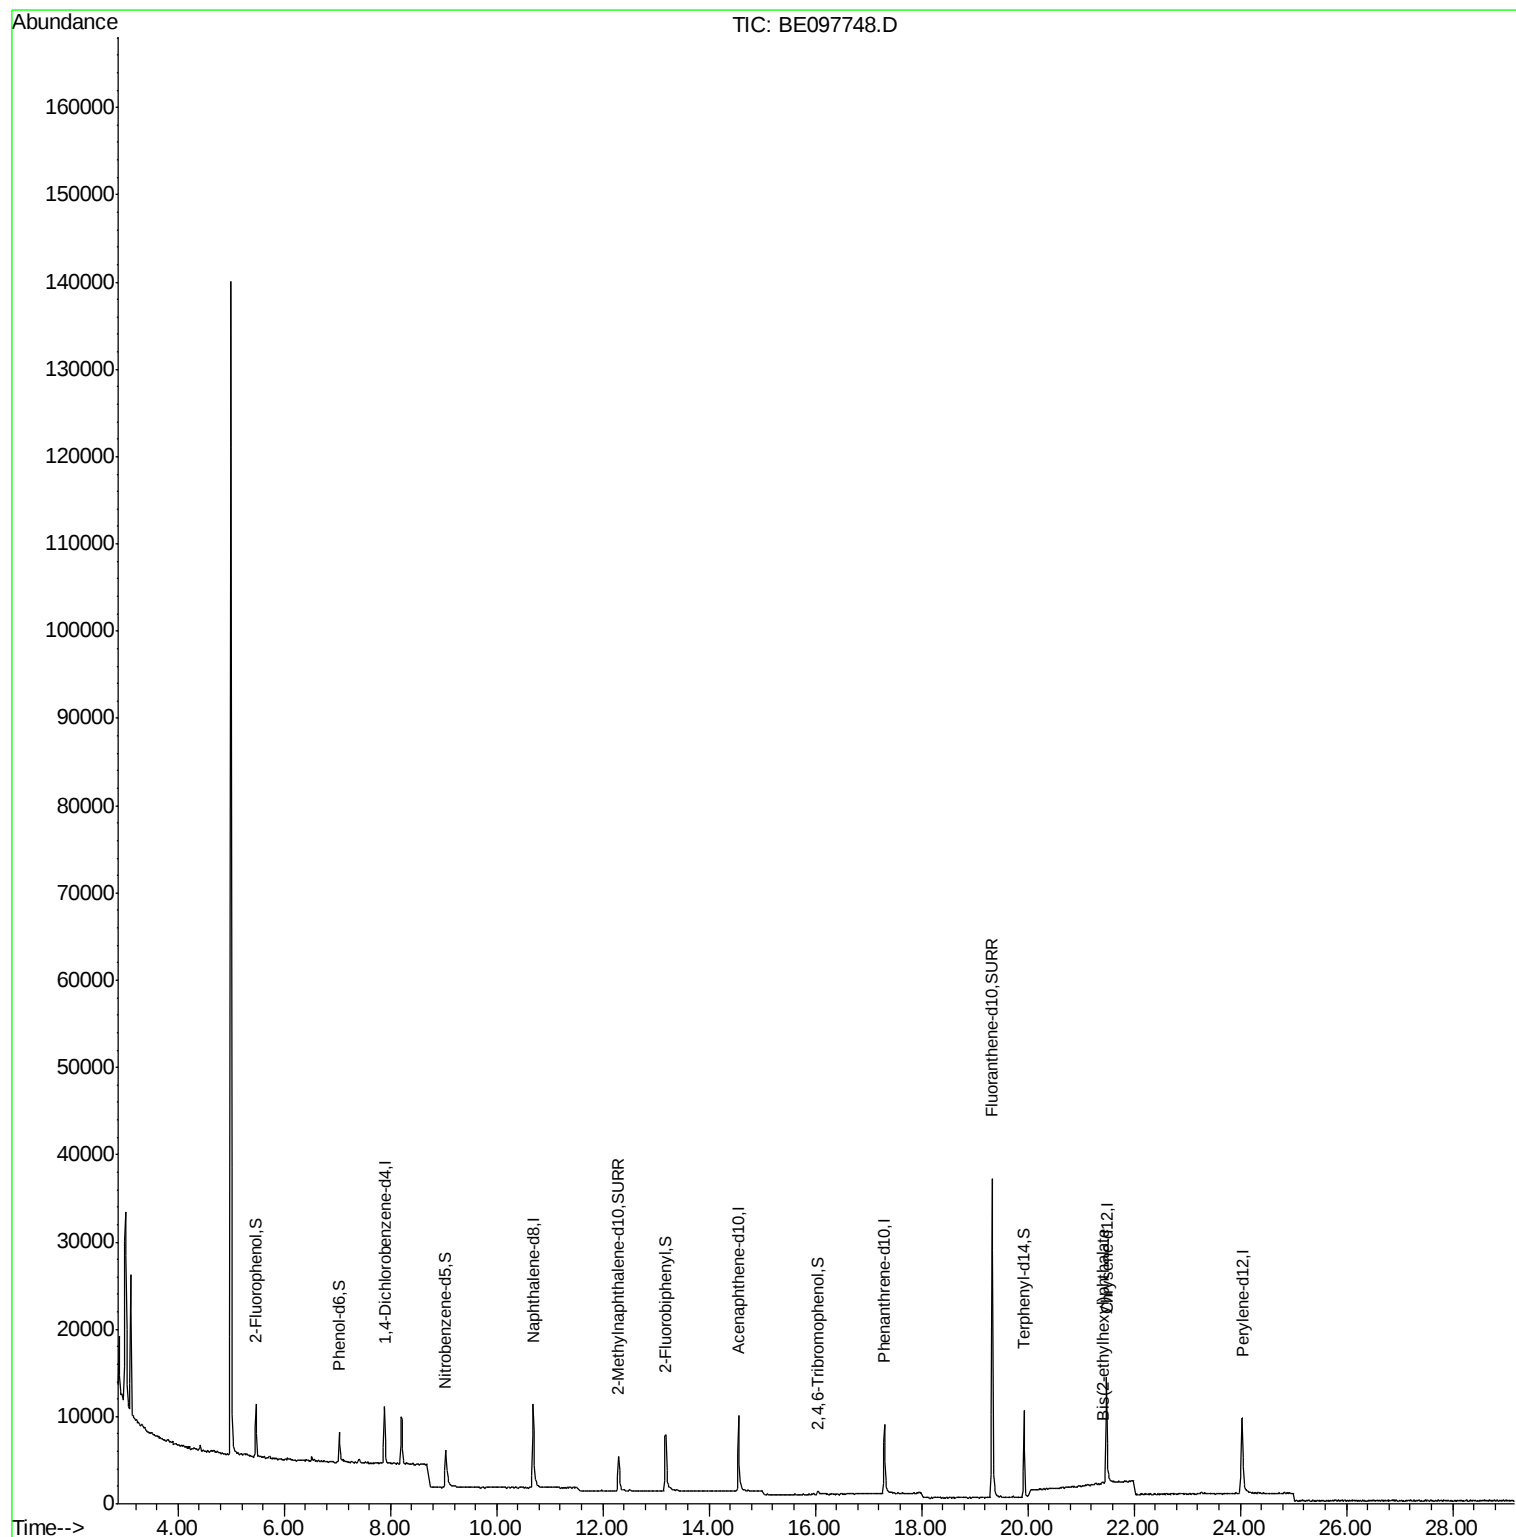




#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.90 min Scan# 437
Delta R.T. -0.00 min
Lab File: BE097748.D
Acq: 5 Oct 2018 10:36

Instrument :
BNA_E
ClientSampleId :

Tot Ion:152 Resp: 3550
Ion Ratio Lower Upper
152 100
150 157.6 120.9 181.3
115 60.7 46.6 69.8

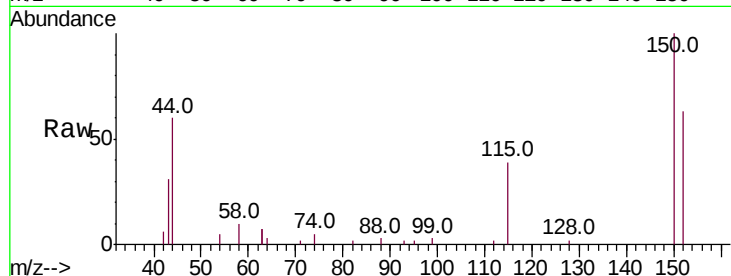


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

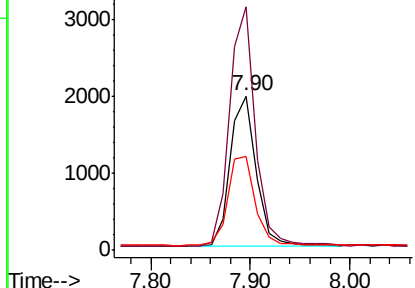



#4


2-Fluorophenol
Concen: 0.359 ng
RT: 5.47 min Scan# 226
Delta R.T. -0.00 min
Lab File: BE097748.D
Acq: 5 Oct 2018 10:36

Tgt Ion:112 Resp: 3013
Ion Ratio Lower Upper
112 100
64 71.1 56.6 84.8
63 143.2 119.4 179.0



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BE0
Ion 63.00 (62.70 to 63.70): BE0

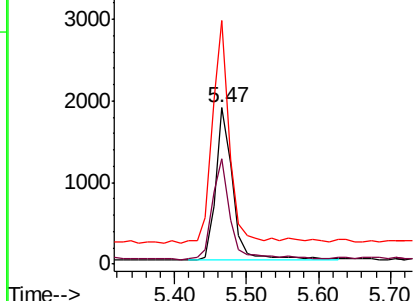



#5

Phenol-d6

Concen: 0.288 ng

RT: 7.04 min Scan# 363

Delta R.T. -0.00 min

Lab File: BE097748.D

Acq: 5 Oct 2018 10:36

Instrument :

BNA_E

ClientSampleId :


Tot Ion: 99 Resp: 3702

Ion Ratio Lower Upper

99 100

42 25.6 19.9 29.9




71 36.7 25.4 38.2



Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

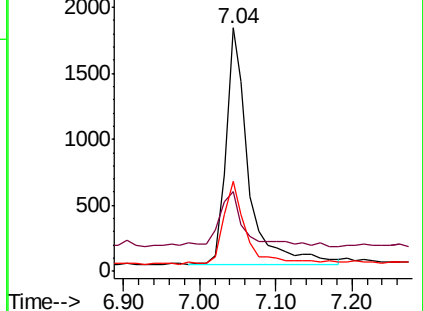

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.69 min Scan# 656

Delta R.T. 0.00 min

Lab File: BE097748.D

Acq: 5 Oct 2018 10:36

Tgt Ion: 136 Resp: 12943


Ion Ratio Lower Upper

136 100

137 11.2 9.0 13.4

54 44.3 37.8 56.6

68 7.6 6.4 9.6






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

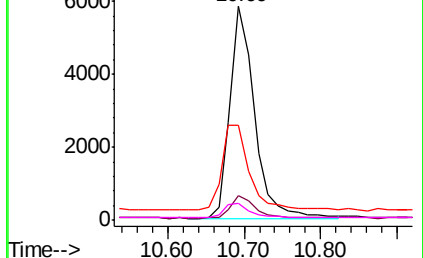



#8

Nitrobenzene-d5

Concen: 0.591 ng

RT: 9.04 min Scan# 529

Delta R.T. 0.00 min

Lab File: BE097748.D

Acq: 5 Oct 2018 10:36

Instrument :

BNA_E

ClientSampleId :


Tot Ion: 82 Resp: 2483

Ion Ratio Lower Upper

82 100

128 116.2 97.0 145.4




54 255.2 206.9 310.3

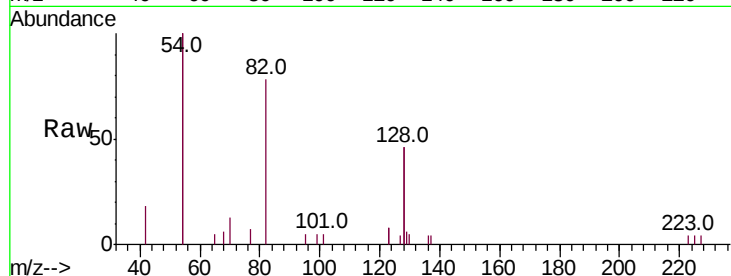

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0

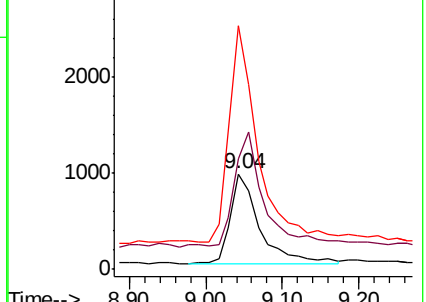

#11

2-Methylnaphthalene-d10

Concen: 0.325 ng

RT: 12.30 min Scan# 769

Delta R.T. -0.00 min

Lab File: BE097748.D


Acq: 5 Oct 2018 10:36

Tgt Ion: 152 Resp: 6688

Ion Ratio Lower Upper



152 100


151 18.8 15.4 23.2



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

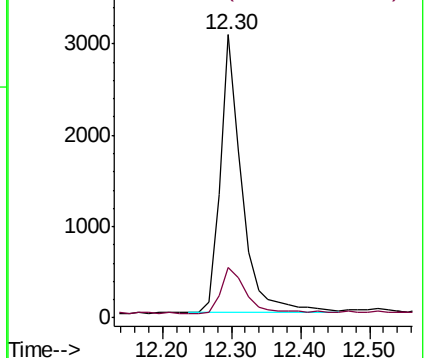







#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.56 min Scan# 926
 Delta R.T. -0.00 min
 Lab File: BE097748.D
 Acq: 5 Oct 2018 10:36

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:164 Resp: 6021
 Ion Ratio Lower Upper
 164 100
 162 97.0 78.6 117.8
 160 48.7 37.8 56.6




Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E


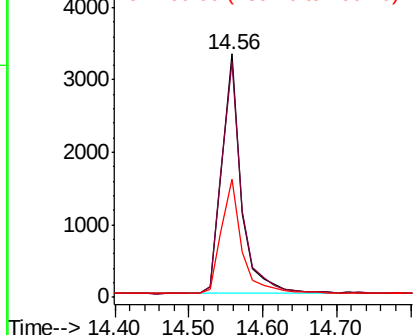



#14
 2,4,6-Tribromophenol
 Concen: 0.329 ng
 RT: 16.05 min Scan# 1043
 Delta R.T. 0.00 min
 Lab File: BE097748.D
 Acq: 5 Oct 2018 10:36

Tgt Ion:330 Resp: 359
 Ion Ratio Lower Upper
 330 100
 332 84.1 83.5 125.3
 141 40.7 34.9 52.3



Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

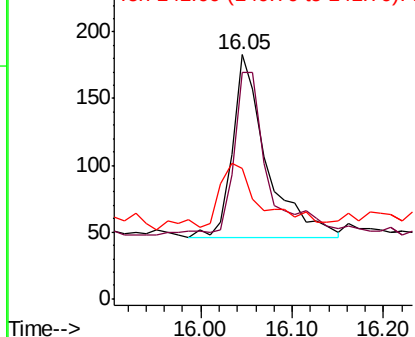


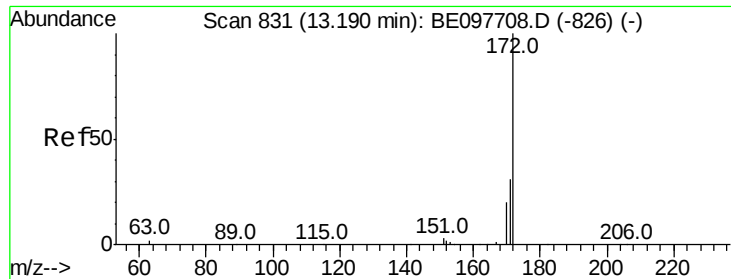




#15
2-Fluorobiphenyl
Concen: 0.385 ng
RT: 13.19 min Scan# 831
Delta R.T. -0.00 min
Lab File: BE097748.D
Acq: 5 Oct 2018 10:36

Instrument :
BNA_E
ClientSampled :

Tot Ion:172 Resp: 10203
Ion Ratio Lower Upper
172 100
171 32.5 25.2 37.8
170 22.8 16.2 24.2




Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

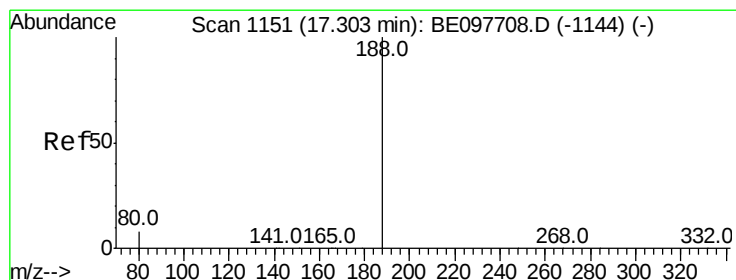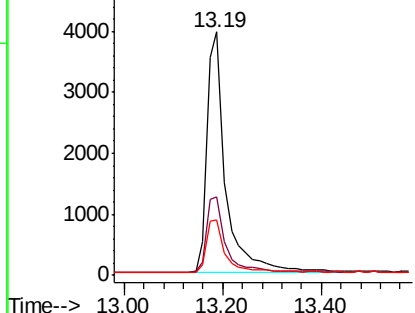




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.30 min Scan# 1151
Delta R.T. 0.00 min
Lab File: BE097748.D
Acq: 5 Oct 2018 10:36

Tgt Ion:188 Resp: 13801
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 9.2 6.6 9.8

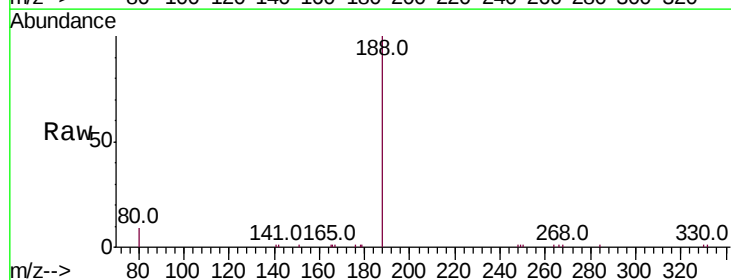

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BE0
Ion 80.00 (79.70 to 80.70): BE0

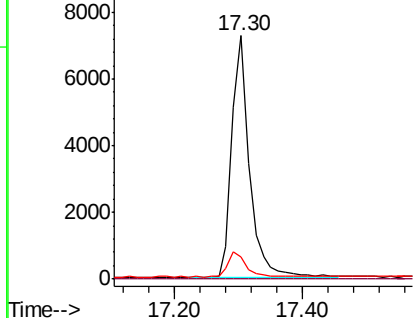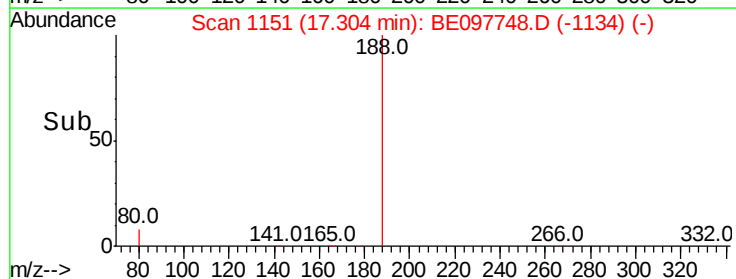



#25

Fluoranthene-d10

Concen: 0.331 ng

RT: 19.33 min Scan# 1437

Delta R.T. -0.00 min

Lab File: BE097748.D

Acq: 5 Oct 2018 10:36

Instrument :

BNA_E

ClientSampleId :


Tot Ion:212 Resp: 57773

Ion Ratio Lower Upper

212 100

106 2.6 2.2 3.2




104 1.5 1.2 1.8

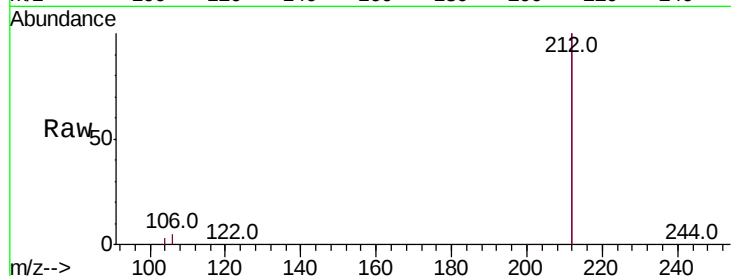

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

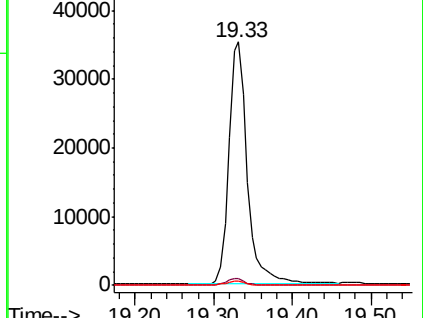

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.49 min Scan# 1673

Delta R.T. -0.00 min

Lab File: BE097748.D

Acq: 5 Oct 2018 10:36


Tgt Ion:240 Resp: 14703

Ion Ratio Lower Upper

240 100

120 6.8 4.7 7.1



236 28.0 20.8 31.2




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E




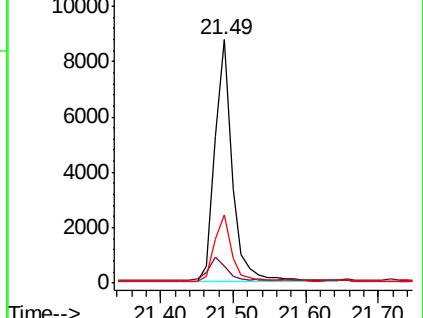




#29
 Terphenyl-d14
 Concen: 0.322 ng
 RT: 19.93 min Scan# 1541
 Delta R.T. -0.01 min
 Lab File: BE097748.D
 Acq: 5 Oct 2018 10:36




Instrument :
 BNA_E
 ClientSampleId :




Tot Ion:244 Resp: 9671
 Ion Ratio Lower Upper
 244 100
 212 35.1 25.8 38.8
 122 11.4 8.7 13.1

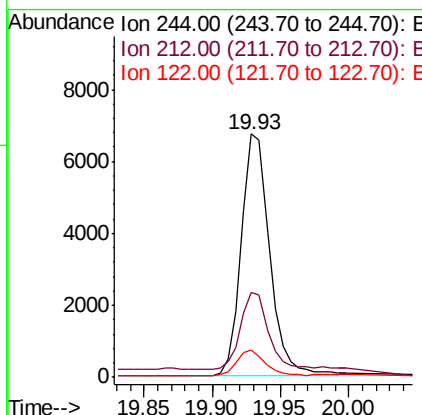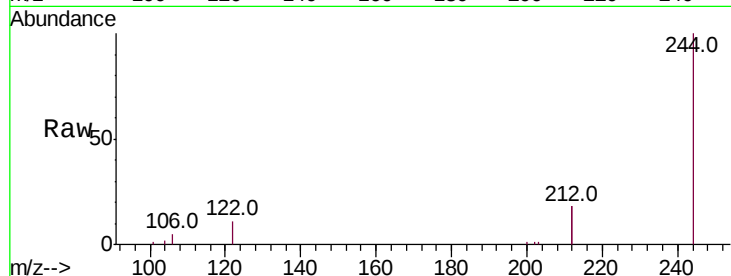

#32
 Bis(2-ethylhexyl)phthalate
 Concen: 0.020 ng
 RT: 21.41 min Scan# 1667
 Delta R.T. 0.00 min
 Lab File: BE097748.D
 Acq: 5 Oct 2018 10:36

Tgt Ion:149 Resp: 591
 Ion Ratio Lower Upper
 149 100
 167 3.7 5.5 8.3#
 279 0.0 0.9 1.3#

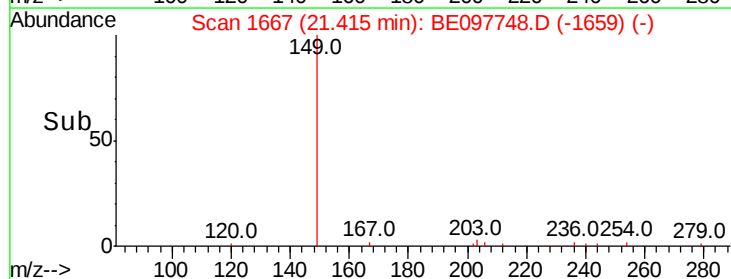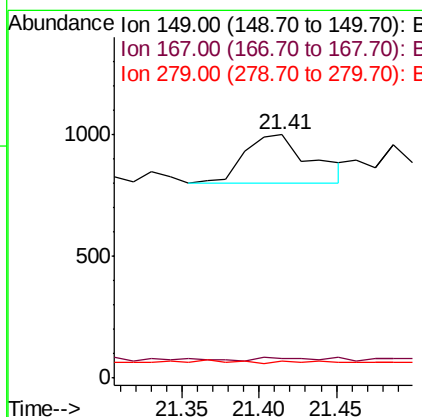

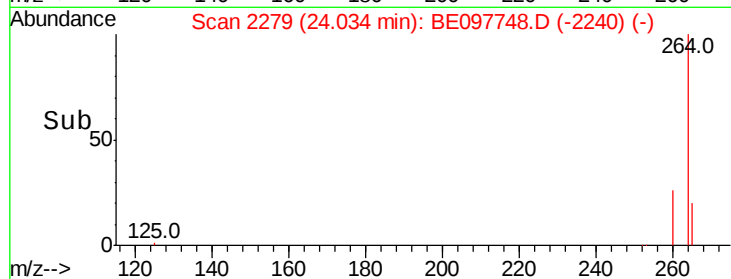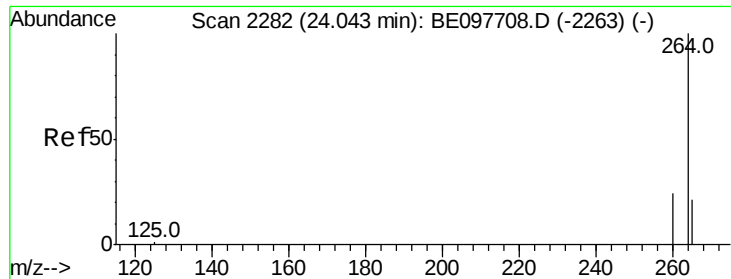

#34

Pervlene-d12

Concen: 0.400 ng

RT: 24.03 min Scan# 2279

Delta R.T. -0.01 min

Lab File: BE097748.D

Acq: 5 Oct 2018 10:36

Instrument :

BNA_E

ClientSampleId :

Tot Ion:264 Resp: 15485

Ion Ratio Lower Upper

264 100

260 26.1 19.1 28.7

265 31.8 21.9 32.9

