

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE100518\
 Data File : BE097783.D
 Acq On : 6 Oct 2018 9:25
 Operator : SJ/JU
 Sample : J5189-12DL 5X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 TT-DUP01-20180928DL

Quant Time: Oct 08 06:39:21 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE100318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 08 06:37:06 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	4596	0.40	ng	-0.01
7) Naphthalene-d8	10.69	136	18240	0.40	ng	0.00
13) Acenaphthene-d10	14.56	164	11036	0.40	ng	0.00
19) Phenanthrene-d10	17.29	188	30769	0.40	ng	-0.01
27) Chrysene-d12	21.47	240	34383	0.40	ng	-0.01
34) Perylene-d12	24.03	264	34183	0.40	ng	-0.02
System Monitoring Compounds						
4) 2-Fluorophenol	5.47	112	457	0.04	ng	0.00
5) Phenol-d6	7.05	99	354	0.02	ng	0.00
8) Nitrobenzene-d5	9.04	82	882	0.15	ng	0.00
11) 2-Methylnaphthalene-d10	12.30	152	2516	0.09	ng	0.00
14) 2,4,6-Tribromophenol	16.04	330	208	0.10	ng	0.00
15) 2-Fluorobiphenyl	13.17	172	4639	0.10	ng	-0.02
25) Fluoranthene-d10	19.33	212	33168	0.09	ng	0.00
29) Terphenyl-d14	19.92	244	9577	0.14	ng	-0.01
Target Compounds						
2) 1,4-Dioxane	3.40	88	9353	1.021	ng	97
32) Bis(2-ethylhexyl)phthalate	21.40	149	1906	0.028	ng	# 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE100518\
Data File : BE097783.D
Acq On : 6 Oct 2018 9:25
Operator : SJ/JU
Sample : J5189-12DL 5X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
TT-DUP01-20180928DL

Quant Time: Oct 08 06:39:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE100318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 08 06:37:06 2018
Response via : Initial Calibration

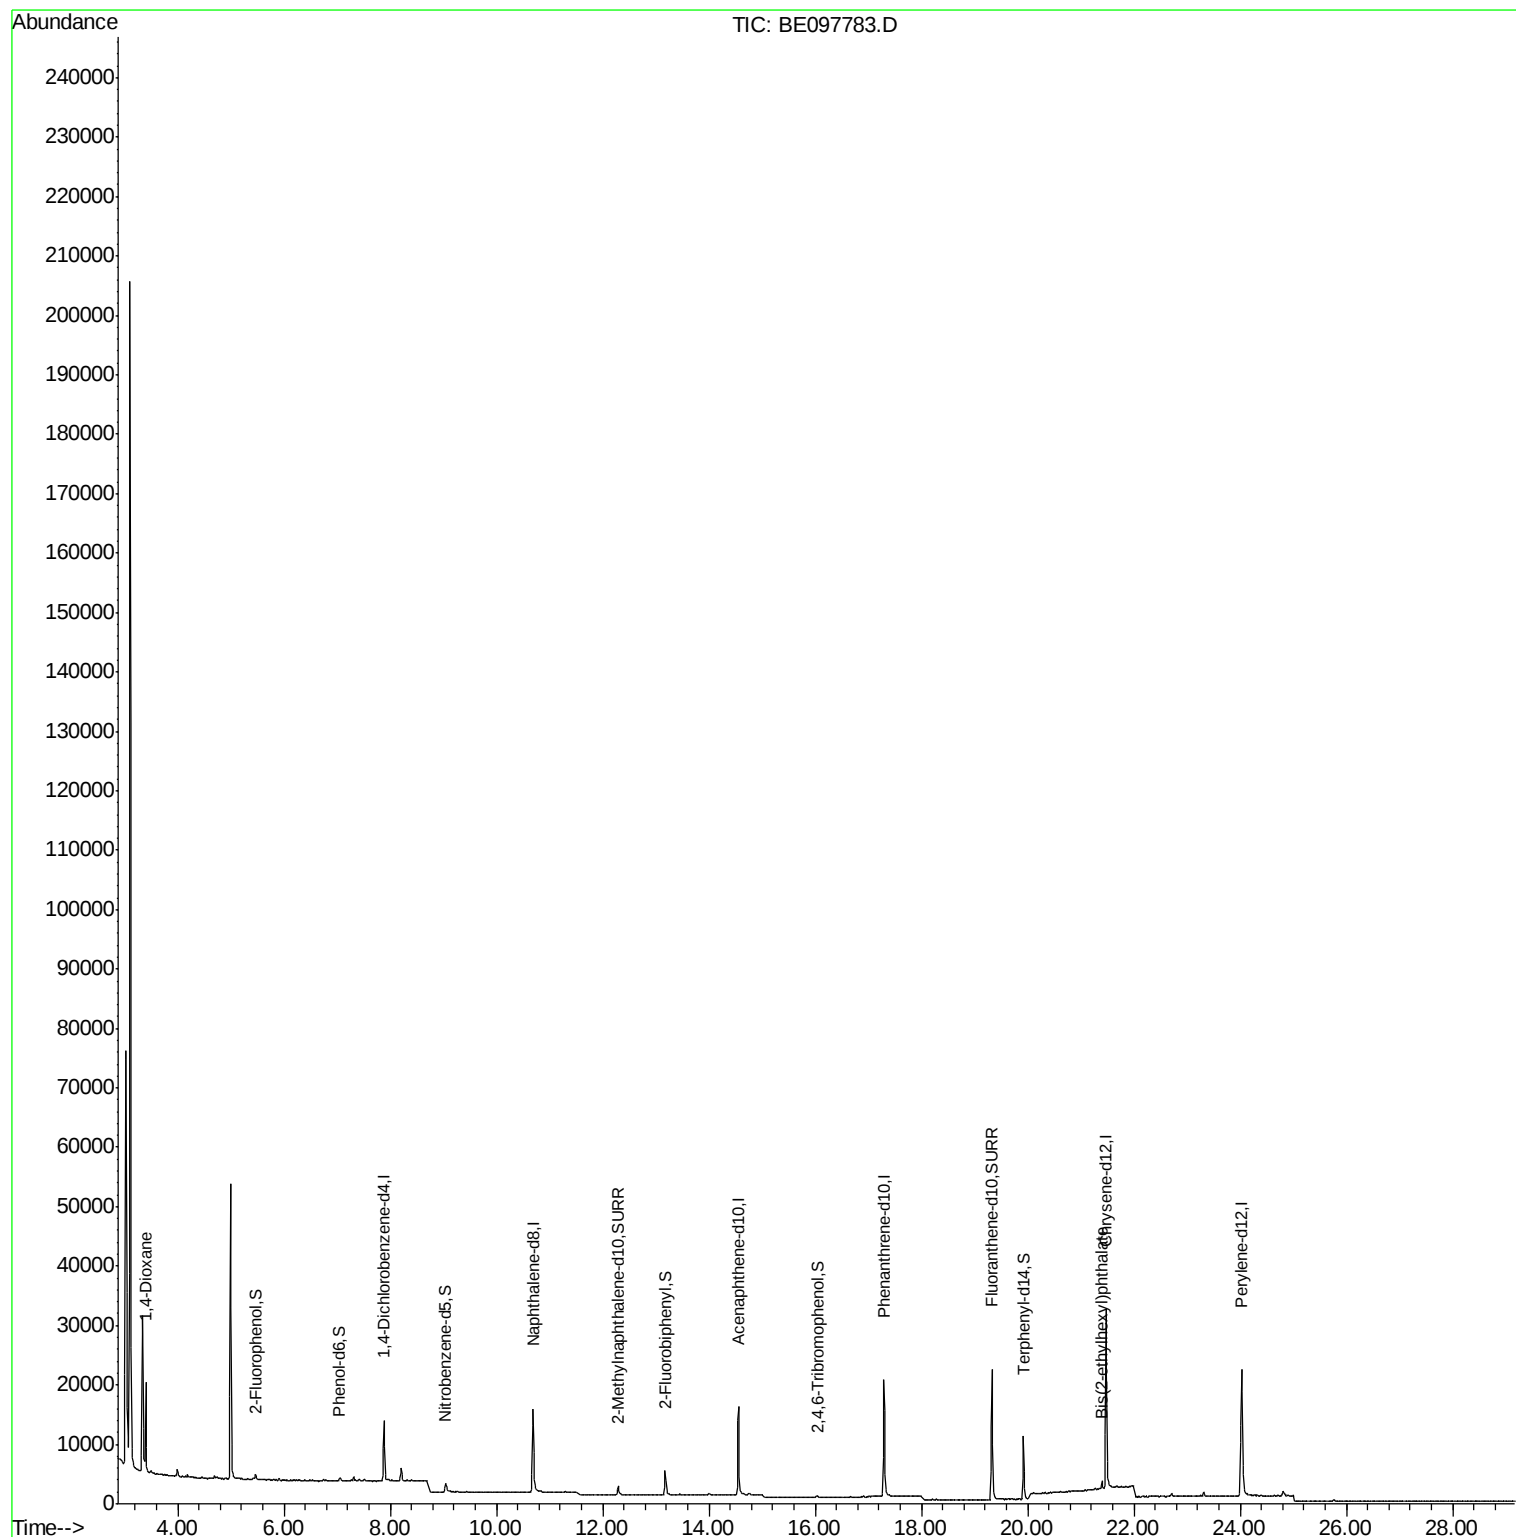



#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.89 min Scan# 436

Delta R.T. -0.01 min

Lab File: BE097783.D

Acq: 6 Oct 2018 9:25

Instrument :

BNA_E

ClientSampleId :

TT-DUP01-20180928DL


Tgt Ion:152 Resp: 4596

Ion Ratio Lower Upper

152 100

150 152.7 120.9 181.3




115 62.4 46.6 69.8

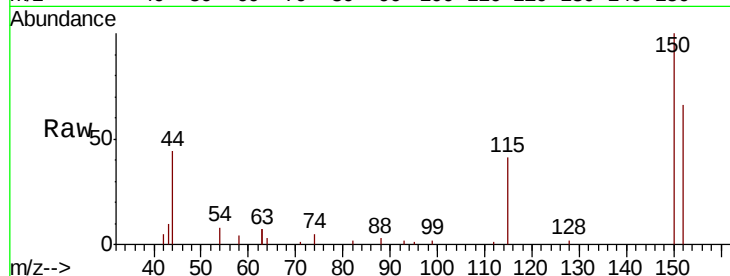

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

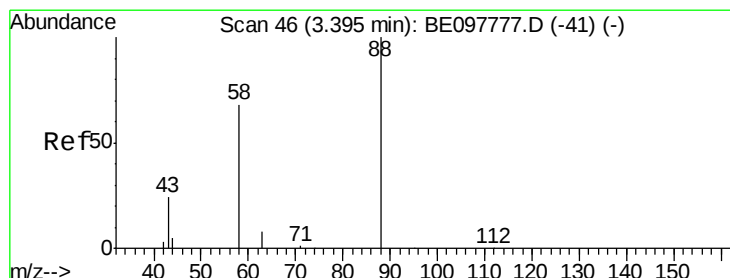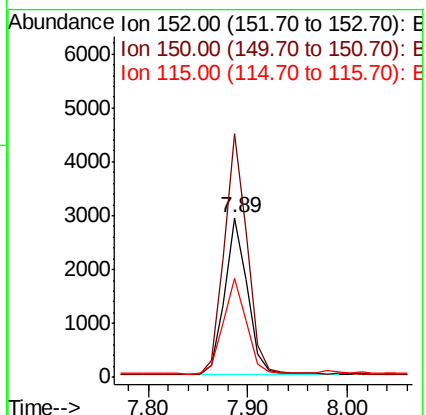

#2

1,4-Dioxane

Concen: 1.021 ng

RT: 3.40 min Scan# 46

Delta R.T. 0.00 min

Lab File: BE097783.D

Acq: 6 Oct 2018 9:25


Tgt Ion: 88 Resp: 9353

Ion Ratio Lower Upper

88 100

58 86.1 70.8 106.2



43 38.6 33.3 49.9

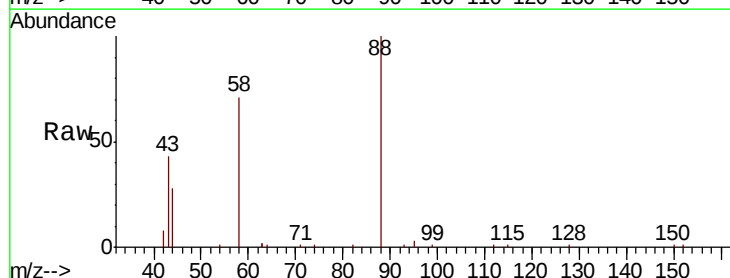


Abundance Ion 88.00 (87.70 to 88.70): BE0

Ion 58.00 (57.70 to 58.70): BE0

Ion 43.00 (42.70 to 43.70): BE0

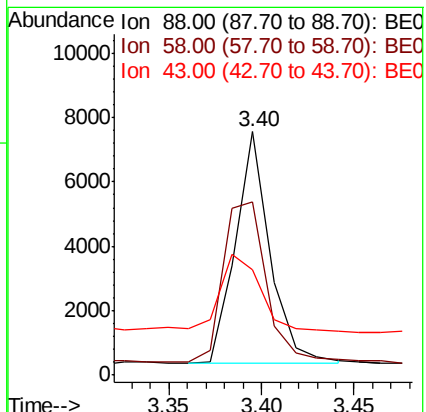

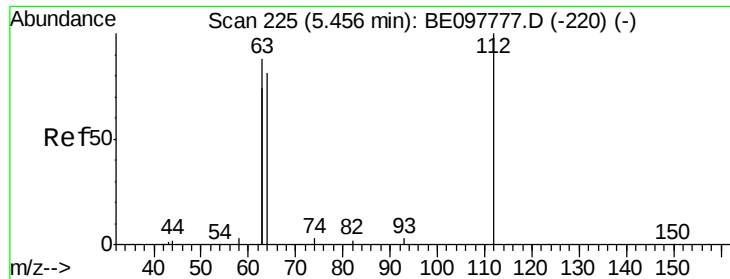

#4

2-Fluorophenol

Concen: 0.042 ng

RT: 5.47 min Scan# 226

Delta R.T. 0.00 min

Lab File: BE097783.D

Acq: 6 Oct 2018 9:25

Instrument :

BNA_E

ClientSampleId :

TT-DUP01-20180928DL


Tgt Ion: 112 Resp: 457

Ion Ratio Lower Upper

112 100

64 82.1 56.6 84.8

63 155.8 119.4 179.0

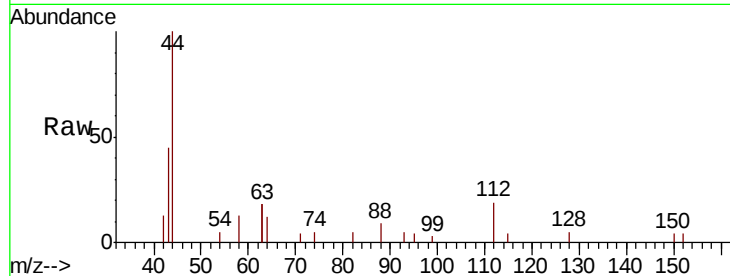

Abundance Ion 112.00 (111.70 to 112.70): BE0

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

800

600



400

200

0

5.40 5.50

Time-->

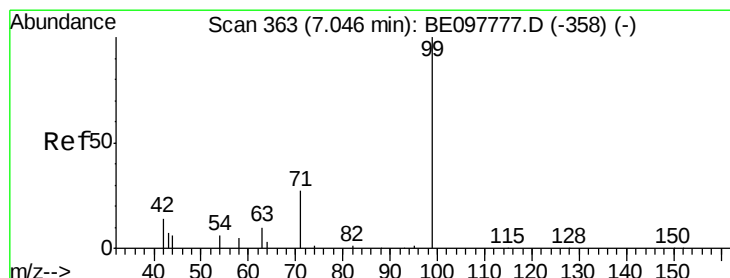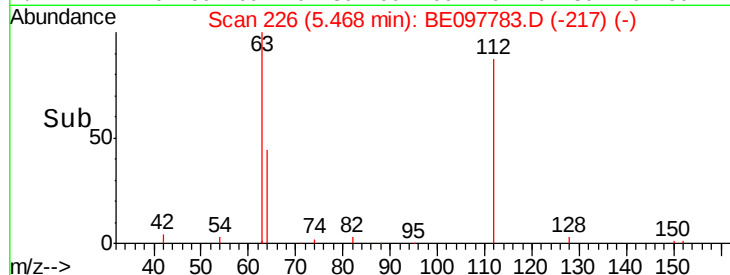

#5

Phenol-d6

Concen: 0.021 ng

RT: 7.05 min Scan# 363

Delta R.T. 0.00 min

Lab File: BE097783.D

Acq: 6 Oct 2018 9:25


Tgt Ion: 99 Resp: 354

Ion Ratio Lower Upper

99 100

42 92.7 19.9 29.9#

71 50.8 25.4 38.2#

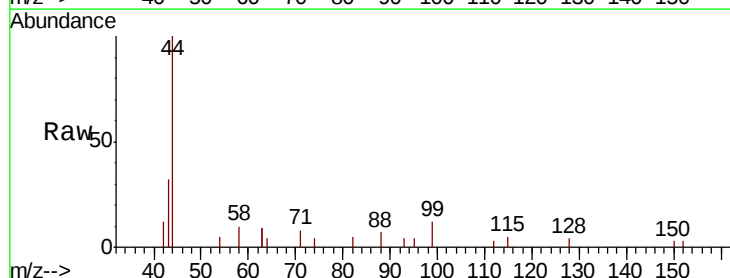

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

300

250

200

150


100


50

0

6.95 7.00 7.05 7.10 7.15

Time-->



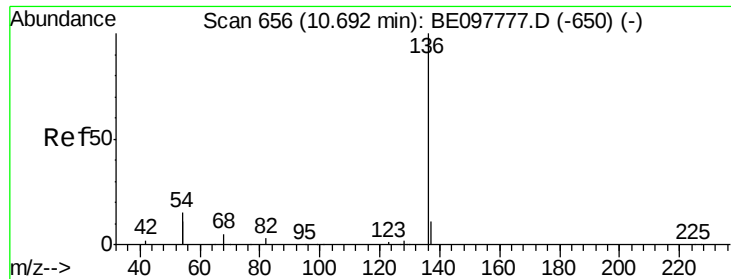

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.69 min Scan# 656

Delta R.T. 0.00 min

Lab File: BE097783.D

Acq: 6 Oct 2018 9:25

Instrument :

BNA_E

ClientSampleId :

TT-DUP01-20180928DL

Tgt Ion: 136 Resp: 18240


Ion Ratio Lower Upper

136 100

137 11.5 9.0 13.4

54 35.7 37.8 56.6#

68 6.5 6.4 9.6



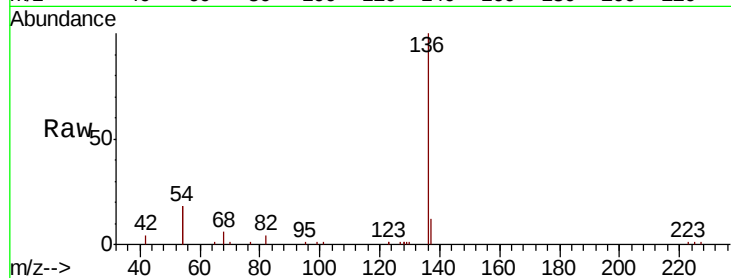


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

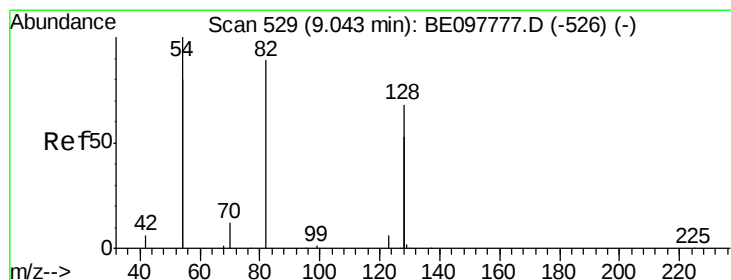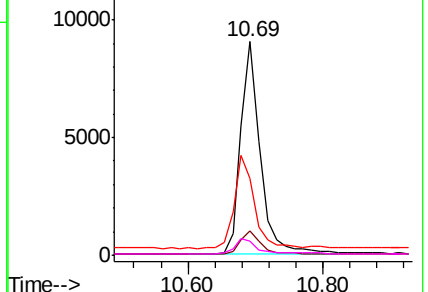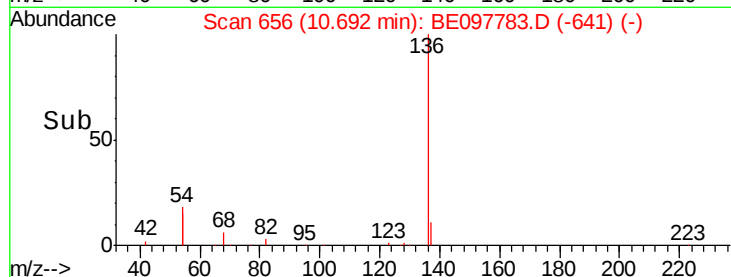

#8

Nitrobenzene-d5

Concen: 0.149 ng

RT: 9.04 min Scan# 529

Delta R.T. 0.00 min

Lab File: BE097783.D

Acq: 6 Oct 2018 9:25


Tgt Ion: 82 Resp: 882

Ion Ratio Lower Upper

82 100

128 168.7 97.0 145.4#



54 286.8 206.9 310.3

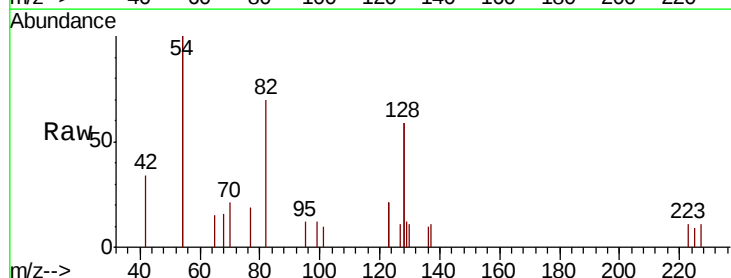


Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0

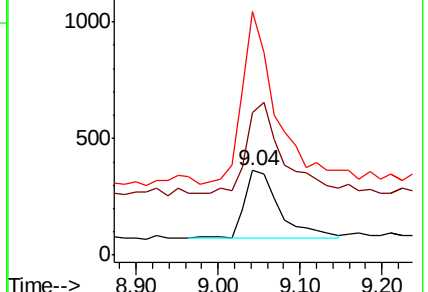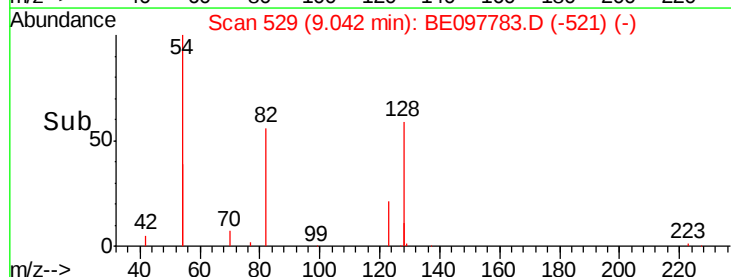

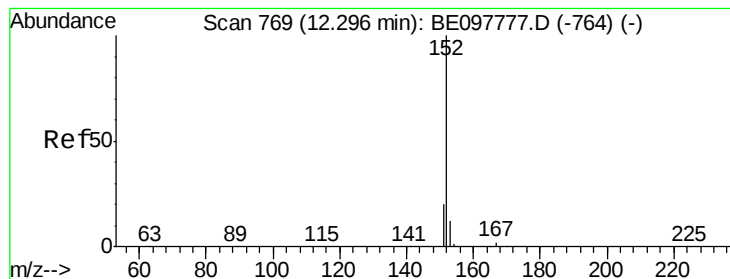

#11

2-Methylnaphthalene-d10

Concen: 0.087 ng

RT: 12.30 min Scan# 769

Delta R.T. -0.00 min

Lab File: BE097783.D

Acq: 6 Oct 2018 9:25

Instrument :

BNA_E

ClientSampleId :


TT-DUP01-20180928DL

Tgt Ion:152 Resp: 2516

Ion Ratio Lower Upper

152 100

151 21.1 15.4 23.2

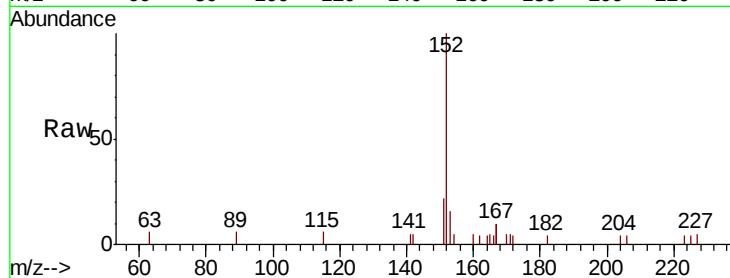

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

12.30



1000

500

0

Time-->

12.20 12.30 12.40 12.50

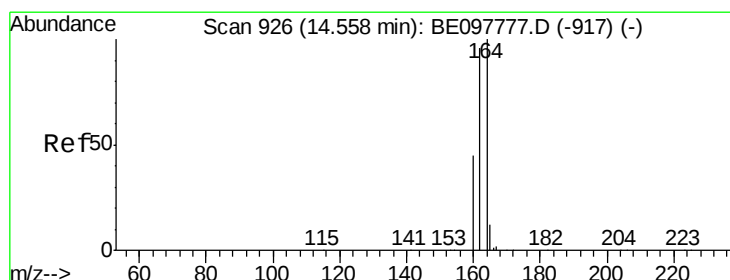

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.56 min Scan# 926

Delta R.T. -0.00 min

Lab File: BE097783.D

Acq: 6 Oct 2018 9:25


Tgt Ion:164 Resp: 11036

Ion Ratio Lower Upper

164 100

162 89.2 78.6 117.8

160 45.5 37.8 56.6

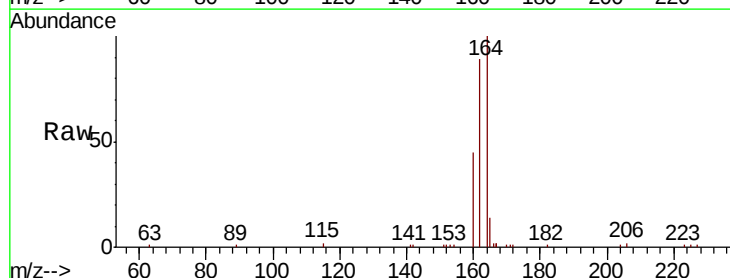

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

8000

6000


4000


2000

0

Time-->

14.40 14.50 14.60









#14
 2,4,6-Tribromophenol
 Concen: 0.104 ng
 RT: 16.04 min Scan# 1043
 Delta R.T. 0.00 min
 Lab File: BE097783.D
 Acq: 6 Oct 2018 9:25

Instrument :
 BNA_E
 ClientSampleId :
 TT-DUP01-20180928DL

Tgt Ion:330 Resp: 208
 Ion Ratio Lower Upper
 330 100
 332 124.5 83.5 125.3
 141 41.8 34.9 52.3

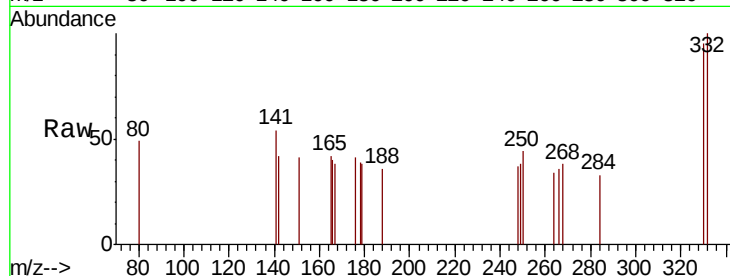


Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

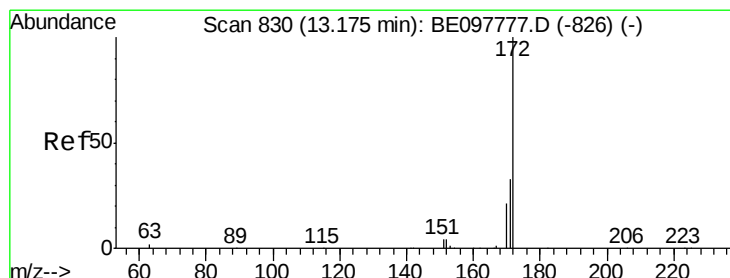
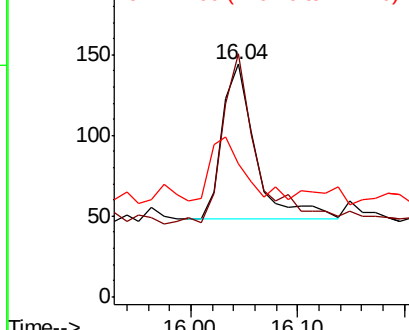



#15
 2-Fluorobiphenyl
 Concen: 0.095 ng
 RT: 13.17 min Scan# 830
 Delta R.T. -0.02 min
 Lab File: BE097783.D
 Acq: 6 Oct 2018 9:25

Tgt Ion:172 Resp: 4639
 Ion Ratio Lower Upper
 172 100
 171 34.9 25.2 37.8
 170 24.4 16.2 24.2#

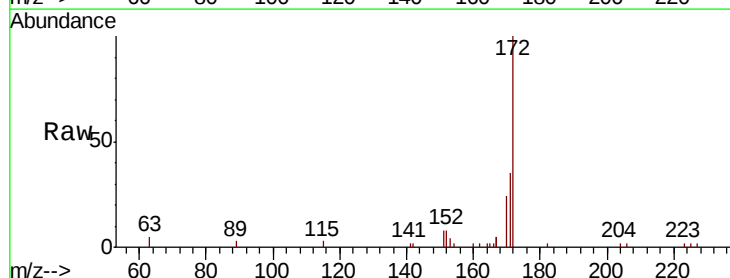

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

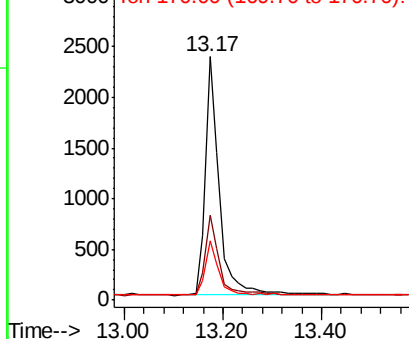

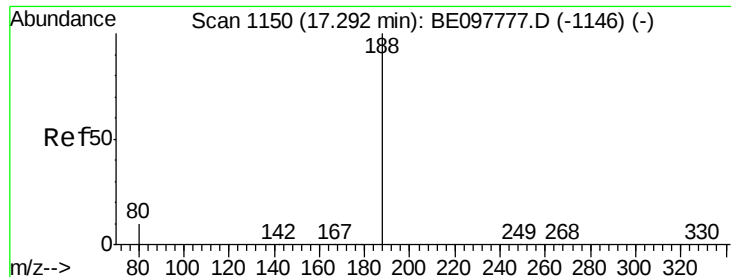

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.29 min Scan# 1150

Delta R.T. -0.01 min

Lab File: BE097783.D

Acq: 6 Oct 2018 9:25

Instrument :

BNA_E

ClientSampleId :

TT-DUP01-20180928DL


Tgt Ion:188 Resp: 30769

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 11.8 6.6 9.8#

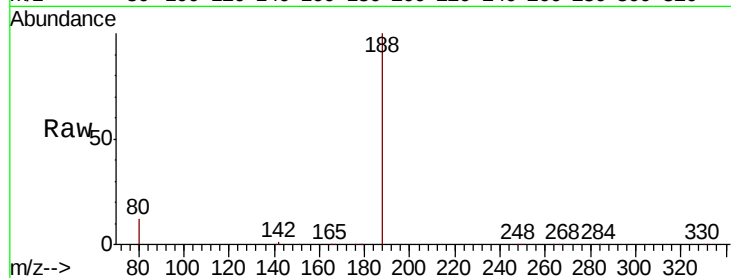

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

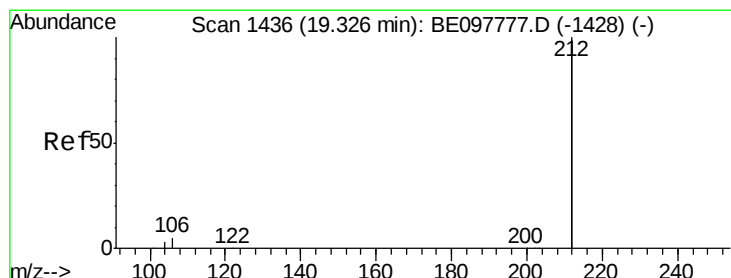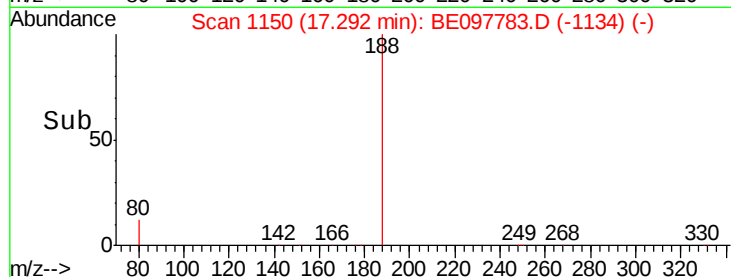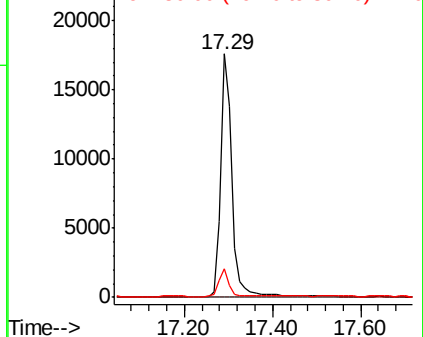

#25

Fluoranthene-d10

Concen: 0.085 ng

RT: 19.33 min Scan# 1436

Delta R.T. -0.01 min

Lab File: BE097783.D

Acq: 6 Oct 2018 9:25


Tgt Ion:212 Resp: 33168

Ion Ratio Lower Upper

212 100

106 2.6 2.2 3.2



104 1.6 1.2 1.8

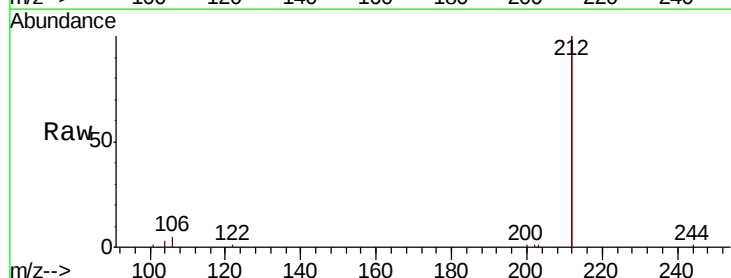


Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

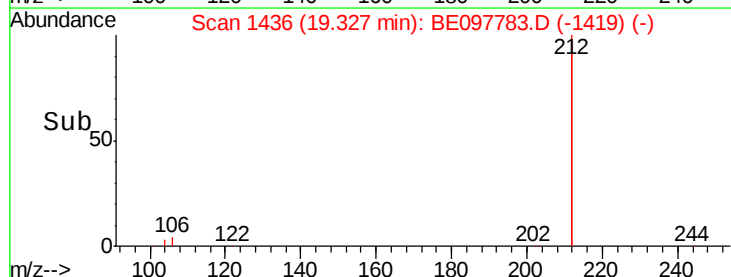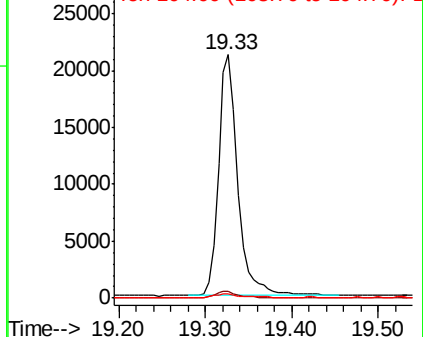

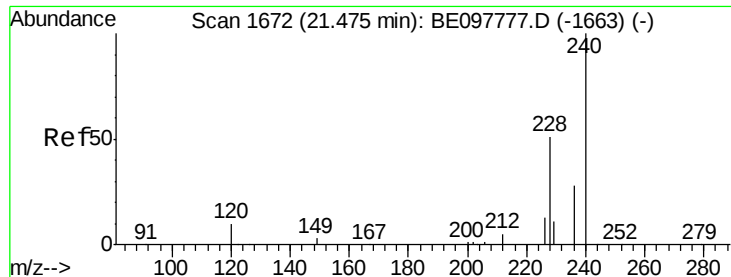

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.47 min Scan# 1672

Delta R.T. -0.01 min

Lab File: BE097783.D

Acq: 6 Oct 2018 9:25

Instrument :

BNA_E

ClientSampleId :

TT-DUP01-20180928DL


Tgt Ion:240 Resp: 34383

Ion Ratio Lower Upper

240 100

120 9.3 4.7 7.1#




236 28.0 20.8 31.2

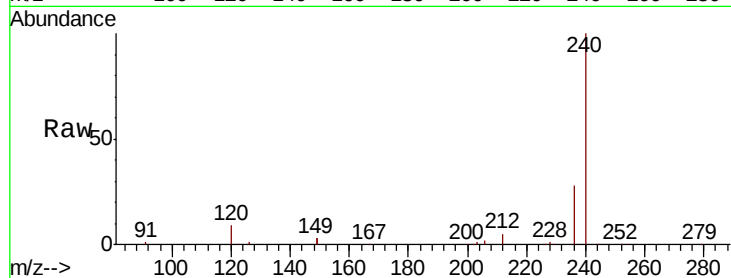

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

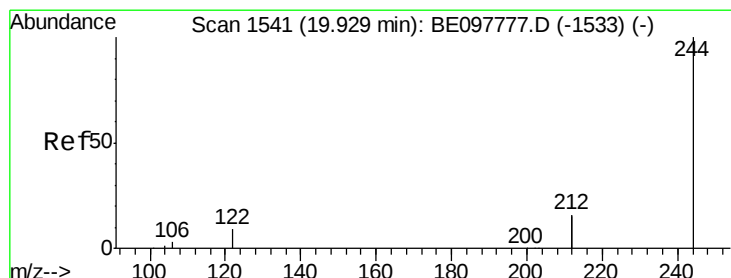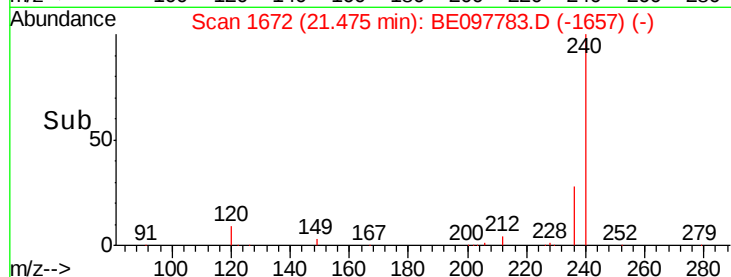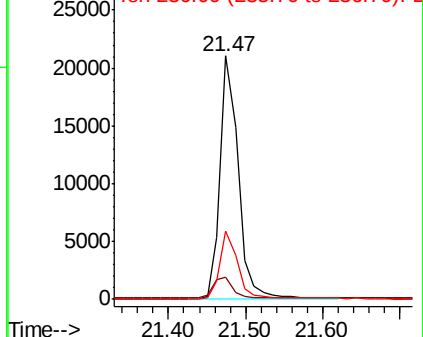

#29

Terphenyl-d14

Concen: 0.136 ng

RT: 19.92 min Scan# 1540

Delta R.T. -0.01 min

Lab File: BE097783.D

Acq: 6 Oct 2018 9:25


Tgt Ion:244 Resp: 9577

Ion Ratio Lower Upper

244 100

212 33.3 25.8 38.8



122 10.7 8.7 13.1

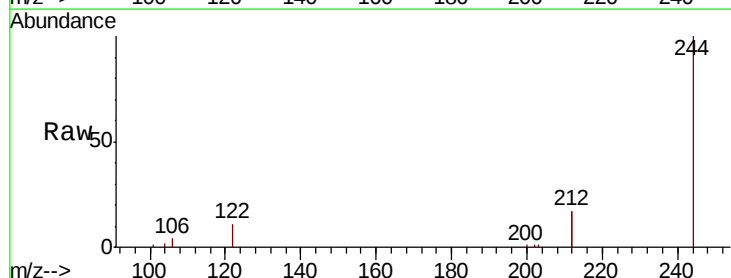


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

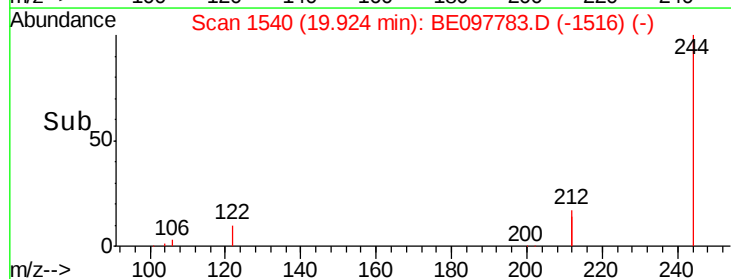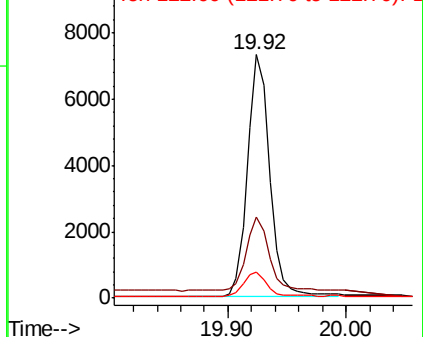







#32
 Bis(2-ethylhexyl)phthalate
 Concen: 0.028 ng
 RT: 21.40 min Scan# 1666
 Delta R.T. -0.01 min
 Lab File: BE097783.D
 Acq: 6 Oct 2018 9:25

Instrument :
 BNA_E
 ClientSampleID :
 TT-DUP01-20180928DL

Tgt Ion: 149 Resp: 1906
 Ion Ratio Lower Upper
 149 100
 167 8.7 5.5 8.3#
 279 0.0 0.9 1.3#

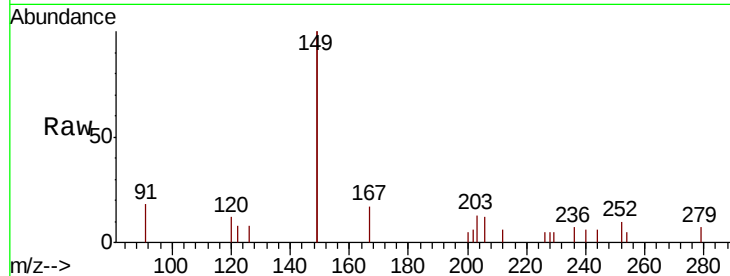


Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 167.00 (166.70 to 167.70): E
 Ion 279.00 (278.70 to 279.70): E

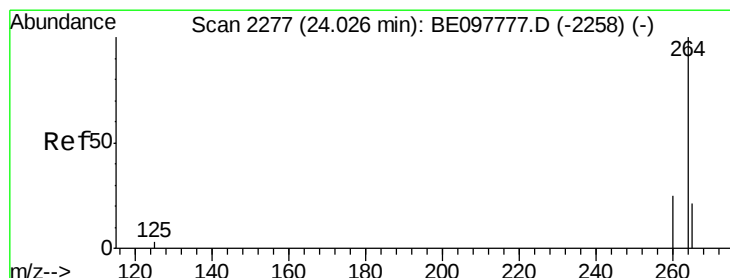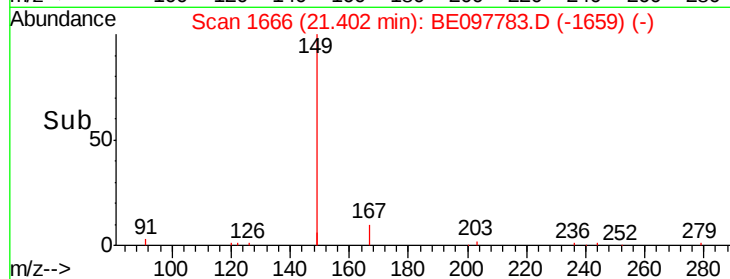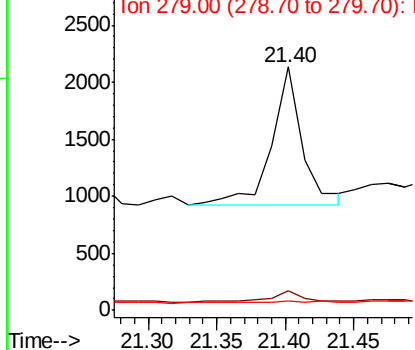

#34
 Perylene-d12
 Concen: 0.400 ng
 RT: 24.03 min Scan# 2277
 Delta R.T. -0.02 min
 Lab File: BE097783.D
 Acq: 6 Oct 2018 9:25

Tgt Ion: 264 Resp: 34183
 Ion Ratio Lower Upper
 264 100
 260 24.9 19.1 28.7
 265 26.6 21.9 32.9

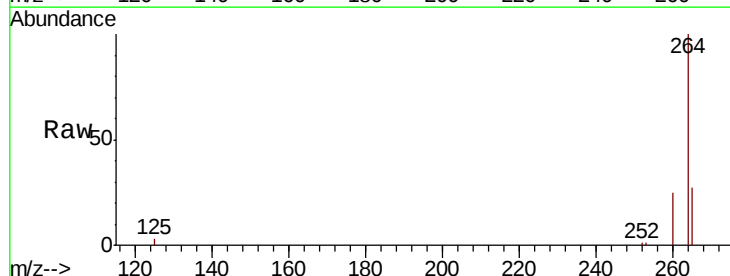

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

