
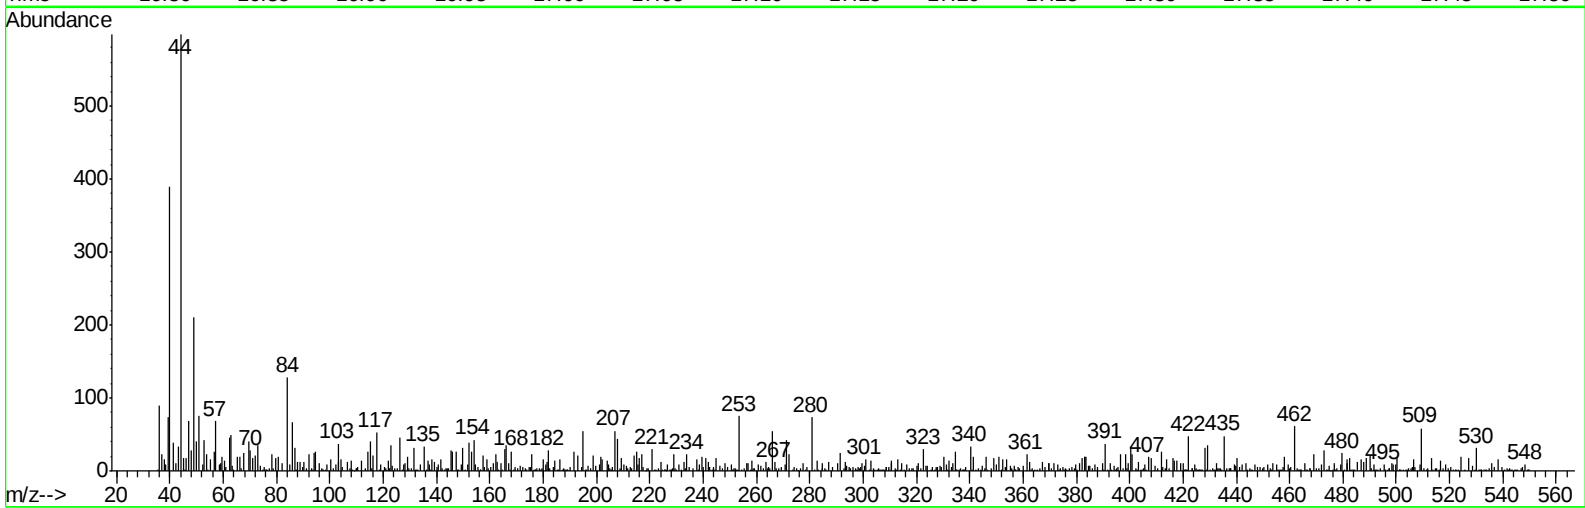


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE100518\
Data File : BE097744.D
Acq On : 5 Oct 2018 8:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 08:33:25 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 22 13:32:18 2018
Response via : Initial Calibration

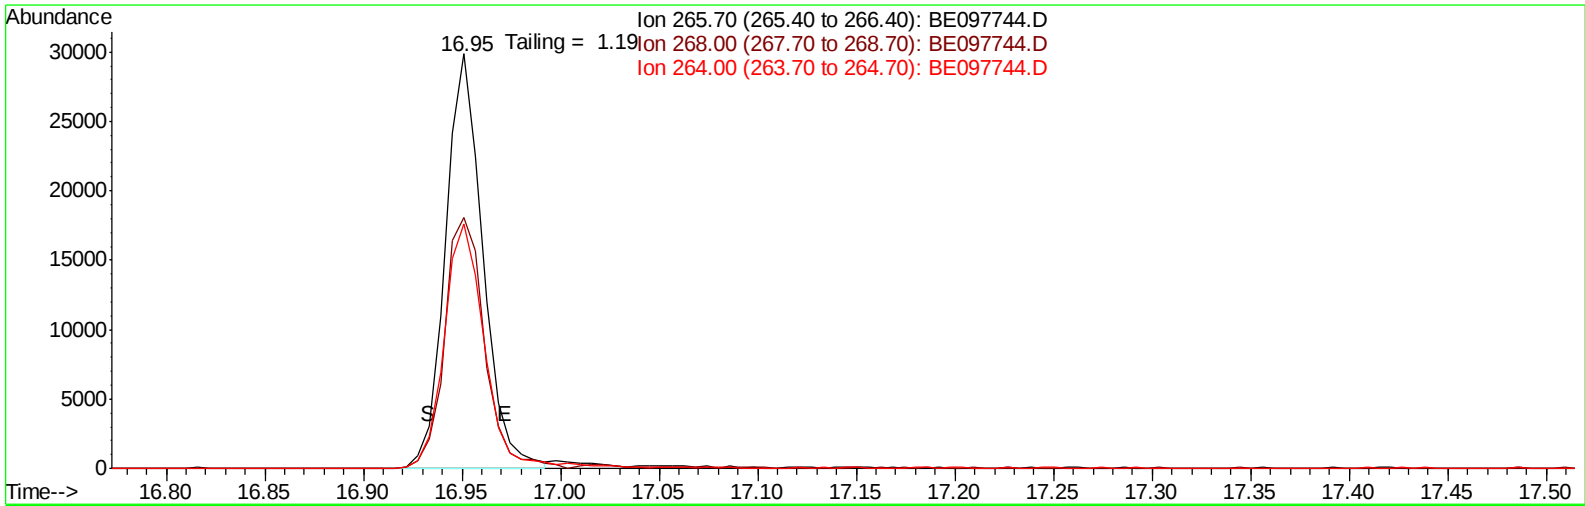

TIC: BE097744.D

(69) Pentachlorophenol (C)



11.058min (+0.030) 289.50ng

response 47

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	7.27#
264.00	61.90	18.18#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE100518\
 Data File : BE097744.D
 Acq On : 5 Oct 2018 8:08
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 08:33:25 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 22 13:32:18 2018
 Response via : Initial Calibration

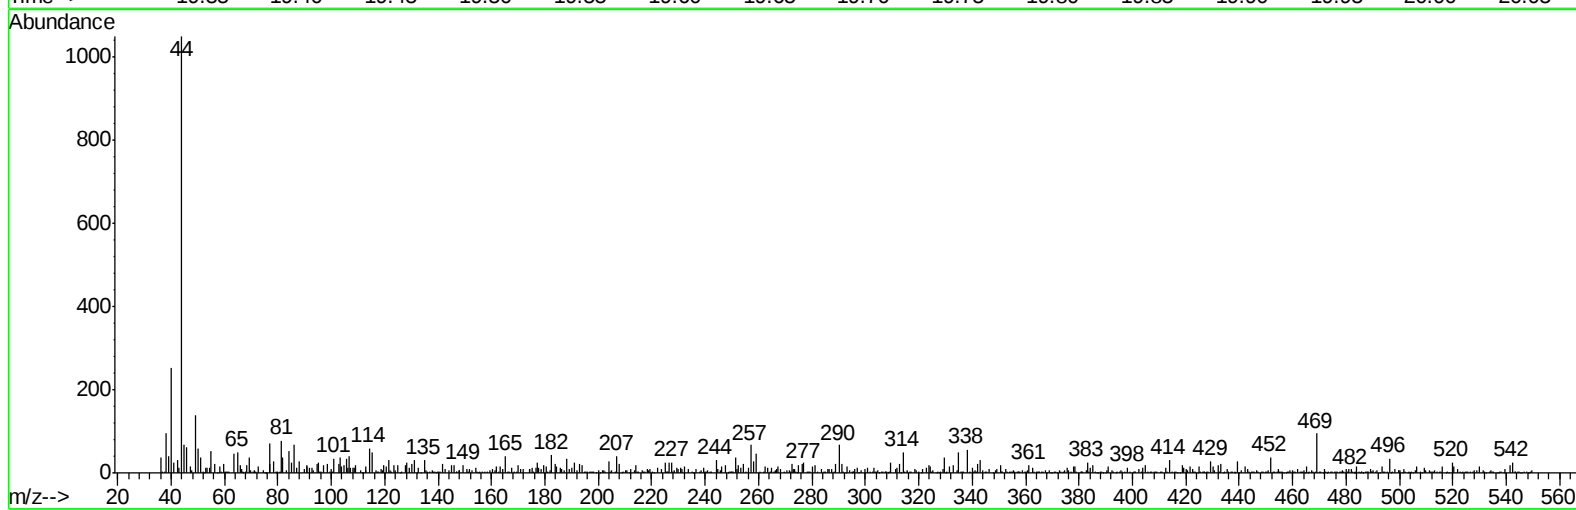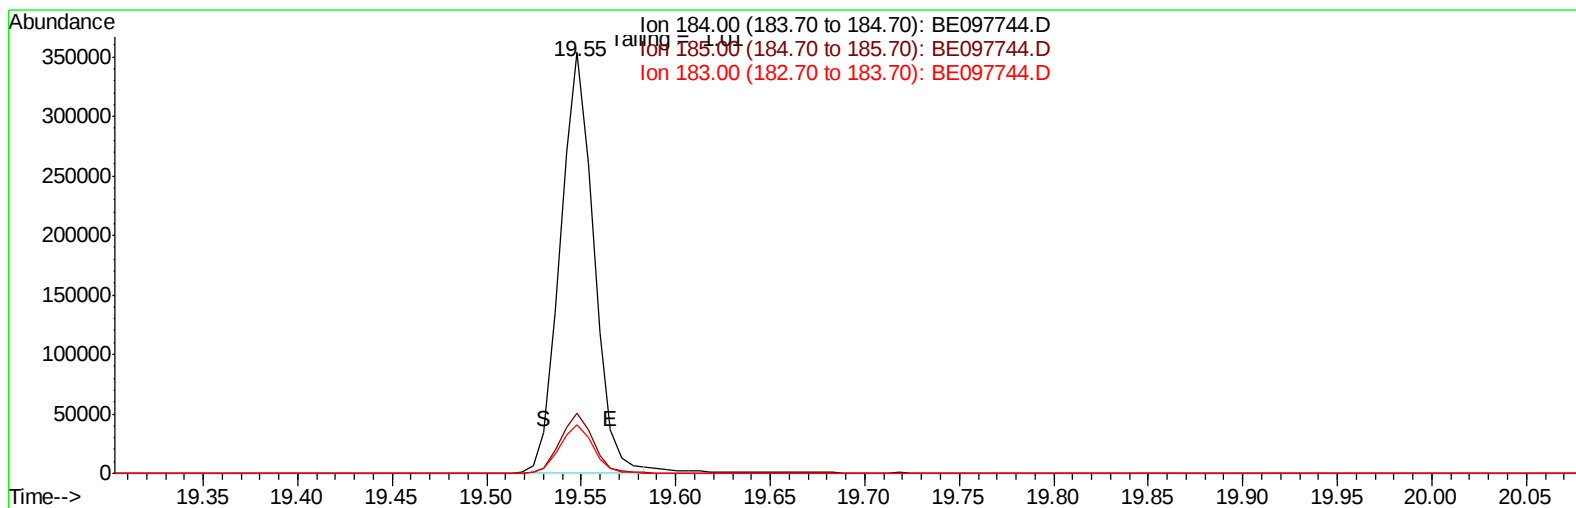

TIC: BE097744.D

(76) Benzidine

12.585min (+0.040) 12.80ng

response 30

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	33.33#
183.00	11.60	0.00#
0.00	0.00	0.00