
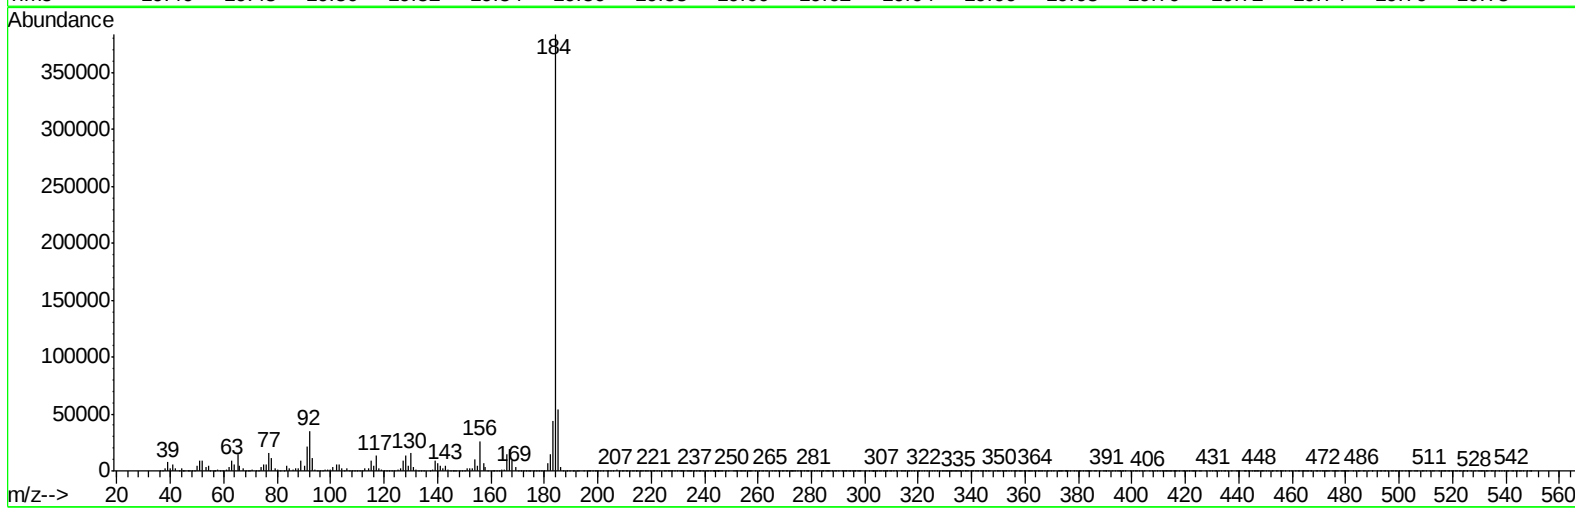


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE100518\
Data File : BE097758.D
Acq On : 5 Oct 2018 17:02
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 08:47:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 22 13:32:18 2018
Response via : Initial Calibration

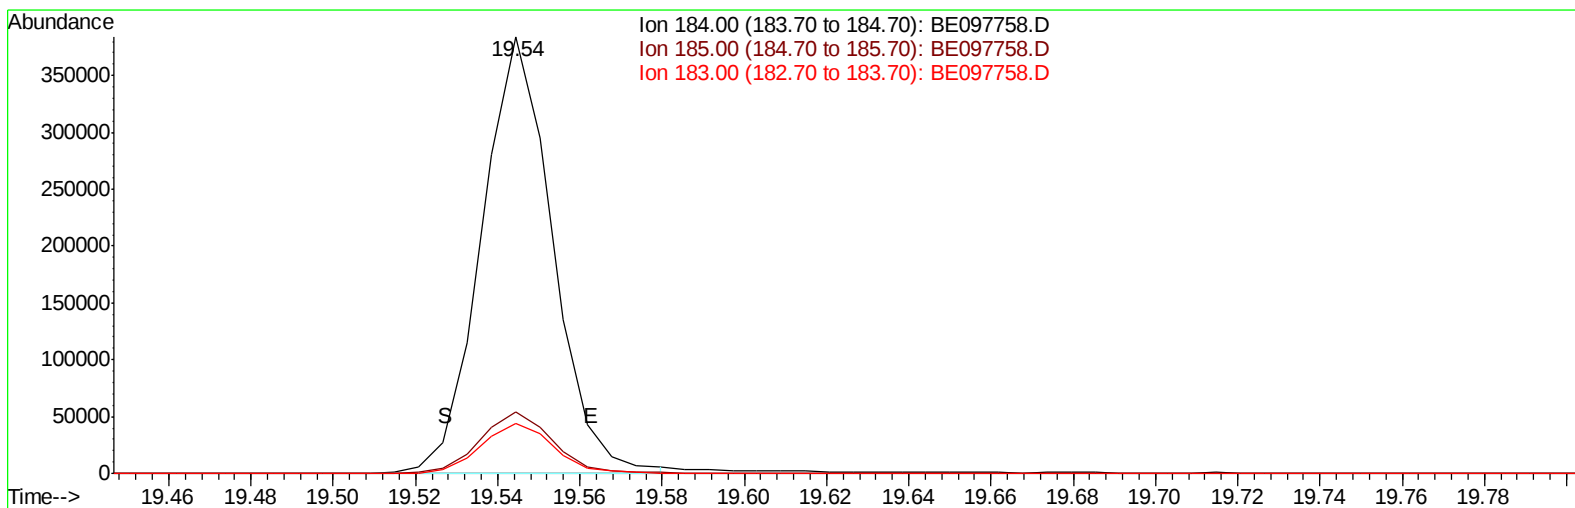

TIC: BE097758.D

(76) Benzidine



19.544min (+6.999) 712348.51ng m

response 462304

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.01
183.00	11.60	11.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE100518\
Data File : BE097758.D
Acq On : 5 Oct 2018 17:02
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 08:47:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 22 13:32:18 2018
Response via : Initial Calibration

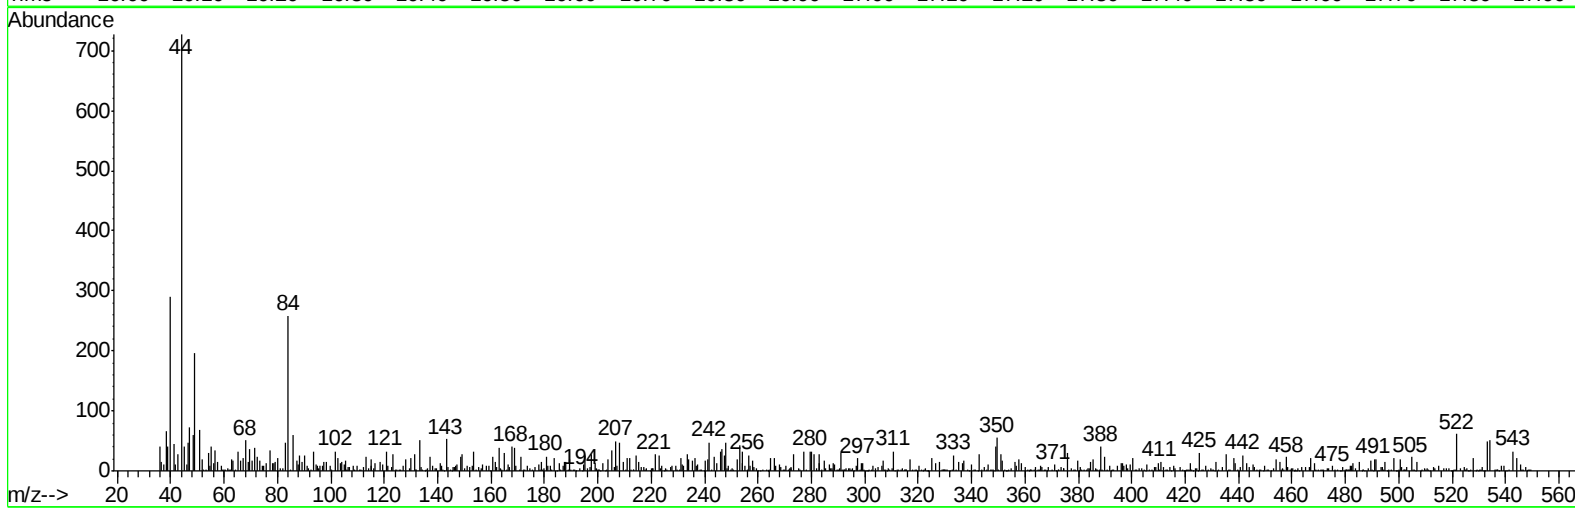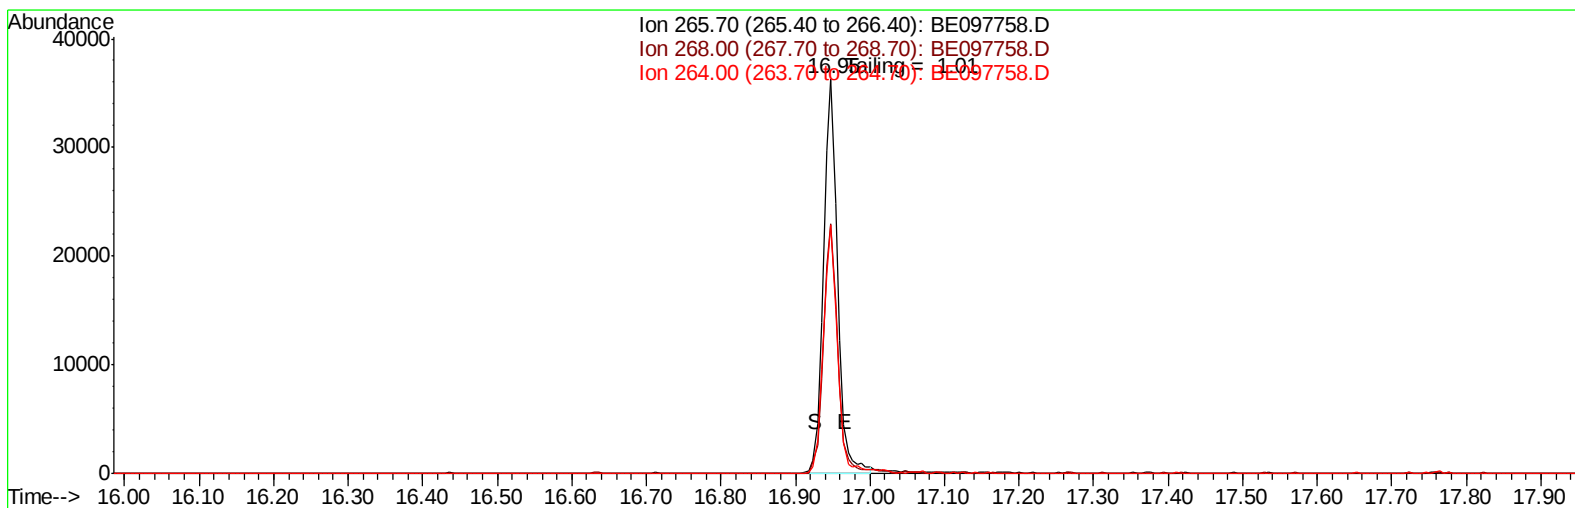

TIC: BE097758.D

(69) Pentachlorophenol (C)

11.072min (+0.044) 64.93ng

response 11

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	81.82#
264.00	61.90	13.64#
0.00	0.00	0.00