

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE100518\
 Data File : BE097778.D
 Acq On : 6 Oct 2018 6:20
 Operator : SJ/JU
 Sample : J5284-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 RE-125D2-2018001

Quant Time: Oct 08 06:45:37 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE100318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 08 06:37:06 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	4073	0.40	ng	0.00
7) Naphthalene-d8	10.70	136	16210	0.40	ng	0.01
13) Acenaphthene-d10	14.56	164	9152	0.40	ng	0.00
19) Phenanthrene-d10	17.30	188	26699	0.40	ng	0.00
27) Chrysene-d12	21.49	240	33433	0.40	ng	0.00
34) Perylene-d12	24.03	264	31383	0.40	ng	0.00

System Monitoring Compounds						
4) 2-Fluorophenol	5.47	112	1733	0.18	ng	0.00
5) Phenol-d6	7.06	99	1417	0.10	ng	0.01
8) Nitrobenzene-d5	9.05	82	4110	0.78	ng	0.01
11) 2-Methylnaphthalene-d10	12.30	152	10197	0.40	ng	0.00
14) 2,4,6-Tribromophenol	16.04	330	876	0.53	ng	0.00
15) 2-Fluorobiphenyl	13.19	172	18965	0.47	ng	0.00
25) Fluoranthene-d10	19.33	212	147528	0.44	ng	0.00
29) Terphenyl-d14	19.93	244	30132	0.44	ng	0.00


Target Compounds				Qvalue		
2) 1,4-Dioxane	3.39	88	49429	6.090	ng	97
6) bis(2-Chloroethyl)ether	7.32	93	341	0.022	ng	# 78
9) Naphthalene	10.76	128	6244	0.038	ng	# 97
12) 2-Methylnaphthalene	12.38	142	550	0.021	ng	# 89
32) Bis(2-ethylhexyl)phthalate	21.40	149	3699	0.056	ng	# 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE100518\
Data File : BE097778.D
Acq On : 6 Oct 2018 6:20
Operator : SJ/JU
Sample : J5284-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
RE-125D2-2018001

Quant Time: Oct 08 06:45:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE100318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 08 06:37:06 2018
Response via : Initial Calibration

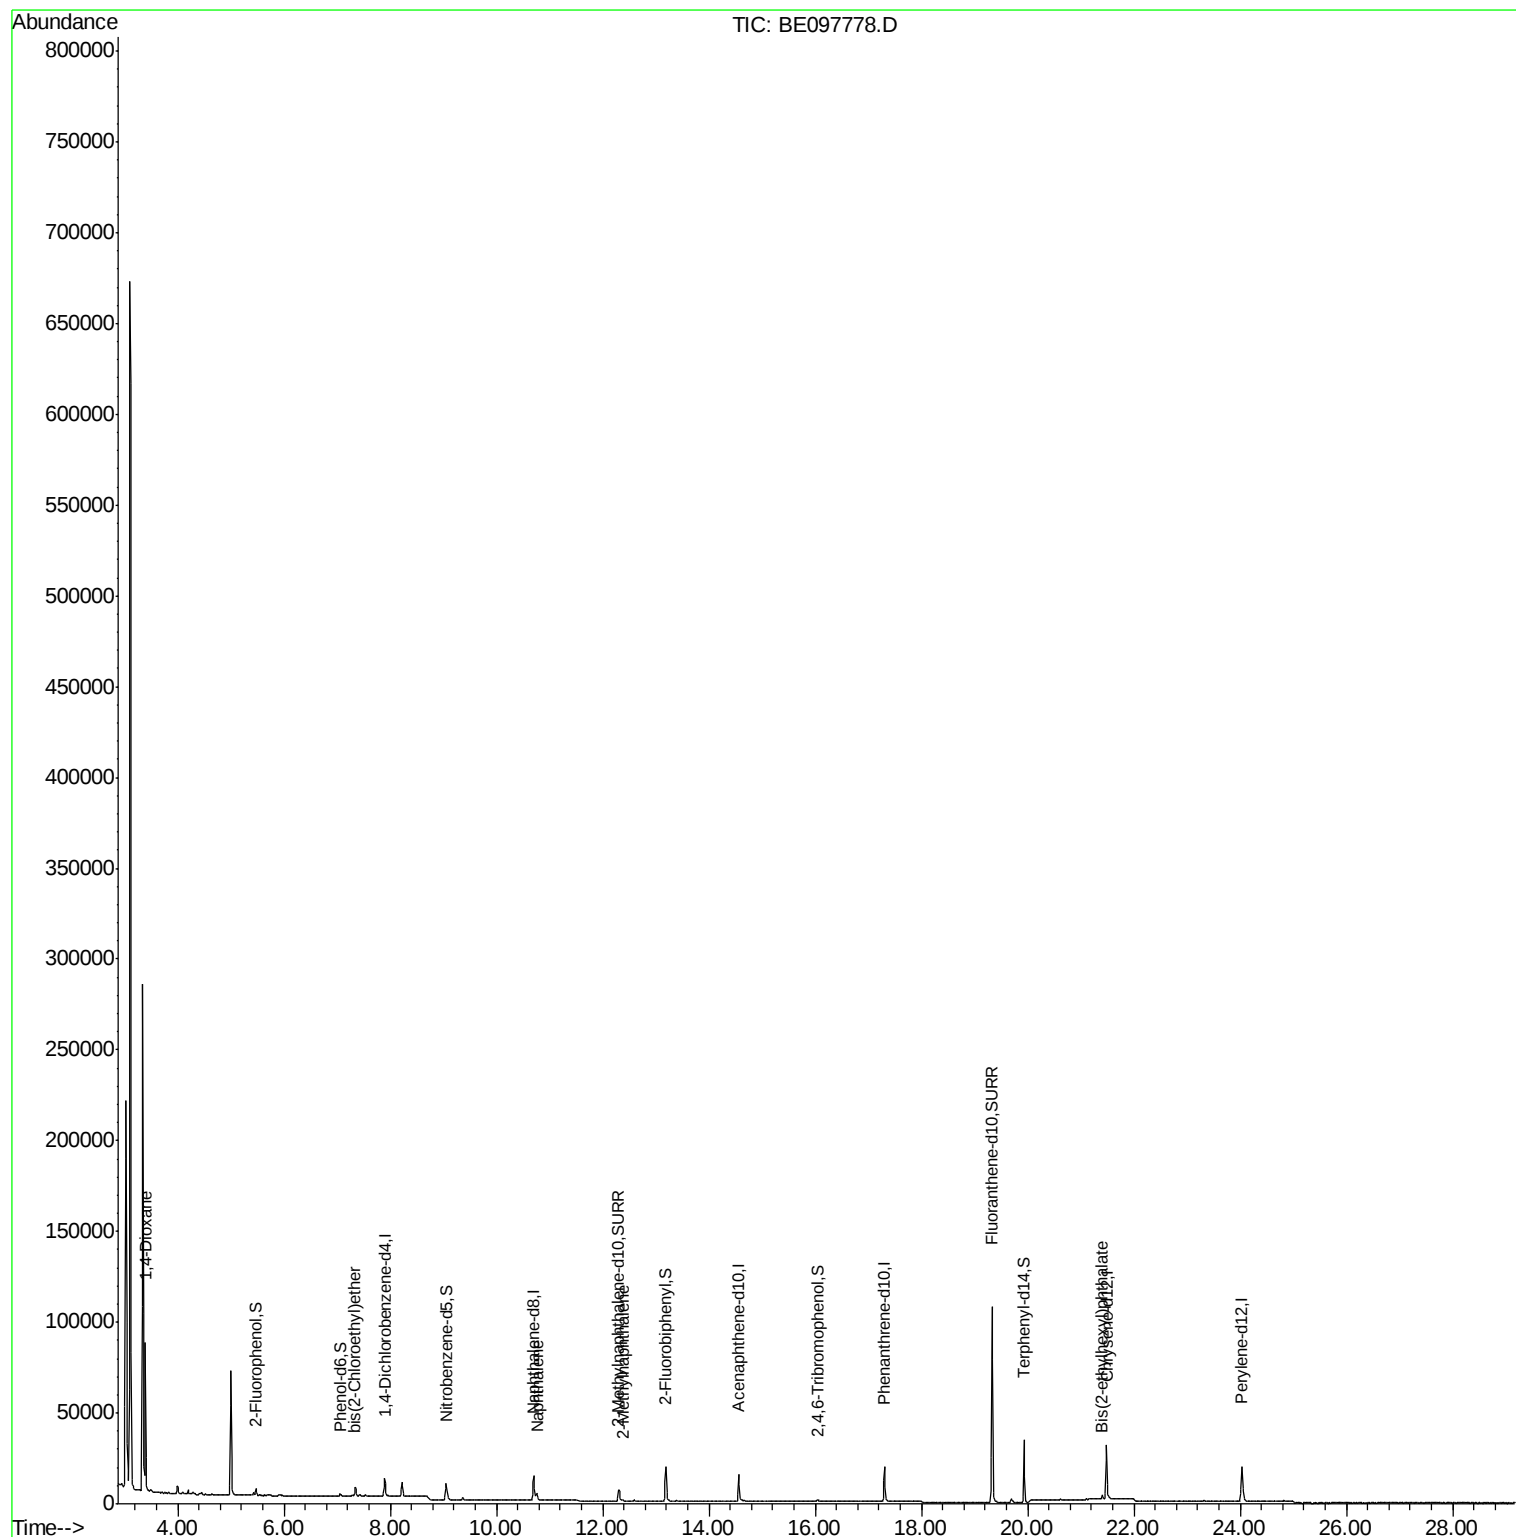



#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.90 min Scan# 437

Delta R.T. -0.00 min

Lab File: BE097778.D

Acq: 6 Oct 2018 6:20

Instrument :

BNA_E

ClientSampleId :

RE-125D2-2018001


Tot Ion:152 Resp: 4073

Ion Ratio Lower Upper

152 100

150 164.5 120.9 181.3




115 68.6 46.6 69.8

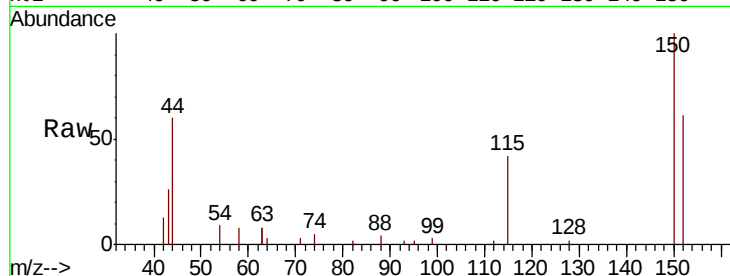

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

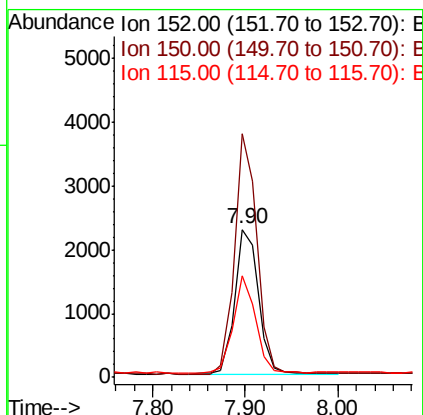

#2

1,4-Dioxane

Concen: 6.090 ng

RT: 3.39 min Scan# 46

Delta R.T. -0.00 min

Lab File: BE097778.D

Acq: 6 Oct 2018 6:20


Tgt Ion: 88 Resp: 49429

Ion Ratio Lower Upper

88 100

58 87.2 70.8 106.2



43 37.7 33.3 49.9




Abundance Ion 88.00 (87.70 to 88.70): BE0

Ion 58.00 (57.70 to 58.70): BE0

Ion 43.00 (42.70 to 43.70): BE0

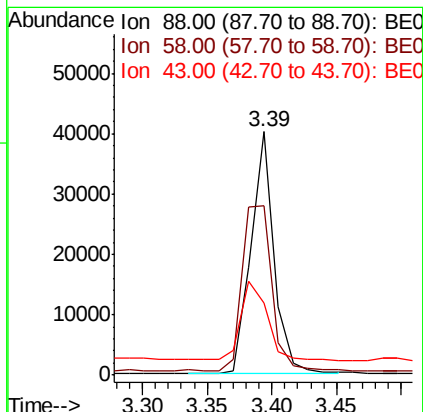



#4

2-Fluorophenol

Concen: 0.180 ng

RT: 5.47 min Scan# 226

Delta R.T. -0.00 min

Lab File: BE097778.D

Acq: 6 Oct 2018 6:20

Instrument :

BNA_E

ClientSampleId :

RE-125D2-2018001


Tot Ion: 112 Resp: 1733

Ion Ratio Lower Upper

112 100

64 67.2 56.6 84.8




63 155.2 119.4 179.0

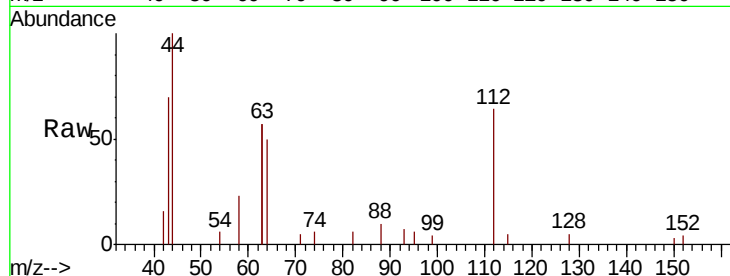

Abundance Ion 112.00 (111.70 to 112.70): BE0

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

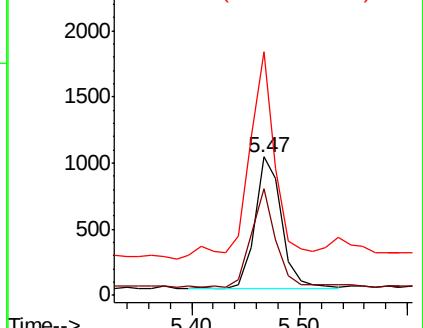

#5

Phenol-d6

Concen: 0.096 ng

RT: 7.06 min Scan# 364

Delta R.T. 0.01 min

Lab File: BE097778.D

Acq: 6 Oct 2018 6:20


Tgt Ion: 99 Resp: 1417

Ion Ratio Lower Upper

99 100

42 23.4 19.9 29.9



71 44.6 25.4 38.2#




Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

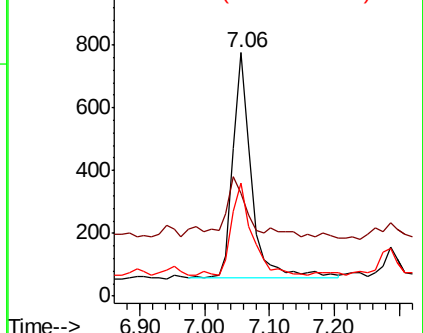



#6

bis(2-Chloroethyl)ether

Concen: 0.022 ng

RT: 7.32 min Scan# 387

Delta R.T. 0.01 min

Lab File: BE097778.D

Acq: 6 Oct 2018 6:20

Instrument :

BNA_E

ClientSampleId :

RE-125D2-2018001





Tot Ion: 93 Resp: 341

Ion Ratio Lower Upper

93 100

63 284.5 266.9 400.3

95 40.2 26.2 39.2#

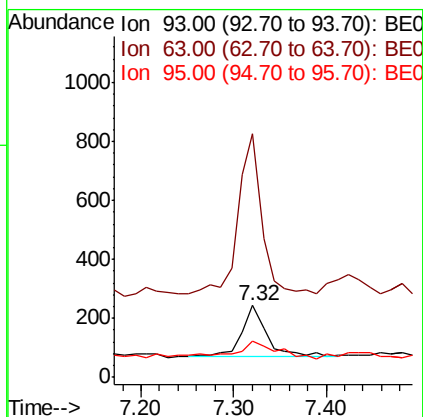

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.70 min Scan# 657

Delta R.T. 0.01 min

Lab File: BE097778.D

Acq: 6 Oct 2018 6:20

Tgt Ion: 136 Resp: 16210




Ion Ratio Lower Upper


136 100

137 11.0 9.0 13.4

54 34.5 37.8 56.6#

68 5.9 6.4 9.6#

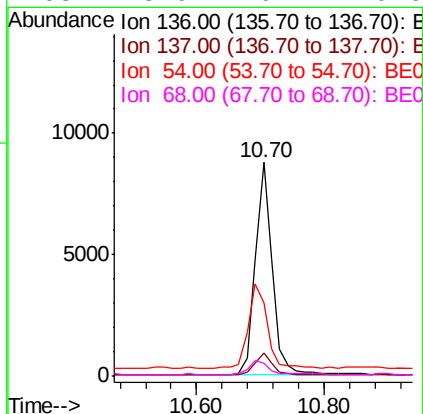

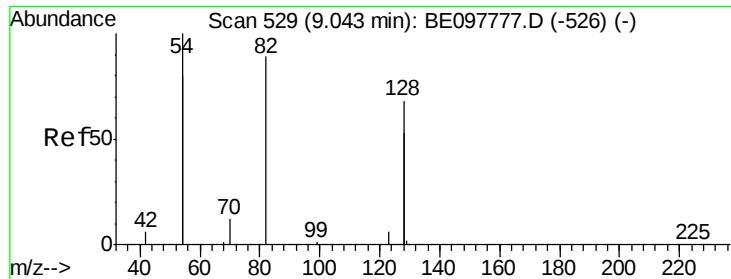

#8

Nitrobenzene-d5

Concen: 0.781 ng

RT: 9.05 min Scan# 530

Delta R.T. 0.01 min

Lab File: BE097778.D

Acq: 6 Oct 2018 6:20

Instrument :

BNA_E

ClientSampleId :

RE-125D2-2018001





Tot Ion: 82 Resp: 4110

Ion Ratio Lower Upper

82 100

128 136.8 97.0 145.4

54 215.2 206.9 310.3

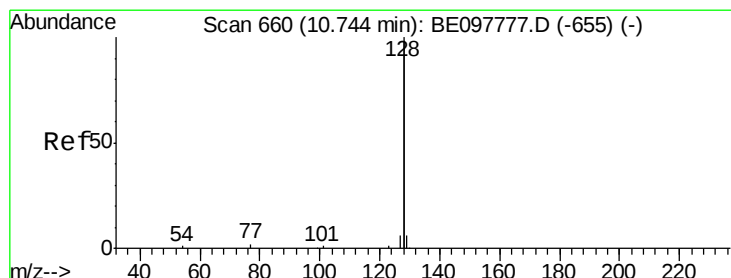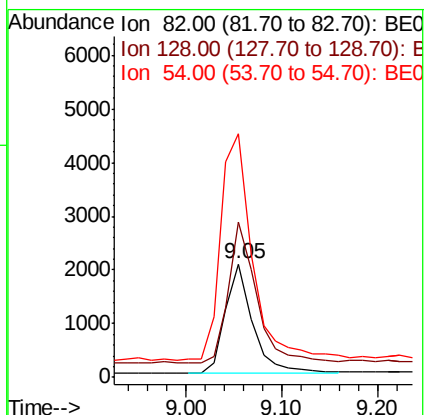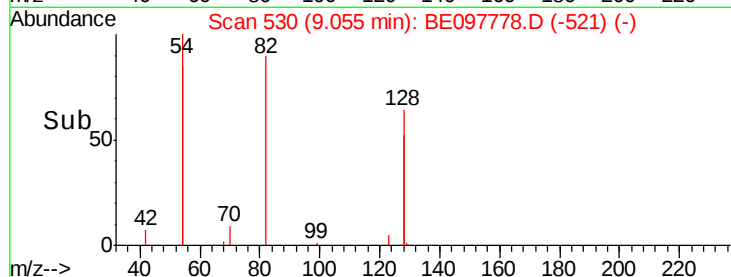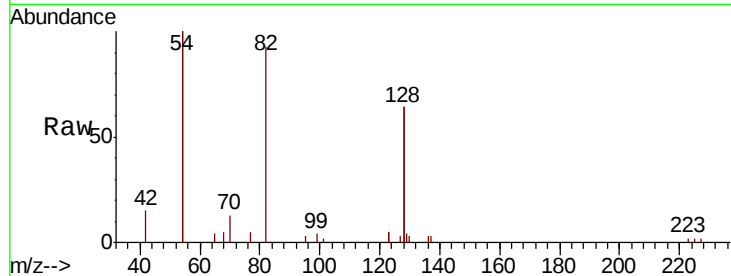

#9

Naphthalene

Concen: 0.038 ng

RT: 10.76 min Scan# 661

Delta R.T. 0.01 min

Lab File: BE097778.D

Acq: 6 Oct 2018 6:20




Tgt Ion: 128 Resp: 6244


Ion Ratio Lower Upper

128 100

129 4.4 2.2 3.2#

127 3.9 2.7 4.1

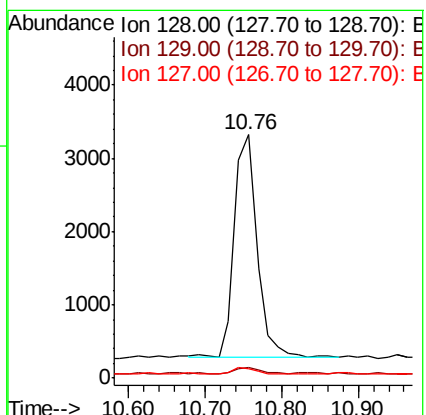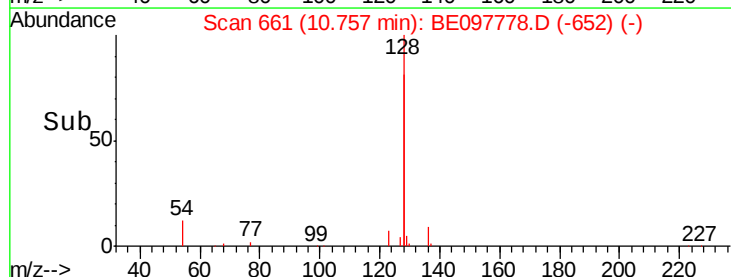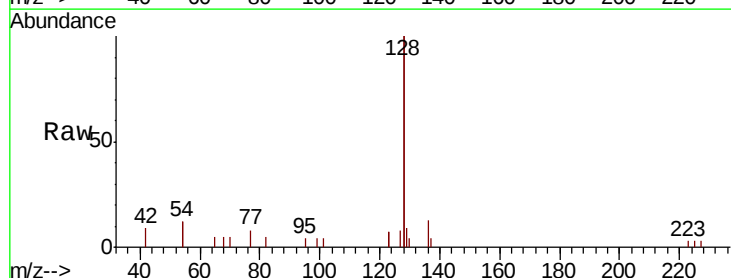

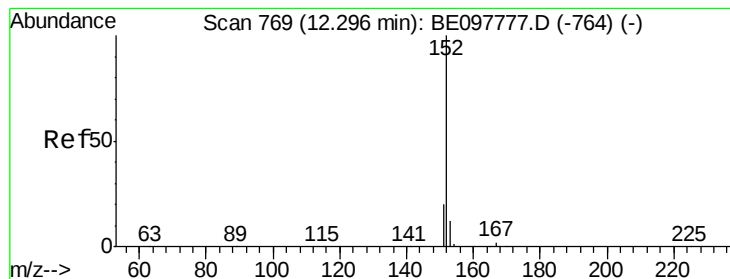

#11

2-Methylnaphthalene-d10

Concen: 0.395 ng

RT: 12.30 min Scan# 769

Delta R.T. -0.00 min

Lab File: BE097778.D

Acq: 6 Oct 2018 6:20

Instrument :

BNA_E

ClientSampleId :


RE-125D2-2018001

Tot Ion:152 Resp: 10197

Ion Ratio Lower Upper




152 100

151 18.6 15.4 23.2



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

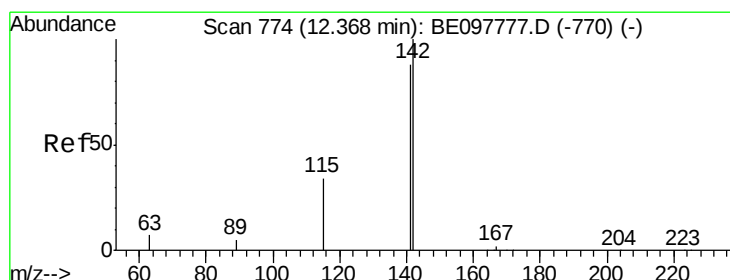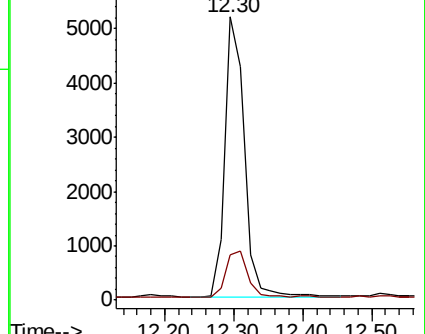

#12

2-Methylnaphthalene

Concen: 0.021 ng

RT: 12.38 min Scan# 775

Delta R.T. 0.01 min

Lab File: BE097778.D

Acq: 6 Oct 2018 6:20


Tgt Ion:142 Resp: 550

Ion Ratio Lower Upper

142 100

141 83.6 69.4 104.2



115 51.9 28.0 42.0#




Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 115.00 (114.70 to 115.70): E

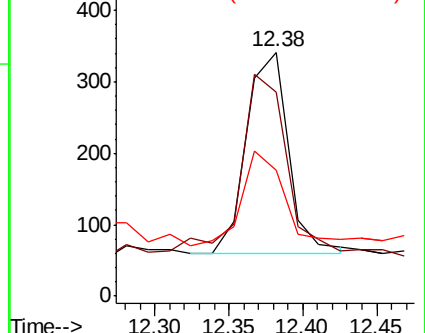


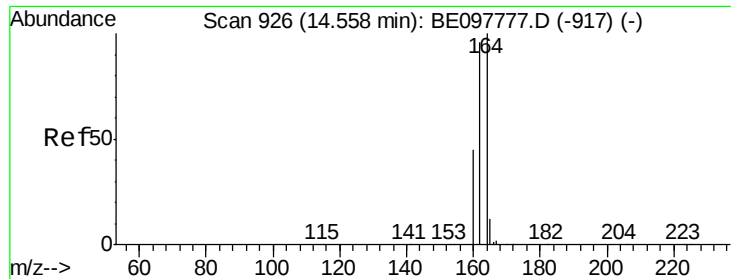




#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.56 min Scan# 926
 Delta R.T. -0.00 min
 Lab File: BE097778.D
 Acq: 6 Oct 2018 6:20

Instrument :
 BNA_E
 ClientSampleId :
 RE-125D2-2018001

Tot Ion:164 Resp: 9152
 Ion Ratio Lower Upper
 164 100
 162 97.5 78.6 117.8
 160 48.8 37.8 56.6

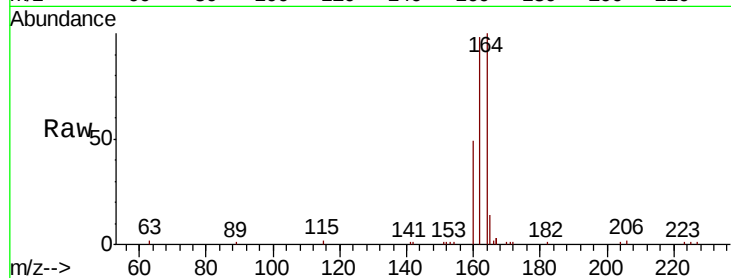


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

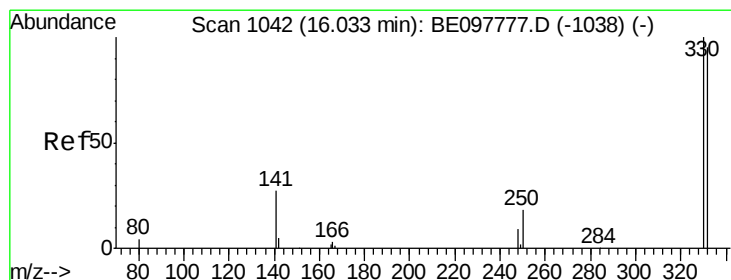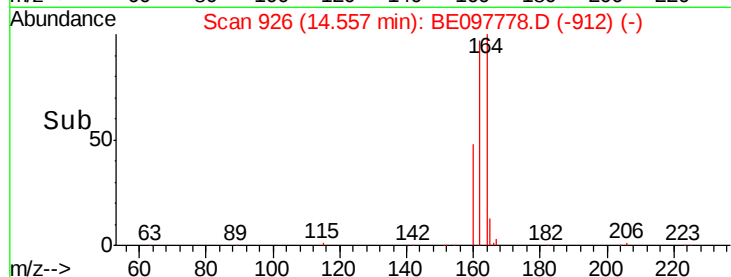
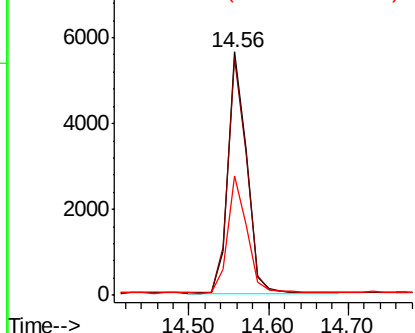



#14
 2,4,6-Tribromophenol
 Concen: 0.528 ng
 RT: 16.04 min Scan# 1043
 Delta R.T. 0.00 min
 Lab File: BE097778.D
 Acq: 6 Oct 2018 6:20

Tgt Ion:330 Resp: 876
 Ion Ratio Lower Upper
 330 100
 332 92.0 83.5 125.3
 141 34.5 34.9 52.3#

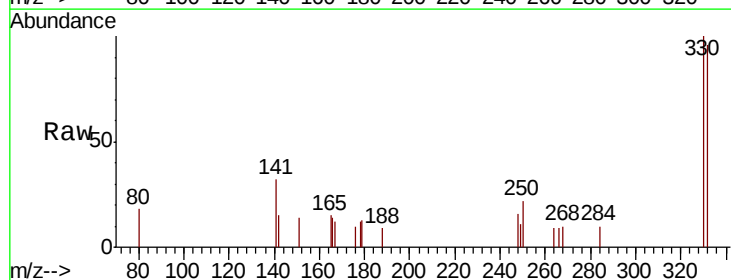

Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

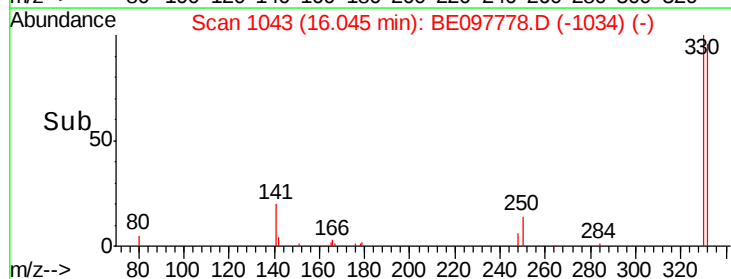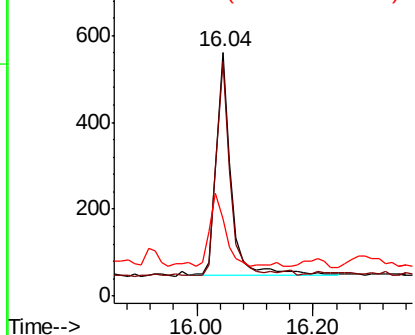


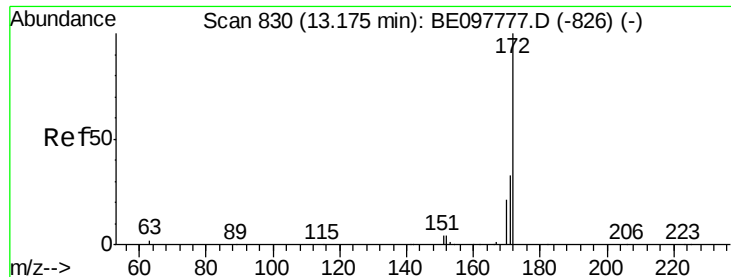




#15
2-Fluorobiphenyl
Concen: 0.471 ng
RT: 13.19 min Scan# 831
Delta R.T. -0.00 min
Lab File: BE097778.D
Acq: 6 Oct 2018 6:20

Instrument :
BNA_E
ClientSampleId :
RE-125D2-2018001

Tot Ion:172 Resp: 18965
Ion Ratio Lower Upper
172 100
171 32.1 25.2 37.8
170 21.1 16.2 24.2

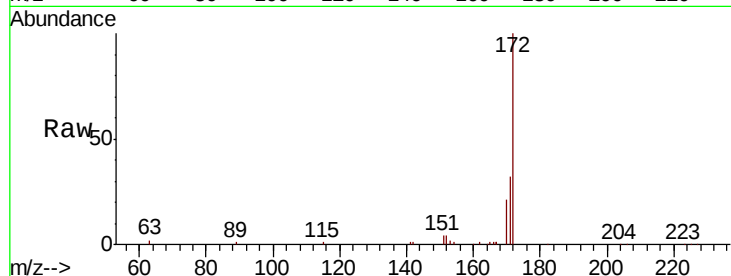


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

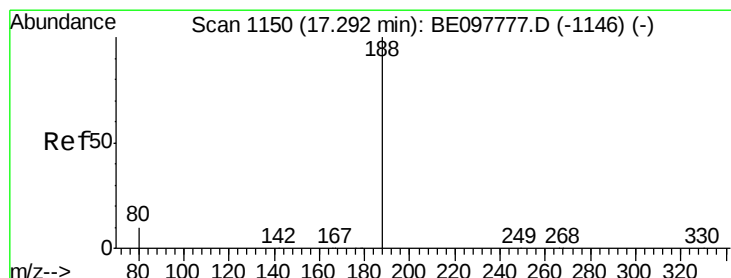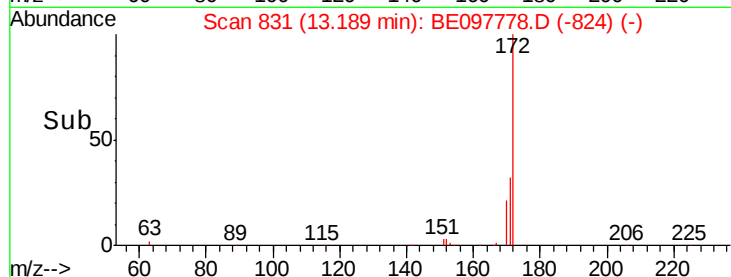
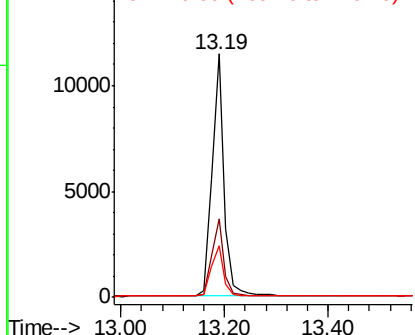



#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.30 min Scan# 1151
Delta R.T. -0.00 min
Lab File: BE097778.D
Acq: 6 Oct 2018 6:20

Tgt Ion:188 Resp: 26699
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.0 6.6 9.8

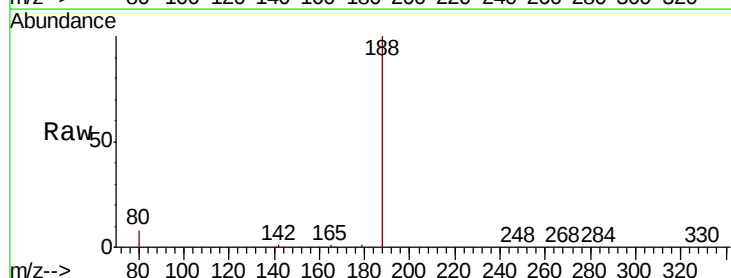

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BE0
Ion 80.00 (79.70 to 80.70): BE0

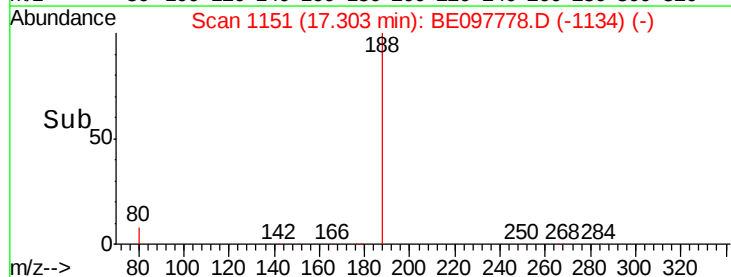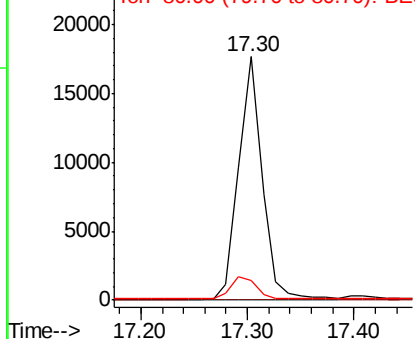


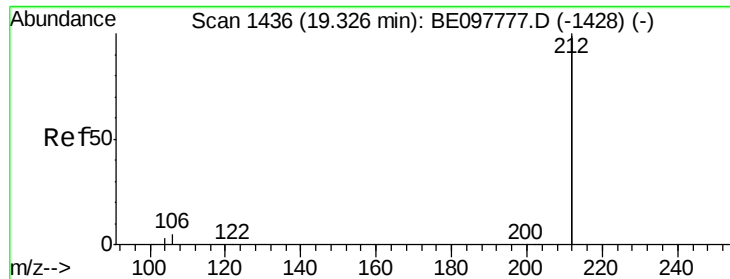




#25
 Fluoranthene-d10
 Concen: 0.437 ng
 RT: 19.33 min Scan# 1437
 Delta R.T. 0.00 min
 Lab File: BE097778.D
 Acq: 6 Oct 2018 6:20

Instrument :
 BNA_E
 ClientSampleId :
 RE-125D2-2018001

Tot Ion:212 Resp: 147528
 Ion Ratio Lower Upper
 212 100
 106 2.6 2.2 3.2
 104 1.5 1.2 1.8

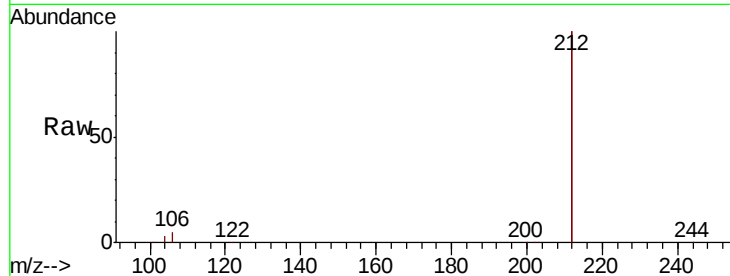


Abundance Ion 212.00 (211.70 to 212.70): E
 Ion 106.00 (105.70 to 106.70): E
 Ion 104.00 (103.70 to 104.70): E


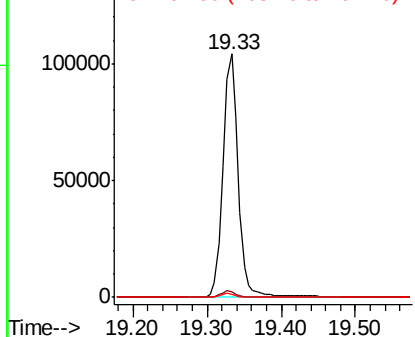



#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.49 min Scan# 1673
 Delta R.T. -0.00 min
 Lab File: BE097778.D
 Acq: 6 Oct 2018 6:20

Tgt Ion:240 Resp: 33433
 Ion Ratio Lower Upper
 240 100
 120 5.0 4.7 7.1
 236 26.3 20.8 31.2



Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

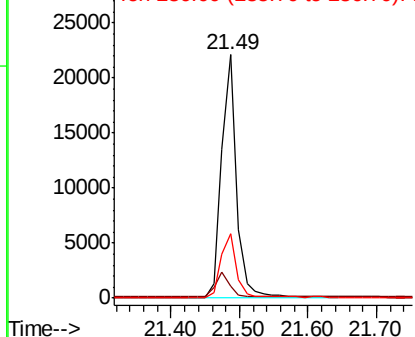



#29

Terphenyl-d14

Concen: 0.441 ng

RT: 19.93 min Scan# 1541

Delta R.T. -0.00 min

Lab File: BE097778.D

Acq: 6 Oct 2018 6:20

Instrument :

BNA_E

ClientSampleId :

RE-125D2-2018001


Tot Ion:244 Resp: 30132

Ion Ratio Lower Upper

244 100

212 31.6 25.8 38.8




122 10.0 8.7 13.1

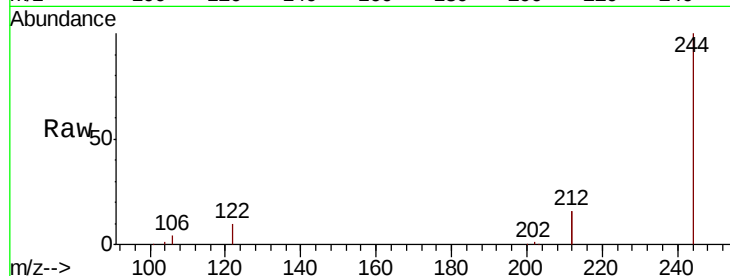

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

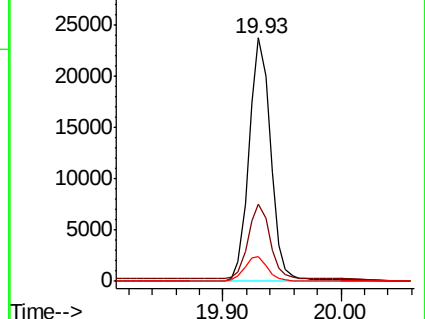

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.056 ng

RT: 21.40 min Scan# 1666

Delta R.T. -0.01 min

Lab File: BE097778.D

Acq: 6 Oct 2018 6:20


Tgt Ion:149 Resp: 3699

Ion Ratio Lower Upper

149 100

167 5.7 5.5 8.3



279 1.3 0.9 1.3#






Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

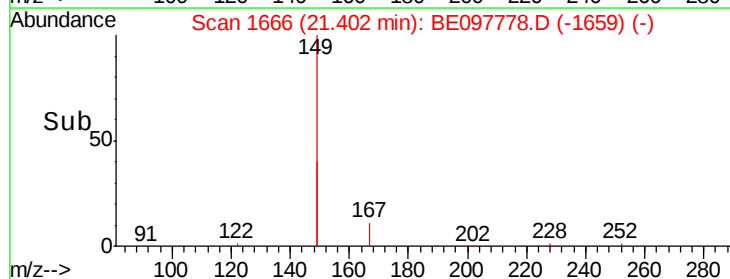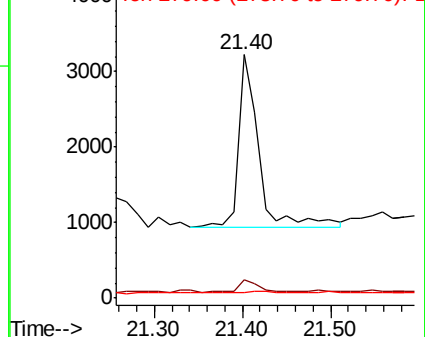

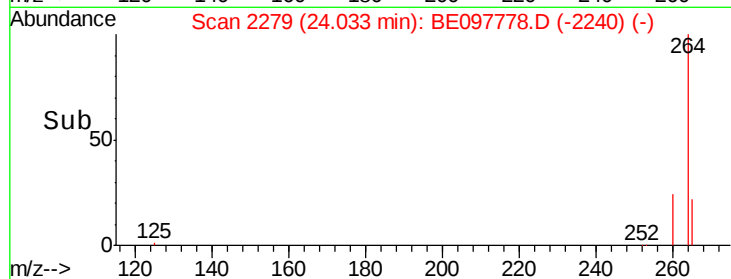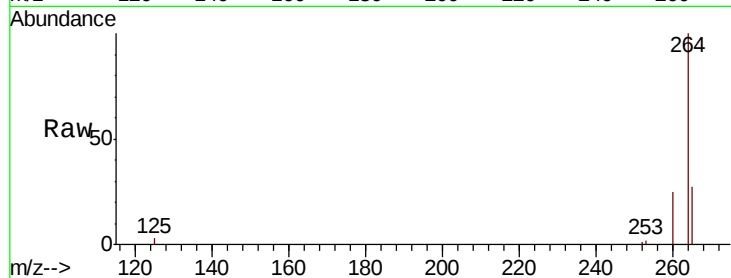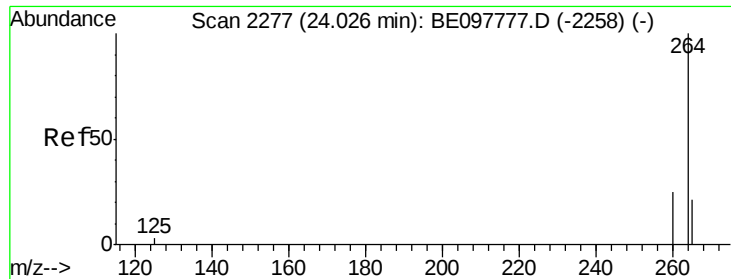

#34

Pervlene-d12

Concen: 0.400 ng

RT: 24.03 min Scan# 2279

Delta R.T. -0.01 min

Lab File: BE097778.D

Acq: 6 Oct 2018 6:20

Instrument :

BNA_E

ClientSampleId :

RE-125D2-2018001

Tot Ion:264 Resp: 31383

Ion Ratio Lower Upper

264 100

260 24.6 19.1 28.7

265 26.8 21.9 32.9

