


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE100518\
Data File : BE097744.D
Acq On : 5 Oct 2018 8:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE100318.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 08 06:37:06 2018

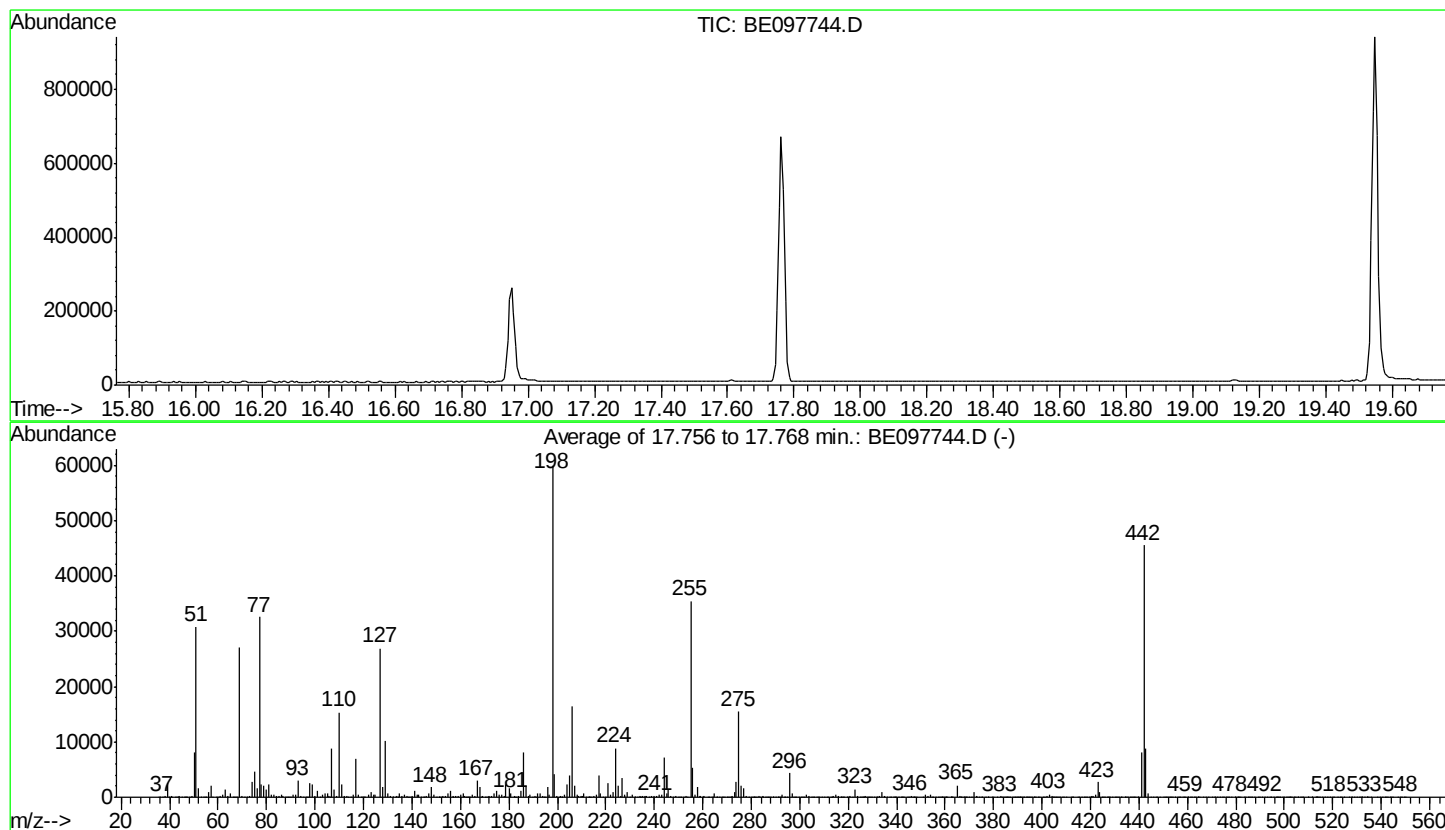

AutoFind: Scans 2581, 2582, 2583; Background Corrected with Scan 2572

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.4	30806	PASS
68	69	0.00	2	0.4	103	PASS
69	198	0.00	100	45.3	27138	PASS
70	69	0.00	2	0.6	171	PASS
127	198	10	80	44.8	26845	PASS
197	198	0.00	2	0.6	384	PASS
198	198	100	100	100.0	59925	PASS
199	198	5	9	6.8	4099	PASS
275	198	10	60	25.7	15411	PASS
365	198	1	100	3.7	2202	PASS
441	198	0.01	100	13.4	8054	PASS
442	198	50	100	76.0	45565	PASS
443	442	15	24	19.5	8876	PASS