


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE100518\
Data File : BE097776.D
Acq On : 6 Oct 2018 4:51
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE100318.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 08 06:37:06 2018

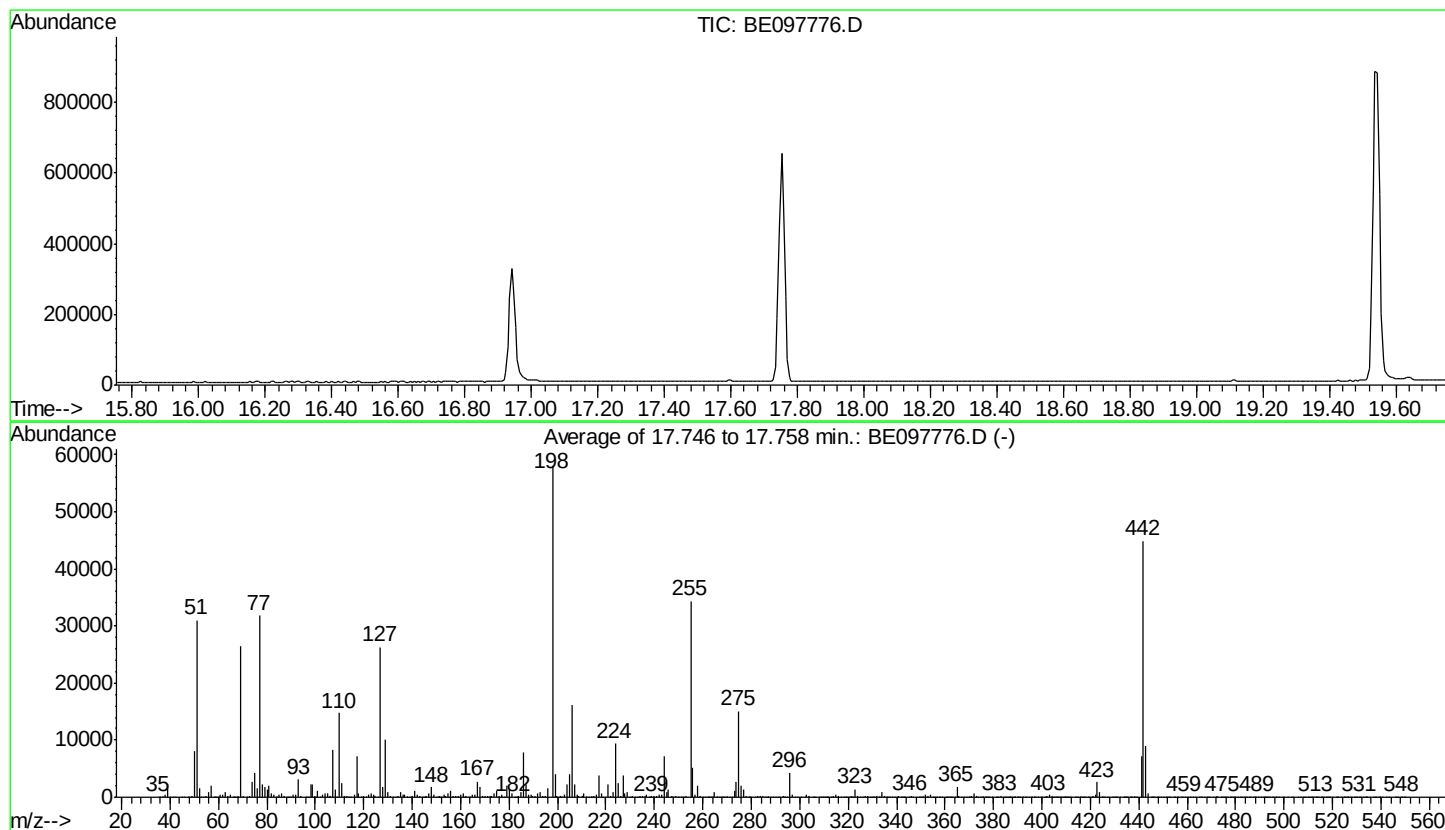

AutoFind: Scans 2580, 2581, 2582; Background Corrected with Scan 2568

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.5	31053	PASS
68	69	0.00	2	1.0	274	PASS
69	198	0.00	100	45.5	26424	PASS
70	69	0.00	2	0.7	193	PASS
127	198	10	80	45.3	26330	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58069	PASS
199	198	5	9	7.0	4039	PASS
275	198	10	60	25.9	15036	PASS
365	198	1	100	3.3	1894	PASS
441	198	0.01	100	12.5	7284	PASS
442	198	50	100	77.2	44846	PASS
443	442	15	24	20.0	8961	PASS