
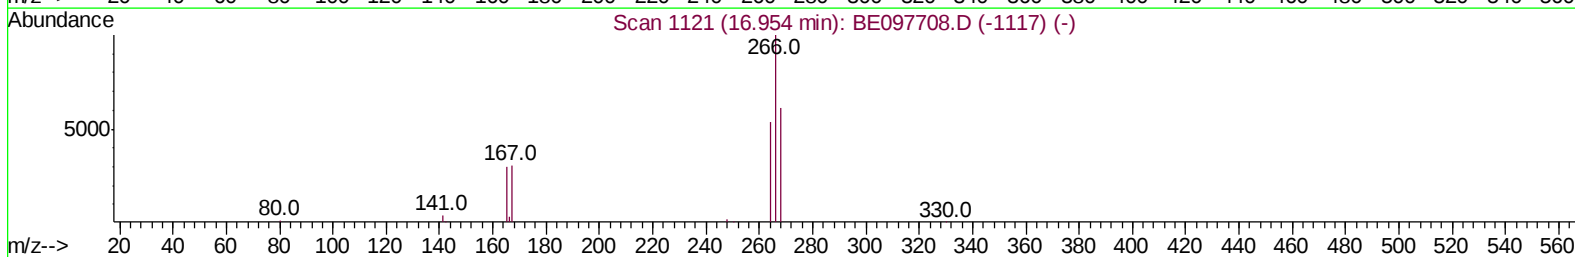
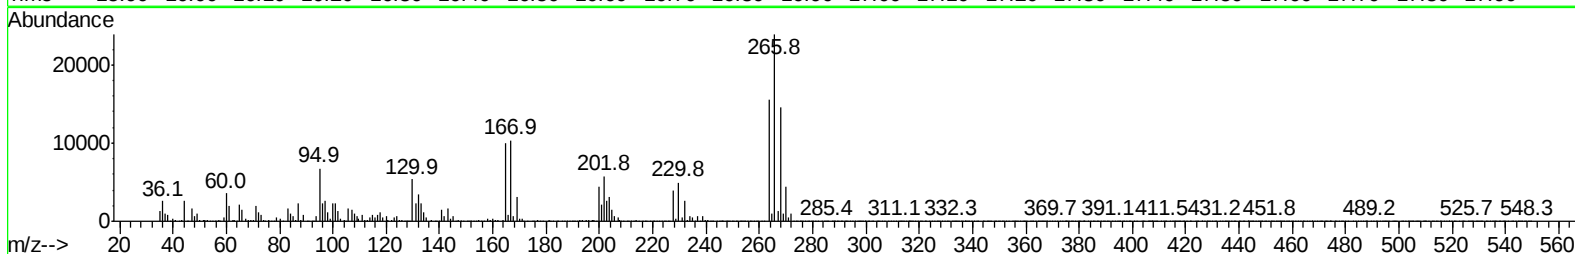


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE100818\
Data File : BE097789.D
Acq On : 8 Oct 2018 11:55
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 09 12:43:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE100318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 09 11:59:33 2018
Response via : Initial Calibration

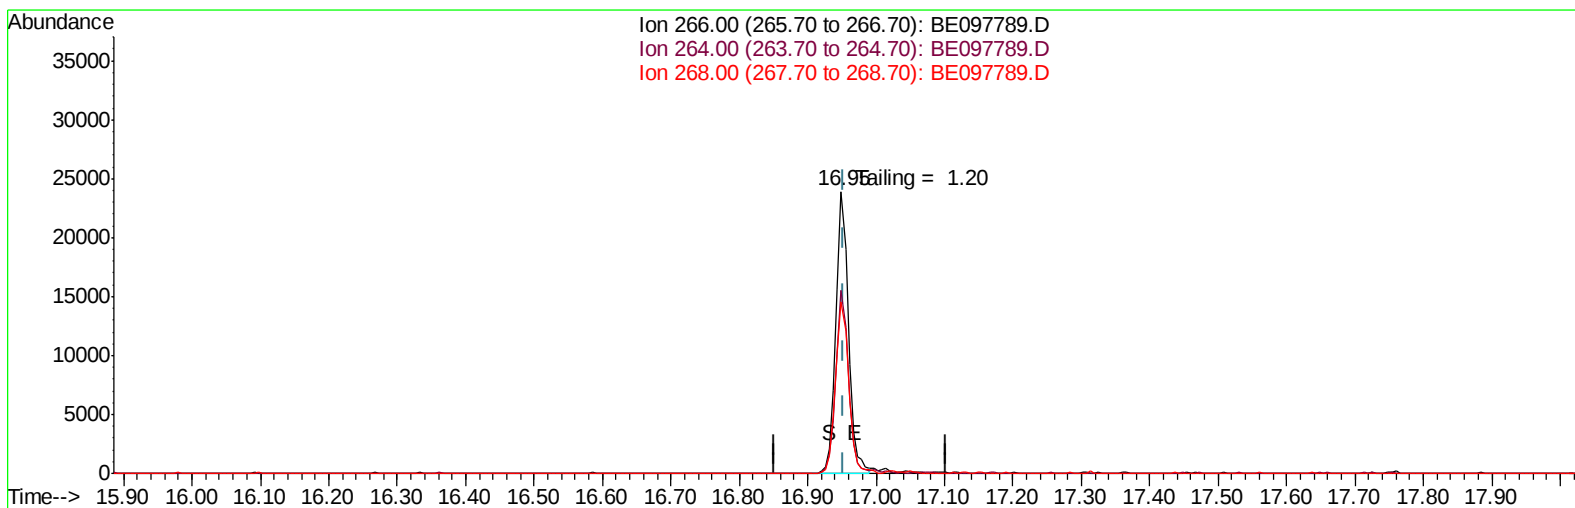

TIC: BE097789.D

(22) Pentachlorophenol

16.949min (-0.004) 47043.23ng

response 30488

Ion	Exp%	Act%
266.00	100	100
264.00	58.50	64.87
268.00	66.30	60.73
0.00	0.00	0.00