


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE100818\
 Data File : BE097789.D
 Acq On : 8 Oct 2018 11:55
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE100318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 09 11:59:33 2018

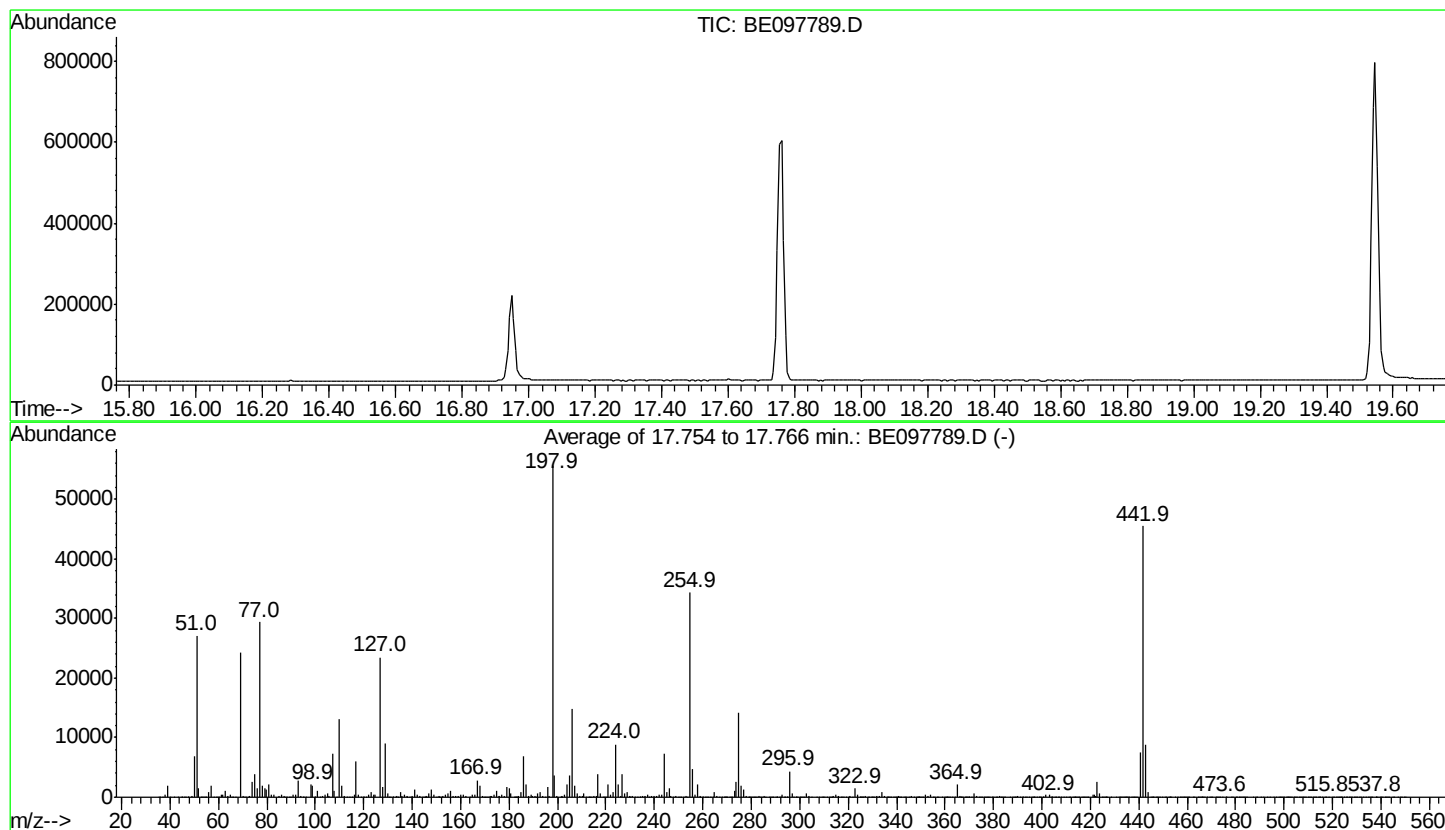

AutoFind: Scans 2581, 2582, 2583; Background Corrected with Scan 2565

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.7	27105	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.5	24224	PASS
70	69	0.00	2	0.7	163	PASS
127	198	10	80	42.2	23464	PASS
197	198	0.00	2	0.4	195	PASS
198	198	100	100	100.0	55646	PASS
199	198	5	9	6.5	3609	PASS
275	198	10	60	25.6	14255	PASS
365	198	1	100	3.8	2113	PASS
441	198	0.01	100	13.5	7534	PASS
442	198	50	100	81.8	45528	PASS
443	442	15	24	19.2	8732	PASS