
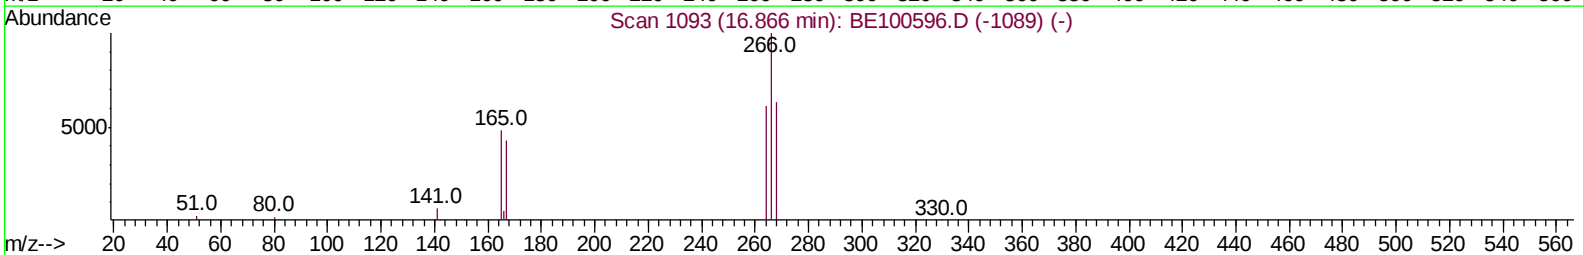
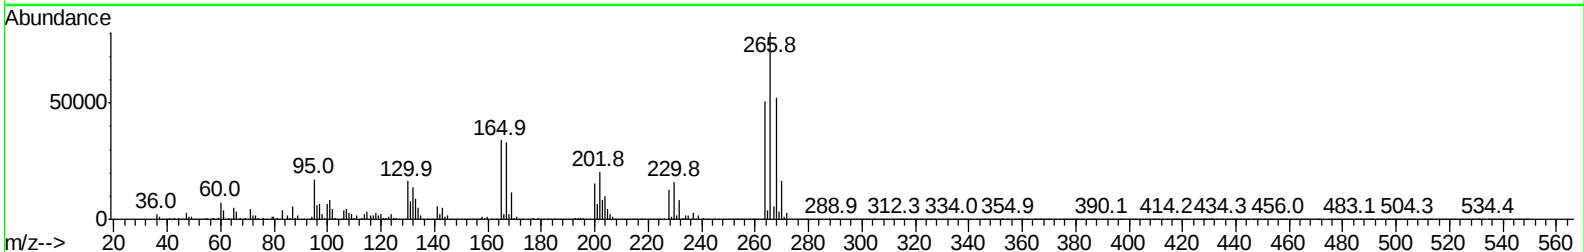


```
Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE100819\  
Data File : BE100602.D  
Acq On    : 8 Oct 2019 11:05  
Operator  : JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Oct 09 05:01:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE100319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 09 01:42:20 2019
Response via : Initial Calibration

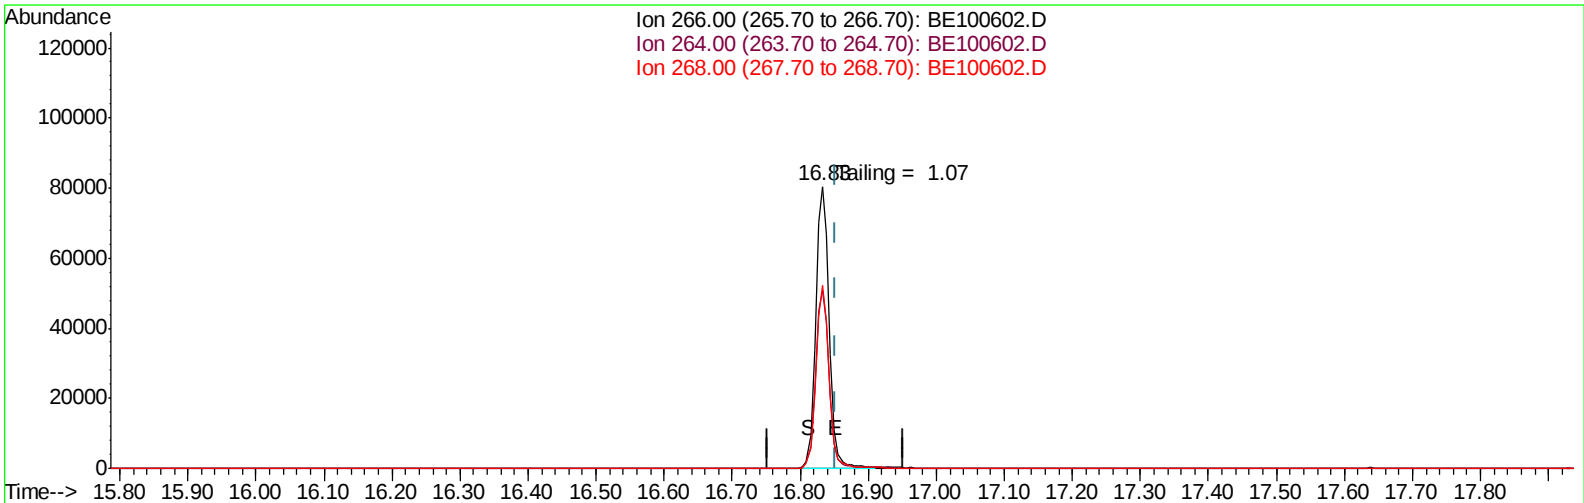

TIC: BE100602.D

(22) Pentachlorophenol

16.833min (-0.020) 7588.42ng

response 112667

Ion	Exp%	Act%
266.00	100	100
264.00	70.40	63.32
268.00	75.40	65.10
0.00	0.00	0.00