


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE100819\
Data File : BE100602.D
Acq On : 8 Oct 2019 11:05
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE100319.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 09 01:42:20 2019

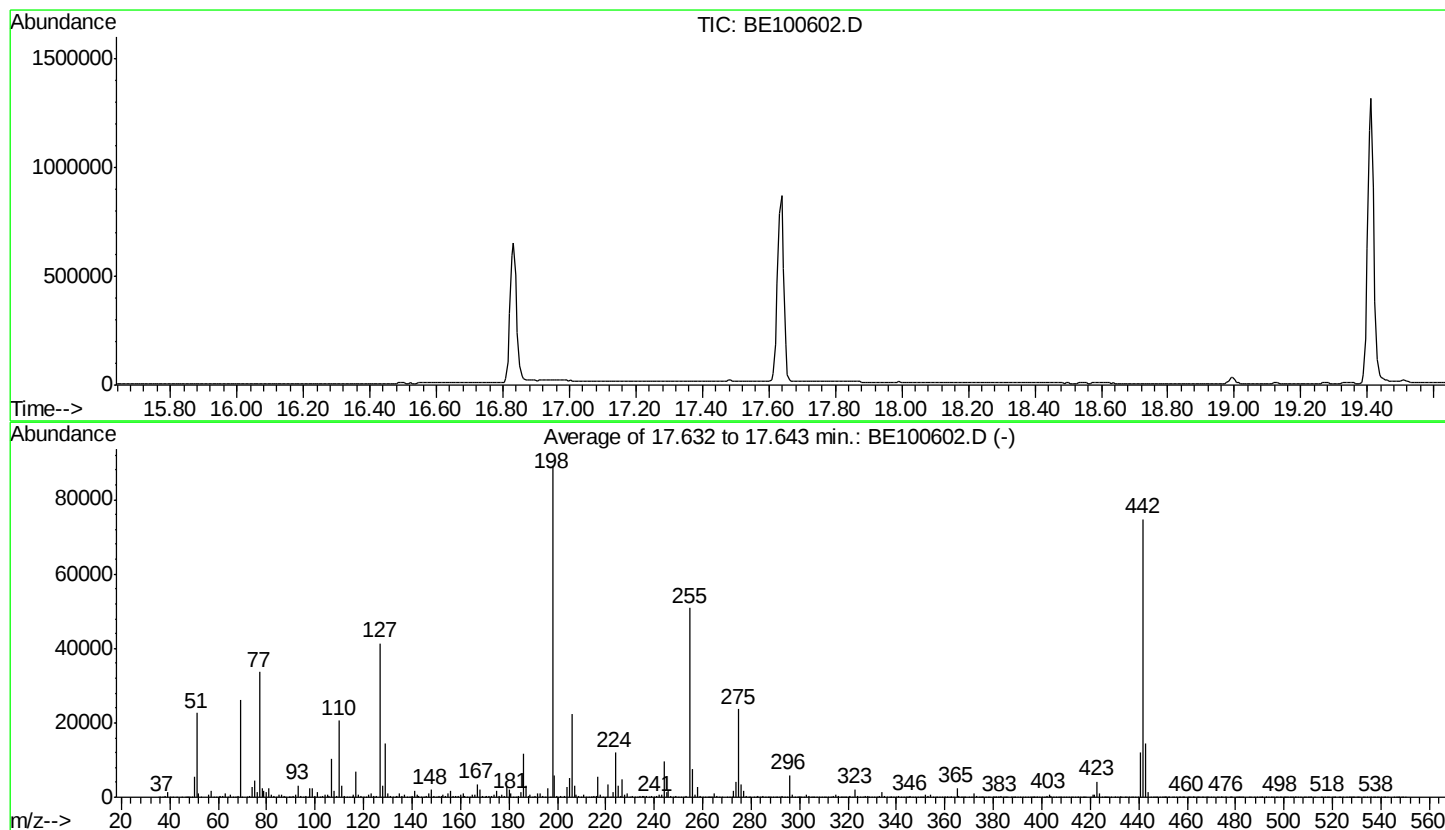

AutoFind: Scans 2560, 2561, 2562; Background Corrected with Scan 2550

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.3	22579	PASS
68	69	0.00	2	1.4	372	PASS
69	198	0.00	100	29.5	26254	PASS
70	69	0.00	2	0.4	102	PASS
127	198	10	80	46.4	41339	PASS
197	198	0.00	2	0.2	164	PASS
198	198	100	100	100.0	89125	PASS
199	198	5	9	6.8	6019	PASS
275	198	10	60	26.5	23583	PASS
365	198	1	100	2.9	2554	PASS
441	198	0.01	100	13.5	12039	PASS
442	198	50	100	83.8	74667	PASS
443	442	15	24	19.6	14616	PASS