


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE100819\
 Data File : BE100615.D
 Acq On : 8 Oct 2019 19:04
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE100319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 09 01:42:20 2019

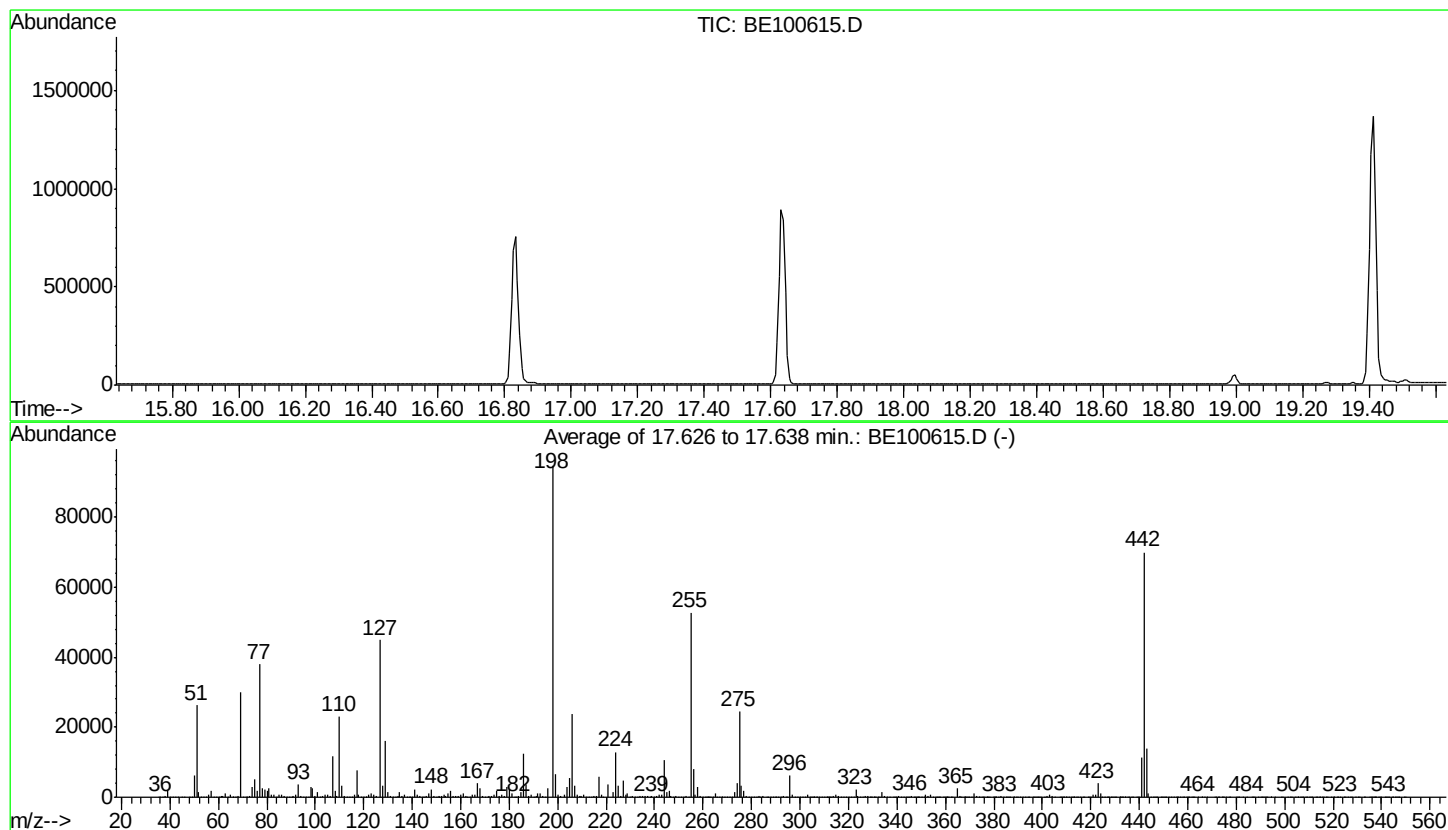

AutoFind: Scans 2559, 2560, 2561; Background Corrected with Scan 2551

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.7	26264	PASS
68	69	0.00	2	1.6	493	PASS
69	198	0.00	100	31.8	30115	PASS
70	69	0.00	2	0.5	150	PASS
127	198	10	80	47.4	44871	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	94711	PASS
199	198	5	9	7.0	6599	PASS
275	198	10	60	25.8	24478	PASS
365	198	1	100	2.6	2486	PASS
441	198	0.01	100	11.9	11281	PASS
442	198	50	100	73.8	69922	PASS
443	442	15	24	19.8	13865	PASS