


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE100918\
 Data File : BE097813.D
 Acq On : 9 Oct 2018 12:08
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE100318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 09 11:59:33 2018

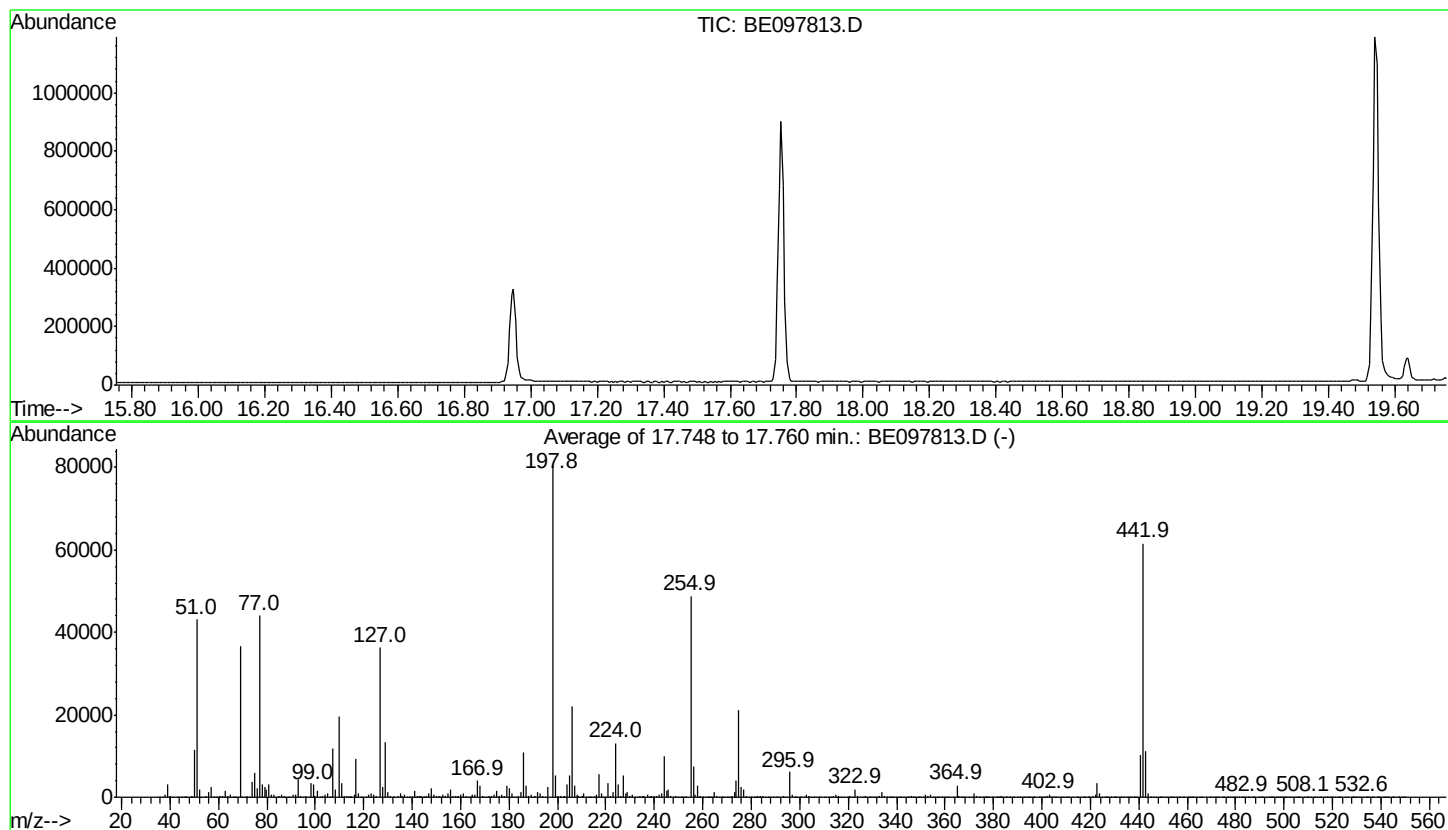

AutoFind: Scans 2580, 2581, 2582; Background Corrected with Scan 2574

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.5	43061	PASS
68	69	0.00	2	0.4	147	PASS
69	198	0.00	100	45.6	36678	PASS
70	69	0.00	2	0.4	154	PASS
127	198	10	80	45.1	36255	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	80441	PASS
199	198	5	9	6.4	5170	PASS
275	198	10	60	26.1	20993	PASS
365	198	1	100	3.5	2806	PASS
441	198	0.01	100	12.8	10265	PASS
442	198	50	100	76.5	61558	PASS
443	442	15	24	18.1	11148	PASS