

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE101018\
 Data File : BE097835.D
 Acq On : 10 Oct 2018 19:39
 Operator : SJ/JU
 Sample : J5184-13
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Oct 11 01:23:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE101018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 01:20:33 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	2933	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	14147	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.54	164	10568	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.39	188	1526426	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.48
20) Perylene-d12	24.03	264	46578	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	6668	0.30	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.86	252	6945	0.063	ng/ul#	Ovalue 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE101018\
Data File : BE097835.D
Acq On : 10 Oct 2018 19:39
Operator : SJ/JU
Sample : J5184-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Oct 11 01:23:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE101018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 01:20:33 2018
Response via : Initial Calibration

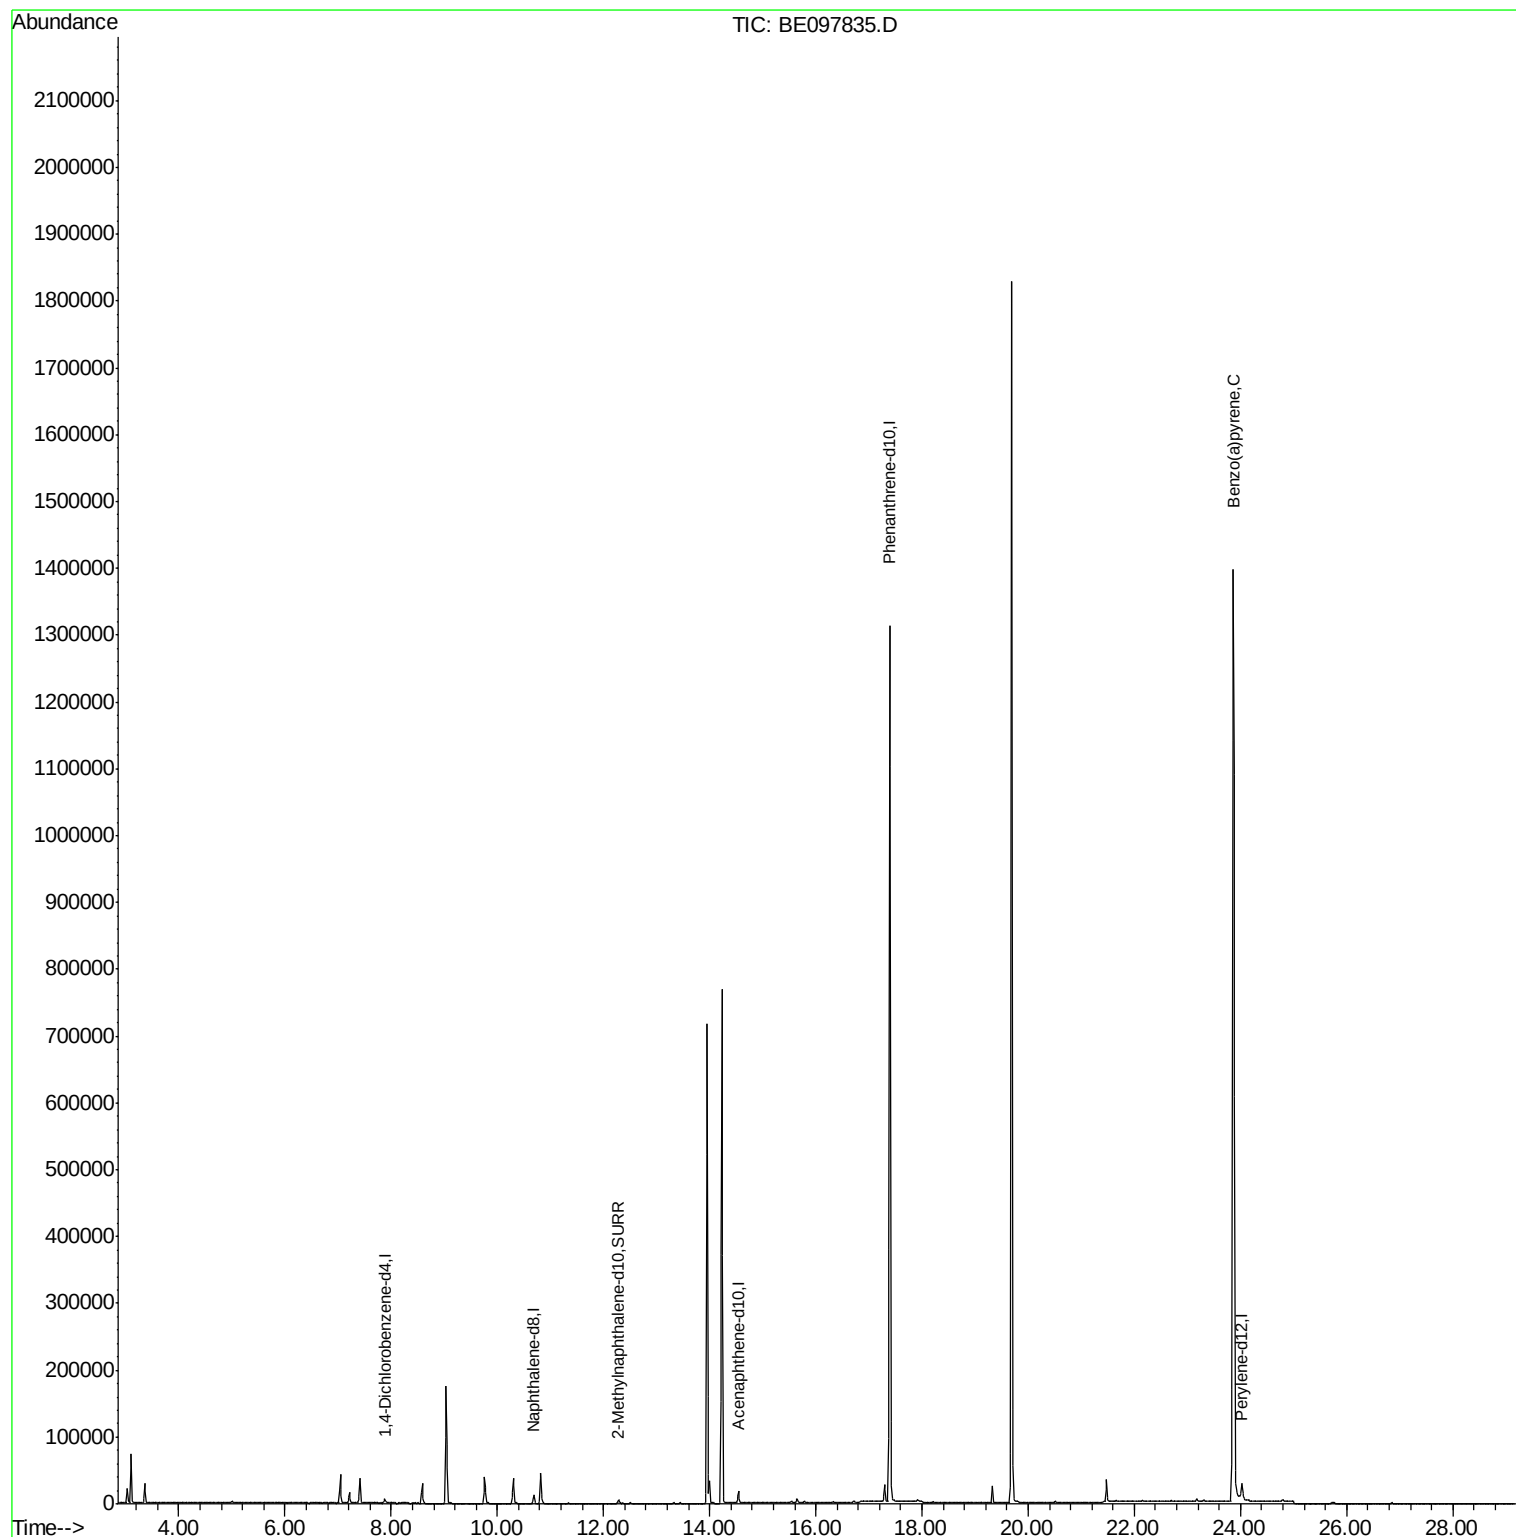

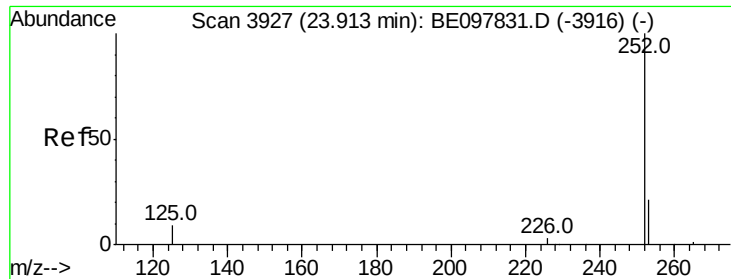

#23

Benzo(a)pyrene

Concen: 0.063 ng/ul

RT: 23.86 min Scan# 3921

Delta R.T. -0.05 min


Lab File: BE097835.D

Acq: 10 Oct 2018 19:39

Instrument :

BNA_E

ClientSampleId :

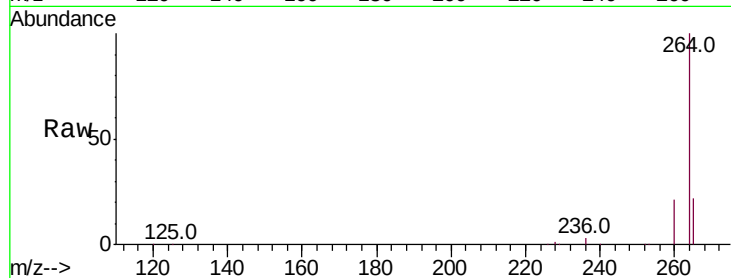

Tot Ion: 252 Resp: 6945

Ion Ratio Lower Upper

252 100

253 32.6 18.2 27.4#

125 30.9 8.3 12.5#

