

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE101018\
 Data File : BE097840.D
 Acq On : 10 Oct 2018 22:43
 Operator : SJ/JU
 Sample : J5183-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Oct 11 01:23:48 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE101018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 01:20:33 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	2715	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	13386	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.54	164	10361	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.40	188	1242856	0.40	ng/ul	0.11
16) Chrysene-d12	21.67	240	78	0.40	ng/ul	0.19
20) Perylene-d12	0.00	264	0	0.00	ng/ul	-24.03
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	5399	0.26	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
17) Pyrene	19.72	202	31282	163.233	ng/ul	96
18) Benzo(a)anthracene	21.52	228	179212	827.804	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE101018\
Data File : BE097840.D
Acq On : 10 Oct 2018 22:43
Operator : SJ/JU
Sample : J5183-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Oct 11 01:23:48 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE101018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 01:20:33 2018
Response via : Initial Calibration

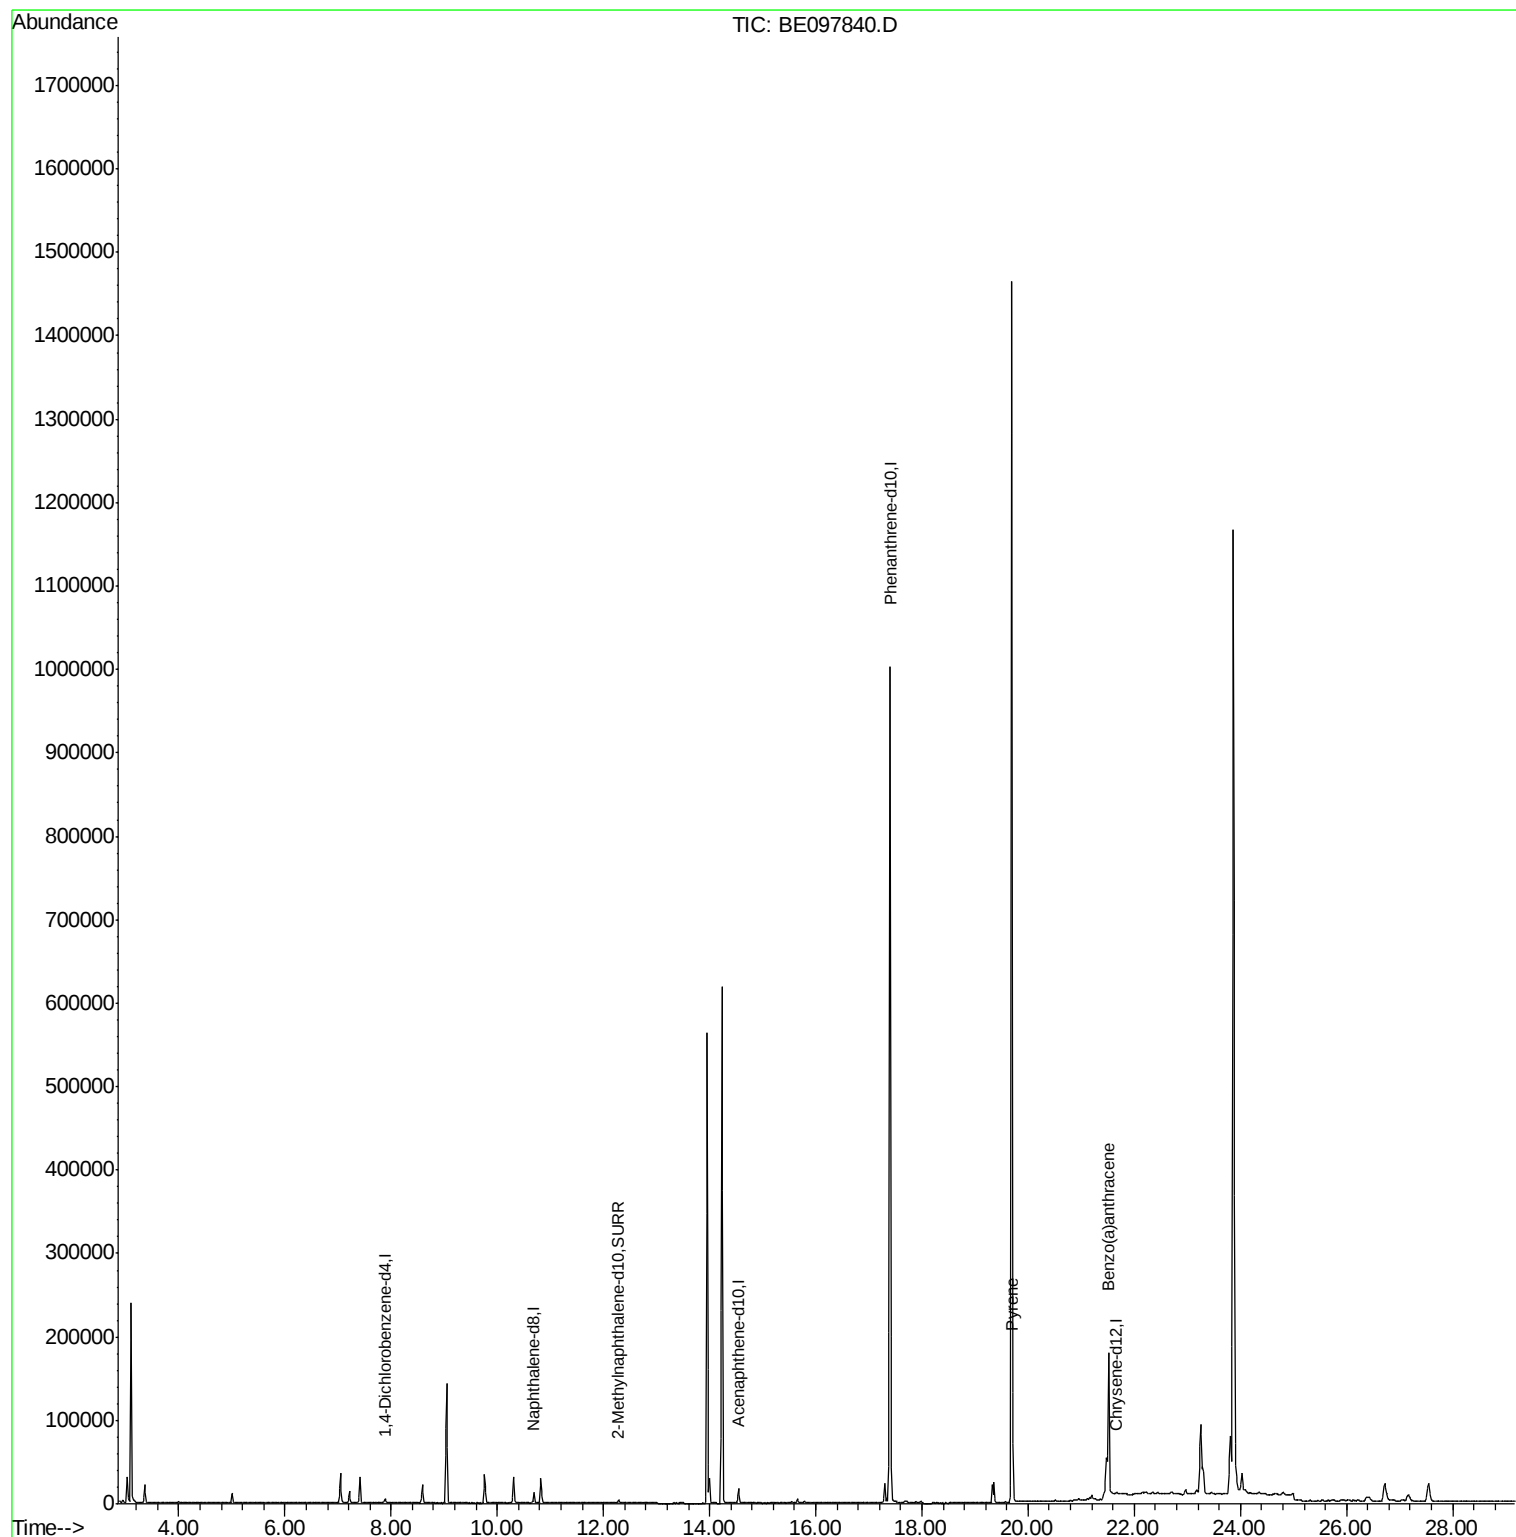

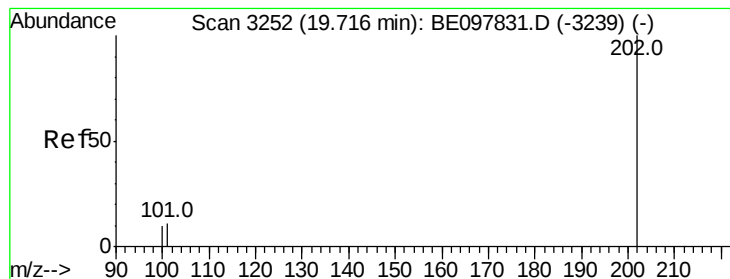

#17

Pvrene

Concen: 163.233 ng/ul

RT: 19.72 min Scan# 3254

Delta R.T. 0.00 min

Lab File: BE097840.D

Acq: 10 Oct 2018 22:43

Instrument :

BNA_E

ClientSampleId :


Tot Ion:202 Resp: 31282

Ion Ratio Lower Upper

202 100

101 12.5 8.8 13.2




100 11.4 7.9 11.9

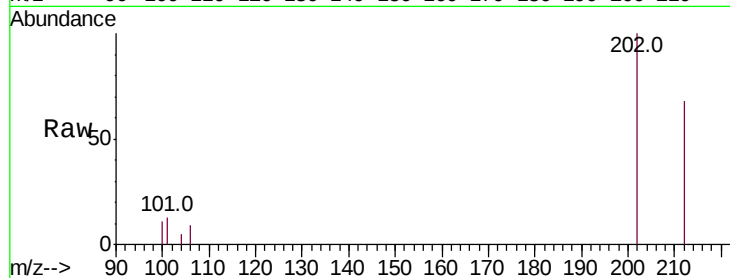

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

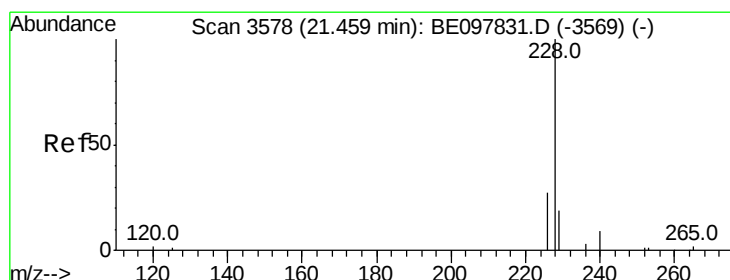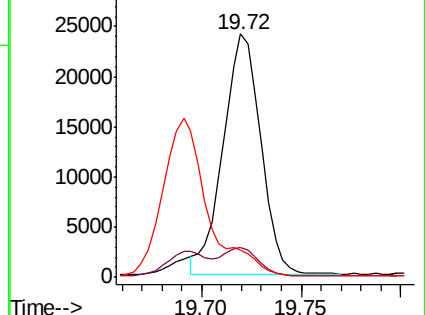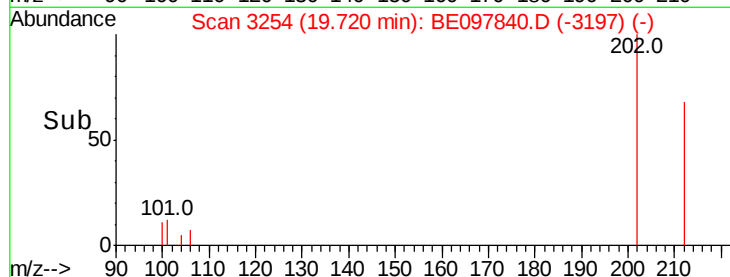

#18

Benzo(a)anthracene

Concen: 827.804 ng/ul

RT: 21.52 min Scan# 3588

Delta R.T. 0.06 min

Lab File: BE097840.D

Acq: 10 Oct 2018 22:43


Tgt Ion:228 Resp: 179212

Ion Ratio Lower Upper

228 100

229 20.5 16.4 24.6

226 30.9 21.5 32.3

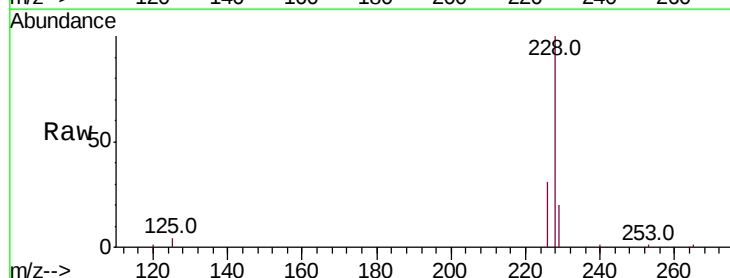

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

