

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE101018\
 Data File : BE097843.D
 Acq On : 11 Oct 2018 00:34
 Operator : SJ/JU
 Sample : J5183-07
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Oct 11 01:24:00 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE101018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 01:20:33 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	2724	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	13812	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.54	164	11311	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.40	188	2753836	0.40	ng/ul	0.11
16) Chrysene-d12	21.67	240	82	0.40	ng/ul	0.19
20) Perylene-d12	0.00	264	0	0.00	ng/ul	-24.03
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	13245	0.61	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.54	166	3955	0.099	ng/ul#	14
18) Benzo(a)anthracene	21.62	228	78	0.343	ng/ul#	1
19) Chrysene	21.70	228	59	0.269	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE101018\
Data File : BE097843.D
Acq On : 11 Oct 2018 00:34
Operator : SJ/JU
Sample : J5183-07
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Oct 11 01:24:00 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE101018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 01:20:33 2018
Response via : Initial Calibration




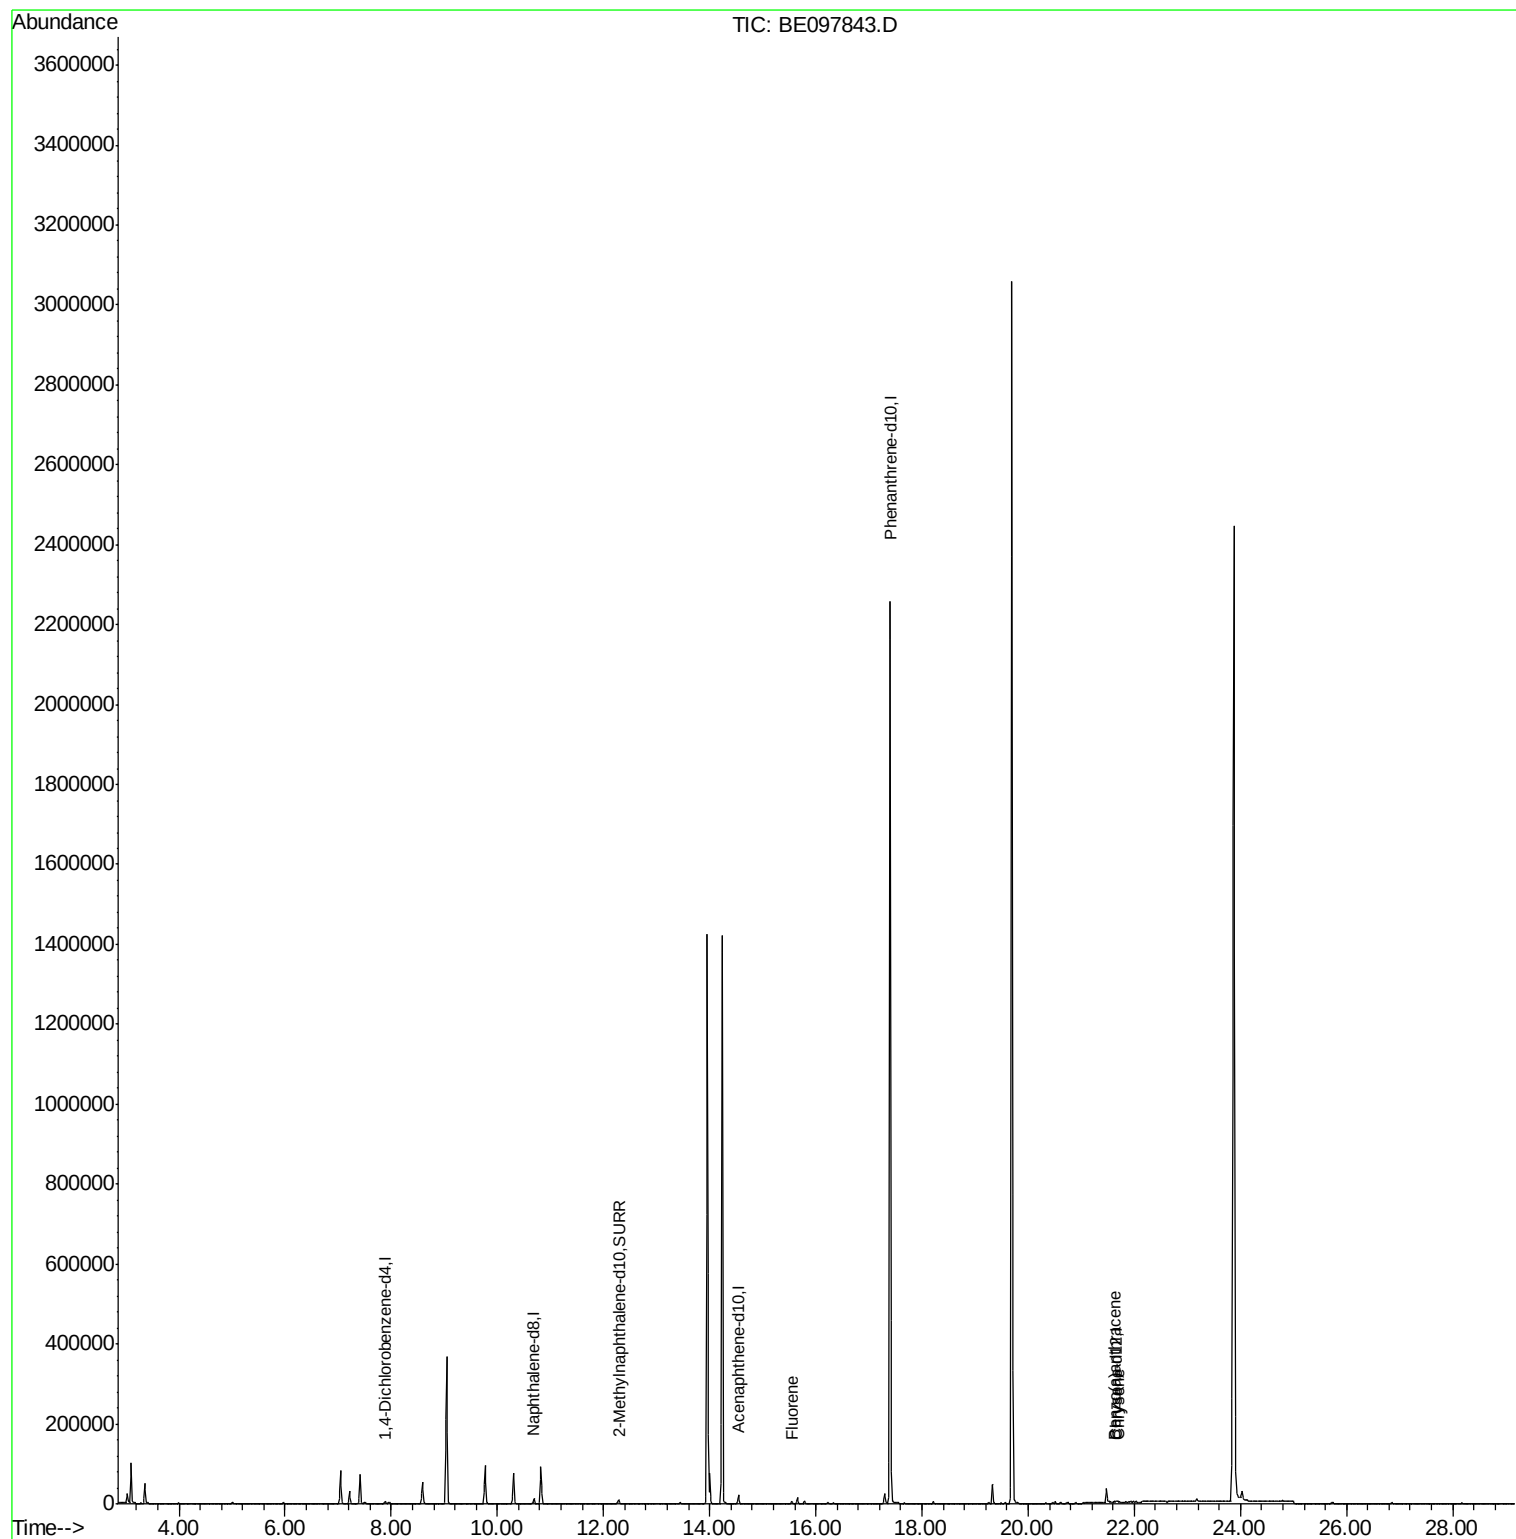


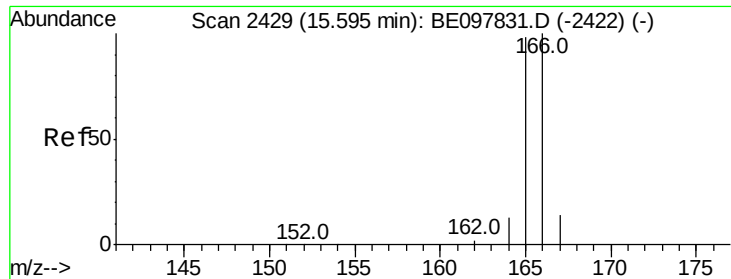

#9
Fluorene
 Concen: 0.099 ng/ul
 RT: 15.54 min Scan# 2421
 Delta R.T. -0.05 min
 Lab File: BE097843.D
 Acq: 11 Oct 2018 00:34




Instrument :
 BNA_E
 ClientSampleId :




Tot Ion:166 Resp: 3955
 Ion Ratio Lower Upper
 166 100
 165 7.2 79.2 118.8#
 167 31.4 11.3 16.9#

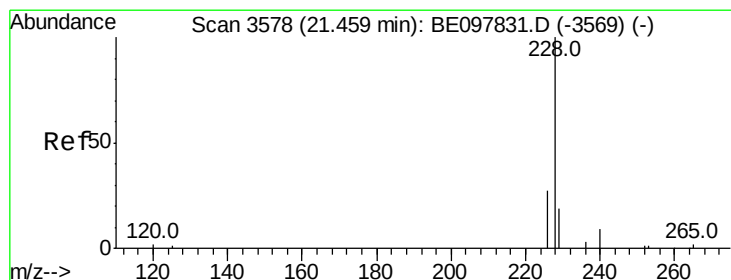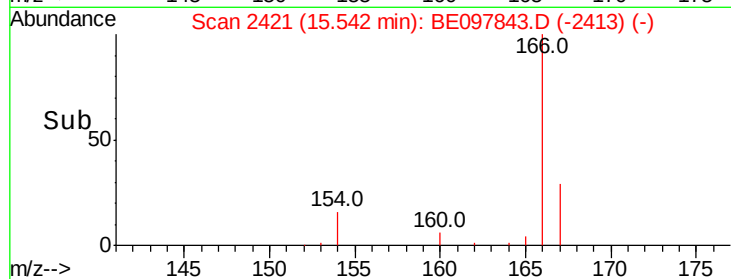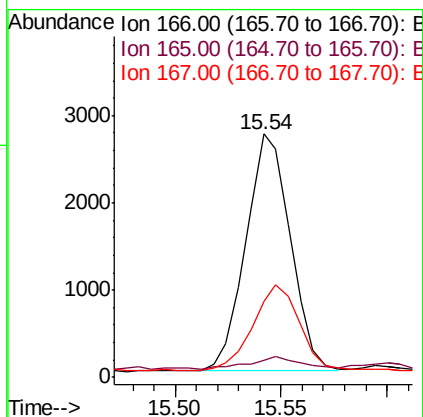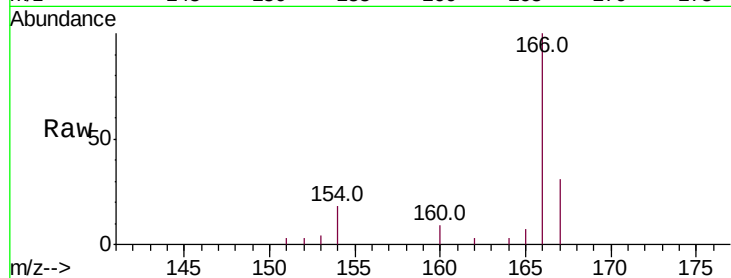

#18
Benzo(a)anthracene
 Concen: 0.343 ng/ul
 RT: 21.62 min Scan# 3603
 Delta R.T. 0.16 min
 Lab File: BE097843.D
 Acq: 11 Oct 2018 00:34

Tgt Ion:228 Resp: 78
 Ion Ratio Lower Upper
 228 100
 229 163.9 16.4 24.6#
 226 86.8 21.5 32.3#

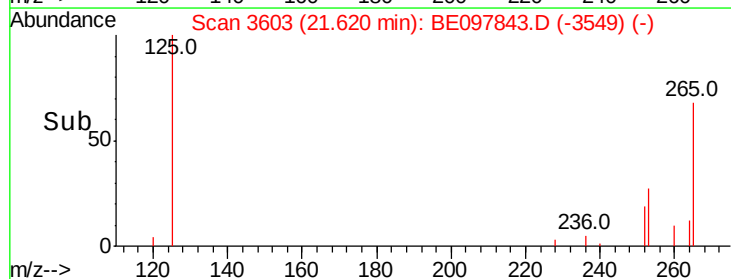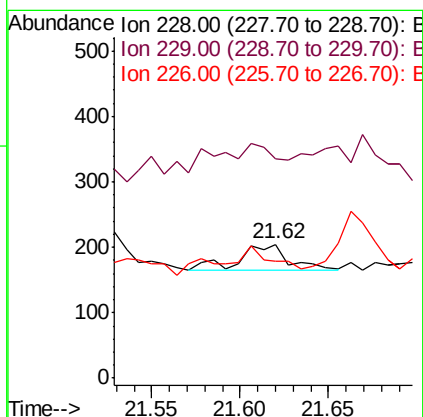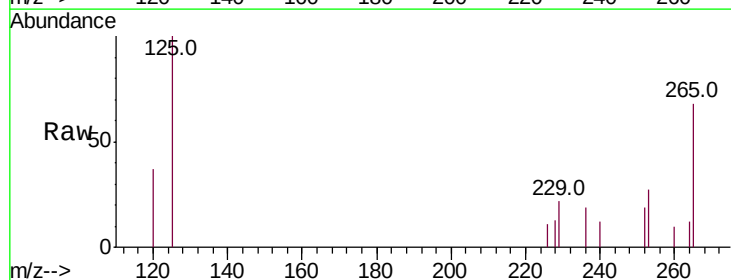

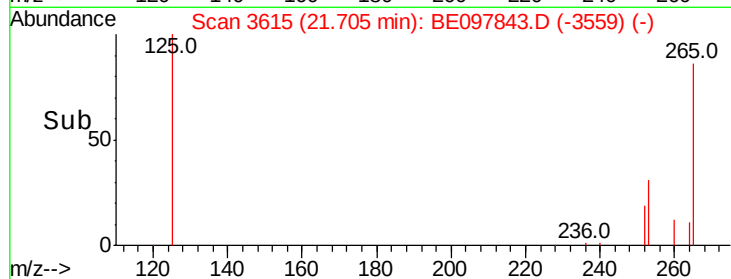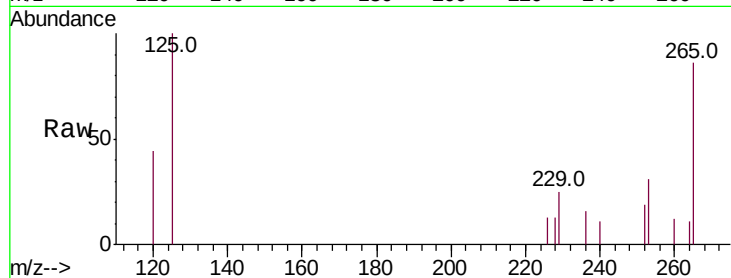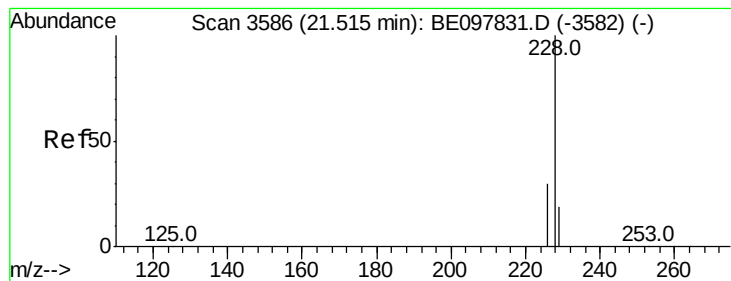

#19

Chrysene

Concen: 0.269 ng/ul

RT: 21.70 min Scan# 3615

Delta R.T. 0.19 min

Lab File: BE097843.D

Acq: 11 Oct 2018 00:34

Instrument :

BNA_E

ClientSampleId :

Tot Ion:228 Resp: 59

Ion Ratio Lower Upper

228 100

226 93.2 23.0 34.4#

229 184.2 15.5 23.3#

