


```
Data Path   : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE101018\  
Data File  : BE097832.D  
Acq On     : 10 Oct 2018   17:48  
Operator   : SJ/JU  
Sample     : J5184-05  
Misc      :  
ALS Vial   : 14      Sample Multiplier: 1
```

Instrument :
BNA_E
ClientSampleId :
JLC24

Manual Integrations

Sohil
10/11/2018 5:33:27 PM

Quant Time: Oct 10 18:50:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 12:43:48 2018
Response via : Initial Calibration

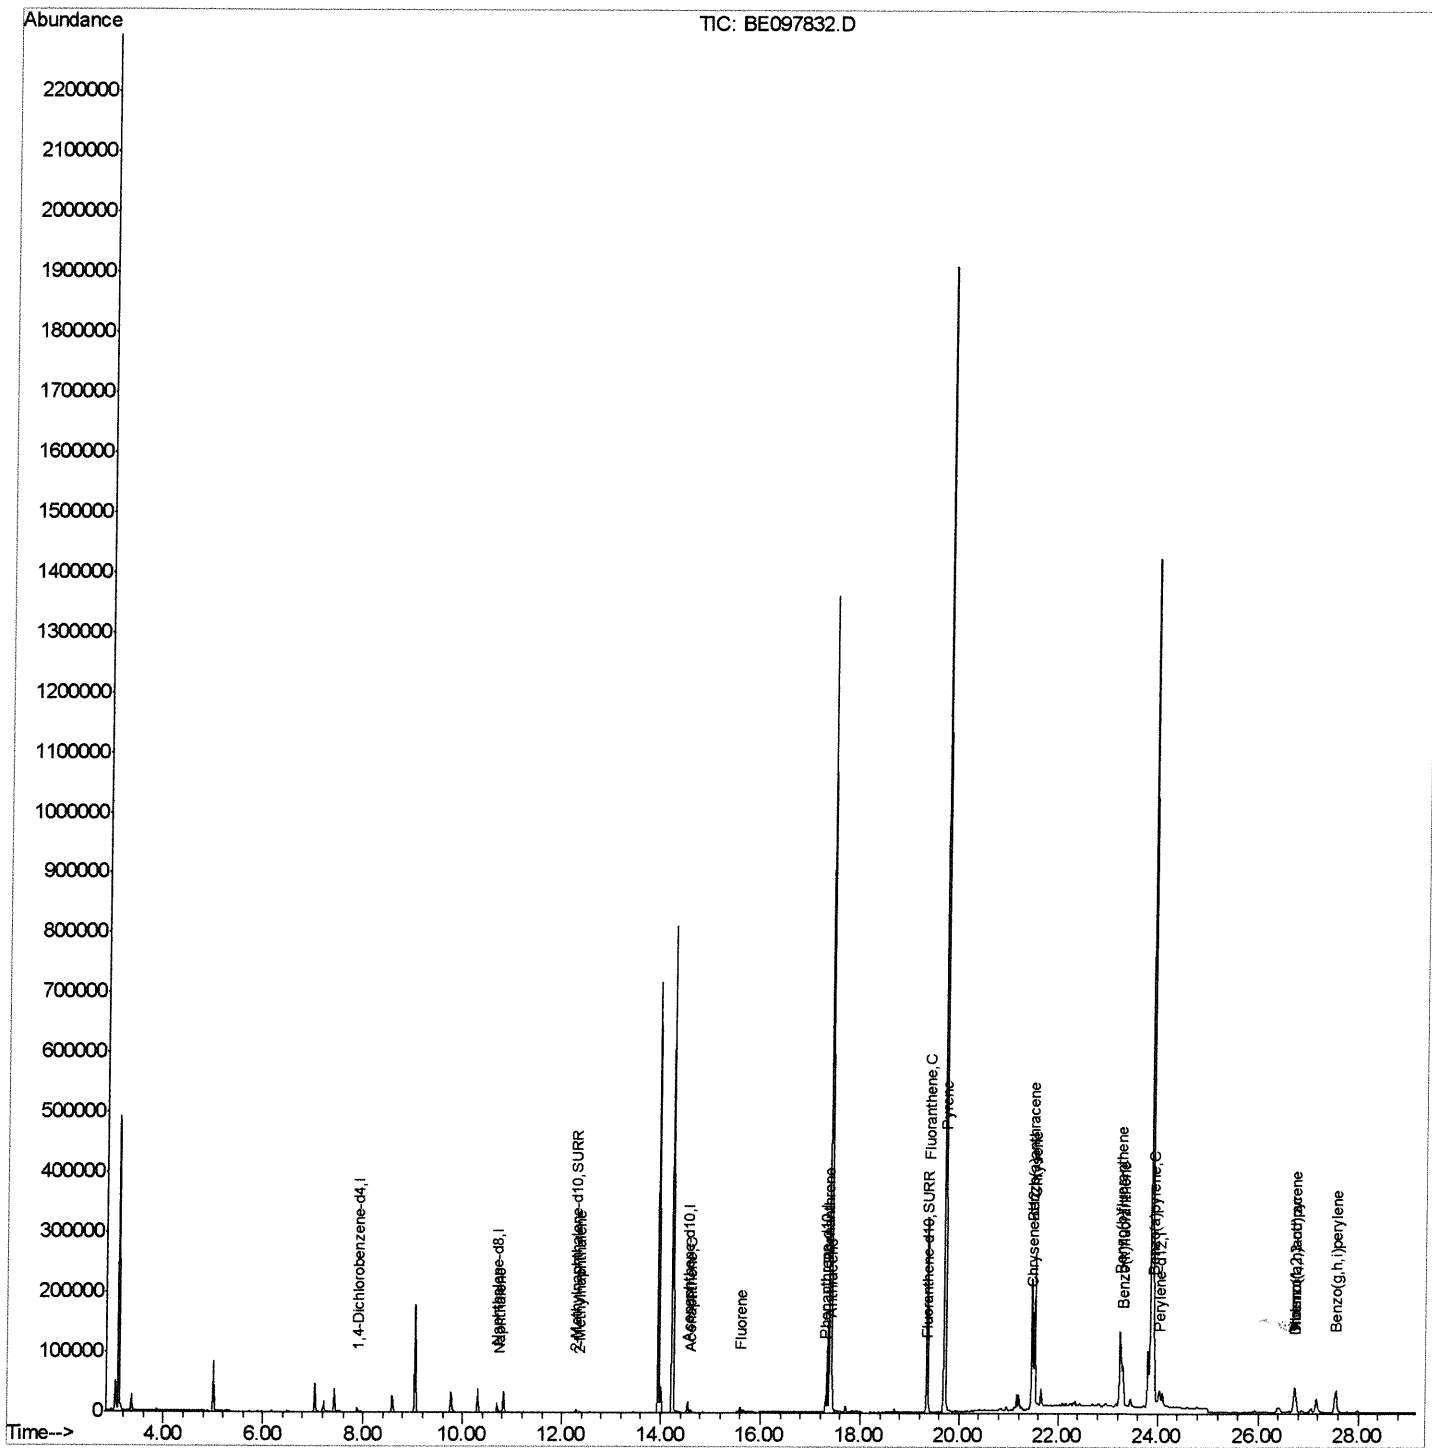

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE101018\
 Data File : BE097832.D
 Acq On : 10 Oct 2018 17:48
 Operator : SJ/JU
 Sample : J5184-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JLC24

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:33:27 PM

Quant Time: Oct 10 18:46:31 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 12:43:48 2018
 Response via : Initial Calibration

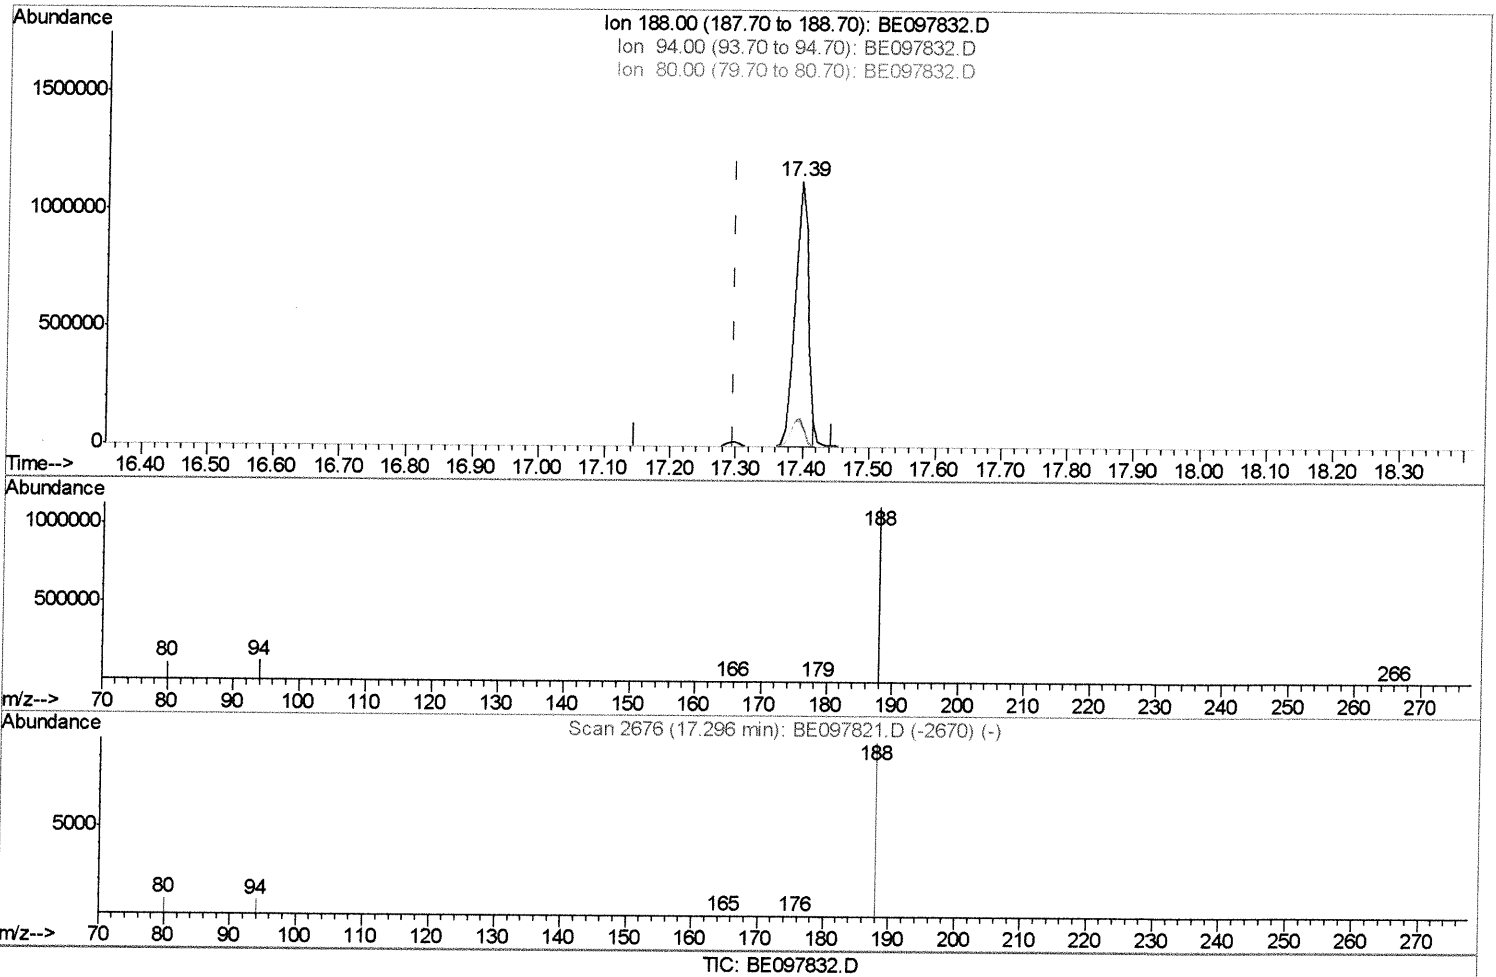

(10) Phenanthrene-d10 (I)
 17.395min (+0.099) 0.40ng/ul
 response 1593489

Ion	Exp%	Act%
188.00	100	100
94.00	8.60	10.82#
80.00	9.30	9.86
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE101018\
Data File : BE097832.D
Acq On : 10 Oct 2018 17:48
Operator : SJ/JU
Sample : J5184-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JLC24

Manual Integrations
APPROVED

Sohil
10/11/2018 5:33:27 PM

Quant Time: Oct 10 18:46:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 12:43:48 2018
Response via : Initial Calibration

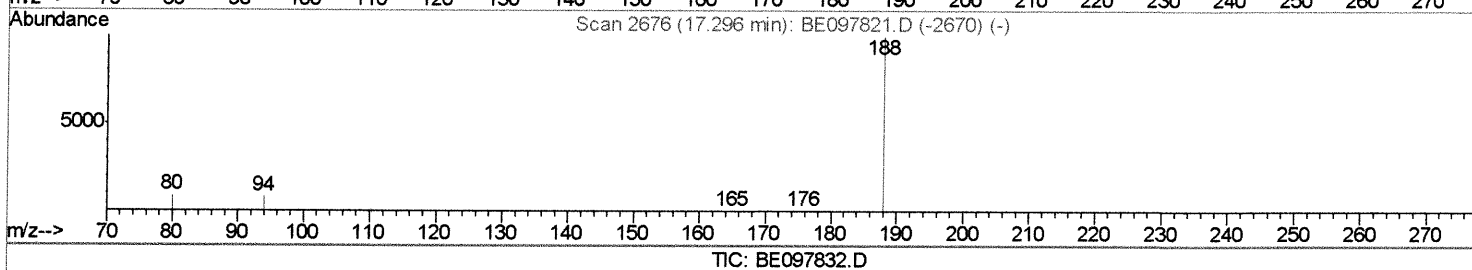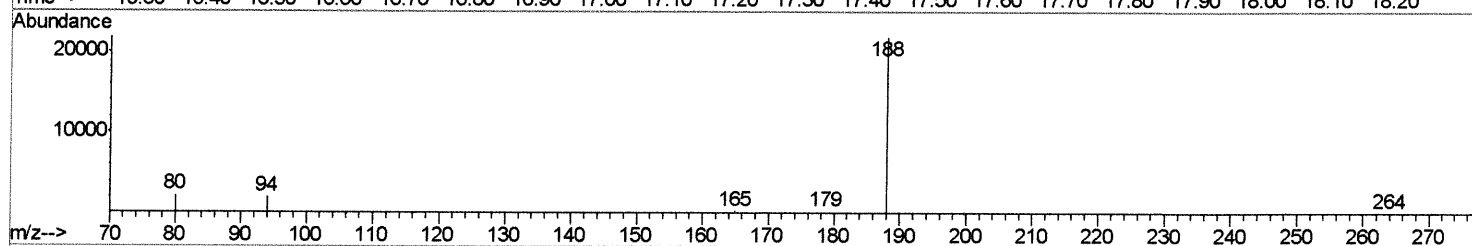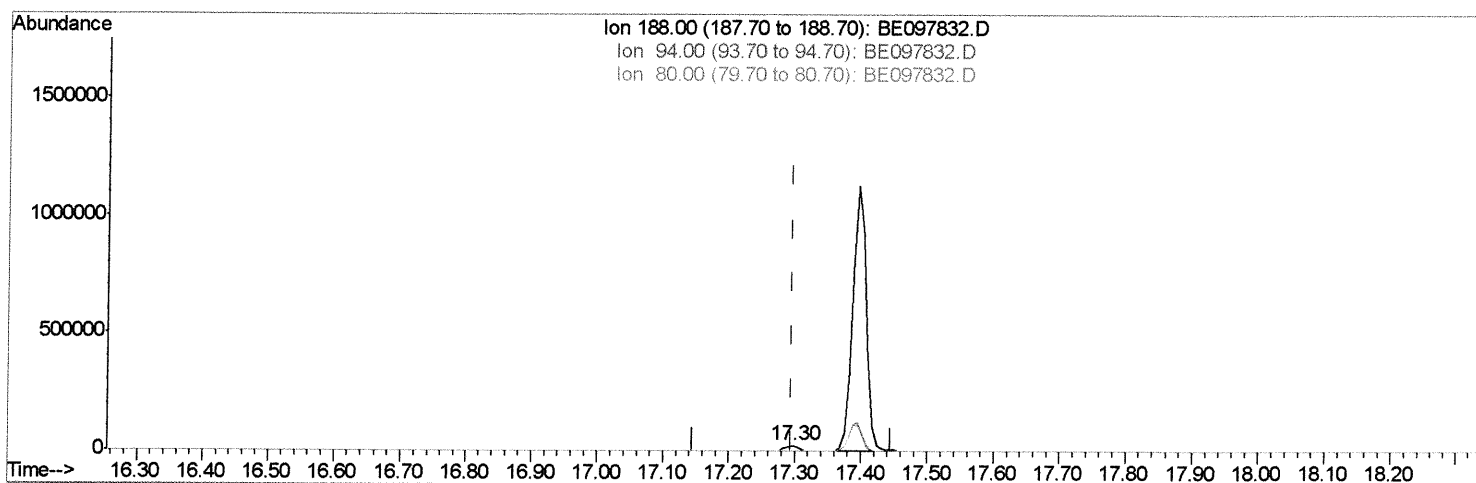

(10) Phenanthrene-d10 (I)

17.296min (+0.001) 0.40ng/ul m> SJ 10/16/18

response 31177

Ion	Exp%	Act%
188.00	100	100
94.00	8.60	9.06
80.00	9.30	9.84
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE101018\
Data File : BE097832.D
Acq On : 10 Oct 2018 17:48
Operator : SJ/JU
Sample : J5184-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JLC24

Manual Integrations
APPROVED

Sohil
10/11/2018 5:33:27 PM

Quant Time: Oct 10 18:47:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 12:43:48 2018
Response via : Initial Calibration

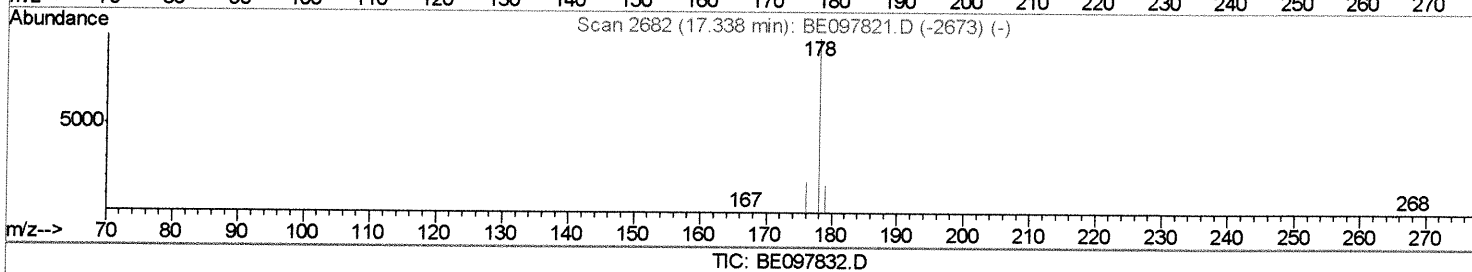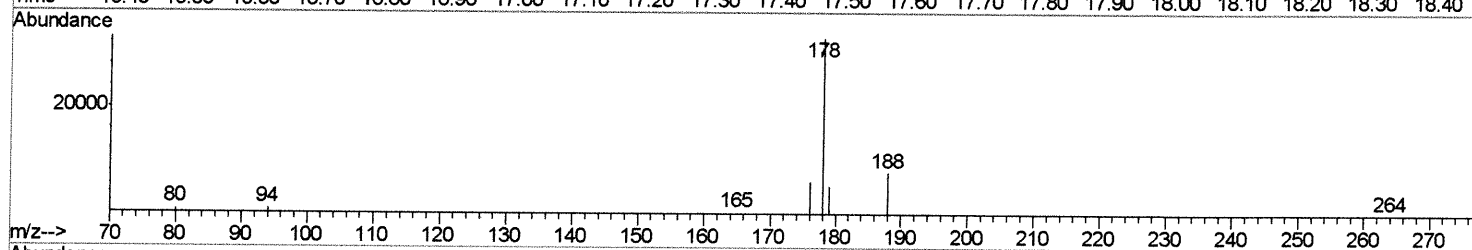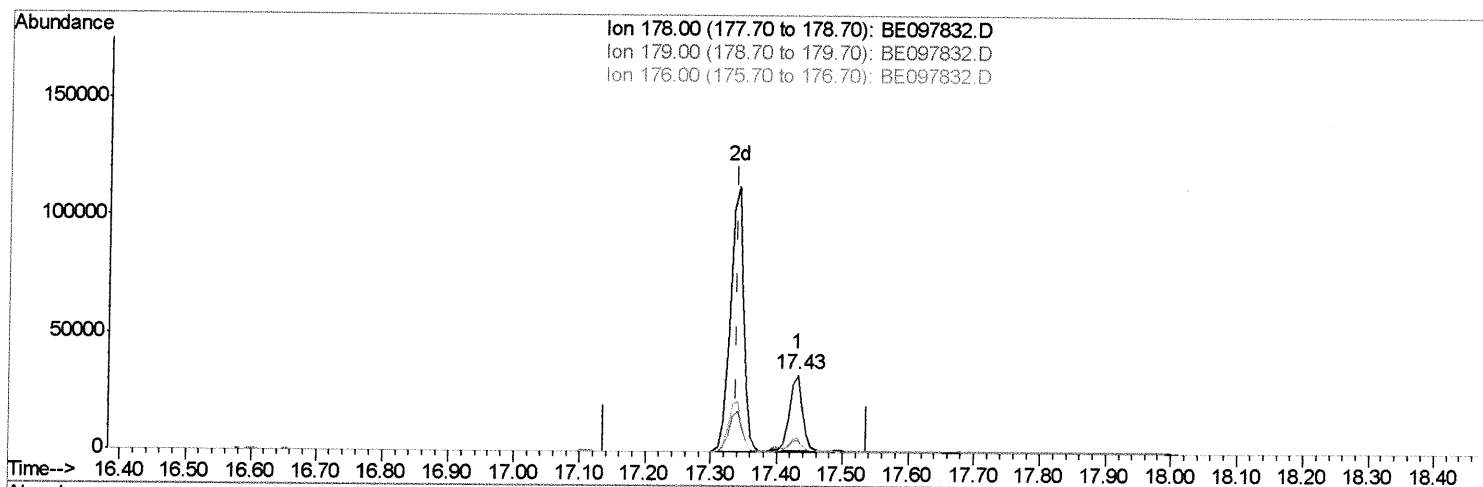

(12) Phenanthrene

17.430min (+0.092) 0.62ng/ul

response 46147

Ion	Exp%	Act%
178.00	100	100
179.00	16.00	15.89
176.00	18.60	18.96
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE101018\
Data File : BE097832.D
Acq On : 10 Oct 2018 17:48
Operator : SJ/JU
Sample : J5184-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JLC24

Manual Integrations
APPROVED

Sohil
10/11/2018 5:33:27 PM

Quant Time: Oct 10 18:47:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 12:43:48 2018
Response via : Initial Calibration

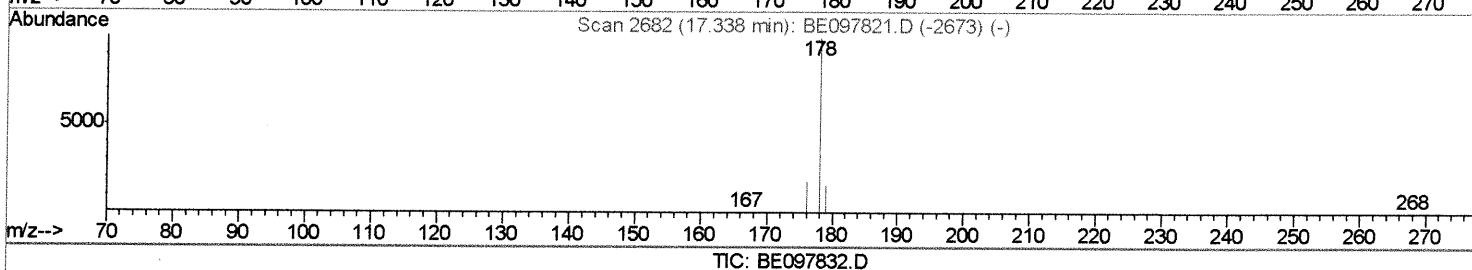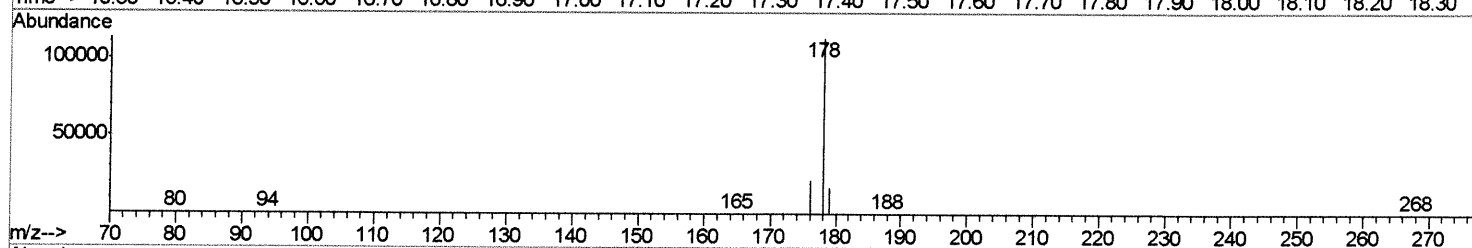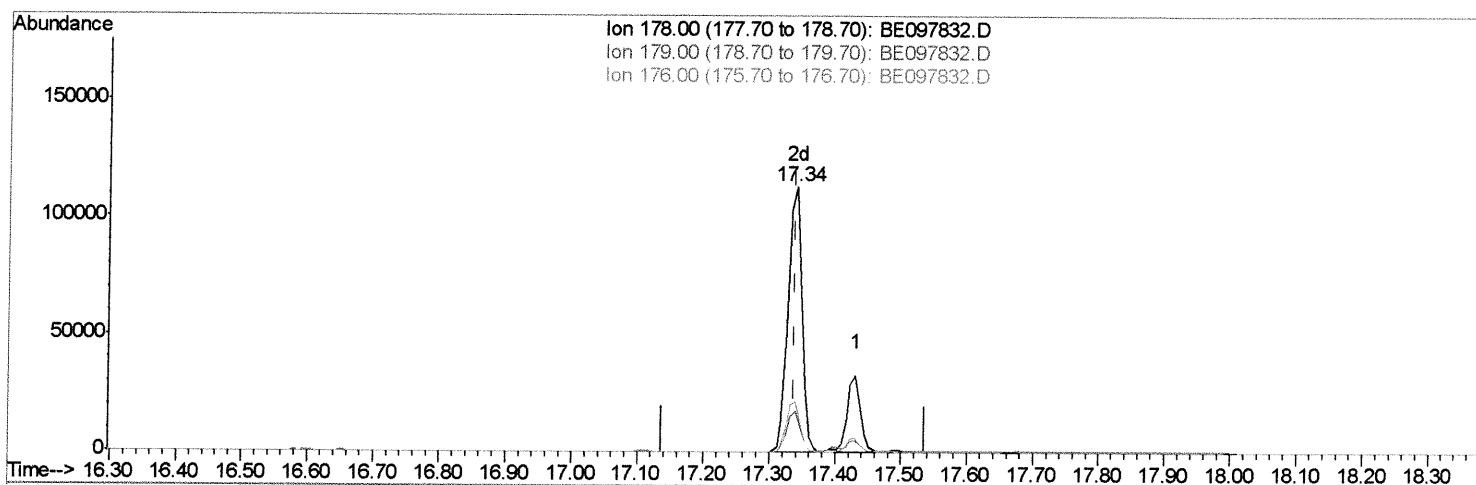

(12) Phenanthrene

17.339min (+0.001) 2.19ng/ul m > SJ 10/16/18

response 163280

Ion	Exp%	Act%
178.00	100	100
179.00	16.00	15.41
176.00	18.60	19.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE101018\
 Data File : BE097832.D
 Acq On : 10 Oct 2018 17:48
 Operator : SJ/JU
 Sample : J5184-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JLC24

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:33:27 PM

Quant Time: Oct 10 18:47:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 12:43:48 2018
 Response via : Initial Calibration

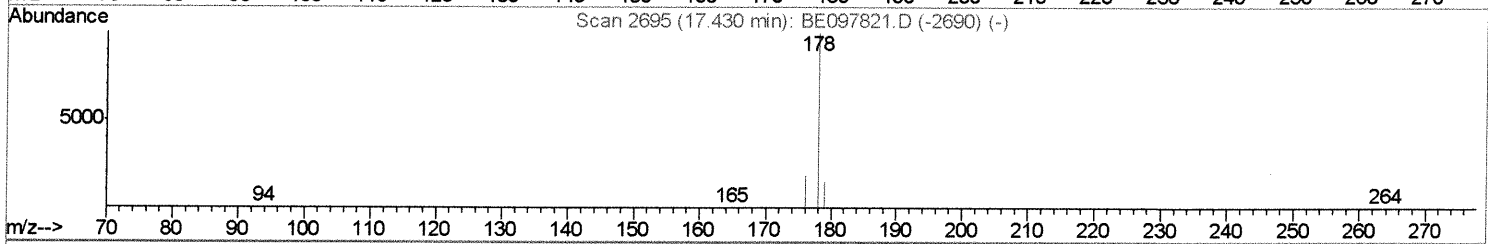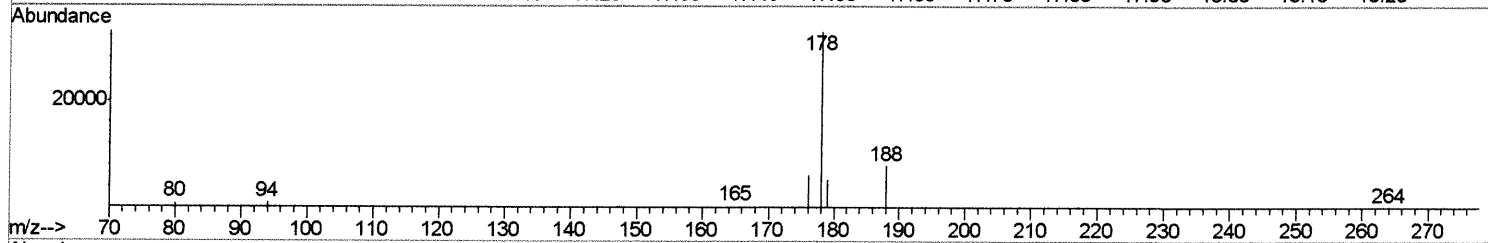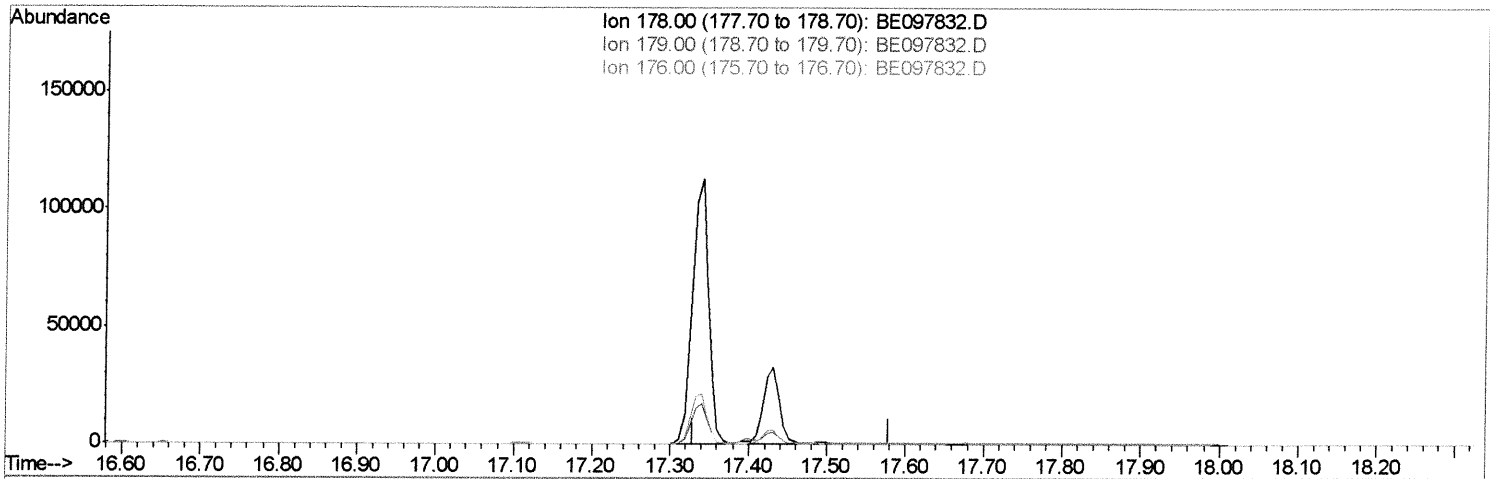

TIC: BE097832.D

(13) Anthracene

17.430min (-17.430) 0.00ng/ul

response 0

Ion	Exp%	Act%
178.00	100	0.00
179.00	16.10	0.00#
176.00	19.40	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE101018\
Data File : BE097832.D
Acq On : 10 Oct 2018 17:48
Operator : SJ/JU
Sample : J5184-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
JLC24

Manual Integrations
APPROVED

Sohil
10/11/2018 5:33:27 PM

Quant Time: Oct 10 18:47:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 12:43:48 2018
Response via : Initial Calibration

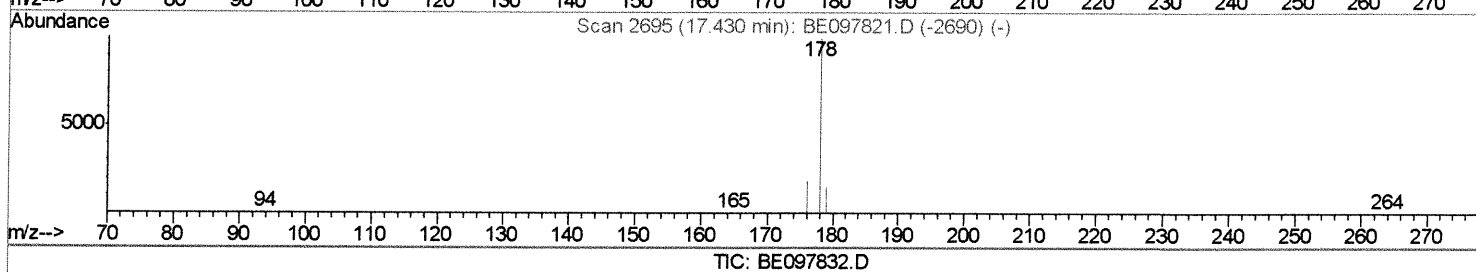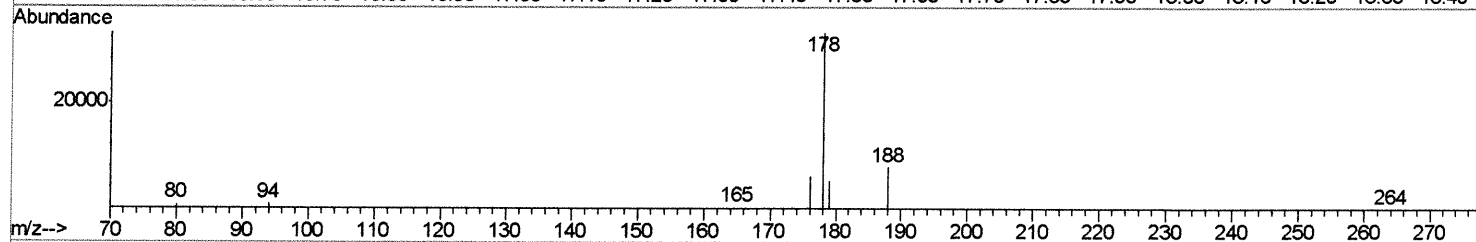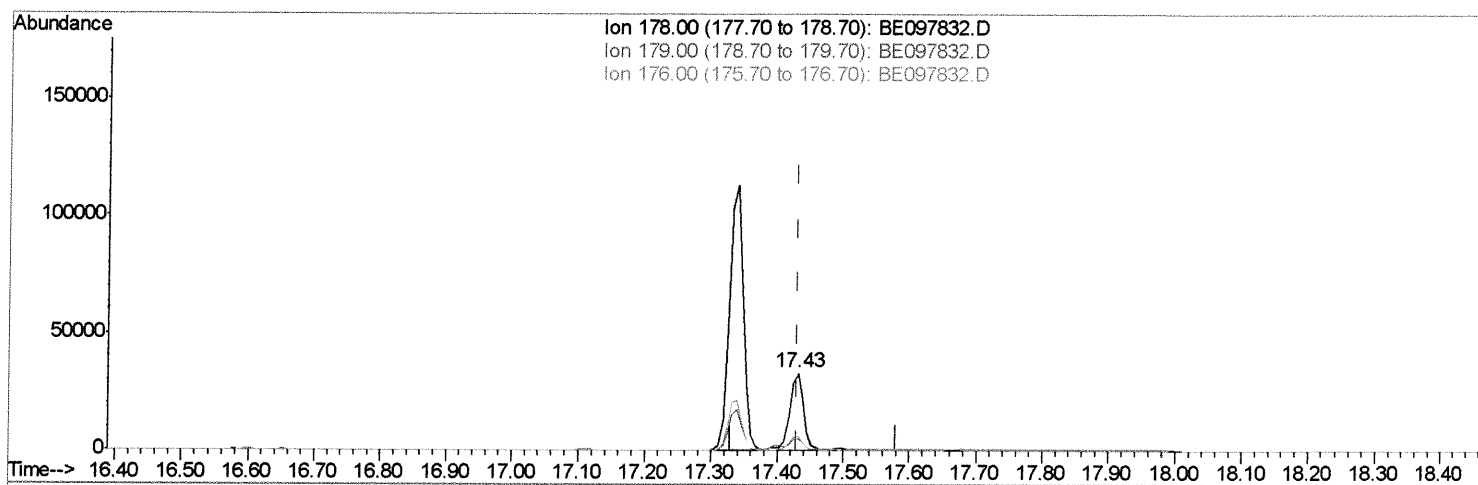

(13) Anthracene

17.430min (+0.001) 0.76ng/ul m> SJ 10/16/18

response 47903

Ion	Exp%	Act%
178.00	100	100
179.00	16.10	15.89
176.00	19.40	18.96
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE101018\
Data File : BE097832.D
Acq On : 10 Oct 2018 17:48
Operator : SJ/JU
Sample : J5184-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JLC24

Manual Integrations
APPROVED

Sohil
10/11/2018 5:33:27 PM

Quant Time: Oct 10 18:47:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 12:43:48 2018
Response via : Initial Calibration

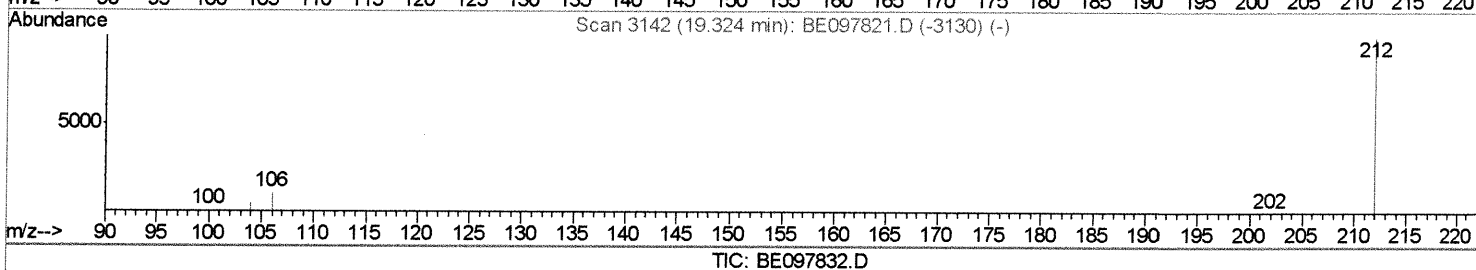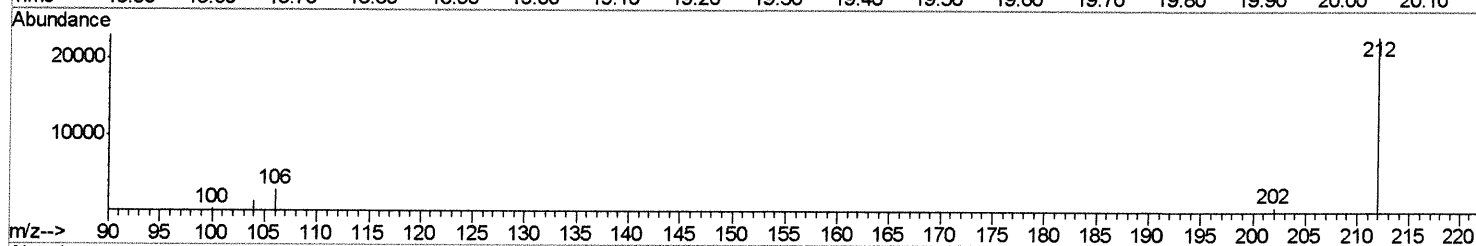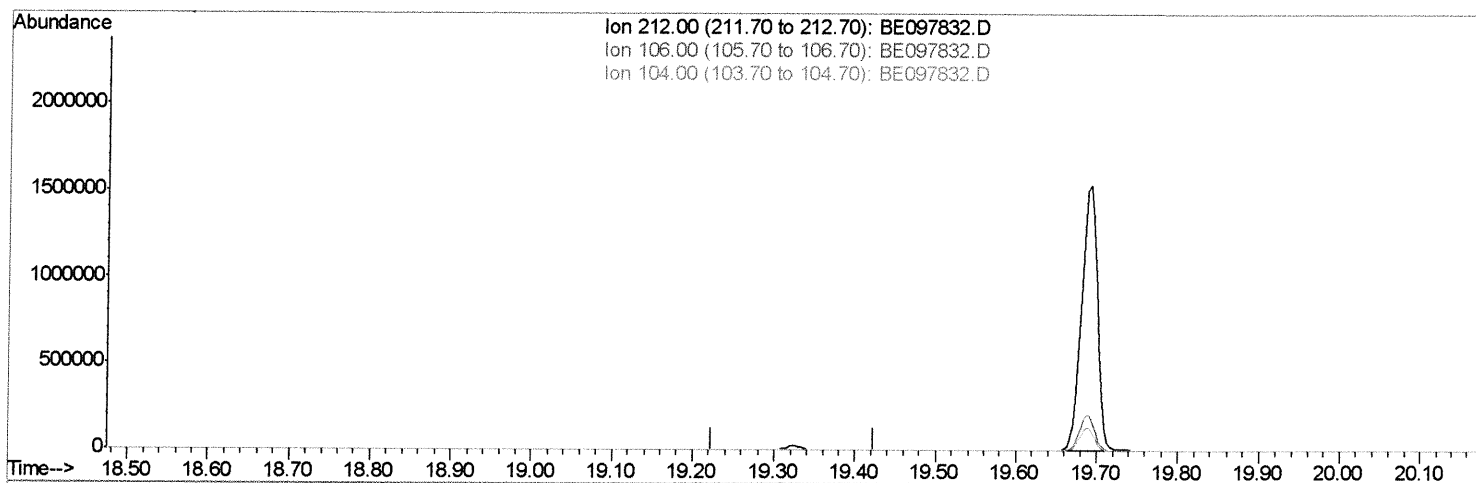

(14) Fluoranthene-d10 (SURR)

19.324min (-19.324) 0.00ng/ui

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	10.20	0.00#
104.00	5.80	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE101018\
Data File : BE097832.D
Acq On : 10 Oct 2018 17:48
Operator : SJ/JU
Sample : J5184-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JLC24

Manual Integrations
APPROVED

Sohil
10/11/2018 5:33:27 PM

Quant Time: Oct 10 18:47:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 12:43:48 2018
Response via : Initial Calibration

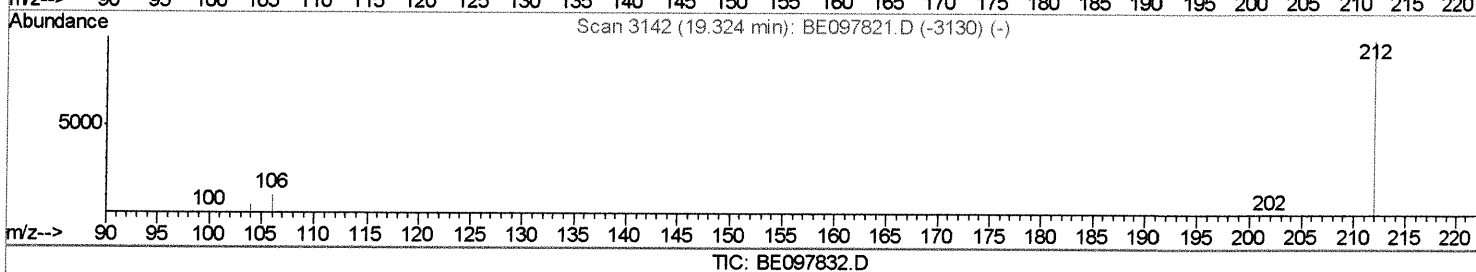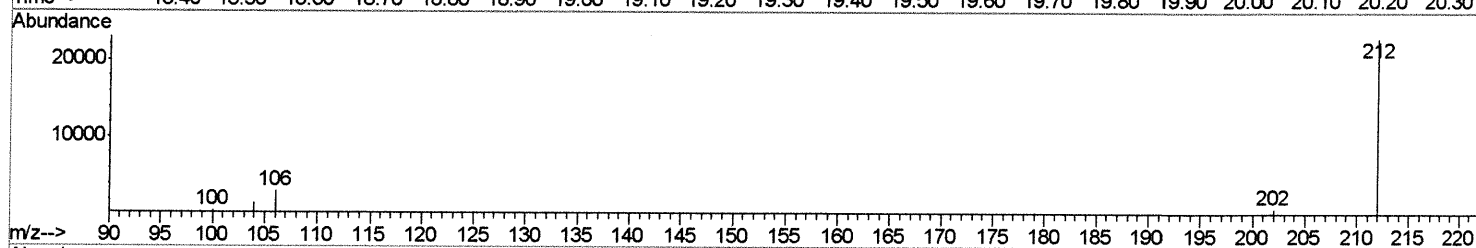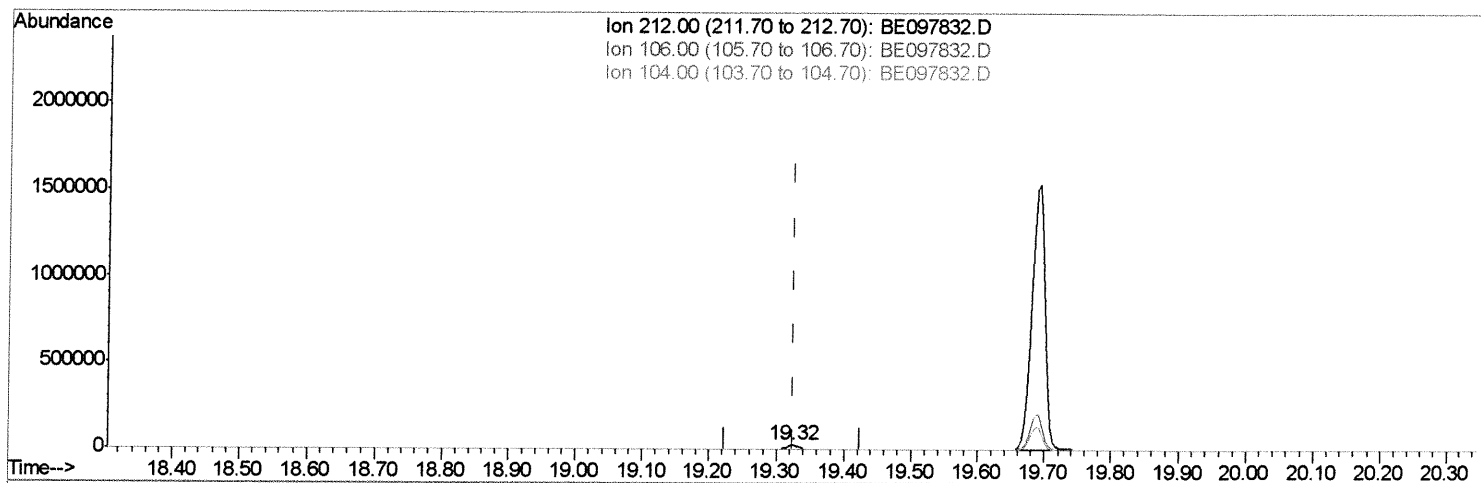

(14) Fluoranthene-d10 (SURR)

19.323min (-0.000) 0.30ng/ul m> SJ 10/16/18

response 30618

Ion	Exp%	Act%
212.00	100	100
106.00	10.20	0.00#
104.00	5.80	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE101018\
 Data File : BE097832.D
 Acq On : 10 Oct 2018 17:48
 Operator : SJ/JU
 Sample : J5184-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JLC24

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:33:27 PM

Quant Time: Oct 10 18:47:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 12:43:48 2018
 Response via : Initial Calibration

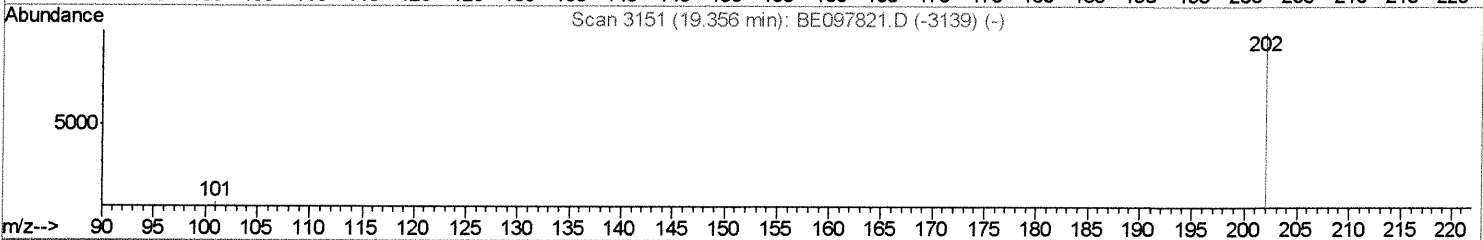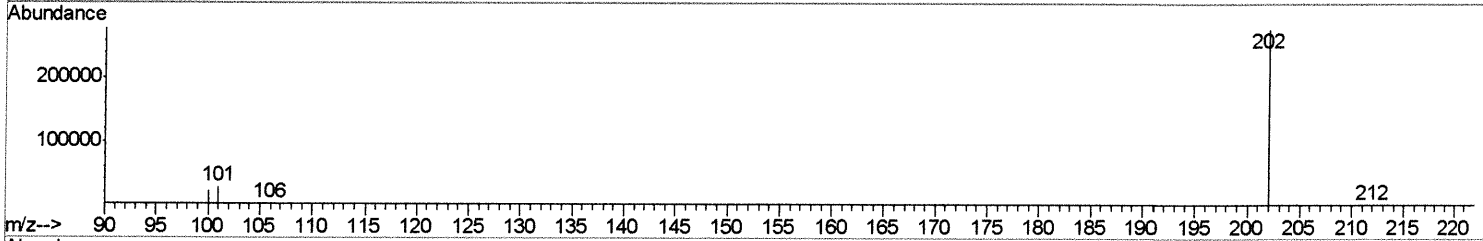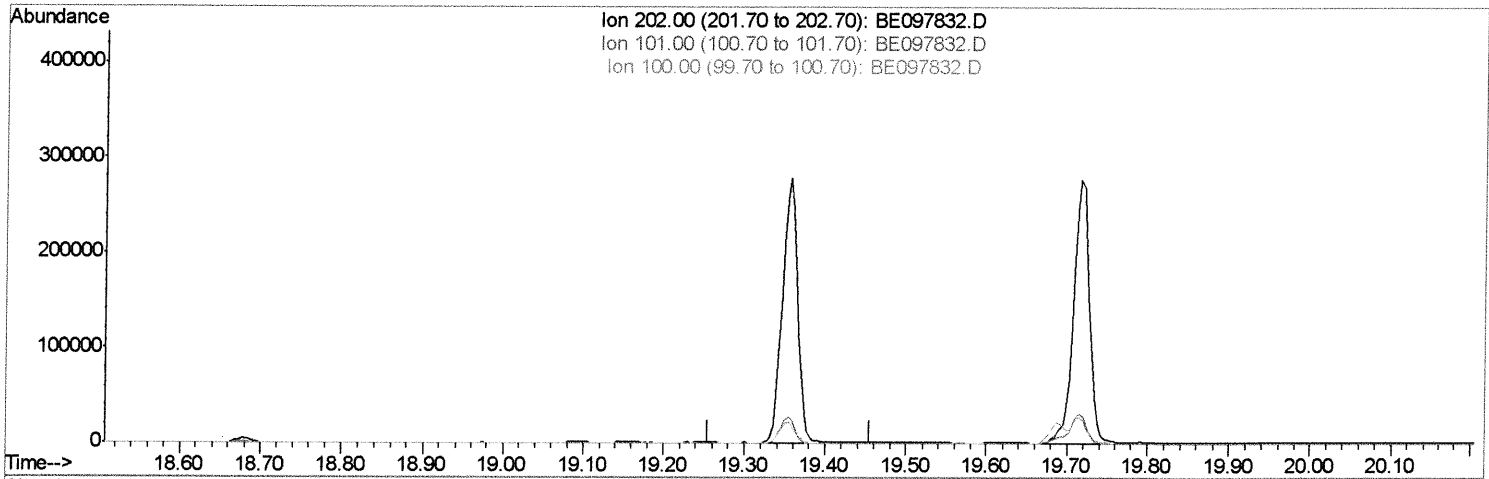

TIC: BE097832.D

(15) Fluoranthene (C)

19.356min (-19.356) 0.00ng/ul

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	9.30	0.00
100.00	7.50	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE101018\
 Data File : BE097832.D
 Acq On : 10 Oct 2018 17:48
 Operator : SJ/JU
 Sample : J5184-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JLC24

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:33:27 PM

Quant Time: Oct 10 18:47:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 12:43:48 2018
 Response via : Initial Calibration

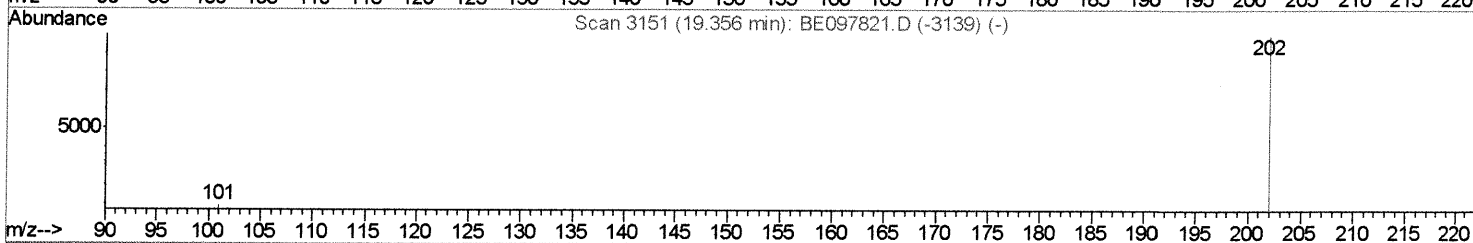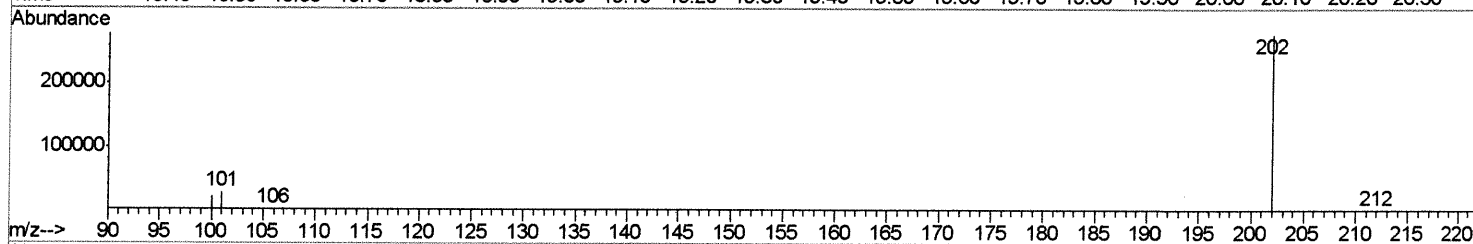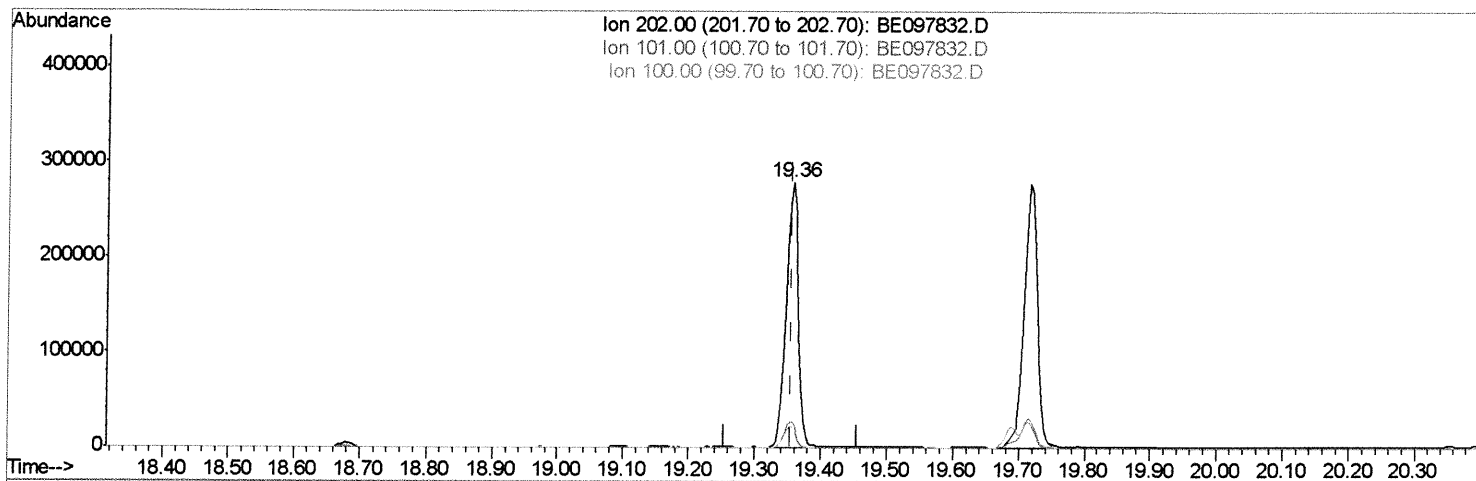

TIC: BE097832.D

(15) Fluoranthene (C)

19.355min (-0.000) 3.75ng/ul m> SJ 10/16/18

response 367915

Ion	Exp%	Act%
202.00	100	100
101.00	9.30	9.71
100.00	7.50	7.71
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE101018\
 Data File : BE097832.D
 Acq On : 10 Oct 2018 17:48
 Operator : SJ/JU
 Sample : J5184-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JLC24

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:33:27 PM

Quant Time: Oct 10 18:47:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 12:43:48 2018
 Response via : Initial Calibration

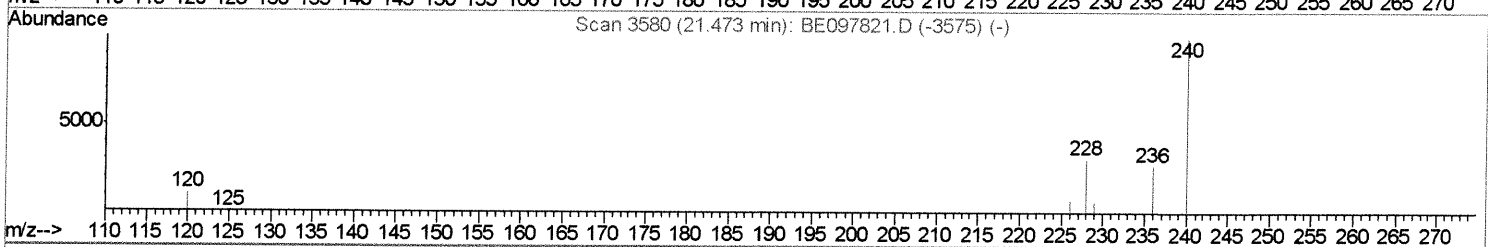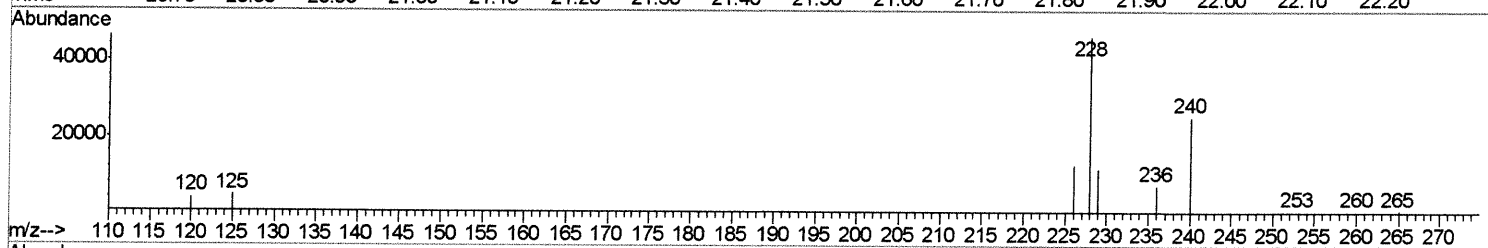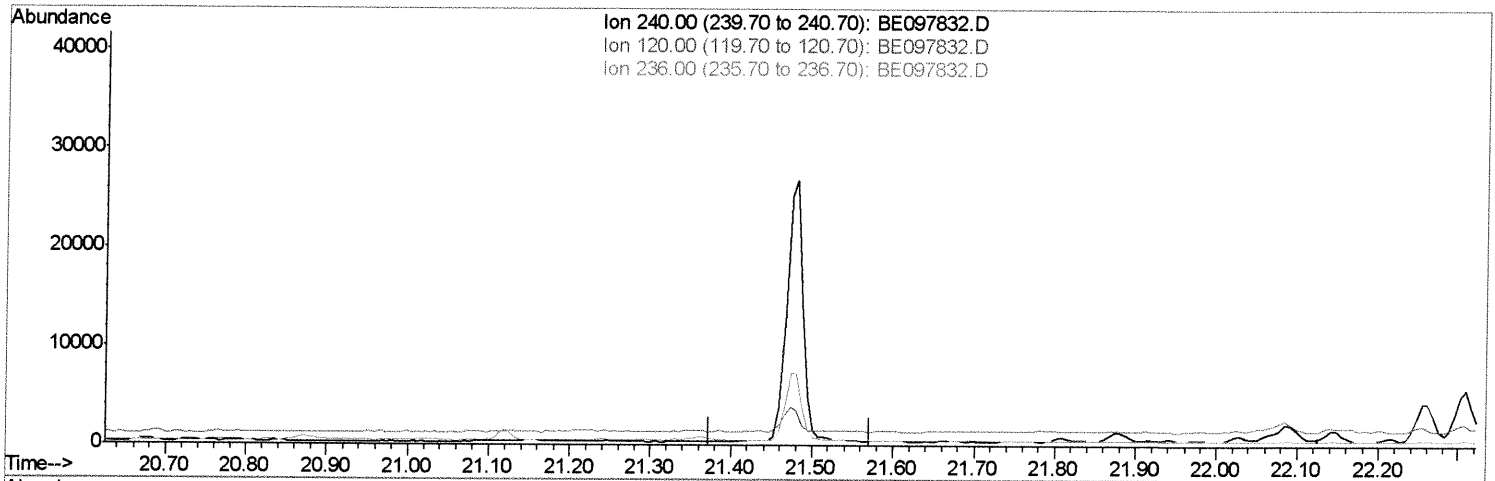

TIC: BE097832.D

(16) Chrysene-d12 (I)

21.473min (-21.473) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	10.70	0.00#
236.00	27.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE101018\
Data File : BE097832.D
Acq On : 10 Oct 2018 17:48
Operator : SJ/JU
Sample : J5184-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JLC24

Manual Integrations
APPROVED

Sohil
10/11/2018 5:33:27 PM

Quant Time: Oct 10 18:47:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 12:43:48 2018
Response via : Initial Calibration

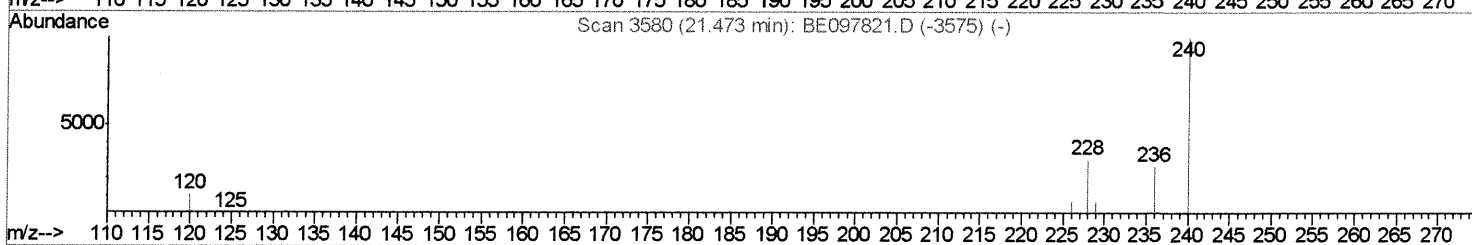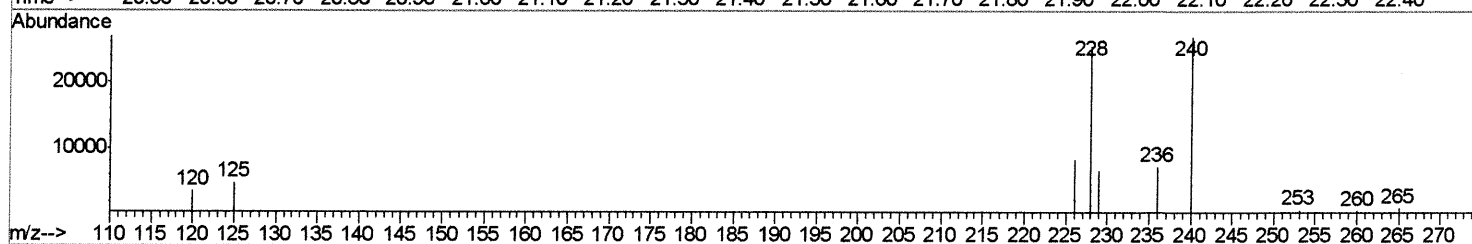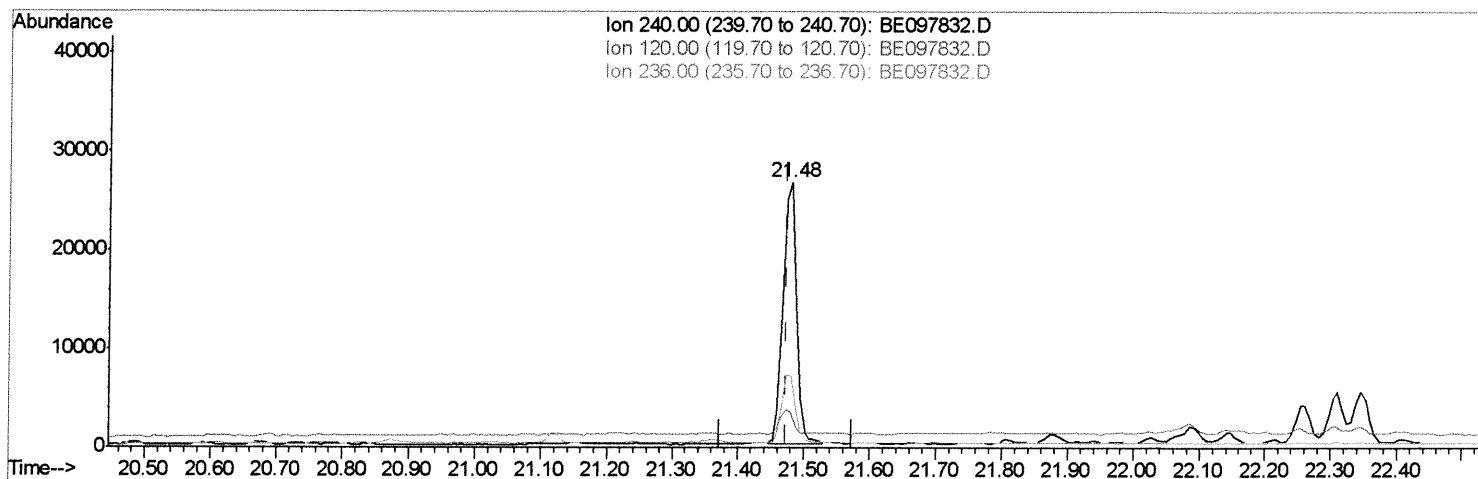

TIC: BE097832.D

(16) Chrysene-d12 (I)

21.480min (+0.007) 0.40ng/ul m > 5 10/16/18

response 37701

Ion	Exp%	Act%
240.00	100	100
120.00	10.70	13.15#
236.00	27.00	27.27
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE101018\
Data File : BE097832.D
Acq On : 10 Oct 2018 17:48
Operator : SJ/JU
Sample : J5184-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JLC24

Manual Integrations
APPROVED

Sohil
10/11/2018 5:33:27 PM

Quant Time: Oct 10 18:49:15 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 12:43:48 2018
Response via : Initial Calibration

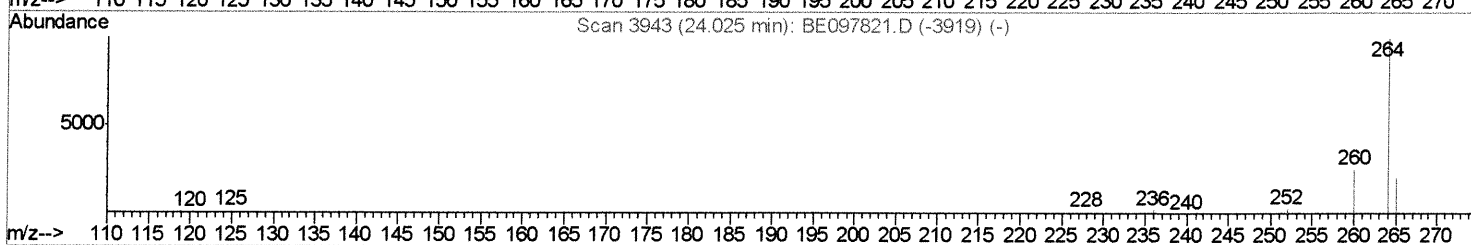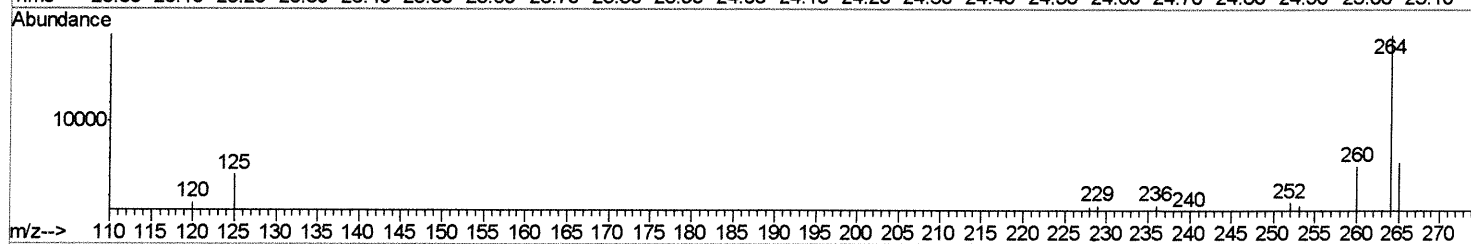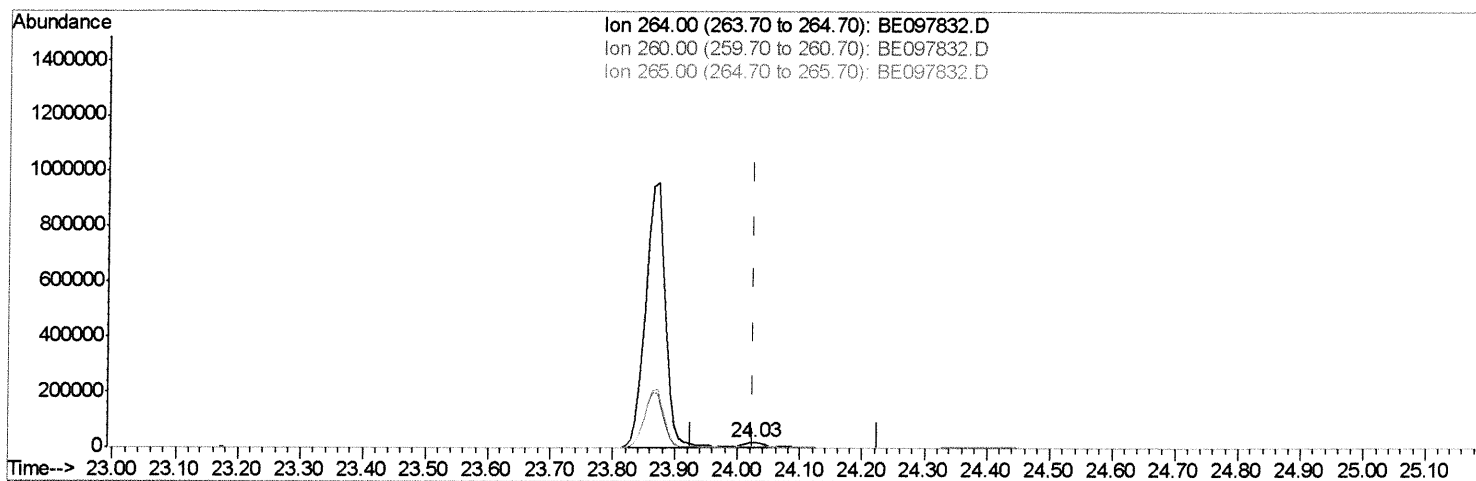

TIC: BE097832.D

(20) Perylene-d12 (I)

24.025min (-0.000) 0.40ng/ul

response 47408

Ion	Exp%	Act%
264.00	100	100
260.00	25.40	26.50
265.00	26.90	28.74
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE101018\
 Data File : BE097832.D
 Acq On : 10 Oct 2018 17:48
 Operator : SJ/JU
 Sample : J5184-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JLC24

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:33:27 PM

Quant Time: Oct 10 18:49:15 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 12:43:48 2018
 Response via : Initial Calibration

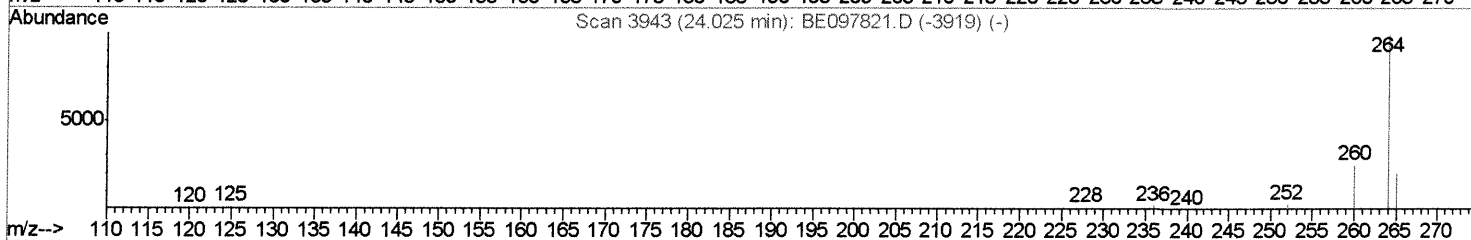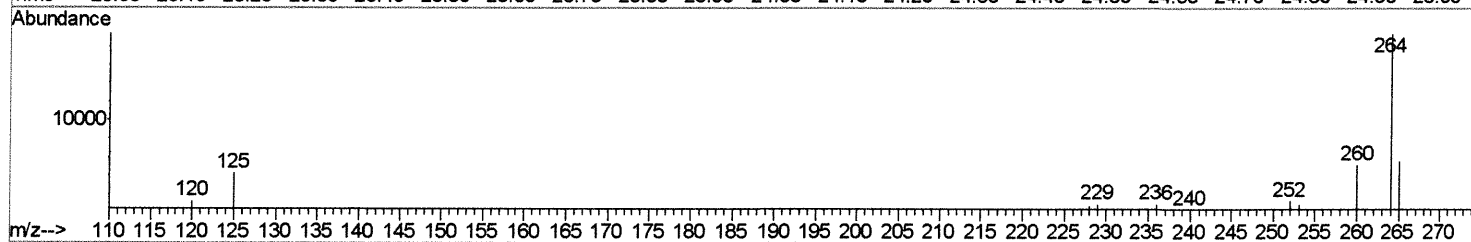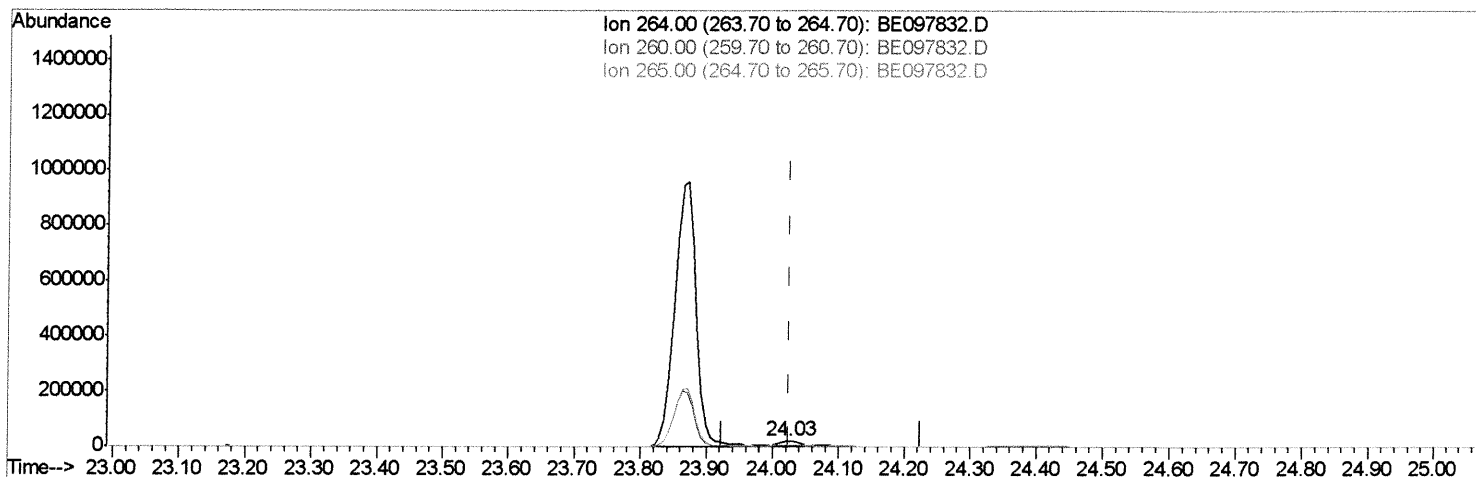

TIC: BE097832.D

(20) Perylene-d12 (I)

24.025min (-0.000) 0.40ng/ul m > SJ 10/16/18

response 31648

Ion	Exp%	Act%
264.00	100	100
260.00	25.40	26.50
265.00	26.90	28.74
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE101018\
Data File : BE097832.D
Acq On : 10 Oct 2018 17:48
Operator : SJ/JU
Sample : J5184-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JLC24

Manual Integrations
APPROVED

Sohil
10/11/2018 5:33:27 PM

Quant Time: Oct 10 18:49:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 12:43:48 2018
Response via : Initial Calibration

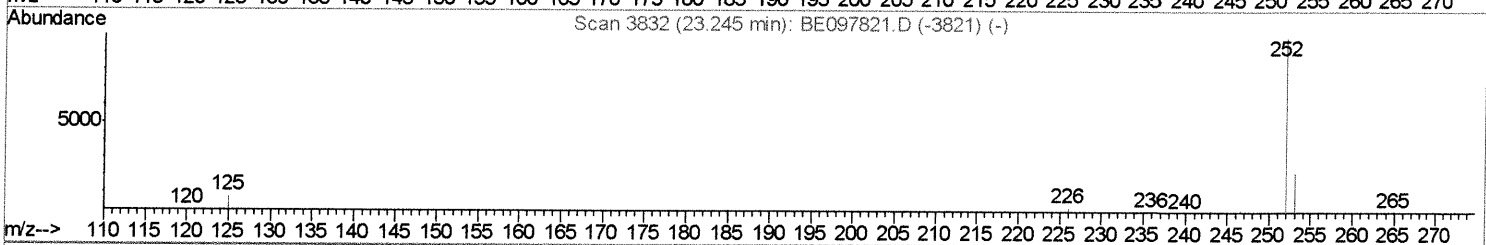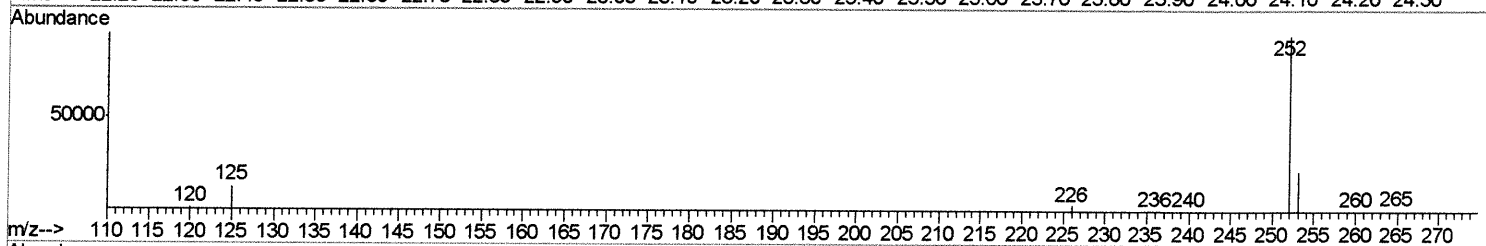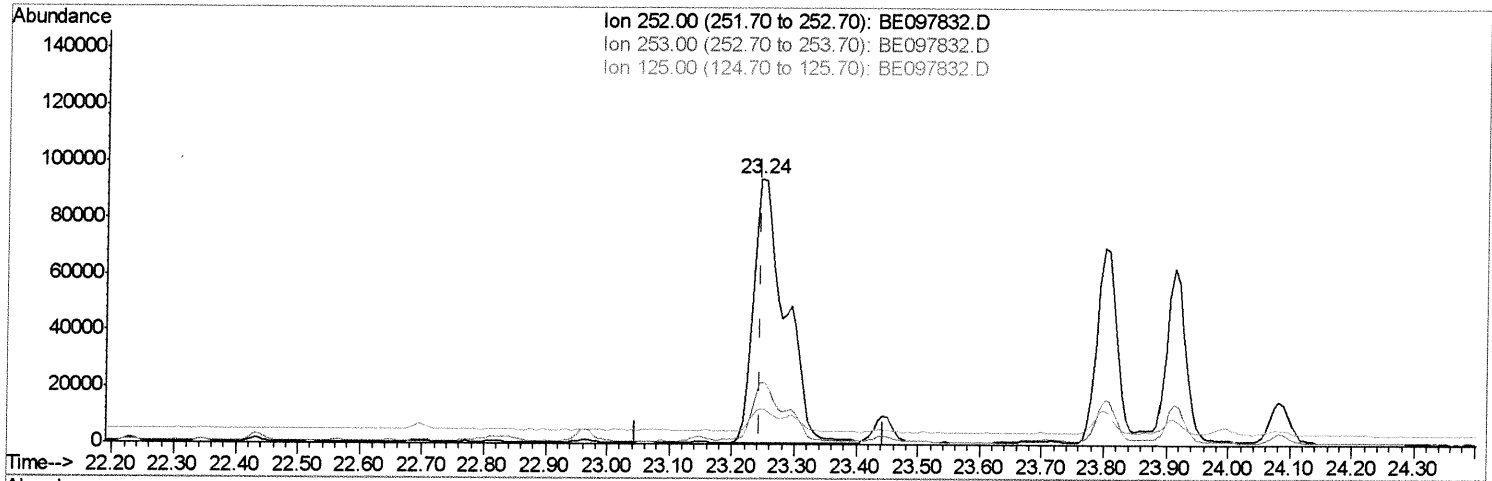

TIC: BE097832.D

(21) Benzo(b)fluoranthene

23.244min (-0.000) 4.04ng/ul

response 330120

Ion	Exp%	Act%
252.00	100	100
253.00	23.50	22.97
125.00	9.10	13.55
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE101018\
Data File : BE097832.D
Acq On : 10 Oct 2018 17:48
Operator : SJ/JU
Sample : J5184-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JLC24

Manual Integrations
APPROVED

Sohil
10/11/2018 5:33:27 PM

Quant Time: Oct 10 18:49:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 12:43:48 2018
Response via : Initial Calibration

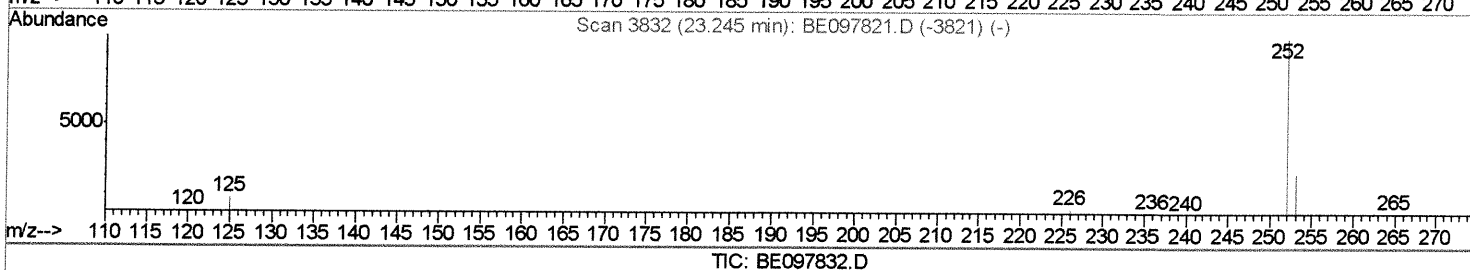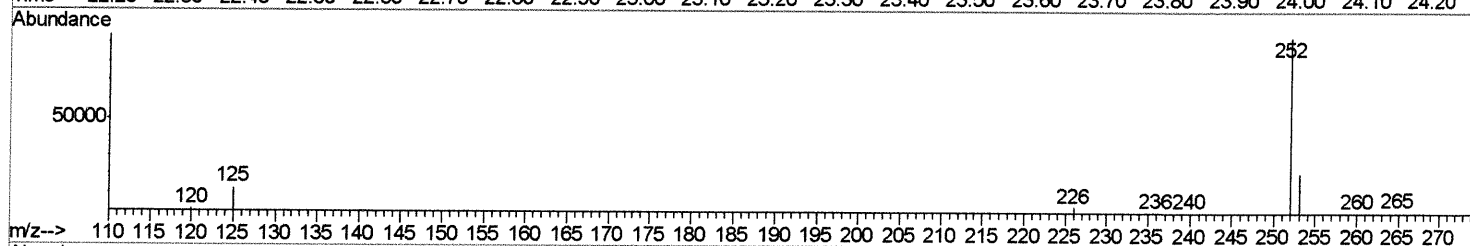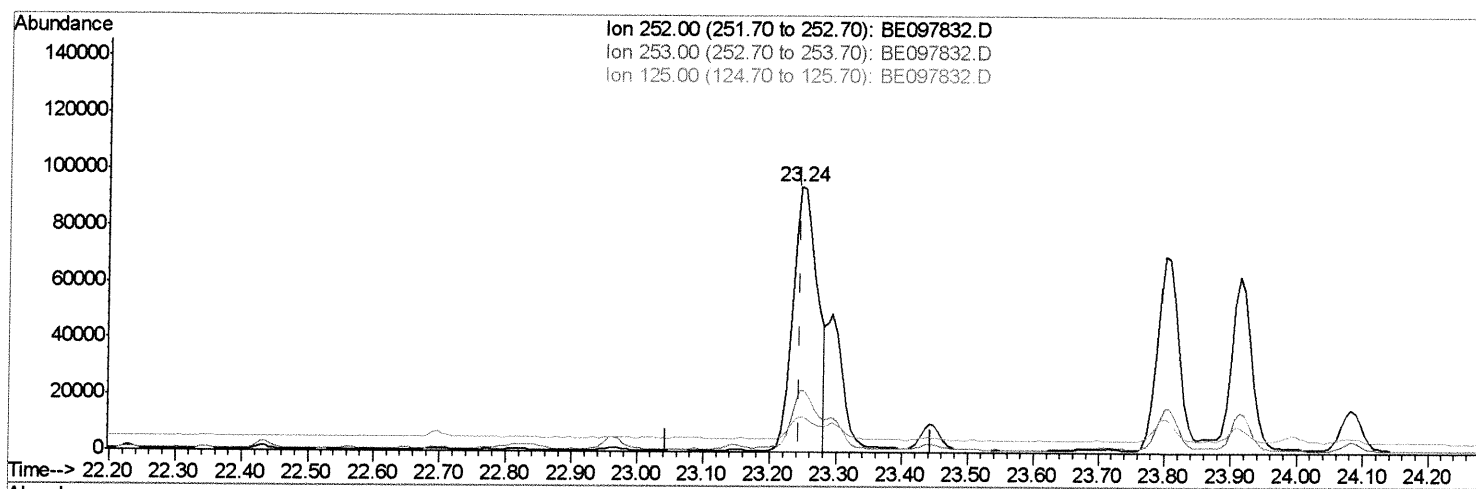

(21) Benzo(b)fluoranthene

23.244min (-0.000) 2.99ng/ul m > 5.0 10/16/18

response 244701

Ion	Exp%	Act%
252.00	100	100
253.00	23.50	22.97
125.00	9.10	13.55
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE101018\
Data File : BE097832.D
Acq On : 10 Oct 2018 17:48
Operator : SJ/JU
Sample : J5184-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JLC24

Manual Integrations
APPROVED

Sohil
10/11/2018 5:33:27 PM

Quant Time: Oct 10 18:49:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 12:43:48 2018
Response via : Initial Calibration

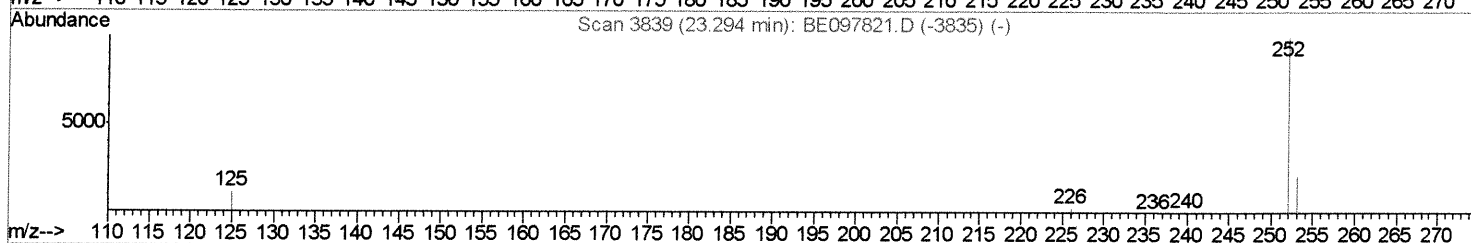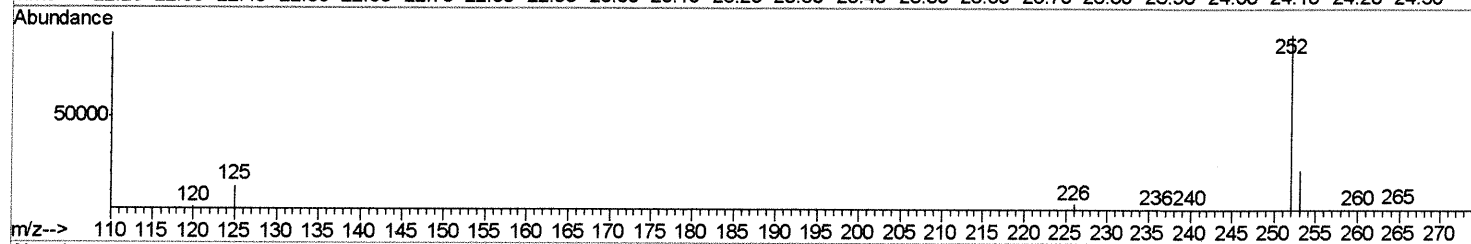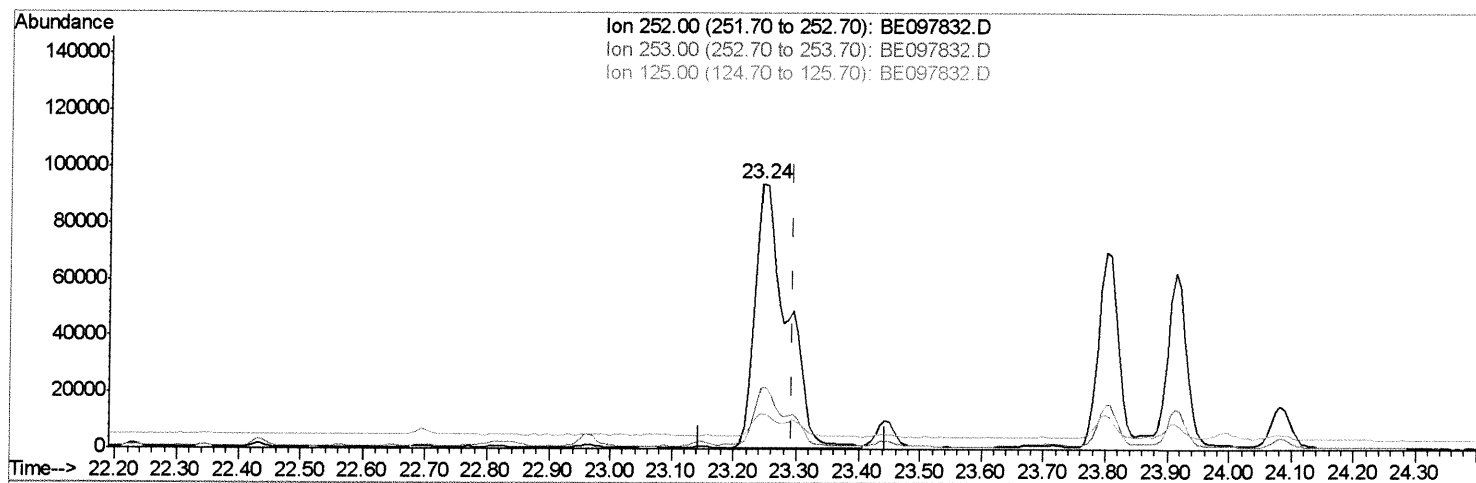

TIC: BE097832.D

(22) Benzo(k)fluoranthene

23.244min (-0.049) 3.56ng/ul

response 330120

Ion	Exp%	Act%
252.00	100	100
253.00	22.20	22.97
125.00	11.70	13.55
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE101018\
Data File : BE097832.D
Acq On : 10 Oct 2018 17:48
Operator : SJ/JU
Sample : J5184-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JLC24

Manual Integrations
APPROVED

Sohil
10/11/2018 5:33:27 PM

Quant Time: Oct 10 18:49:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 12:43:48 2018
Response via : Initial Calibration

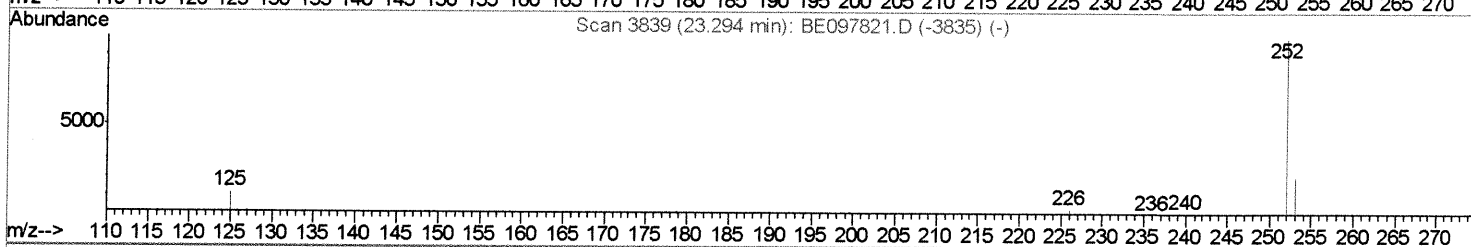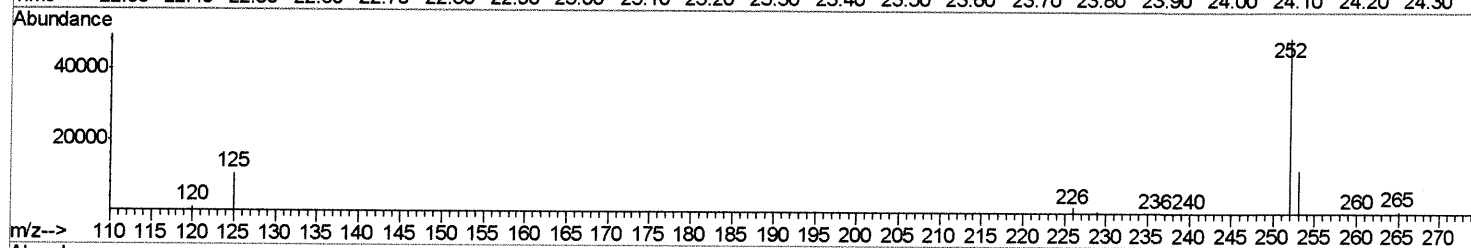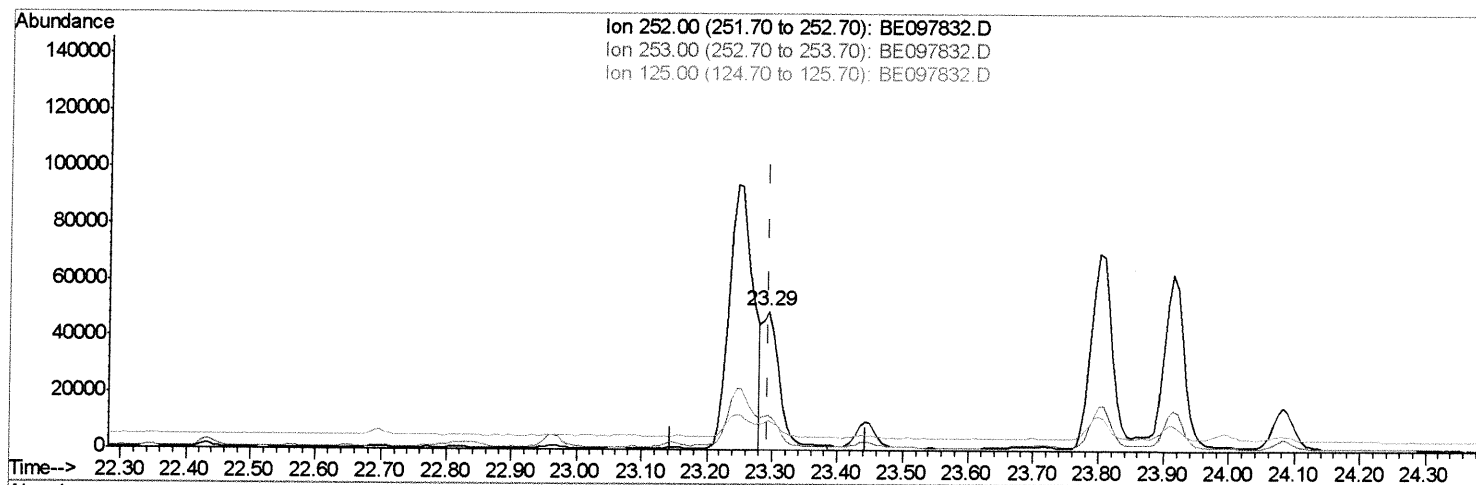

TIC: BE097832.D

(22) Benzo(k)fluoranthene

23.294min (-0.000) 0.98ng/ul m

response 90677

Ion	Exp%	Act%
252.00	100	100
253.00	22.20	25.48
125.00	11.70	21.91#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE101018\
 Data File : BE097832.D
 Acq On : 10 Oct 2018 17:48
 Operator : SJ/JU
 Sample : J5184-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JLC24

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:33:27 PM

Quant Time: Oct 10 18:50:52 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 12:43:48 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.88	152	3124	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	15349	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.54	164	11090	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.30	188	31177m	0.40	ng/ul	0.00
16) Chrysene-d12	21.48	240	37701m	0.40	ng/ul	0.00
20) Perylene-d12	24.03	264	31648m	0.40	ng/ul	0.00

SJ 10/16/18

System Monitoring Compounds
 4) 2-Methylnaphthalene-d10
 14) Fluoranthene-d10

12.28	152	7102	0.30	ng/ul	0.00
19.32	212	30618m	0.30	ng/ul	0.00

SJ 10/16/18

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Naphthalene	10.74	128	1052	0.028	ng/ul#	71
5) 2-Methylnaphthalene	12.36	142	713	0.029	ng/ul	94
8) Acenaphthene	14.60	153	3008	0.092	ng/ul	96
9) Fluorene	15.59	166	4861	0.124	ng/ul	96
12) Phenanthrene	17.34	178	163280m	2.192	ng/ul	
13) Anthracene	17.43	178	47903m	0.757	ng/ul	
15) Fluoranthene	19.36	202	367915m	3.747	ng/ul	
17) Pyrene	19.72	202	384324	4.149	ng/ul	99
18) Benzo(a)anthracene	21.46	228	204961	1.959	ng/ul	99
19) Chrysene	21.51	228	261421	2.590	ng/ul	96
21) Benzo(b)fluoranthene	23.24	252	244701m	2.992	ng/ul	
22) Benzo(k)fluoranthene	23.29	252	90677m	0.978	ng/ul	
23) Benzo(a)pyrene	23.91	252	129247	1.727	ng/ul#	95
24) Indeno(1,2,3-cd)pyrene	26.71	276	85541	1.007	ng/ul#	100
25) Dibenzo(a,h)anthracene	26.73	278	21709	0.306	ng/ul#	84
26) Benzo(g,h,i)perylene	27.54	276	97623	1.217	ng/ul	99

SJ 10/16/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed