


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE101019\
Data File : BE100623.D
Acq On : 10 Oct 2019 9:13
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE101019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 10 14:01:52 2019

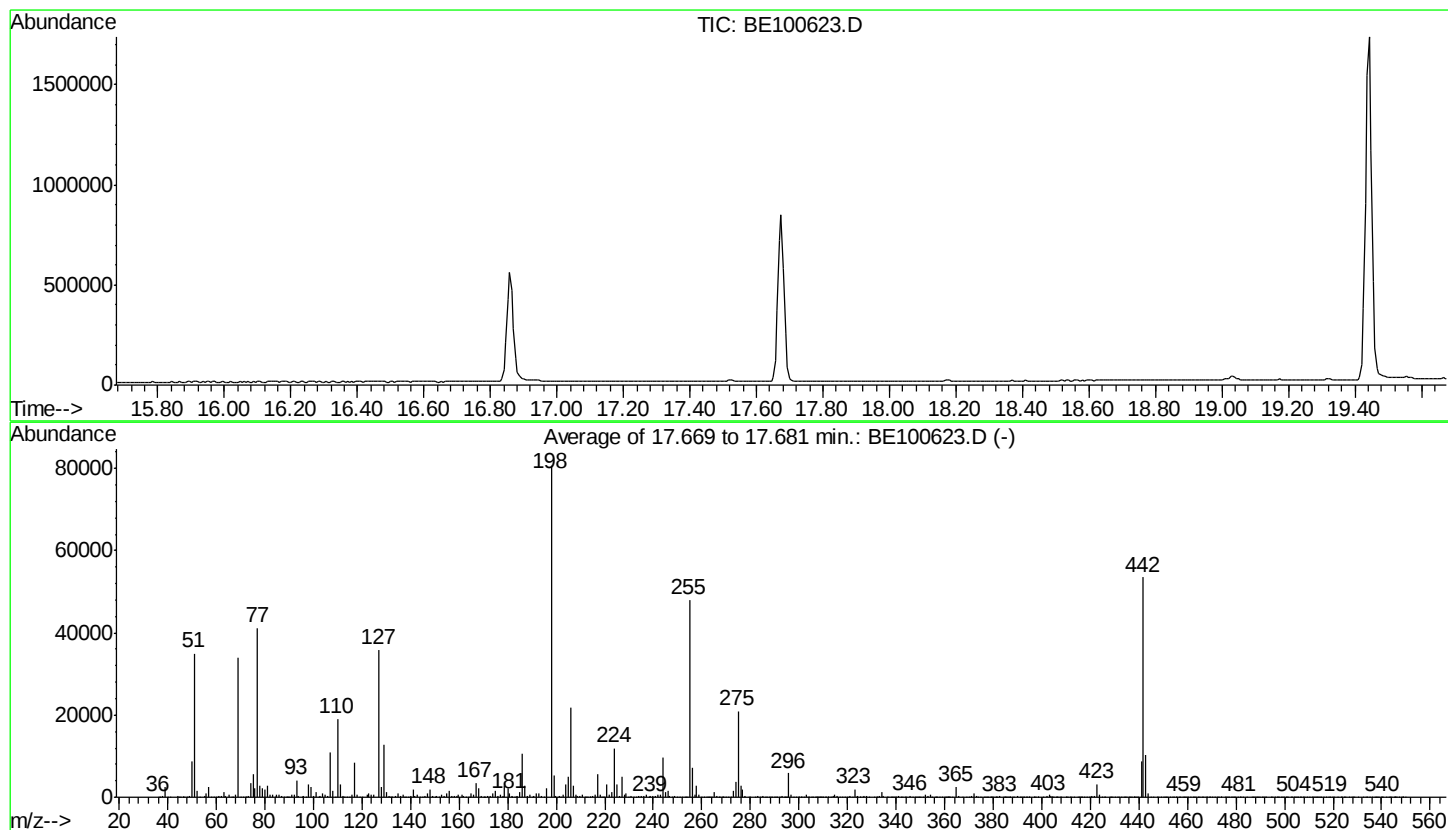

AutoFind: Scans 2567, 2568, 2569; Background Corrected with Scan 2558

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.3	34938	PASS
68	69	0.00	2	1.5	519	PASS
69	198	0.00	100	41.9	33820	PASS
70	69	0.00	2	0.4	152	PASS
127	198	10	80	44.5	35866	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	80683	PASS
199	198	5	9	6.7	5402	PASS
275	198	10	60	26.0	21004	PASS
365	198	1	100	3.2	2571	PASS
441	198	0.01	100	10.7	8613	PASS
442	198	50	100	66.3	53459	PASS
443	442	15	24	19.2	10273	PASS