

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE101118\
 Data File : BE097876.D
 Acq On : 12 Oct 2018 2:43
 Operator : SJ/JU
 Sample : J5184-12DL 5X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Oct 12 04:59:53 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE101118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 12 04:56:57 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	2922	0.40	ng/ul	0.00
2) Naphthalene-d8	10.70	136	15025	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.56	164	10432	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	24158	0.40	ng/ul	0.00
16) Chrysene-d12	21.50	240	23343	0.40	ng/ul	0.00
20) Perylene-d12	24.07	264	27641	0.40	ng/ul	0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	2875	0.11	ng/ul	0.00
14) Fluoranthene-d10	19.34	212	8070	0.10	ng/ul	0.00
Target Compounds				Ovalue		
3) Naphthalene	10.75	128	22483	0.615	ng/ul	98
5) 2-Methylnaphthalene	12.36	142	10144	0.384	ng/ul	98
7) Acenaphthylene	14.27	152	6720	0.170	ng/ul#	88
8) Acenaphthene	14.61	153	24123	0.788	ng/ul	97
9) Fluorene	15.61	166	32018	0.801	ng/ul	98
11) Pentachlorophenol	16.97	266	8600	2.525	ng/ul	98
12) Phenanthrene	17.35	178	928994	16.243	ng/ul	98
13) Anthracene	17.44	178	265823	5.016	ng/ul	99
15) Fluoranthene	19.38	202	2627857	35.778	ng/ul	95
17) Pyrene	19.74	202	2816087	40.496	ng/ul	96
18) Benzo(a)anthracene	21.49	228	2087460	29.576	ng/ul	97
19) Chrysene	21.54	228	2763574	43.580	ng/ul	93
21) Benzo(b)fluoranthene	23.29	252	3736436	50.578	ng/ul	99
22) Benzo(k)fluoranthene	23.29	252	3736436	47.251	ng/ul	97
23) Benzo(a)pyrene	23.96	252	1373887	18.942	ng/ul	99
24) Indeno(1,2,3-cd)pyrene	26.79	276	939294	11.408	ng/ul#	100
25) Dibenzo(a,h)anthracene	26.81	278	275186	4.044	ng/ul#	94
26) Benzo(g,h,i)perylene	27.63	276	841483	11.729	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE101118\
Data File : BE097876.D
Acq On : 12 Oct 2018 2:43
Operator : SJ/JU
Sample : J5184-12DL 5X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Oct 12 04:59:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE101118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 04:56:57 2018
Response via : Initial Calibration

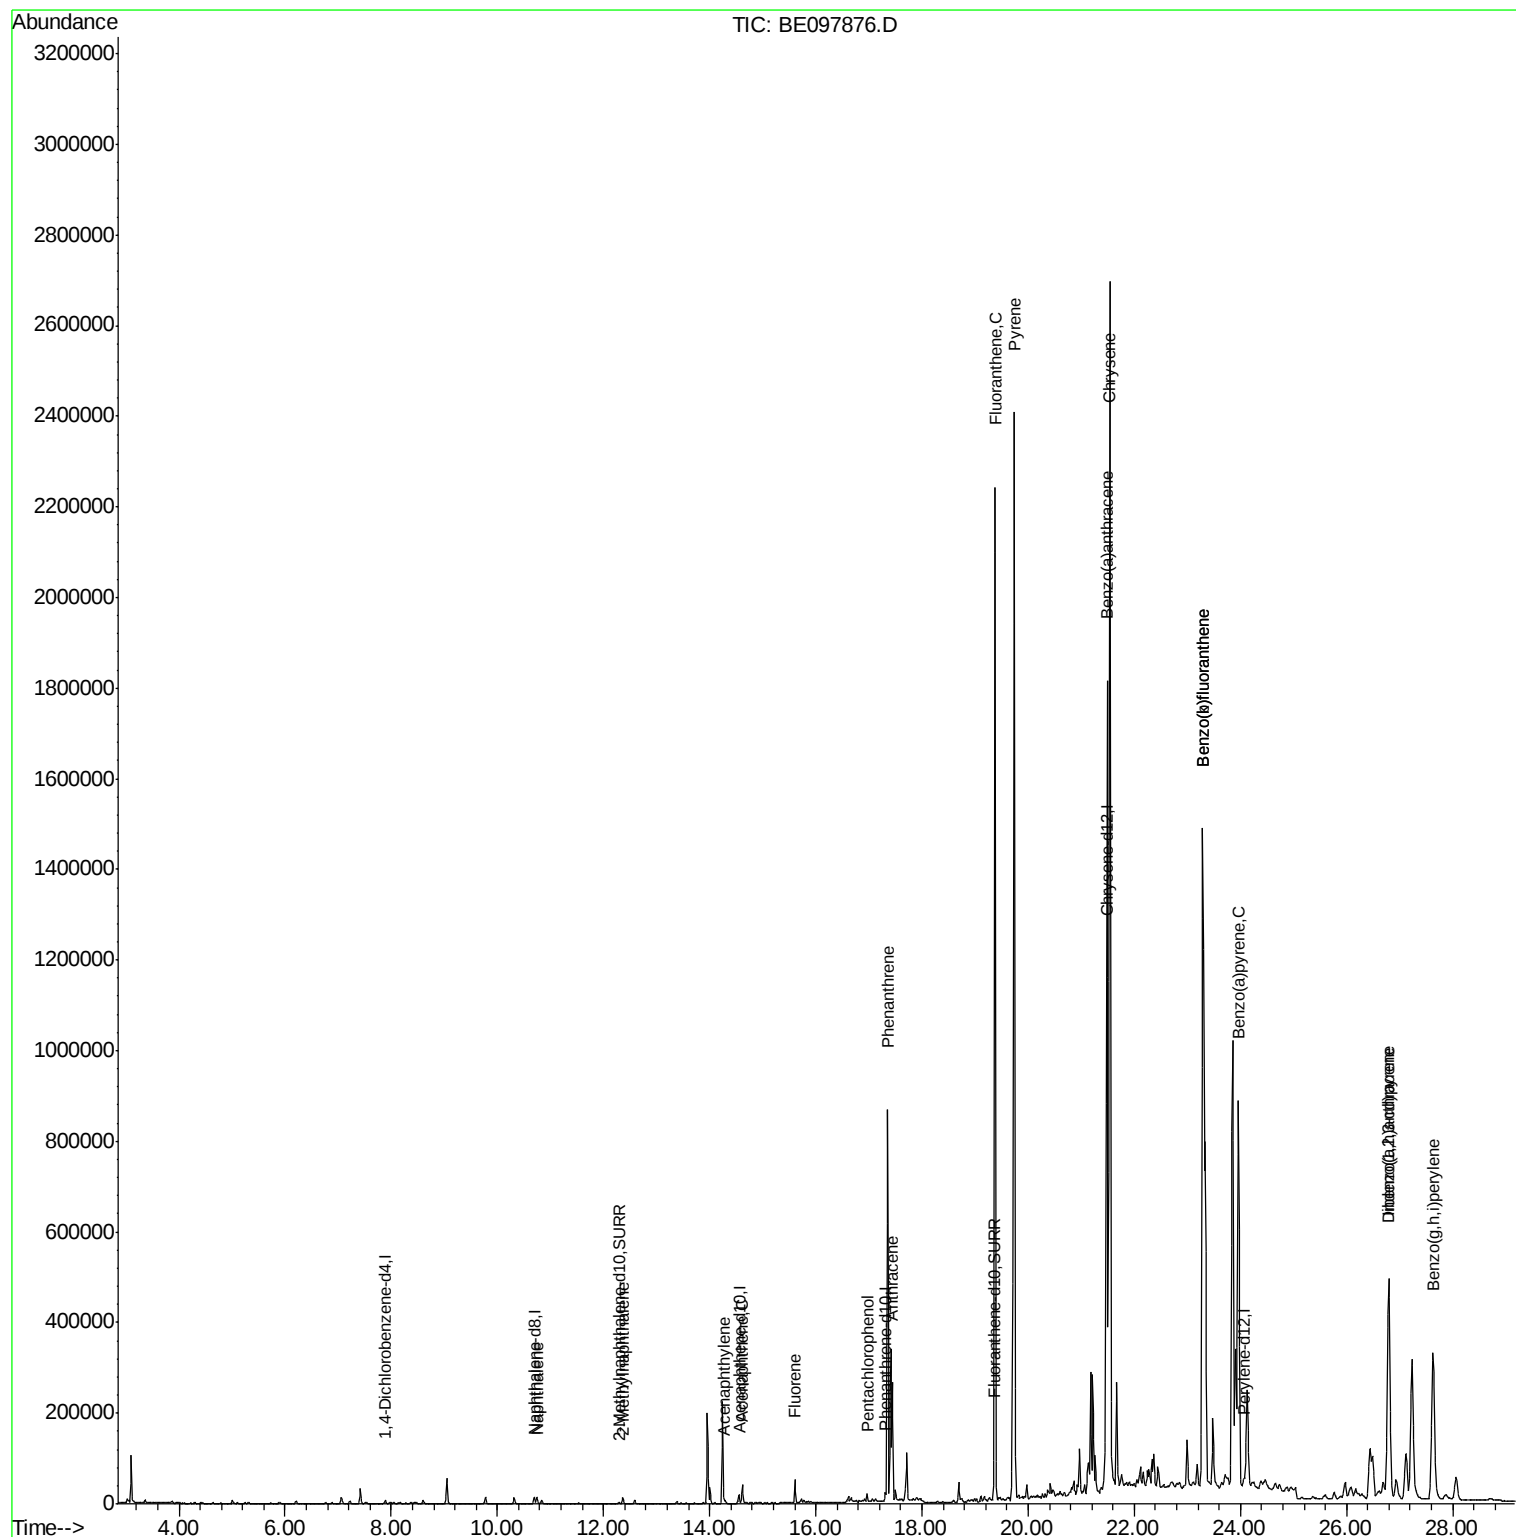

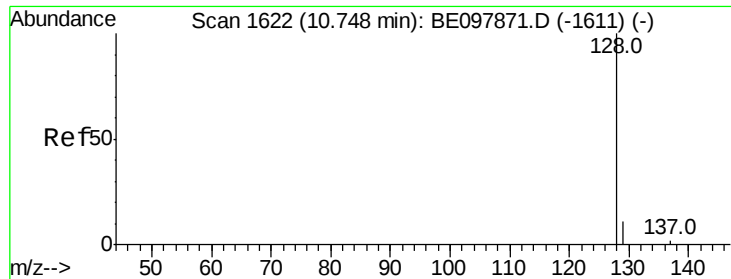

#3

Naphthalene

Concen: 0.615 ng/ul

RT: 10.75 min Scan# 1623

Delta R.T. -0.00 min

Lab File: BE097876.D

Acq: 12 Oct 2018 2:43

Instrument :

BNA_E

ClientSampleId :


Tot Ion:128 Resp: 22483

Ion Ratio Lower Upper

128 100

129 12.1 9.1 13.7




127 0.0 0.0 0.0



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

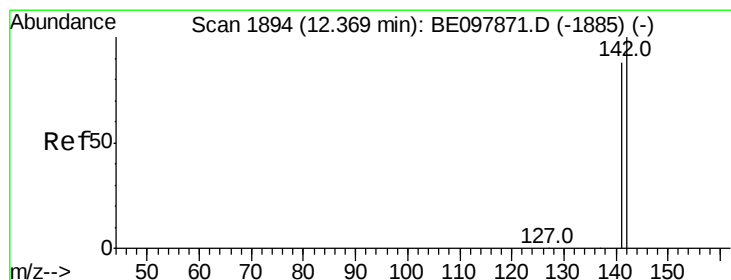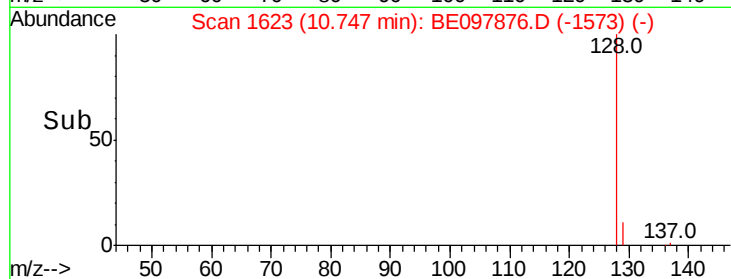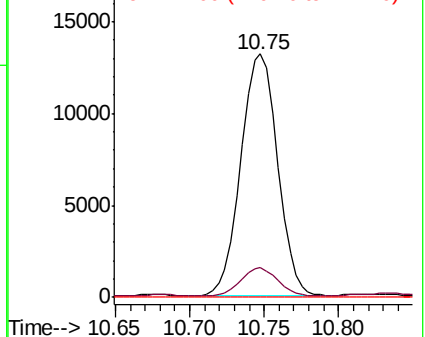

#5

2-Methylnaphthalene

Concen: 0.384 ng/ul

RT: 12.36 min Scan# 1894

Delta R.T. -0.01 min

Lab File: BE097876.D


Acq: 12 Oct 2018 2:43

Tgt Ion:142 Resp: 10144

Ion Ratio Lower Upper



142 100


141 87.4 71.6 107.4

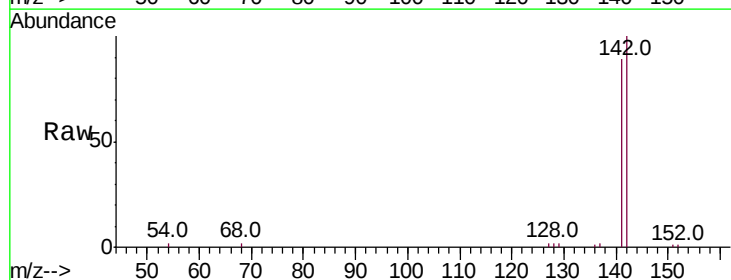

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

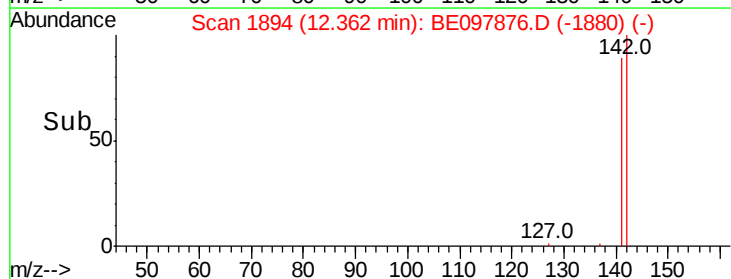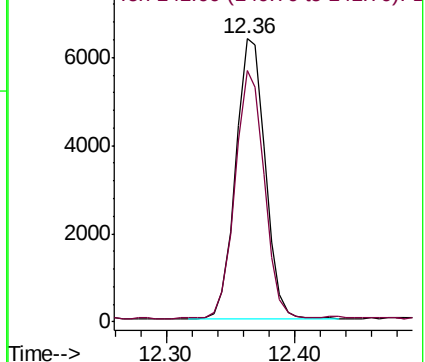



#7

Acenaphthylene

Concen: 0.170 ng/ul

RT: 14.27 min Scan# 2206

Delta R.T. 0.00 min

Lab File: BE097876.D

Acq: 12 Oct 2018 2:43

Instrument :

BNA_E

ClientSampleId :





Tot Ion:152 Resp: 6720

Ion Ratio Lower Upper

152 100

151 23.2 15.0 22.6#

153 18.8 10.5 15.7#

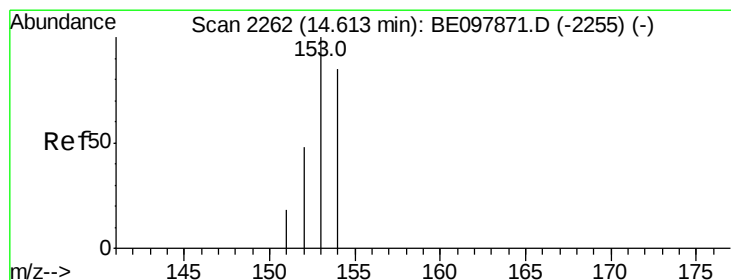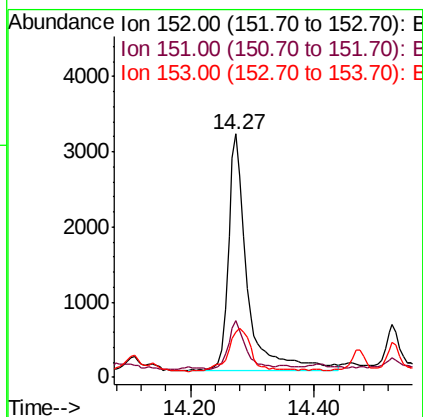

#8

Acenaphthene

Concen: 0.788 ng/ul

RT: 14.61 min Scan# 2264

Delta R.T. 0.00 min

Lab File: BE097876.D

Acq: 12 Oct 2018 2:43




Tgt Ion:153 Resp: 24123


Ion Ratio Lower Upper

153 100

152 48.9 41.2 61.8

154 87.9 68.6 103.0

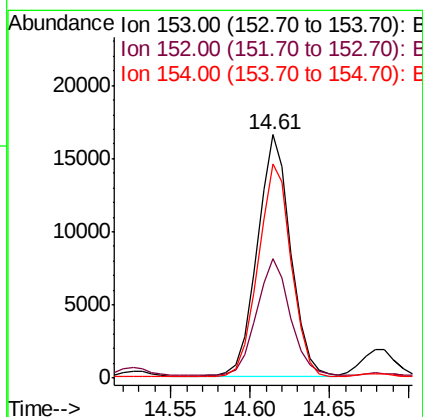



#9

Fluorene

Concen: 0.801 ng/ul

RT: 15.61 min Scan# 2433

Delta R.T. -0.00 min

Lab File: BE097876.D

Acq: 12 Oct 2018 2:43

Instrument :

BNA_E

ClientSampleId :





Tot Ion:166 Resp: 32018

Ion Ratio Lower Upper

166 100

165 100.8 79.2 118.8

167 14.9 11.3 16.9

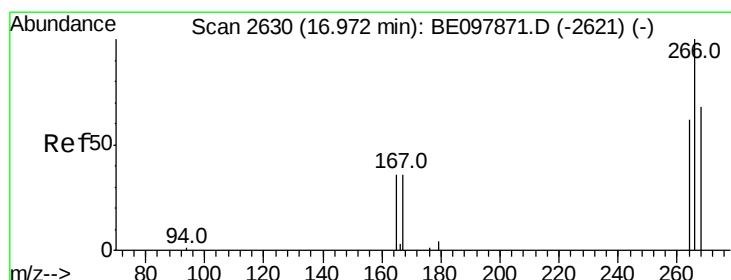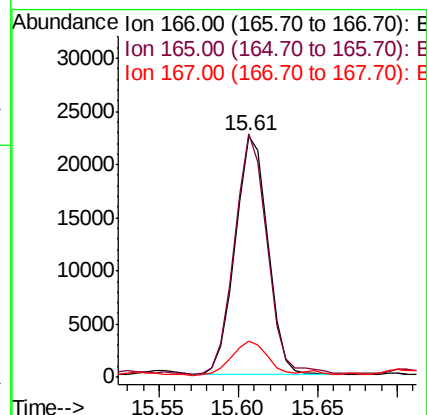

#11

Pentachlorophenol

Concen: 2.525 ng/ul

RT: 16.97 min Scan# 2631

Delta R.T. -0.01 min

Lab File: BE097876.D

Acq: 12 Oct 2018 2:43




Tgt Ion:266 Resp: 8600


Ion Ratio Lower Upper

266 100

264 63.1 49.8 74.8

268 62.8 48.4 72.6

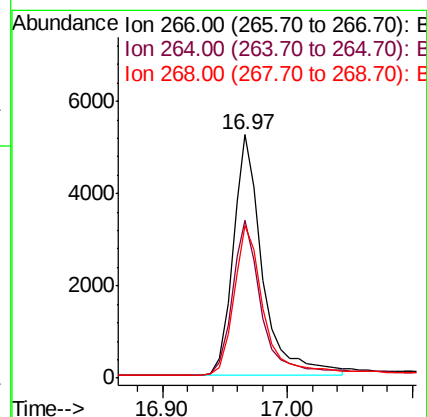



#12

Phenanthrene

Concen: 16.243 ng/ul

RT: 17.35 min Scan# 2686

Delta R.T. 0.00 min

Lab File: BE097876.D

Acq: 12 Oct 2018 2:43

Instrument :

BNA_E

ClientSampleId :


Tot Ion:178 Resp: 928994

Ion Ratio Lower Upper

178 100

179 15.6 12.8 19.2




176 19.9 14.9 22.3

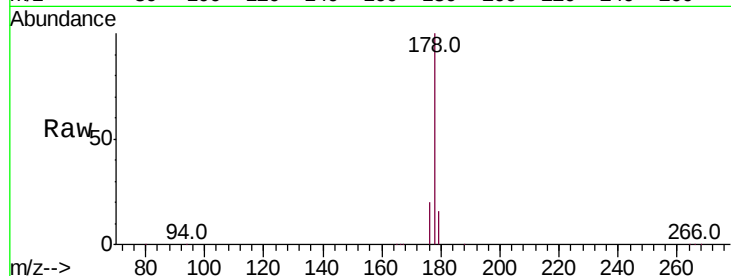

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

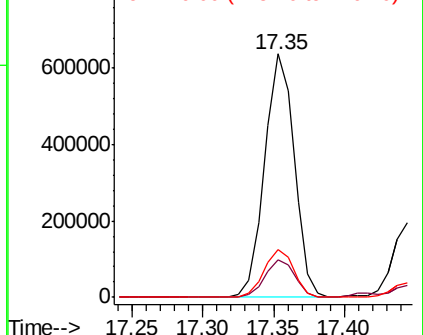

#13

Anthracene

Concen: 5.016 ng/ul

RT: 17.44 min Scan# 2699

Delta R.T. 0.00 min

Lab File: BE097876.D

Acq: 12 Oct 2018 2:43


Tgt Ion:178 Resp: 265823

Ion Ratio Lower Upper

178 100

179 15.7 12.9 19.3



176 18.9 15.5 23.3




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

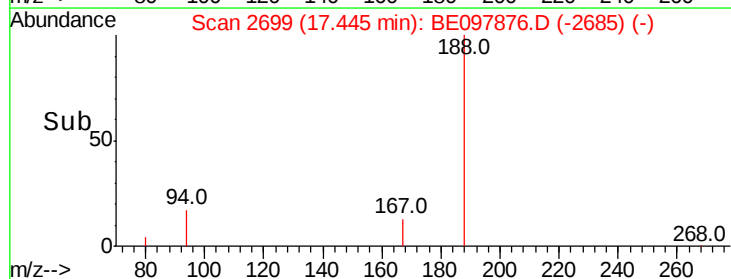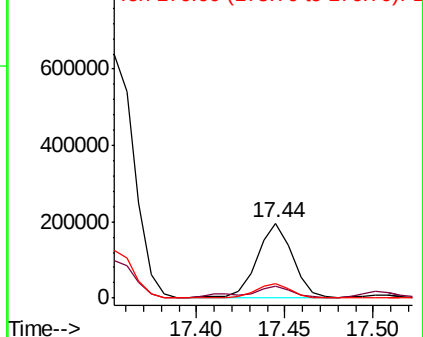

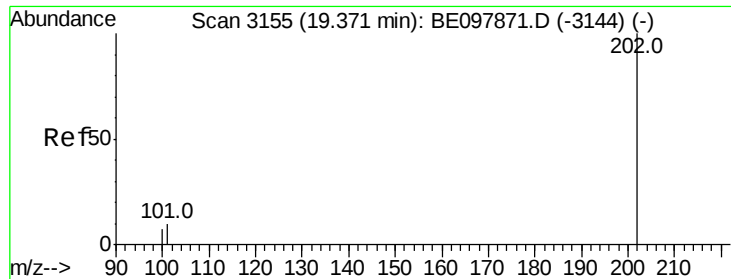

#15

Fluoranthene

Concen: 35.778 ng/ul

RT: 19.38 min Scan# 3158

Delta R.T. 0.01 min

Lab File: BE097876.D

Acq: 12 Oct 2018 2:43

Instrument :

BNA_E

ClientSampleId :





Tot Ion:202 Resp: 2627857

Ion Ratio Lower Upper

202 100

101 11.3 0.0 29.3

100 9.1 0.0 27.5

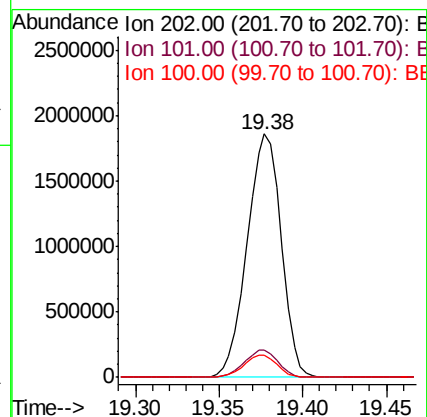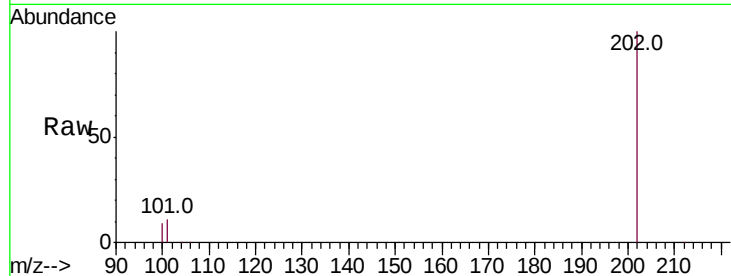

#17

Pyrene

Concen: 40.496 ng/ul

RT: 19.74 min Scan# 3260

Delta R.T. 0.01 min

Lab File: BE097876.D

Acq: 12 Oct 2018 2:43




Tgt Ion:202 Resp: 2816087


Ion Ratio Lower Upper

202 100

101 12.9 8.8 13.2

100 11.3 7.9 11.9

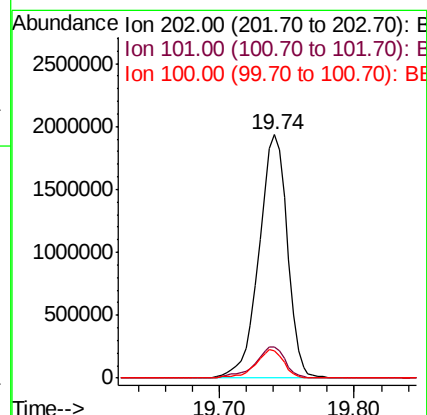

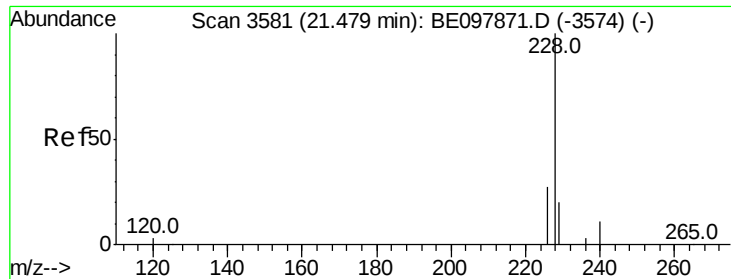

#18

Benzo(a)anthracene

Concen: 29.576 ng/ul

RT: 21.49 min Scan# 3584

Delta R.T. 0.01 min

Lab File: BE097876.D

Acq: 12 Oct 2018 2:43

Instrument :

BNA_E

ClientSampleId :


Tot Ion:228 Resp: 2087460

Ion Ratio Lower Upper

228 100

229 21.7 16.4 24.6




226 28.5 21.5 32.3



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

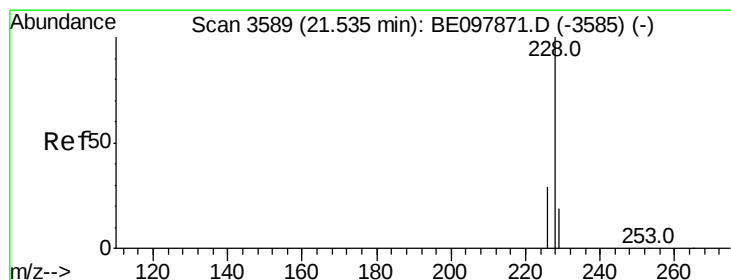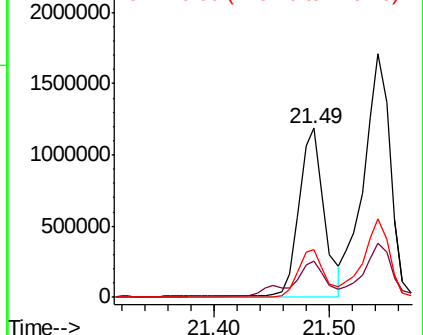

#19

Chrysene

Concen: 43.580 ng/ul

RT: 21.54 min Scan# 3592

Delta R.T. 0.01 min

Lab File: BE097876.D

Acq: 12 Oct 2018 2:43


Tgt Ion:228 Resp: 2763574

Ion Ratio Lower Upper

228 100

226 32.5 23.0 34.4



229 22.5 15.5 23.3

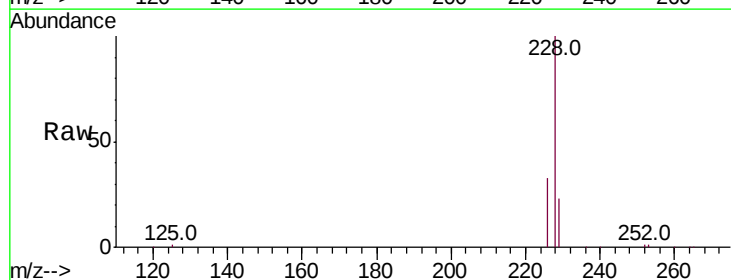


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E



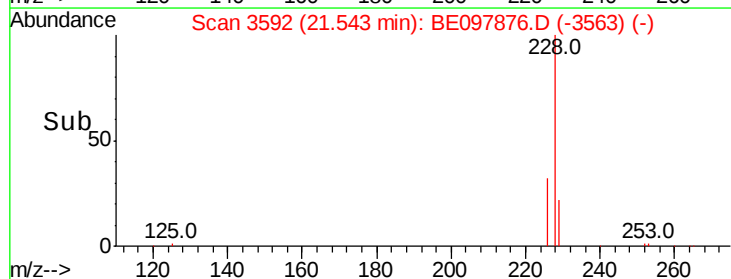
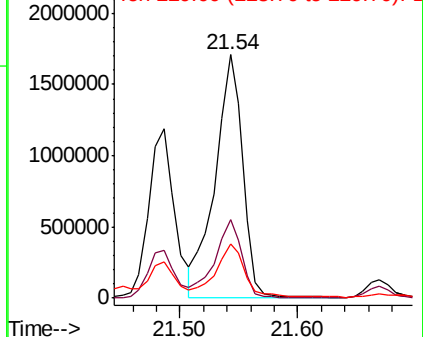


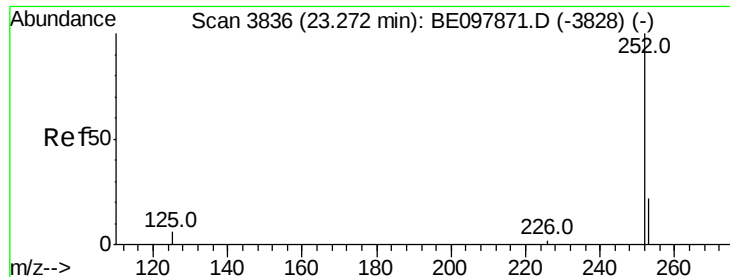

#21
Benzo(b)fluoranthene
Concen: 50.578 ng/ul
RT: 23.29 min Scan# 3841
Delta R.T. 0.02 min
Lab File: BE097876.D
Acq: 12 Oct 2018 2:43




Instrument :
BNA_E
ClientSampleId :


Tot Ion:252 Resp: 3736436
Ion Ratio Lower Upper
252 100
253 23.4 0.0 47.0
125 10.0 0.0 18.2

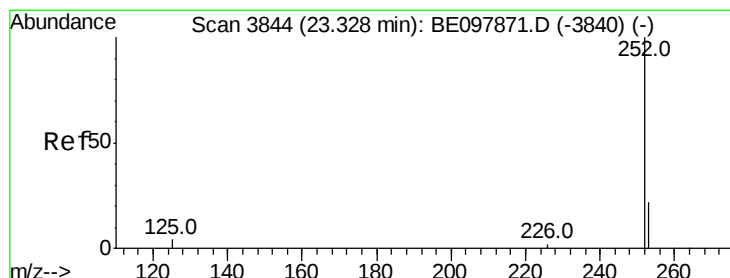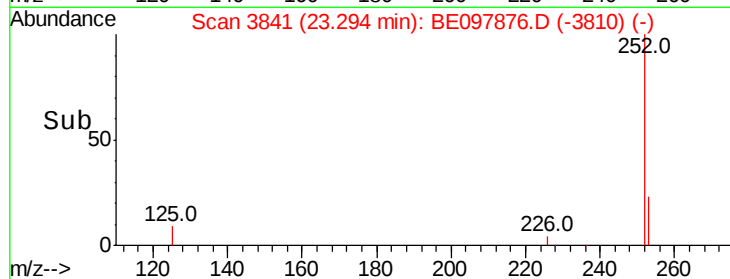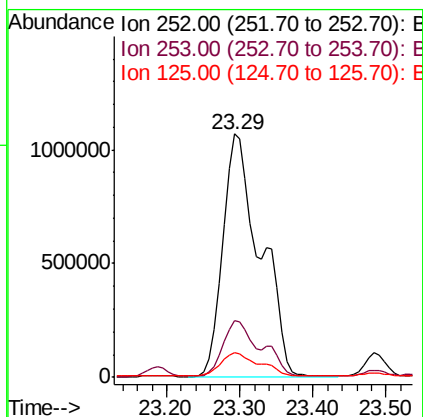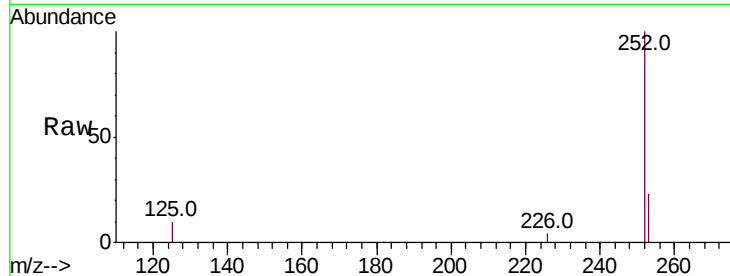

#22
Benzo(k)fluoranthene
Concen: 47.251 ng/ul
RT: 23.29 min Scan# 3841
Delta R.T. -0.03 min
Lab File: BE097876.D
Acq: 12 Oct 2018 2:43

Tgt Ion:252 Resp: 3736436
Ion Ratio Lower Upper
252 100
253 23.4 17.8 26.6
125 10.0 9.4 14.0

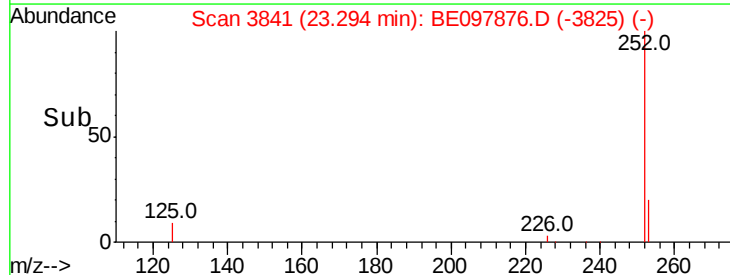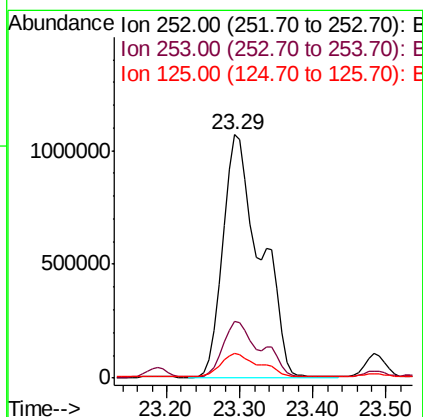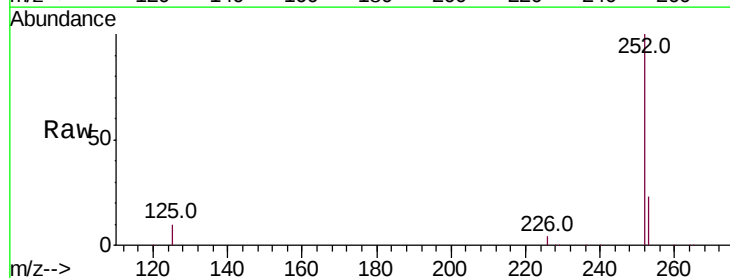

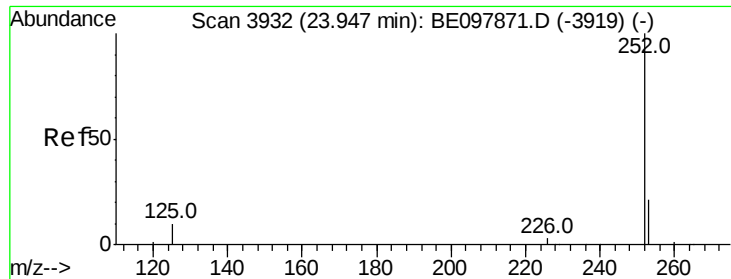

#23

Benzo(a)pyrene

Concen: 18.942 ng/ul

RT: 23.96 min Scan# 3936

Delta R.T. 0.01 min

Lab File: BE097876.D

Acq: 12 Oct 2018 2:43

Instrument :

BNA_E

ClientSampleId :


Tot Ion:252 Resp: 1373887

Ion Ratio Lower Upper

252 100

253 23.3 18.2 27.4




125 10.6 8.3 12.5



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

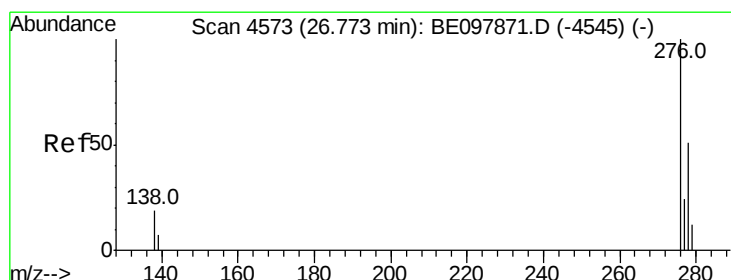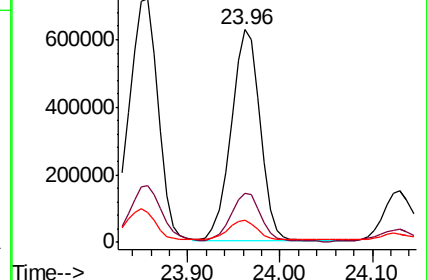

#24

Indeno(1,2,3-cd)pyrene

Concen: 11.408 ng/ul

RT: 26.79 min Scan# 4580

Delta R.T. 0.02 min

Lab File: BE097876.D

Acq: 12 Oct 2018 2:43


Tgt Ion:276 Resp: 939294

Ion Ratio Lower Upper

276 100

138 18.5 0.0 0.0#



227 0.0 0.0 0.0

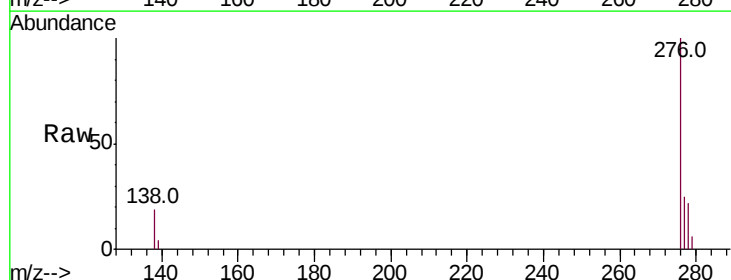


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 227.00 (226.70 to 227.70): E

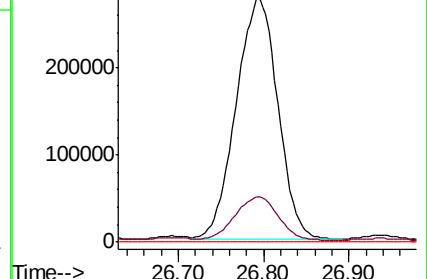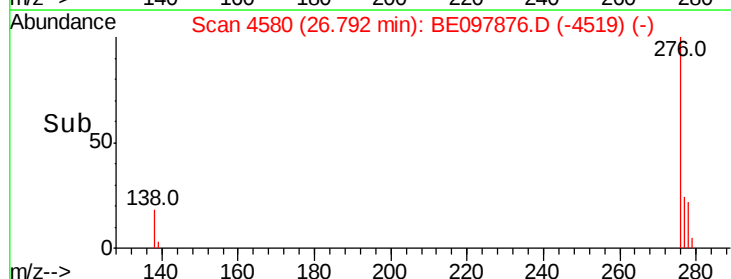



#25

Dibenzo(a,h)anthracene

Concen: 4.044 ng/ul

RT: 26.81 min Scan# 4585

Delta R.T. 0.01 min

Lab File: BE097876.D

Acq: 12 Oct 2018 2:43

Instrument :

BNA_E

ClientSampleId :


Tot Ion:278 Resp: 275186

Ion Ratio Lower Upper

278 100

139 16.4 10.9 16.3#

279 26.0 18.8 28.2

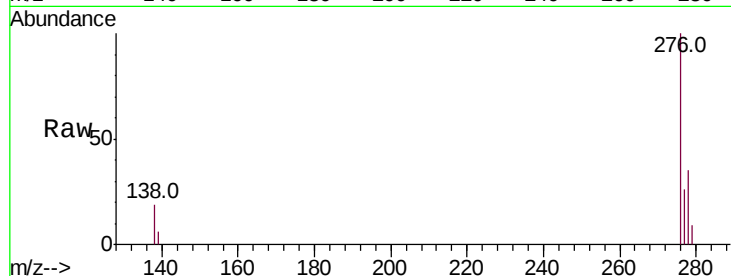


Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E


Ion 279.00 (278.70 to 279.70): E

Time-->



26.81

Time-->



#26

Benzo(g,h,i)perylene

Concen: 11.729 ng/ul

RT: 27.63 min Scan# 4815

Delta R.T. 0.04 min

Lab File: BE097876.D

Acq: 12 Oct 2018 2:43


Tgt Ion:276 Resp: 841483

Ion Ratio Lower Upper

276 100

138 19.3 14.3 21.5

277 24.2 19.5 29.3




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

Time-->



27.63

Time-->