

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE101118\
 Data File : BE097872.D
 Acq On : 12 Oct 2018 00:14
 Operator : SJ/JU
 Sample : J5183-02DL 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JLC17DL

Manual Integrations
 APPROVED

Sohil
 10/12/2018 6:35:03 PM

Quant Time: Oct 12 05:03:13 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 12 04:56:57 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	2587	0.40	ng/ul	0.00
2) Naphthalene-d8	10.70	136	13290	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.55	164	8881	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	21747	0.40	ng/ul	0.00
16) Chrysene-d12	21.49	240	22754	0.40	ng/ul	0.00
20) Perylene-d12	24.06	264	23304	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	991	0.04	ng/ul	0.00
14) Fluoranthene-d10	19.34	212	3044	0.04	ng/ul	0.00
Target Compounds				Qvalue		
3) Naphthalene	10.75	128	912	0.028	ng/ul#	68
5) 2-Methylnaphthalene	12.37	142	587	0.025	ng/ul	95
12) Phenanthrene	17.35	178	8411	0.163	ng/ul	95
13) Anthracene	17.44	178	1551	0.033	ng/ul#	68
15) Fluoranthene	19.37	202	14756	0.223	ng/ul	96
17) Pyrene	19.73	202	20806	0.307	ng/ul	97
18) Benzo(a)anthracene	21.48	228	12854	0.187	ng/ul#	74
19) Chrysene	21.54	228	12703	0.206	ng/ul#	78
21) Benzo(b)fluoranthene	23.27	252	16976m	0.273	ng/ul	
22) Benzo(k)fluoranthene	23.32	252	5391m	0.081	ng/ul	
23) Benzo(a)pyrene	23.95	252	10314	0.169	ng/ul#	6
24) Indeno(1,2,3-cd)pyrene	26.77	276	8591	0.124	ng/ul#	100
25) Dibenzo(a,h)anthracene	26.78	278	2301	0.040	ng/ul#	1
26) Benzo(g,h,i)perylene	27.60	276	9806	0.162	ng/ul#	50

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE101118\
Data File : BE097872.D
Acq On : 12 Oct 2018 00:14
Operator : SJ/JU
Sample : J5183-02DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
JLC17DL

Manual Integrations
APPROVED

Sohil
10/12/2018 6:35:03 PM

Quant Time: Oct 12 05:03:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE101118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 04:56:57 2018
Response via : Initial Calibration

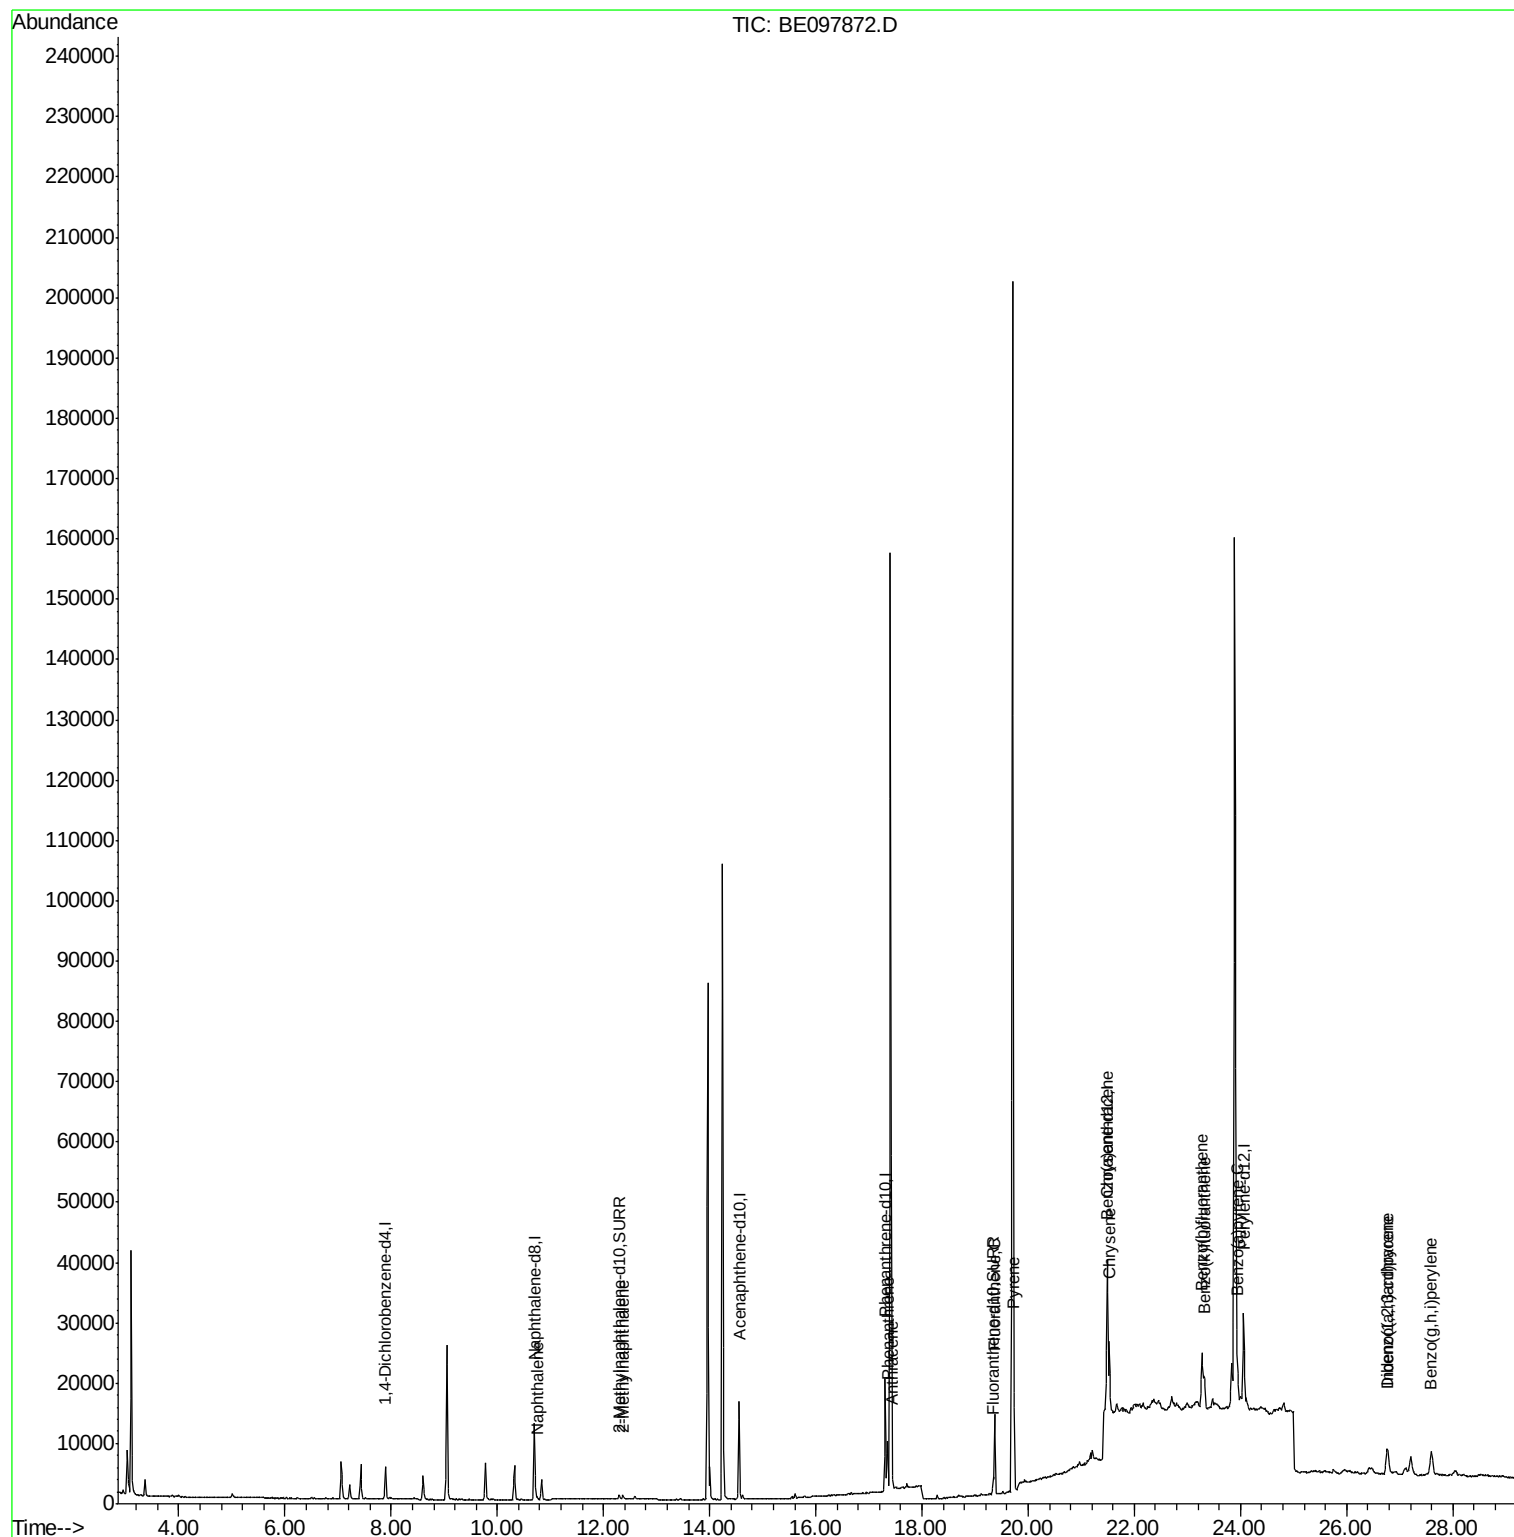

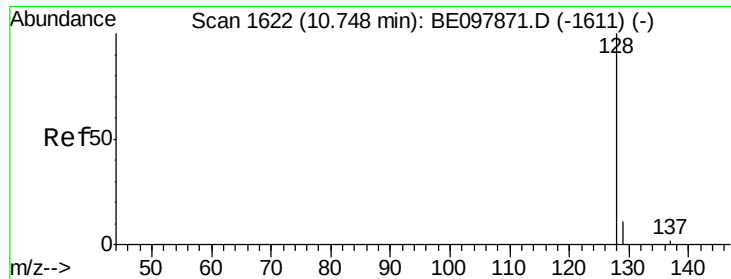

#3

Naphthalene

Concen: 0.028 ng/ul

RT: 10.75 min Scan# 1623

Delta R.T. -0.00 min

Lab File: BE097872.D

Acq: 12 Oct 2018 00:14

Instrument :

BNA_E





ClientSampleId :

JLC17DL

Tgt Ion:	128	Resp:	912
Ion Ratio	Lower	Upper	
128	100		
129	23.8	9.1	13.7#
127	0.0	0.0	0.0

Manual Integrations
APPROVED

Sohil
10/12/2018 6:35:03 PM

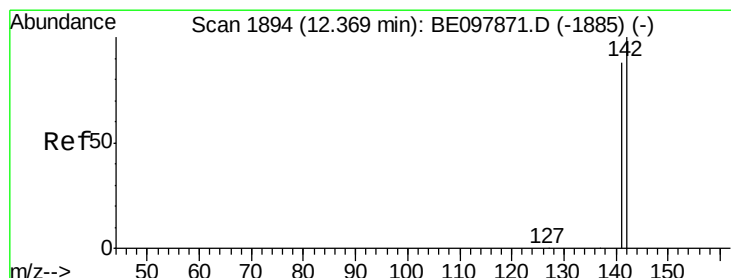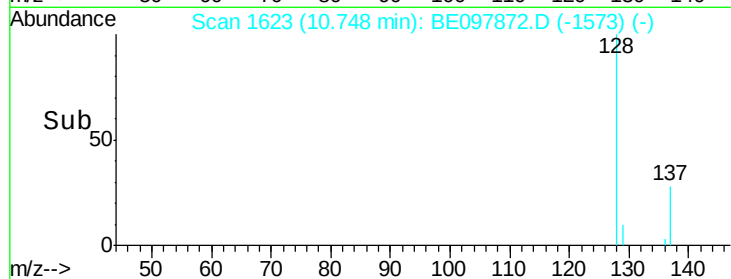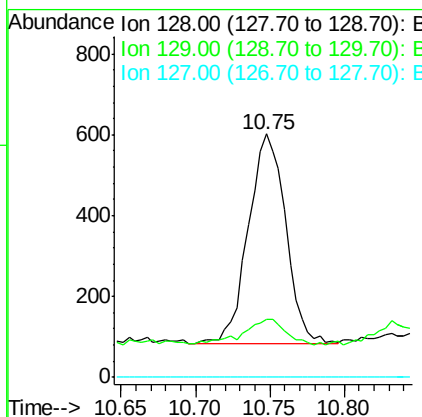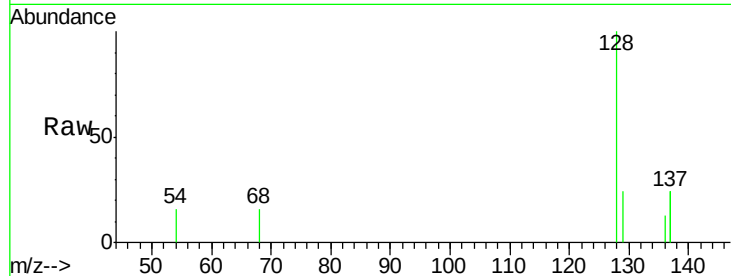

#5

2-Methylnaphthalene

Concen: 0.025 ng/ul




RT: 12.37 min Scan# 1895


Delta R.T. 0.00 min

Lab File: BE097872.D

Acq: 12 Oct 2018 00:14

Tgt Ion:	142	Resp:	587
Ion Ratio	Lower	Upper	
142	100		
141	84.7	71.6	107.4

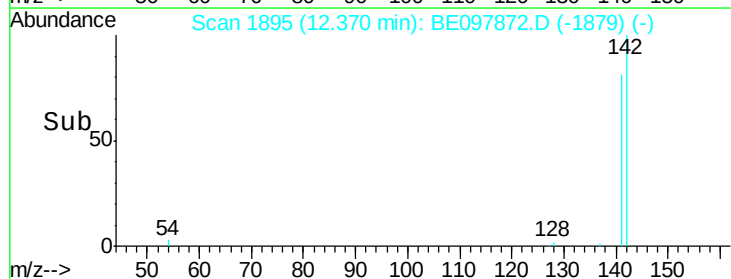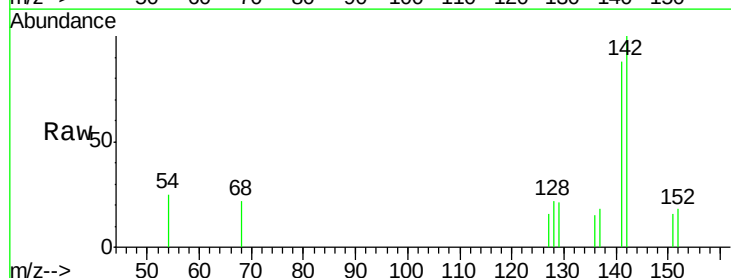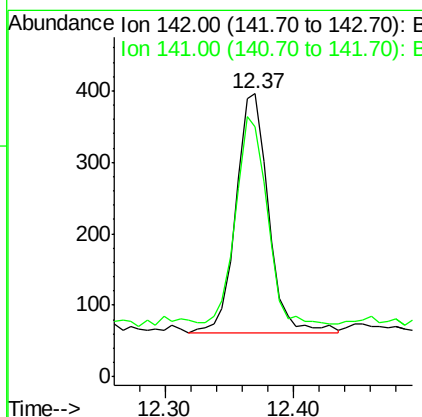

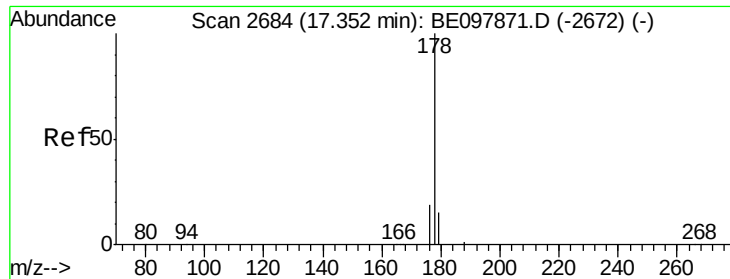

#12

Phenanthrene

Concen: 0.163 ng/ul

RT: 17.35 min Scan# 2685

Delta R.T. -0.00 min

Lab File: BE097872.D

Acq: 12 Oct 2018 00:14

Instrument :

BNA_E





ClientSampleId :

JLC17DL

Tgt Ion:	178	Resp:	8411
Ion Ratio	Lower	Upper	
178	100		
179	18.4	12.8	19.2
176	20.3	14.9	22.3

Manual Integrations
APPROVED

Sohil
10/12/2018 6:35:03 PM

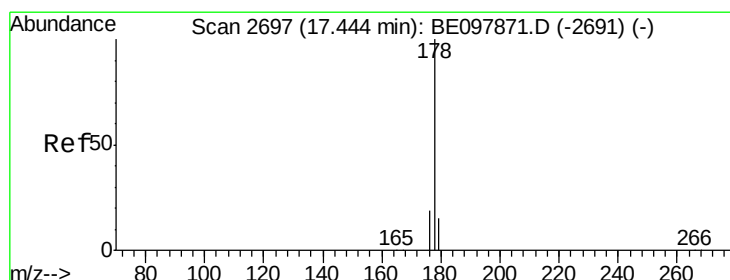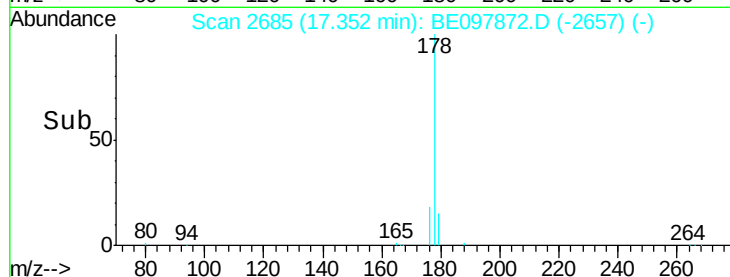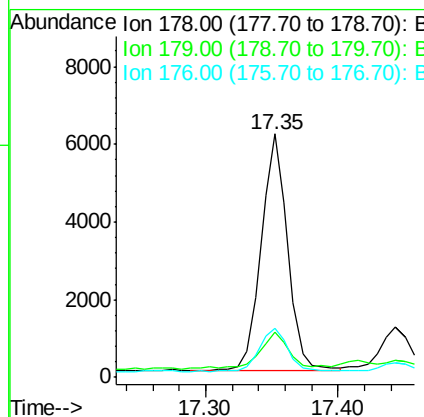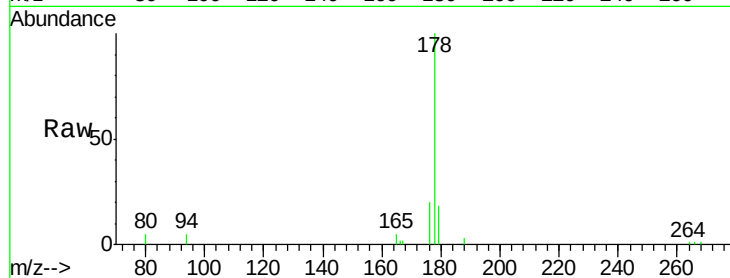

#13

Anthracene

Concen: 0.033 ng/ul




RT: 17.44 min Scan# 2698


Delta R.T. -0.00 min

Lab File: BE097872.D

Acq: 12 Oct 2018 00:14

Tgt Ion:	178	Resp:	1551
Ion Ratio	Lower	Upper	
178	100		
179	34.3	12.9	19.3#
176	29.6	15.5	23.3#

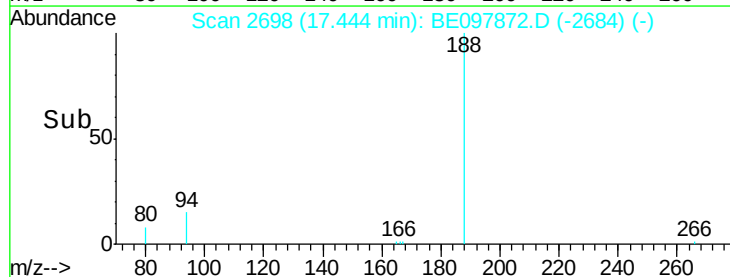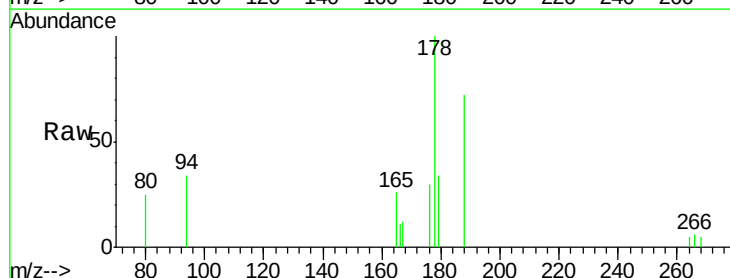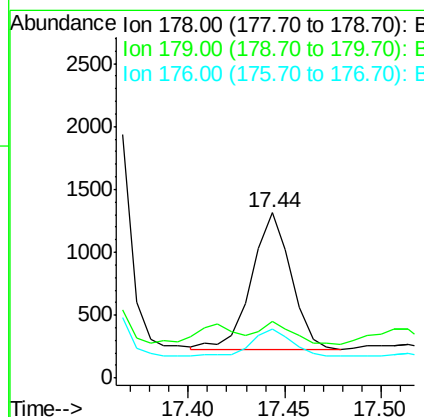

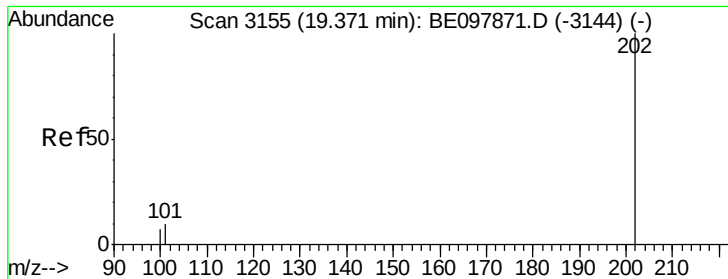





#15
Fluoranthene
Concen: 0.223 ng/ul
RT: 19.37 min Scan# 3156
Delta R.T. -0.00 min
Lab File: BE097872.D
Acq: 12 Oct 2018 00:14

Instrument :
BNA_E
ClientSampleId :
JLC17DL

Tgt Ion	Ratio	Resp Lower	Resp Upper
202	100		
101	10.7	0.0	29.3
100	9.1	0.0	27.5




Manual Integrations
APPROVED


Sohil
10/12/2018 6:35:03 PM

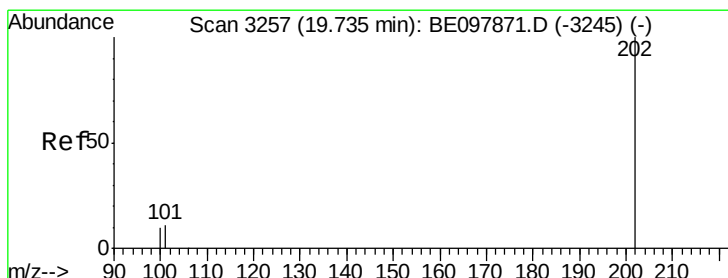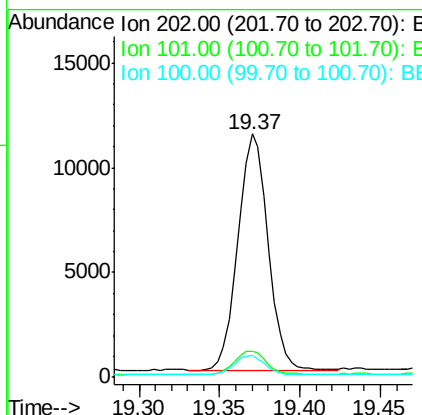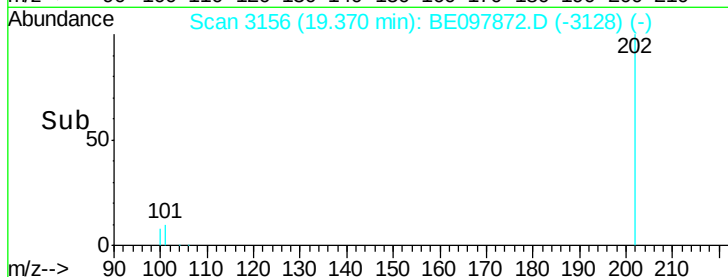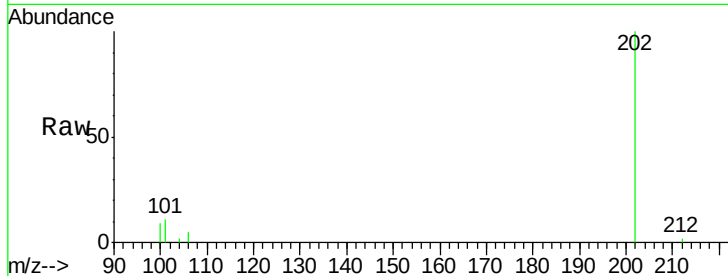

#17
Pyrene
Concen: 0.307 ng/ul
RT: 19.73 min Scan# 3258
Delta R.T. -0.00 min
Lab File: BE097872.D
Acq: 12 Oct 2018 00:14

Tgt Ion	Ratio	Resp Lower	Resp Upper
202	100		
101	12.6	8.8	13.2
100	10.7	7.9	11.9

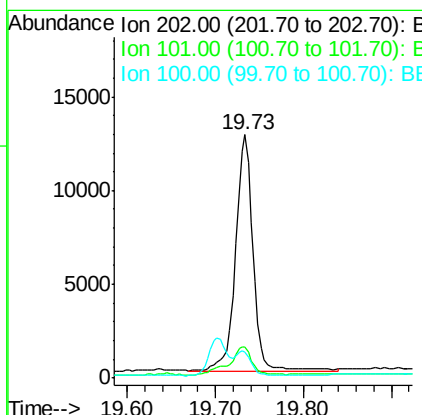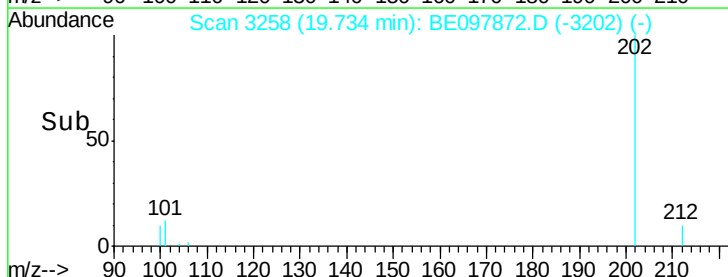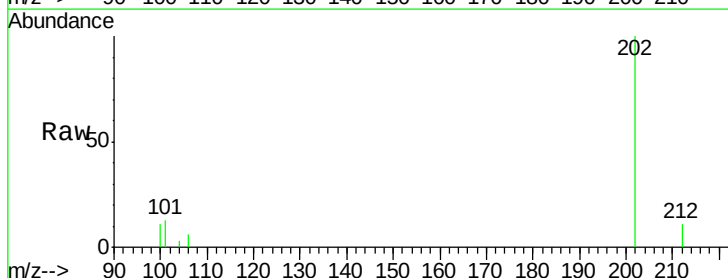

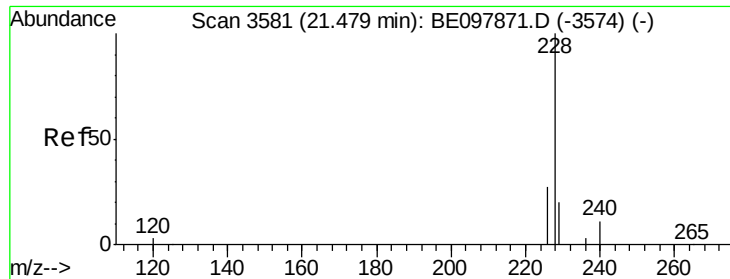

#18

Benzo(a)anthracene

Concen: 0.187 ng/ul

RT: 21.48 min Scan# 3582

Delta R.T. 0.00 min

Lab File: BE097872.D

Acq: 12 Oct 2018 00:14

Instrument :

BNA_E





ClientSampled :

JLC17DL

Tgt Ion:	228	Resp:	12854
Ion Ratio	Lower	Upper	
228	100		
229	39.1	16.4	24.6#
226	35.2	21.5	32.3#

Manual Integrations
APPROVED

Sohil
10/12/2018 6:35:03 PM

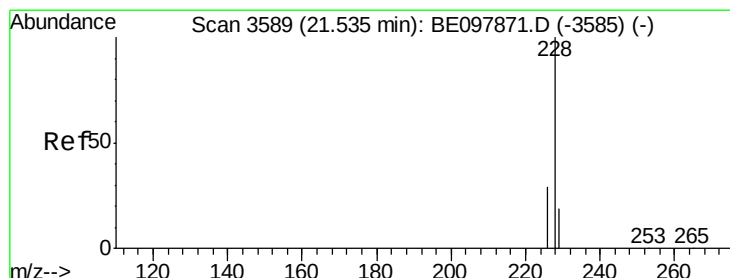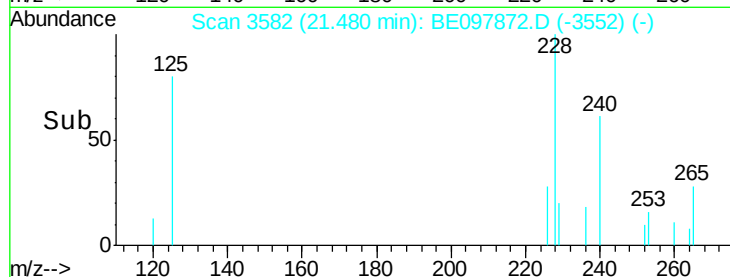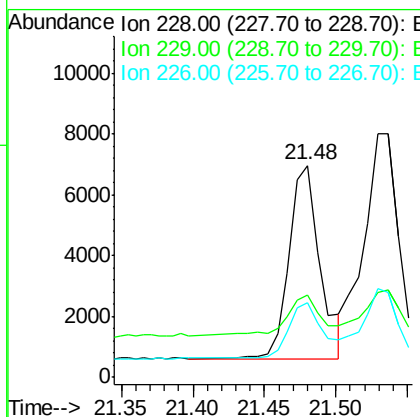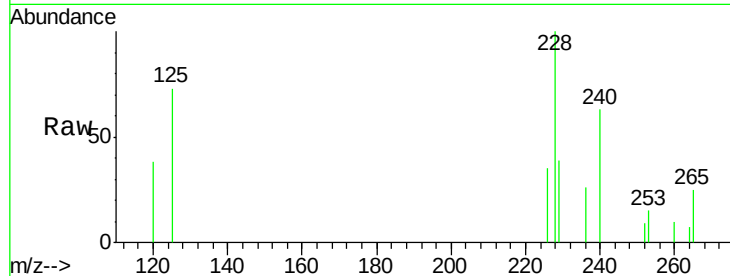

#19

Chrysene

Concen: 0.206 ng/ul




RT: 21.54 min Scan# 3590


Delta R.T. 0.00 min

Lab File: BE097872.D

Acq: 12 Oct 2018 00:14

Tgt Ion:	228	Resp:	12703
Ion Ratio	Lower	Upper	
228	100		
226	35.0	23.0	34.4#
229	36.1	15.5	23.3#

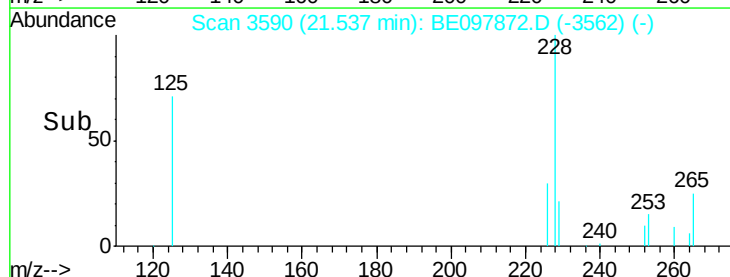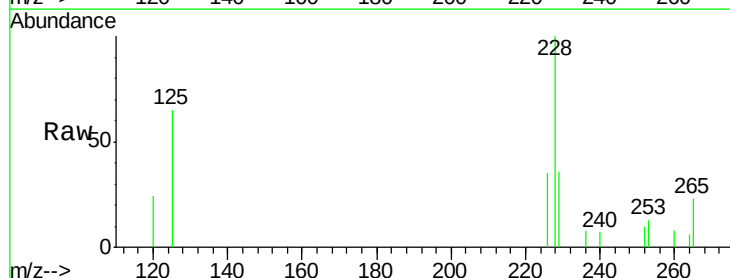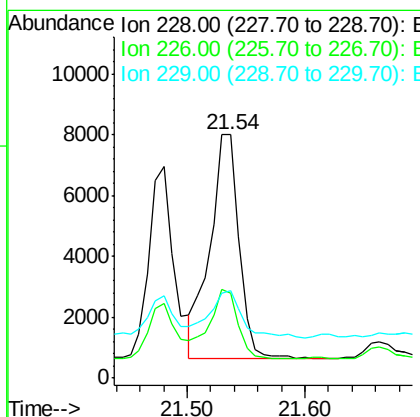

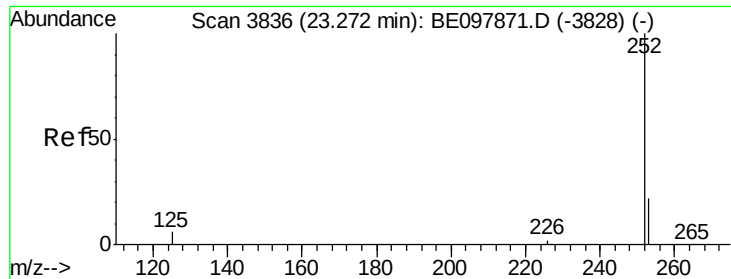





#21
Benzo(b)fluoranthene
Concen: 0.273 ng/ul m
RT: 23.27 min Scan# 3837
Delta R.T. 0.00 min
Lab File: BE097872.D
Acq: 12 Oct 2018 00:14

Instrument :
BNA_E
ClientSampleId :
JLC17DL

Tgt Ion	Ratio	Resp Lower	Resp Upper
252	100		
253	36.0	0.0	47.0
125	70.8	0.0	18.2#




Manual Integrations
APPROVED


Sohil
10/12/2018 6:35:03 PM

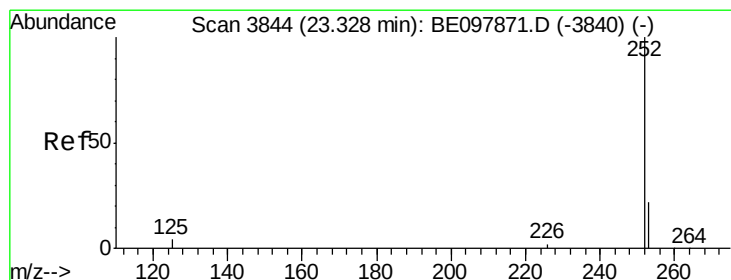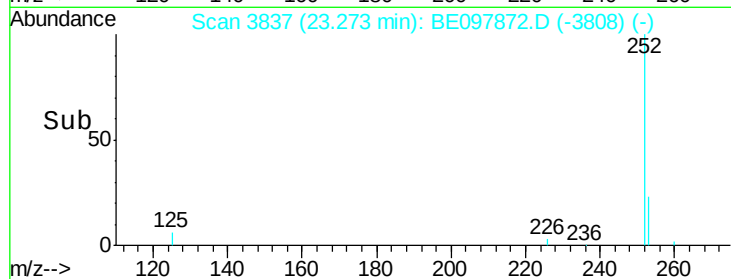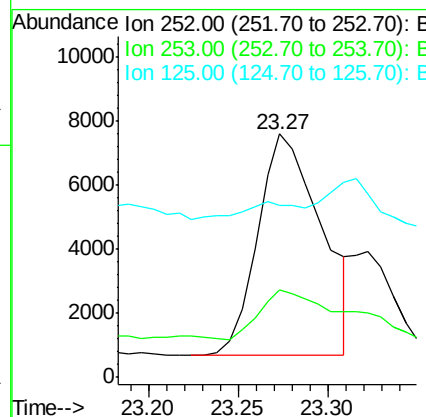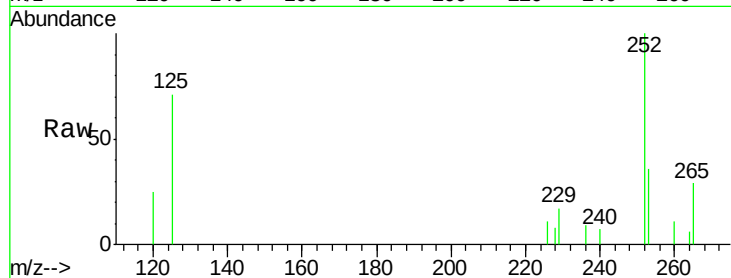

#22
Benzo(k)fluoranthene
Concen: 0.081 ng/ul m
RT: 23.32 min Scan# 3844
Delta R.T. -0.01 min
Lab File: BE097872.D
Acq: 12 Oct 2018 00:14

Tgt Ion	Ratio	Resp Lower	Resp Upper
252	100		
253	51.9	17.8	26.6#
125	146.1	9.4	14.0#

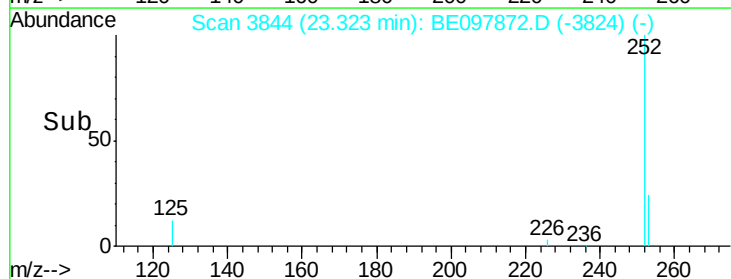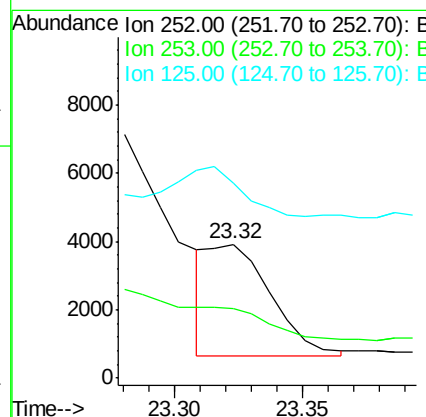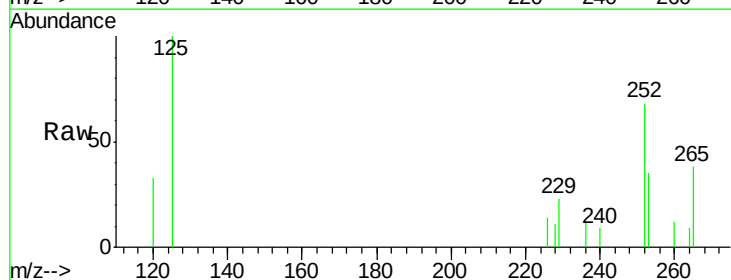

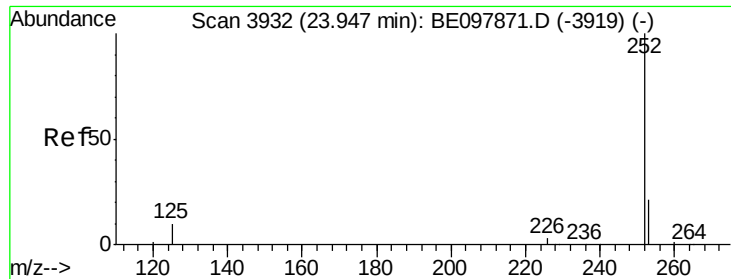

#23

Benzo(a)pyrene

Concen: 0.169 ng/ul

RT: 23.95 min Scan# 3933

Delta R.T. 0.00 min

Lab File: BE097872.D

Acq: 12 Oct 2018 00:14

Instrument :

BNA_E


ClientSampleId :

JLC17DL




Tgt Ion:	252	Resp:	10314
Ion Ratio	Lower	Upper	
252	100		
253	39.7	18.2	27.4#
125	93.9	8.3	12.5#

Manual Integrations
APPROVED

Sohil
10/12/2018 6:35:03 PM

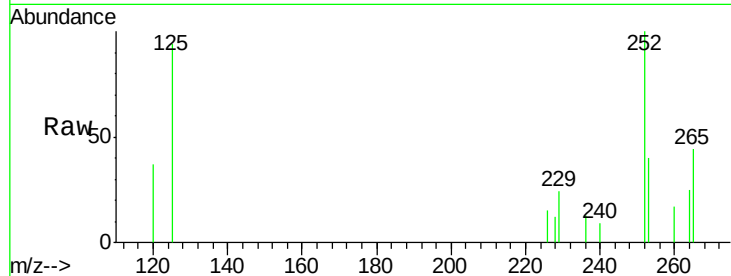

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

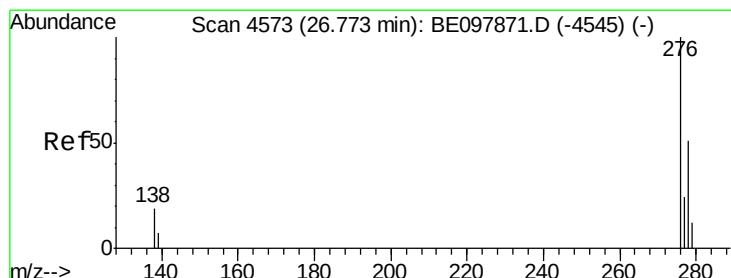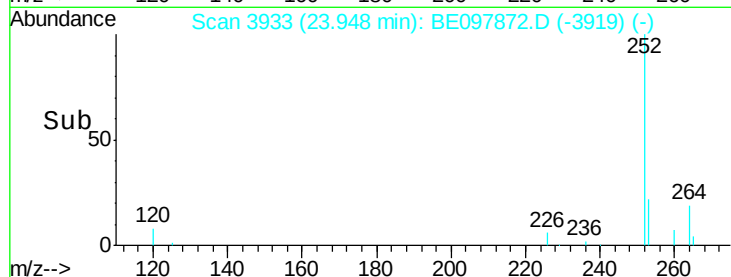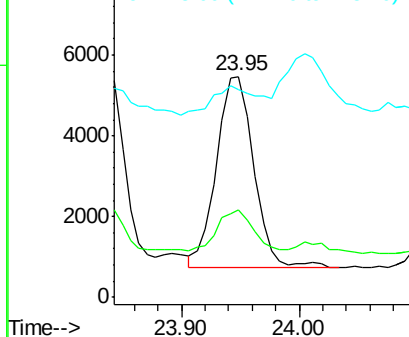

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.124 ng/ul

RT: 26.77 min Scan# 4572




Delta R.T. -0.01 min


Lab File: BE097872.D

Acq: 12 Oct 2018 00:14

Tgt Ion:	276	Resp:	8591
Ion Ratio	Lower	Upper	
276	100		
138	21.0	0.0	0.0#
227	0.0	0.0	0.0

Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 227.00 (226.70 to 227.70): E

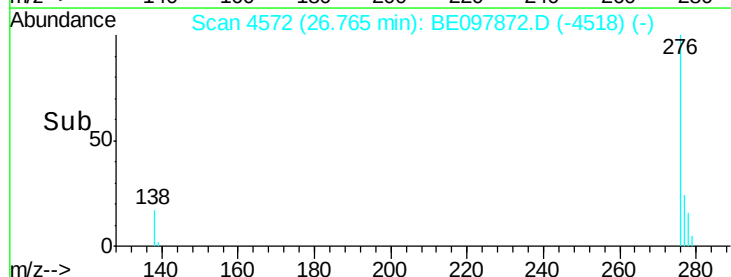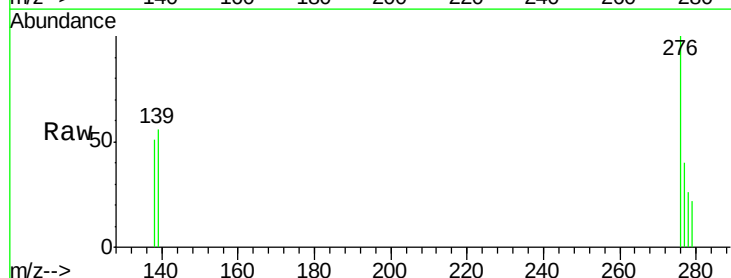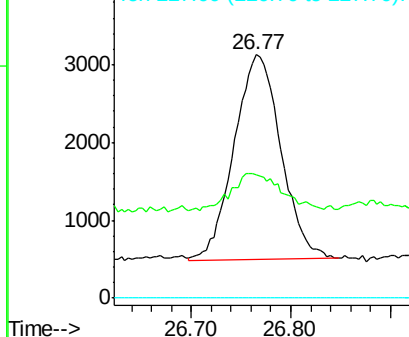

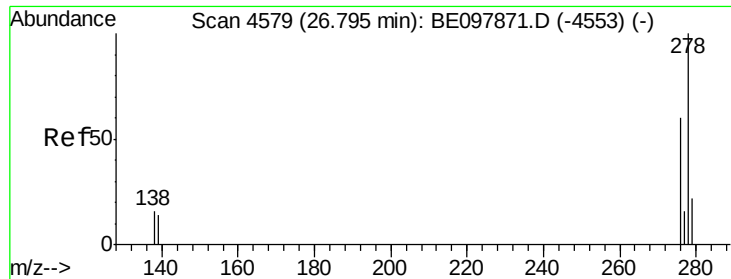

#25

Dibenzo(a,h)anthracene

Concen: 0.040 ng/ul

RT: 26.78 min Scan# 4577

Delta R.T. -0.01 min

Lab File: BE097872.D


Acq: 12 Oct 2018 00:14

Instrument :

BNA_E

ClientSampled :




JLC17DL

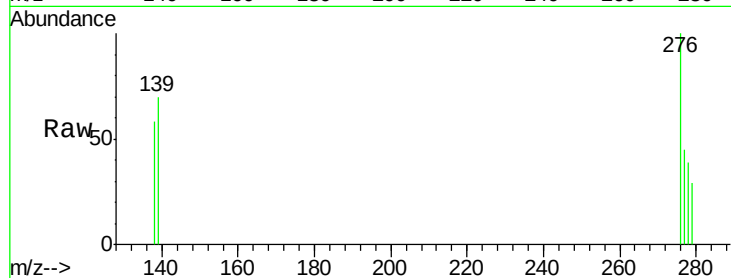

Tgt Ion:	278	Resp:	2301
Ion Ratio	Lower	Upper	
278	100		
139	181.7	10.9	16.3#
279	74.3	18.8	28.2#

Manual Integrations
APPROVED

Sohil
10/12/2018 6:35:03 PM

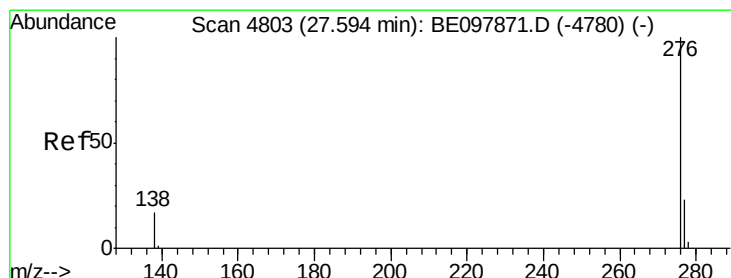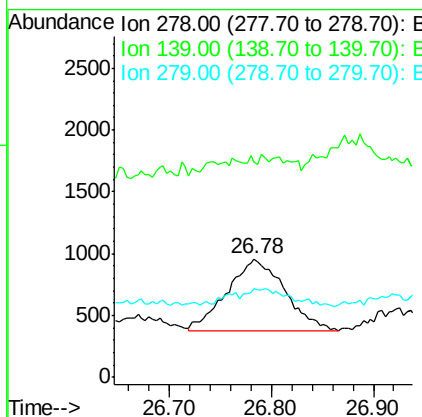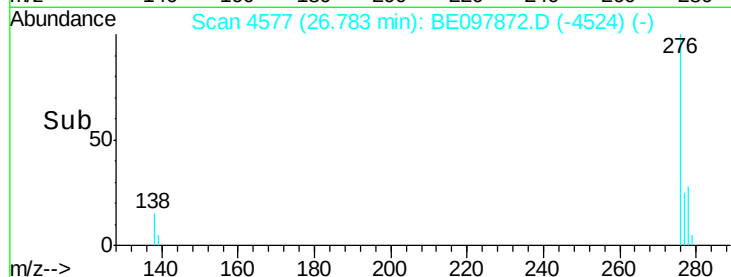

#26

Benzo(g,h,i)perylene


Concen: 0.162 ng/ul

RT: 27.60 min Scan# 4805

Delta R.T. 0.00 min

Lab File: BE097872.D

Acq: 12 Oct 2018 00:14

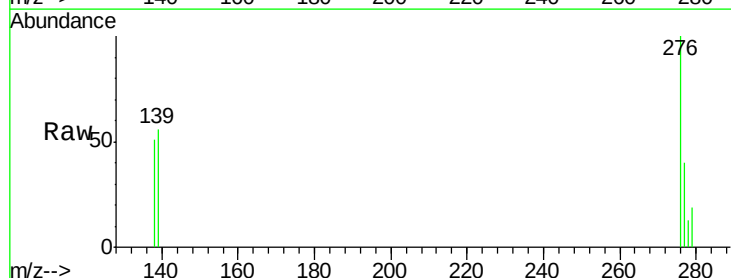

Tgt Ion:	276	Resp:	9806
Ion Ratio	Lower	Upper	
276	100		
138	51.4	14.3	21.5#
277	39.7	19.5	29.3#

